

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
 Data File : VX035148.D
 Acq On : 19 Apr 2023 01:20
 Operator : JC/MD
 Sample : 02397-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035148.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	15	rBV2	18606	17791	0.55%	0.086%
2	1.264	26	29	31	rBV2	6706	6173	0.19%	0.030%
3	1.306	31	36	40	rBV	16164	35099	1.09%	0.169%
4	1.367	43	46	59	rVV	258212	305991	9.48%	1.474%
5	1.672	92	96	104	rBV	178954	227991	7.06%	1.098%
6	2.306	194	200	209	rBV	444245	698647	21.65%	3.366%
7	2.788	275	279	281	rBV4	1158	1647	0.05%	0.008%
8	3.099	325	330	331	rBV4	1291	1880	0.06%	0.009%
9	3.221	348	350	351	rVB2	335	202	0.01%	0.001%
10	3.263	355	357	358	rBV	387	332	0.01%	0.002%
11	3.446	382	387	393	rVB3	1502	3214	0.10%	0.015%
12	3.520	396	399	401	rBV2	280	276	0.01%	0.001%
13	3.605	407	413	415	rBV3	914	1559	0.05%	0.008%
14	3.648	419	420	421	rVV	640	243	0.01%	0.001%
15	3.672	421	424	427	rVB3	272	267	0.01%	0.001%
16	3.897	459	461	463	rBV2	245	269	0.01%	0.001%
17	4.056	485	487	490	rBV2	240	303	0.01%	0.001%
18	4.129	497	499	501	rBV	250	261	0.01%	0.001%
19	4.397	541	543	544	rBV2	234	219	0.01%	0.001%
20	4.458	544	553	576	rVV	119695	368920	11.43%	1.777%
21	4.928	629	630	632	rVB2	386	279	0.01%	0.001%
22	4.958	632	635	636	rBV	320	245	0.01%	0.001%
23	5.056	638	651	669	rVV	244742	760570	23.56%	3.664%
24	5.440	712	714	715	rBV	189	193	0.01%	0.001%
25	5.464	716	718	721	rVV2	277	352	0.01%	0.002%
26	5.653	747	749	751	rBV	257	239	0.01%	0.001%
27	5.775	765	769	772	rVB2	149	218	0.01%	0.001%
28	5.818	772	776	780	rVB3	431	713	0.02%	0.003%
29	5.970	789	801	825	rBV2	670676	2062345	63.90%	9.935%
30	6.360	863	865	868	rBV2	377	325	0.01%	0.002%
31	6.385	868	869	872	rBV3	420	380	0.01%	0.002%
32	6.488	884	886	888	rVB2	280	196	0.01%	0.001%
33	6.549	894	896	900	rBV3	204	240	0.01%	0.001%
34	6.659	911	914	917	rVB2	319	380	0.01%	0.002%
35	6.757	921	930	945	rBV	452369	1100677	34.10%	5.302%
36	7.116	983	989	997	rVB4	1963	4367	0.14%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
 Data File : VX035148.D
 Acq On : 19 Apr 2023 01:20
 Operator : JC/MD
 Sample : 02397-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	7.214	1002	1005	1007	rBV2	311	470	0.01%	0.002%
38	7.305	1011	1020	1038	rBV	414835	906543	28.09%	4.367%
39	7.488	1045	1050	1054	rBV4	1037	2138	0.07%	0.010%
40	7.568	1061	1063	1065	rBV	233	196	0.01%	0.001%
41	7.592	1065	1067	1071	rVB3	314	339	0.01%	0.002%
42	7.744	1088	1092	1097	rBV3	305	492	0.02%	0.002%
43	7.848	1107	1109	1112	rBV2	233	289	0.01%	0.001%
44	7.952	1118	1126	1132	rBV4	1303	3624	0.11%	0.017%
45	8.080	1144	1147	1150	rBV2	198	291	0.01%	0.001%
46	8.324	1180	1187	1203	rBV	249499	420276	13.02%	2.025%
47	8.488	1209	1214	1215	rBV5	733	1370	0.04%	0.007%
48	8.647	1233	1240	1257	rBV	1047379	1662291	51.50%	8.008%
49	8.848	1272	1273	1274	rBV	549	209	0.01%	0.001%
50	8.890	1278	1280	1282	rVB2	266	208	0.01%	0.001%
51	8.951	1284	1290	1305	rBV	176477	270045	8.37%	1.301%
52	9.128	1317	1319	1322	rBV3	430	646	0.02%	0.003%
53	9.171	1324	1326	1327	rBV2	373	192	0.01%	0.001%
54	9.275	1341	1343	1345	rBV3	887	904	0.03%	0.004%
55	9.317	1348	1350	1351	rBV2	272	195	0.01%	0.001%
56	9.384	1355	1361	1377	rBV	562523	816145	25.29%	3.932%
57	9.653	1403	1405	1406	rBV2	413	332	0.01%	0.002%
58	9.671	1406	1408	1410	rVB2	589	371	0.01%	0.002%
59	9.866	1437	1440	1441	rBV2	256	266	0.01%	0.001%
60	10.055	1465	1471	1473	rBV	933977	1484826	46.00%	7.153%
61	10.323	1513	1515	1518	rBV3	501	542	0.02%	0.003%
62	10.671	1571	1572	1573	rVV	410	213	0.01%	0.001%
63	10.719	1577	1580	1582	rVB3	365	301	0.01%	0.001%
64	10.756	1582	1586	1588	rBV2	337	308	0.01%	0.001%
65	10.780	1588	1590	1594	rVB2	190	299	0.01%	0.001%
66	10.915	1609	1612	1613	rVB2	392	286	0.01%	0.001%
67	10.982	1621	1623	1625	rBV2	267	297	0.01%	0.001%
68	11.036	1630	1632	1634	rVB	447	347	0.01%	0.002%
69	11.189	1652	1657	1667	rBV	660397	844677	26.17%	4.069%
70	11.317	1674	1678	1682	rVB4	756	949	0.03%	0.005%
71	11.366	1682	1686	1690	rBV2	6303	7650	0.24%	0.037%
72	11.457	1698	1701	1707	rVB2	3259	3564	0.11%	0.017%
73	11.707	1737	1742	1746	rVB4	868	1367	0.04%	0.007%
74	11.847	1764	1765	1767	rBV2	375	284	0.01%	0.001%
75	11.896	1771	1773	1775	rBV	483	575	0.02%	0.003%
76	11.969	1779	1785	1789	rBV	551474	708253	21.94%	3.412%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
 Data File : VX035148.D
 Acq On : 19 Apr 2023 01:20
 Operator : JC/MD
 Sample : 02397-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041823WMA.M
 Title : VOC Analysis

77	12.036	1789	1796	1807	rVB2	1653966	3227570	100.00%	15.548%
78	12.219	1823	1826	1833	rBV2	7668	11914	0.37%	0.057%
79	12.323	1837	1843	1855	rVV2	1251386	2167091	67.14%	10.439%
80	12.774	1915	1917	1918	rBV	284	194	0.01%	0.001%
81	12.853	1928	1930	1932	rBV2	481	483	0.01%	0.002%
82	12.920	1937	1941	1949	rVB	8916	12492	0.39%	0.060%
83	13.060	1955	1964	1969	rVV3	14852	28952	0.90%	0.139%
84	13.109	1969	1972	1979	rVB	13273	17756	0.55%	0.086%
85	13.195	1982	1986	1990	rVV3	3289	4340	0.13%	0.021%
86	13.262	1994	1997	2000	rBV3	374	559	0.02%	0.003%
87	13.390	2013	2018	2021	rVB4	1563	2326	0.07%	0.011%
88	13.585	2045	2050	2069	rVB	1528664	1881125	58.28%	9.062%
89	13.963	2106	2112	2121	rBV	328997	433999	13.45%	2.091%
90	14.048	2124	2126	2128	rBV2	570	455	0.01%	0.002%
91	14.146	2140	2142	2145	rBV2	515	516	0.02%	0.002%
92	14.213	2151	2153	2155	rVB2	406	309	0.01%	0.001%
93	14.237	2155	2157	2162	rBV4	614	676	0.02%	0.003%
94	14.365	2176	2178	2179	rBV	420	276	0.01%	0.001%
95	14.450	2190	2192	2196	rBV2	491	793	0.02%	0.004%
96	14.536	2204	2206	2209	rBV3	738	799	0.02%	0.004%
97	14.627	2219	2221	2223	rBV2	751	672	0.02%	0.003%
98	14.780	2240	2246	2255	rBV	40081	62190	1.93%	0.300%
99	15.249	2317	2323	2334	rVB	107395	152421	4.72%	0.734%
100	16.511	2526	2530	2536	rVB5	3134	5226	0.16%	0.025%




Sum of corrected areas: 20758707

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
Data File : VX035148.D
Acq On : 19 Apr 2023 01:20
Operator : JC/MD
Sample : 02397-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

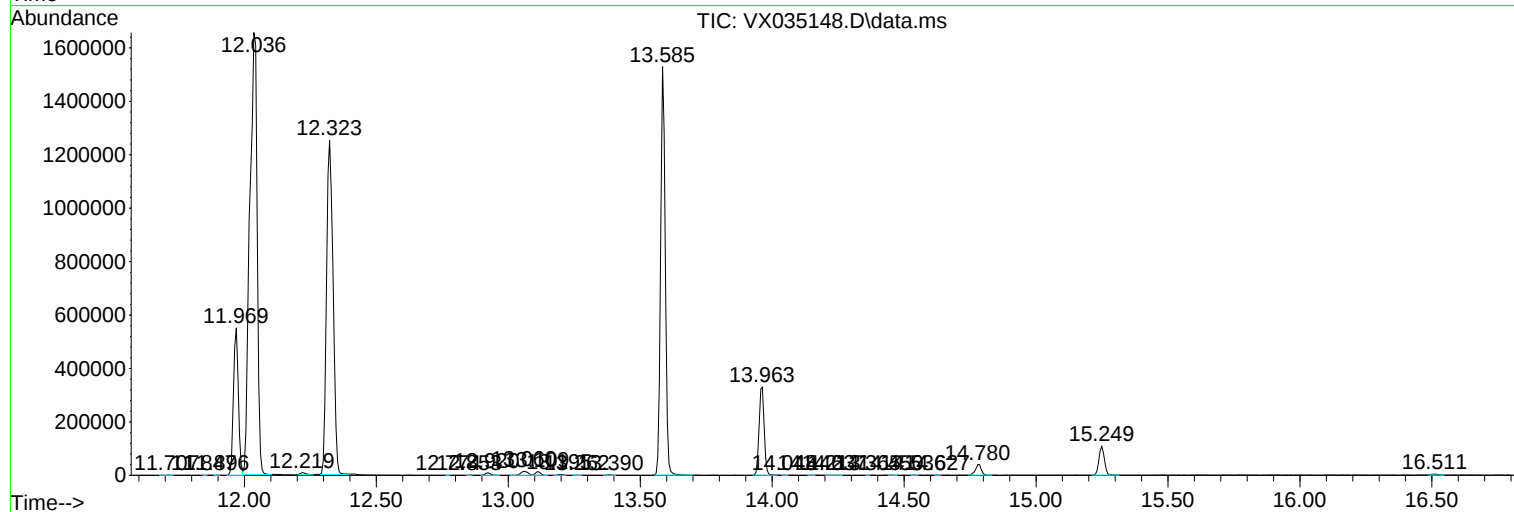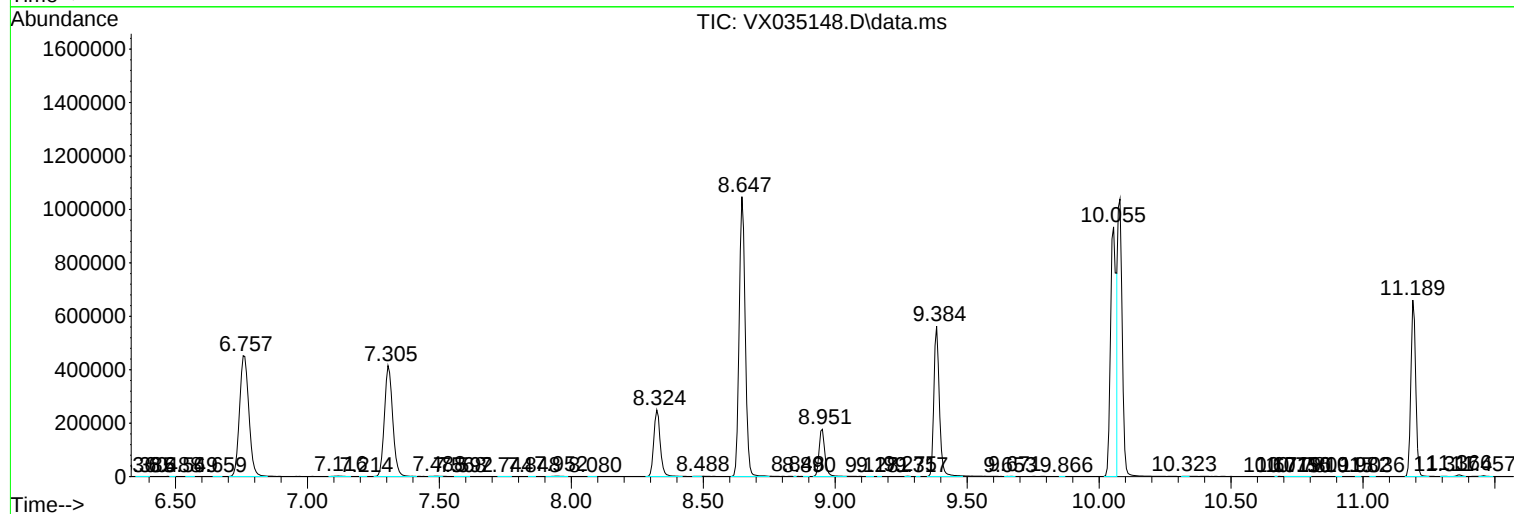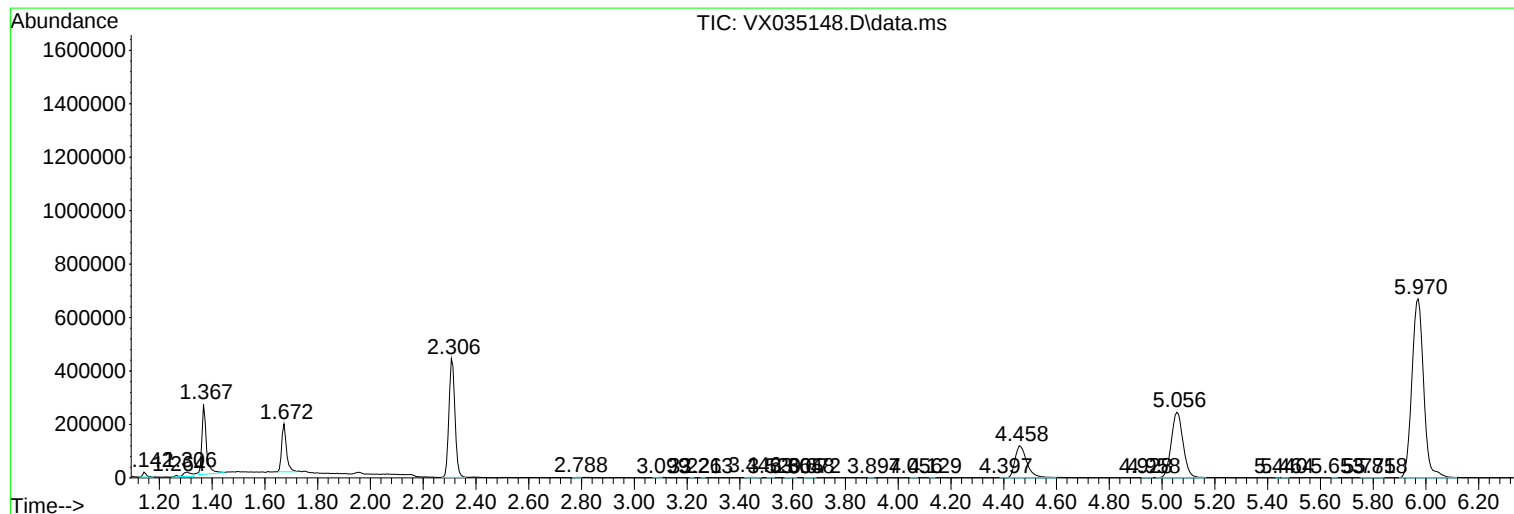

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
Data File : VX035148.D
Acq On : 19 Apr 2023 01:20
Operator : JC/MD
Sample : 02397-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
Data File : VX035148.D
Acq On : 19 Apr 2023 01:20
Operator : JC/MD
Sample : 02397-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------