
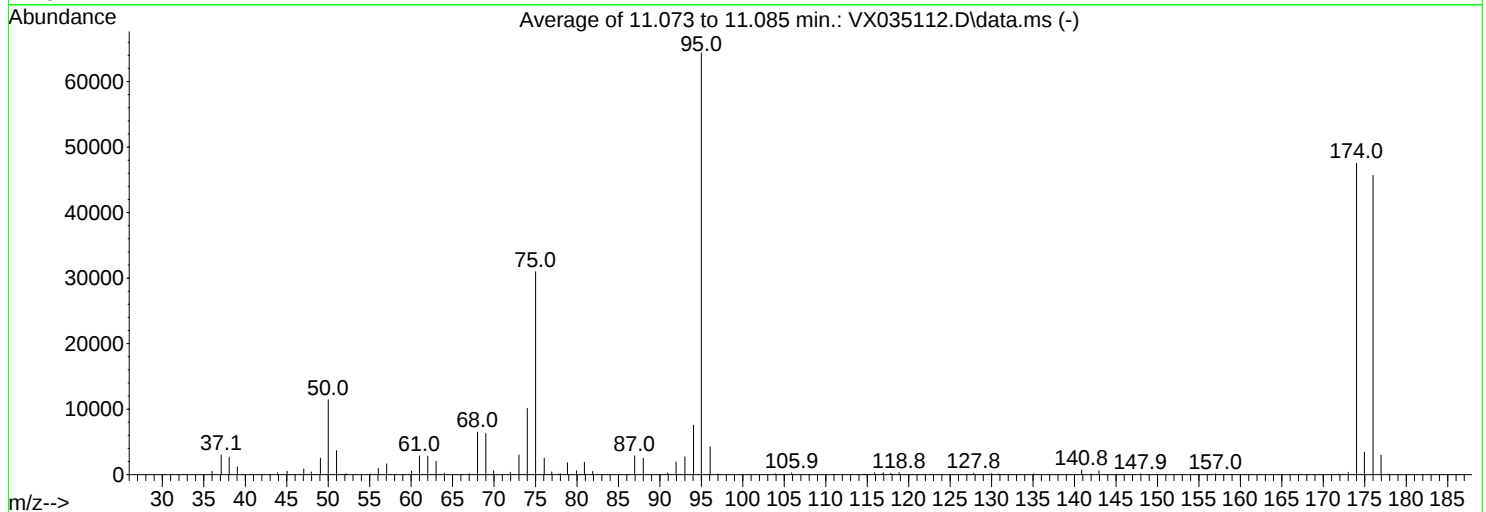


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
Data File : VX035112.D
Acq On : 18 Apr 2023 08:20
Operator : JC/MD
Sample : BFB623
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB623

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041823WMA.M
Title : VOC Analysis
Last Update : Thu Apr 20 23:27:37 2023

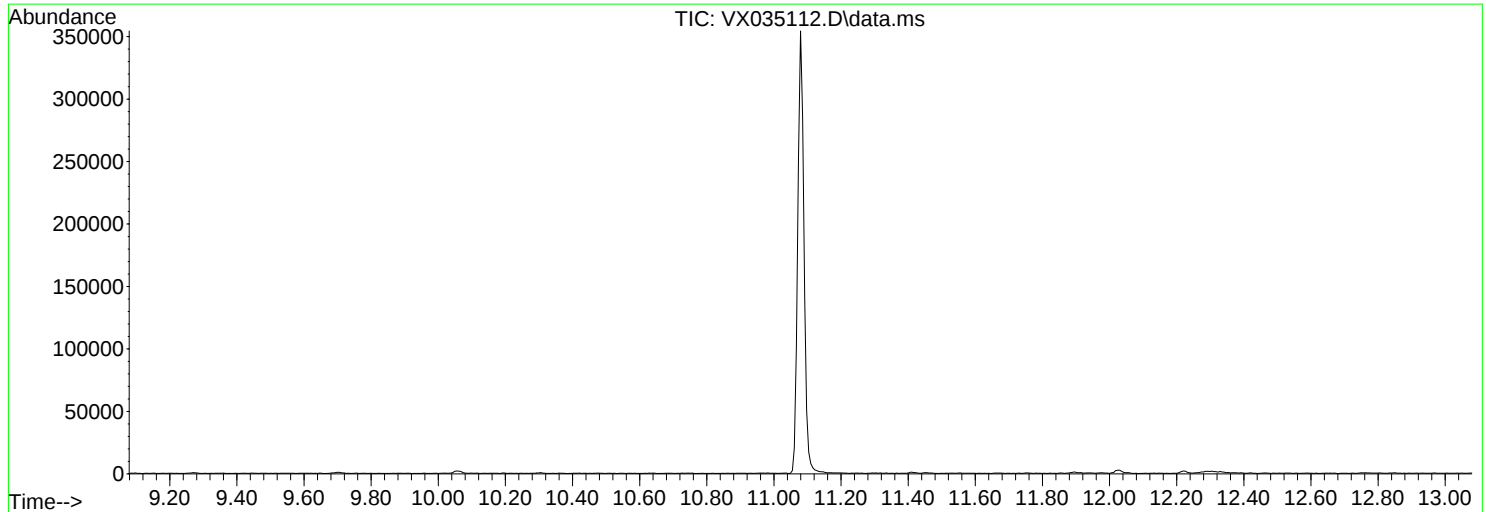

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.8	11435	PASS
75	95	30	80	48.1	30976	PASS
95	95	100	100	100.0	64381	PASS
96	95	5	9	6.7	4282	PASS
173	174	0.00	2	0.8	370	PASS
174	95	50	120	73.8	47517	PASS
175	174	5	9	7.3	3449	PASS
176	174	95	101	96.1	45677	PASS
177	176	5	9	6.5	2989	PASS

m/z	Abundance
40.00	262.0
43.90	335.0

Instrument :
MSVOA_X
ClientSampleId :
BFB623

m/z	Abundance
35.90	500.0
37.10	3030.0
38.00	2978.0
39.00	1080.0
40.00	145.0
44.10	622.0
45.10	566.0
47.00	775.0
47.90	446.0
49.00	2529.0
50.00	11366.0
51.00	3479.0
52.10	152.0
55.10	76.0
56.00	794.0
57.00	1712.0
58.00	64.0
60.10	478.0
61.00	2596.0
62.00	2805.0
63.00	2014.0
64.10	187.0
67.00	158.0
68.00	5809.0
69.00	5703.0
70.00	625.0
71.90	419.0
73.00	2742.0
74.00	8751.0
75.00	27624.0
76.00	2359.0
77.00	358.0
77.80	304.0
78.90	1709.0
80.00	457.0
80.90	1686.0
82.00	482.0
87.00	2714.0
88.00	2276.0
91.00	296.0
92.00	2074.0
93.00	2205.0
94.00	6363.0
95.00	56872.0
96.00	3719.0
97.10	137.0
103.90	177.0
105.00	123.0
106.00	217.0
110.90	86.0
115.90	224.0
116.80	351.0
117.90	205.0
118.80	312.0
128.00	182.0
128.70	64.0
130.10	244.0
135.10	148.0
136.80	119.0
140.90	553.0
141.90	111.0
142.90	300.0
145.00	76.0
145.70	62.0
148.00	104.0
154.80	80.0
156.90	119.0
171.80	149.0
174.00	34456.0
174.90	2331.0
176.00	34456.0
177.00	2307.0
177.90	118.0

Instrument :
MSVOA_X
ClientSampleId :
BFB623

m/z	Abundance
36.00	587.0
37.10	3444.0
38.10	2901.0
39.10	1468.0
39.90	239.0
43.90	686.0
45.00	662.0
46.00	84.0
47.10	1377.0
48.00	432.0
49.10	2974.0
50.00	13460.0
51.00	4472.0
52.20	196.0
55.00	153.0
56.00	1216.0
57.00	1728.0
58.00	99.0
60.10	711.0
61.00	3324.0
62.00	3349.0
63.00	2697.0
64.00	289.0
66.90	222.0
68.00	8110.0
69.00	7668.0
69.90	595.0
71.90	357.0
73.00	3610.0
74.00	12259.0
75.00	37696.0
76.00	2934.0
76.90	564.0
78.00	296.0
78.90	1912.0
80.00	773.0
80.90	2210.0
81.80	510.0
83.20	75.0
87.00	3040.0
87.90	2506.0
91.00	218.0
92.00	2148.0
93.10	3552.0
94.00	9082.0
95.00	76808.0
96.10	5090.0
97.00	143.0
104.00	235.0
105.00	56.0
105.80	303.0
106.80	68.0
113.10	61.0
114.70	59.0
115.10	78.0
116.00	294.0
117.00	512.0
117.80	254.0
118.90	349.0
127.80	343.0
128.70	84.0
129.90	259.0
130.80	146.0
135.10	171.0
136.80	106.0
140.90	825.0
142.00	89.0
143.00	812.0
145.10	63.0
145.70	113.0
147.00	59.0
148.00	161.0
149.90	88.0
152.80	56.0
155.00	153.0
157.00	239.0
158.90	77.0
171.90	179.0
173.00	688.0
174.00	57832.0
175.00	4299.0
176.00	53152.0
176.90	3188.0
177.90	126.0

Instrument :
MSVOA_X
ClientSampleId :
BFB623

m/z	Abundance
36.10	452.0
37.10	2582.0
38.10	2138.0
39.10	1067.0
39.90	183.0
43.90	612.0
45.10	370.0
47.00	484.0
48.00	392.0
49.10	2080.0
50.00	9478.0
51.00	3025.0
52.10	124.0
55.00	121.0
56.10	924.0
57.10	1492.0
59.90	470.0
61.00	2629.0
62.00	2362.0
62.90	1491.0
63.90	202.0
67.10	139.0
68.00	5475.0
69.00	5444.0
70.00	637.0
72.00	300.0
73.00	2677.0
74.00	9436.0
75.00	27608.0
76.10	2294.0
76.90	330.0
78.00	251.0
78.80	1794.0
79.90	565.0
80.90	1761.0
81.90	447.0
86.90	2848.0
88.10	2662.0
90.90	234.0
91.90	1572.0
92.90	2358.0
94.10	7180.0
95.00	59464.0
96.10	4037.0
96.90	140.0
103.70	205.0
105.90	314.0
114.70	99.0
115.10	59.0
115.80	297.0
116.90	388.0
117.80	229.0
118.90	292.0
127.90	207.0
129.00	114.0
129.70	209.0
130.80	120.0
135.10	109.0
140.80	745.0
142.10	145.0
142.90	678.0
147.10	61.0
147.90	179.0
149.90	78.0
152.80	79.0
154.80	98.0
157.10	78.0
159.00	86.0
171.40	82.0
173.00	422.0
174.00	50264.0
175.00	3718.0
176.00	49424.0
177.00	3471.0
177.90	76.0

Instrument :
MSVOA_X
ClientSampleId :
BFB623