


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX041824\  
Data File : VX041152.D  
Acq On : 18 Apr 2024 08:34  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X041624W.M  
Title : SW846 8260  
Last Update : Wed Apr 17 02:04:44 2024

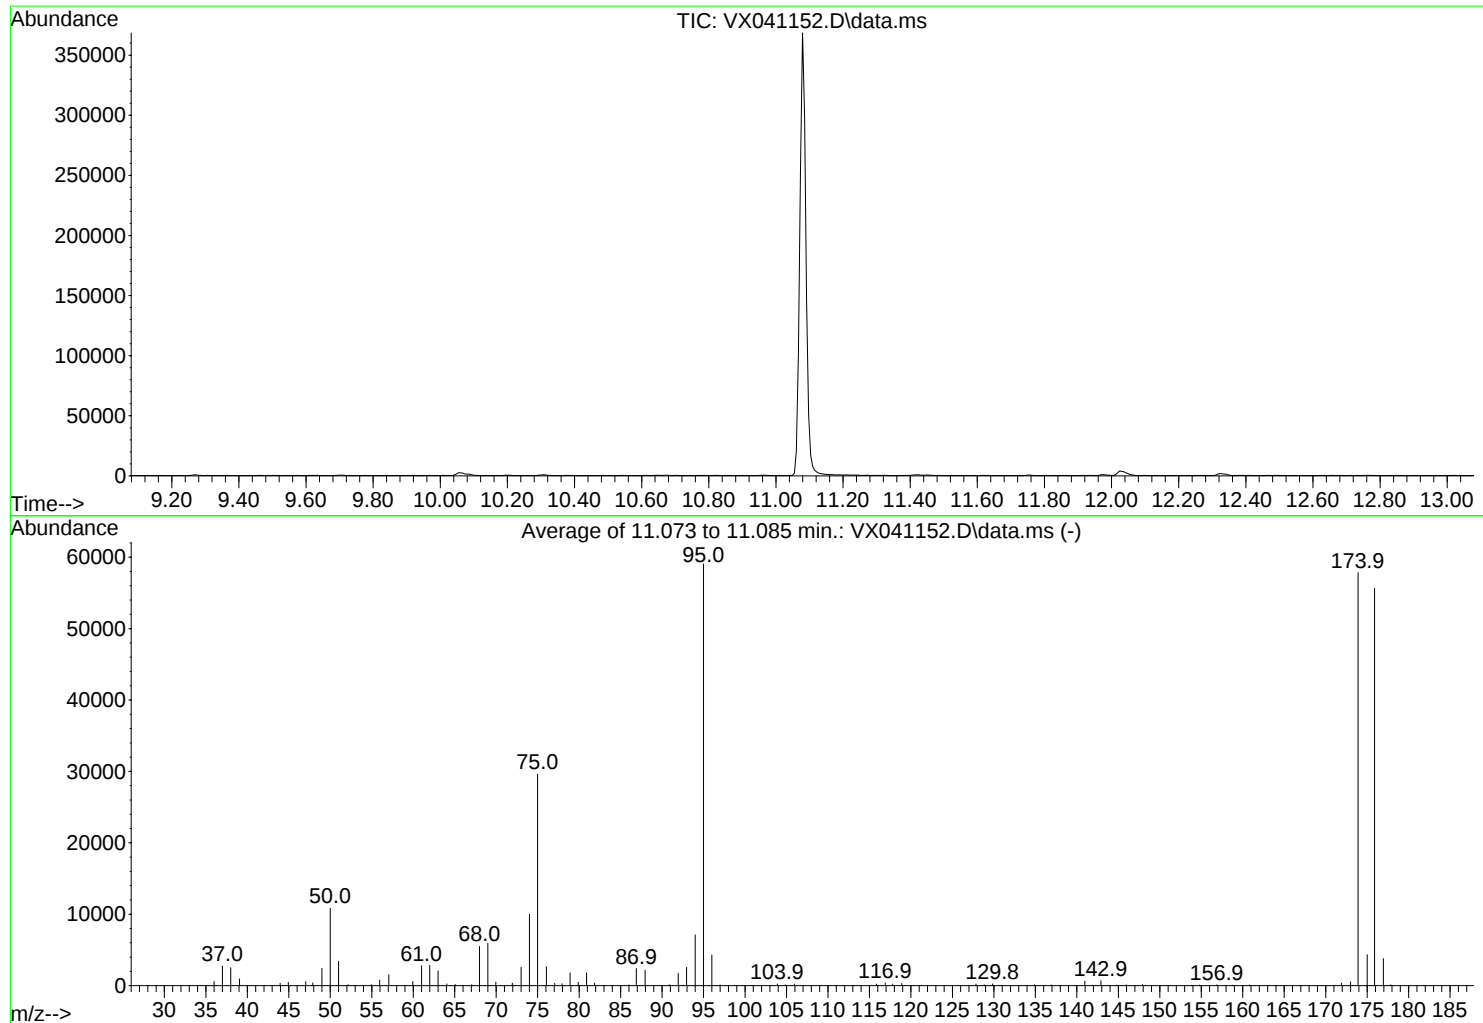

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 18.3  | 10834 | PASS      |
| 75     | 95      | 30     | 60     | 50.1  | 29621 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 59069 | PASS      |
| 96     | 95      | 5      | 9      | 7.3   | 4284  | PASS      |
| 173    | 174     | 0.00   | 2      | 0.9   | 527   | PASS      |
| 174    | 95      | 50     | 100    | 97.9  | 57848 | PASS      |
| 175    | 174     | 5      | 9      | 7.5   | 4329  | PASS      |
| 176    | 174     | 95     | 101    | 96.2  | 55656 | PASS      |
| 177    | 176     | 5      | 9      | 6.8   | 3787  | PASS      |