

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX041919\
 Data File : VX009080.D
 Acq On : 19 Apr 2019 19:01
 Operator : JC/SP
 Sample : K2495-02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SS040RW056-190417

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.404	36	41	47	rBV	14427	17541	1.29%	0.188%
2	1.617	67	76	79	rBV6	7148	16706	1.23%	0.179%
3	2.611	234	239	249	rVB	23134	44395	3.27%	0.475%
4	2.843	270	277	287	rBV2	11226	25159	1.85%	0.269%
5	3.166	322	330	339	rBV4	6574	18266	1.34%	0.195%
6	4.306	508	517	527	rBV3	5227	17702	1.30%	0.189%
7	4.598	546	565	586	rBV	395409	1120094	82.43%	11.984%
8	5.501	701	713	726	rBV2	125796	367104	27.01%	3.928%
9	5.665	727	740	760	rVB	227504	662168	48.73%	7.085%
10	6.068	795	806	823	rBV	156690	418702	30.81%	4.480%
11	6.348	842	852	864	rVB2	38186	115255	8.48%	1.233%
12	6.860	923	936	949	rBV	369734	874949	64.39%	9.361%
13	7.214	984	994	1007	rBV	646717	1358910	100.00%	14.539%
14	8.055	1123	1132	1140	rVB	31315	62846	4.62%	0.672%
15	8.177	1145	1152	1163	rVB	33010	66322	4.88%	0.710%
16	8.714	1225	1240	1250	rBV	774248	1209755	89.02%	12.943%
17	9.335	1333	1342	1351	rBV	311911	448519	33.01%	4.799%
18	10.110	1463	1469	1478	rBV	694707	967308	71.18%	10.349%
19	10.341	1500	1507	1518	rBV3	6871	16829	1.24%	0.180%
20	11.134	1632	1637	1644	rBV	534087	700133	51.52%	7.491%
21	12.079	1786	1792	1800	rBV	639873	817827	60.18%	8.750%


Sum of corrected areas: 9346490

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX041919\
Data File : VX009080.D
Acq On : 19 Apr 2019 19:01
Operator : JC/SP
Sample : K2495-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SS040RW056-190417

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

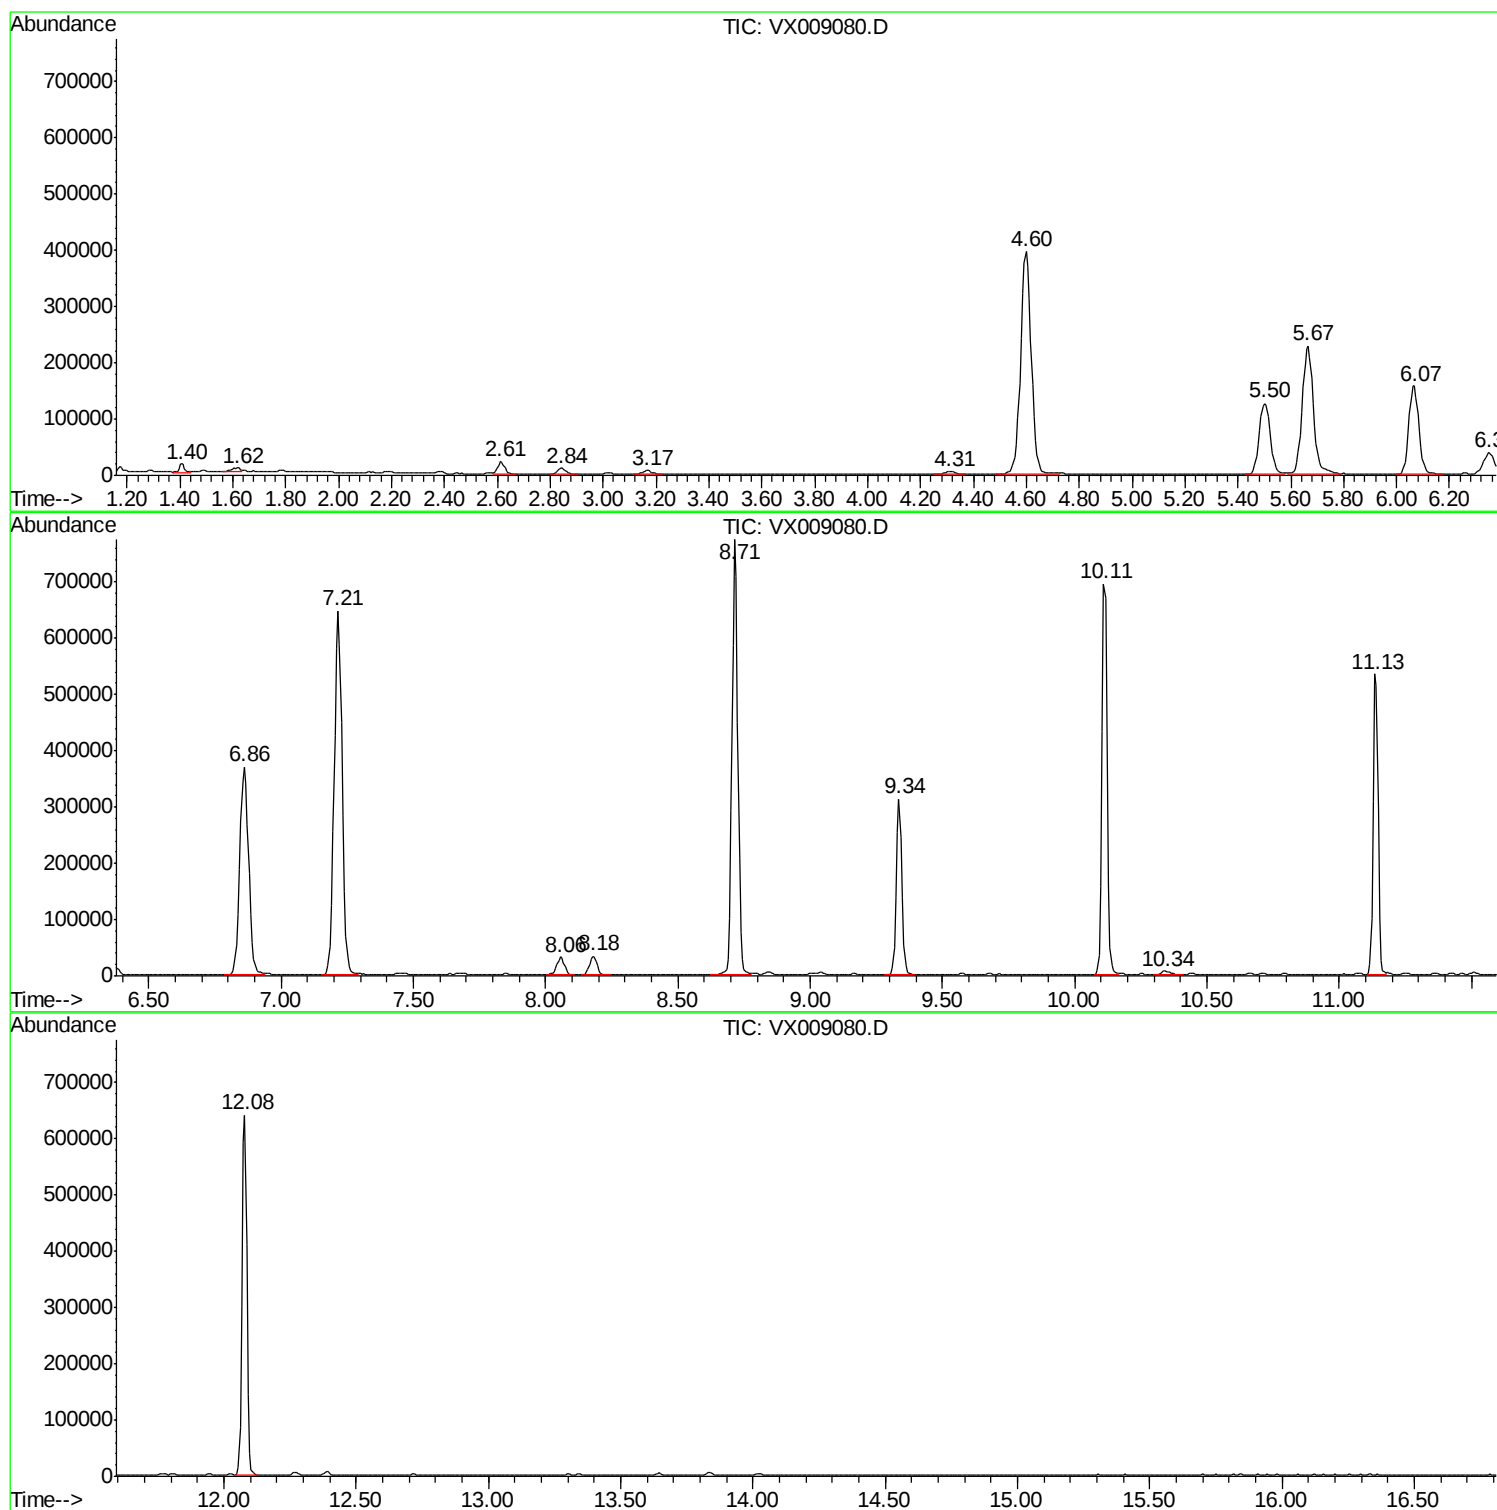

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX041919\
Data File : VX009080.D
Acq On : 19 Apr 2019 19:01
Operator : JC/SP
Sample : K2495-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SS040RW056-190417










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexane, 2,2-dimethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.35	6.59 ug/l	115255	1,4-Difluorobenzene	6.86

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexane, 2,2-dimethyl-	114	C8H18	000590-73-8	72
2			Pentane, 2,2,4-trimethyl-	114	C8H18	000540-84-1	72
3			Butane, 2,2,3,3-tetramethyl-	114	C8H18	000594-82-1	72
4			Hexane, 2,2,4-trimethyl-	128	C9H20	016747-26-5	59
5			Pentane, 2,2,4,4-tetramethyl-	128	C9H20	001070-87-7	59

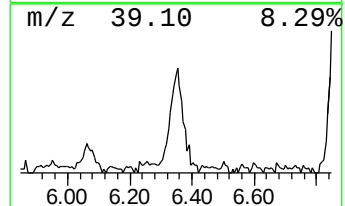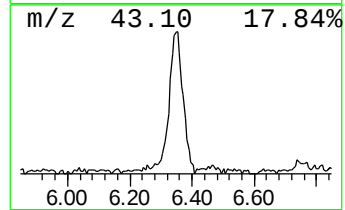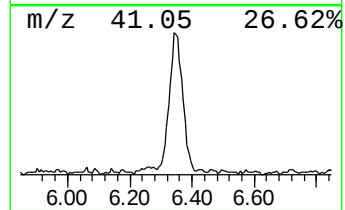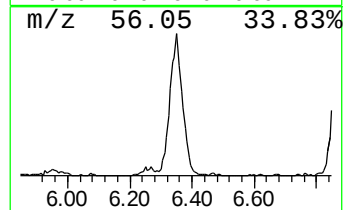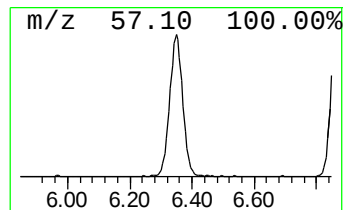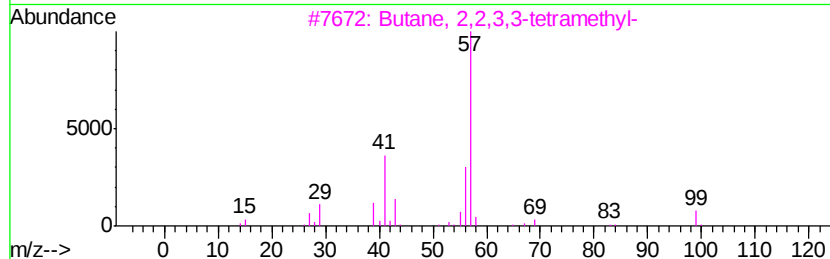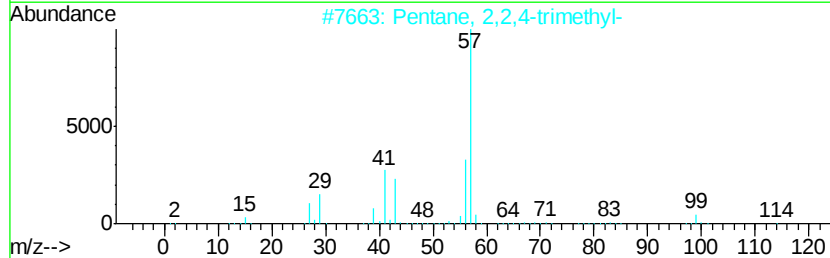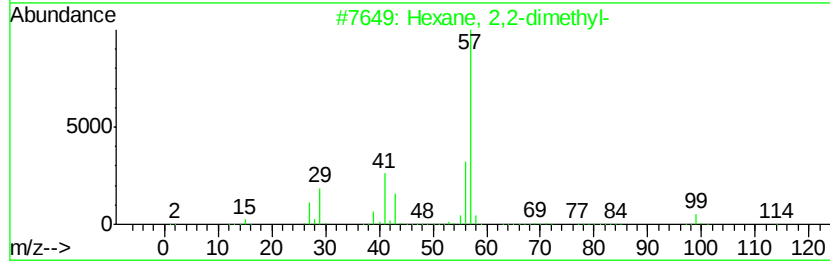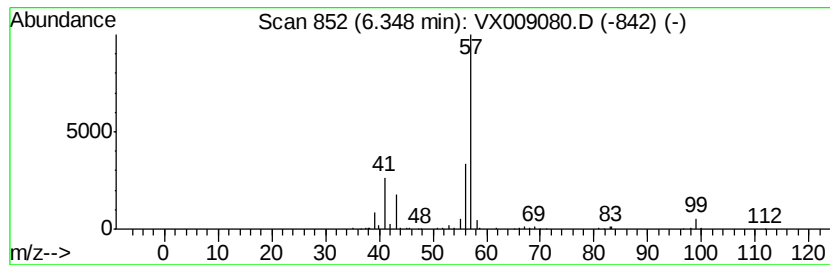

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_X\DATA\VX041919\
Data File : VX009080.D
Acq On : 19 Apr 2019 19:01
Operator : JC/SP
Sample : K2495-02
Misc : 5.0mL/MSV0A_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSV0A_X
ClientSampleId :
SS040RW056-190417

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_X\METHOD\82X041519W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexane, 2,2-dimet...	6.35	6.6	ug/l	115255	2	6.86	874949	50.0