


Chloromethane

Response Ratio

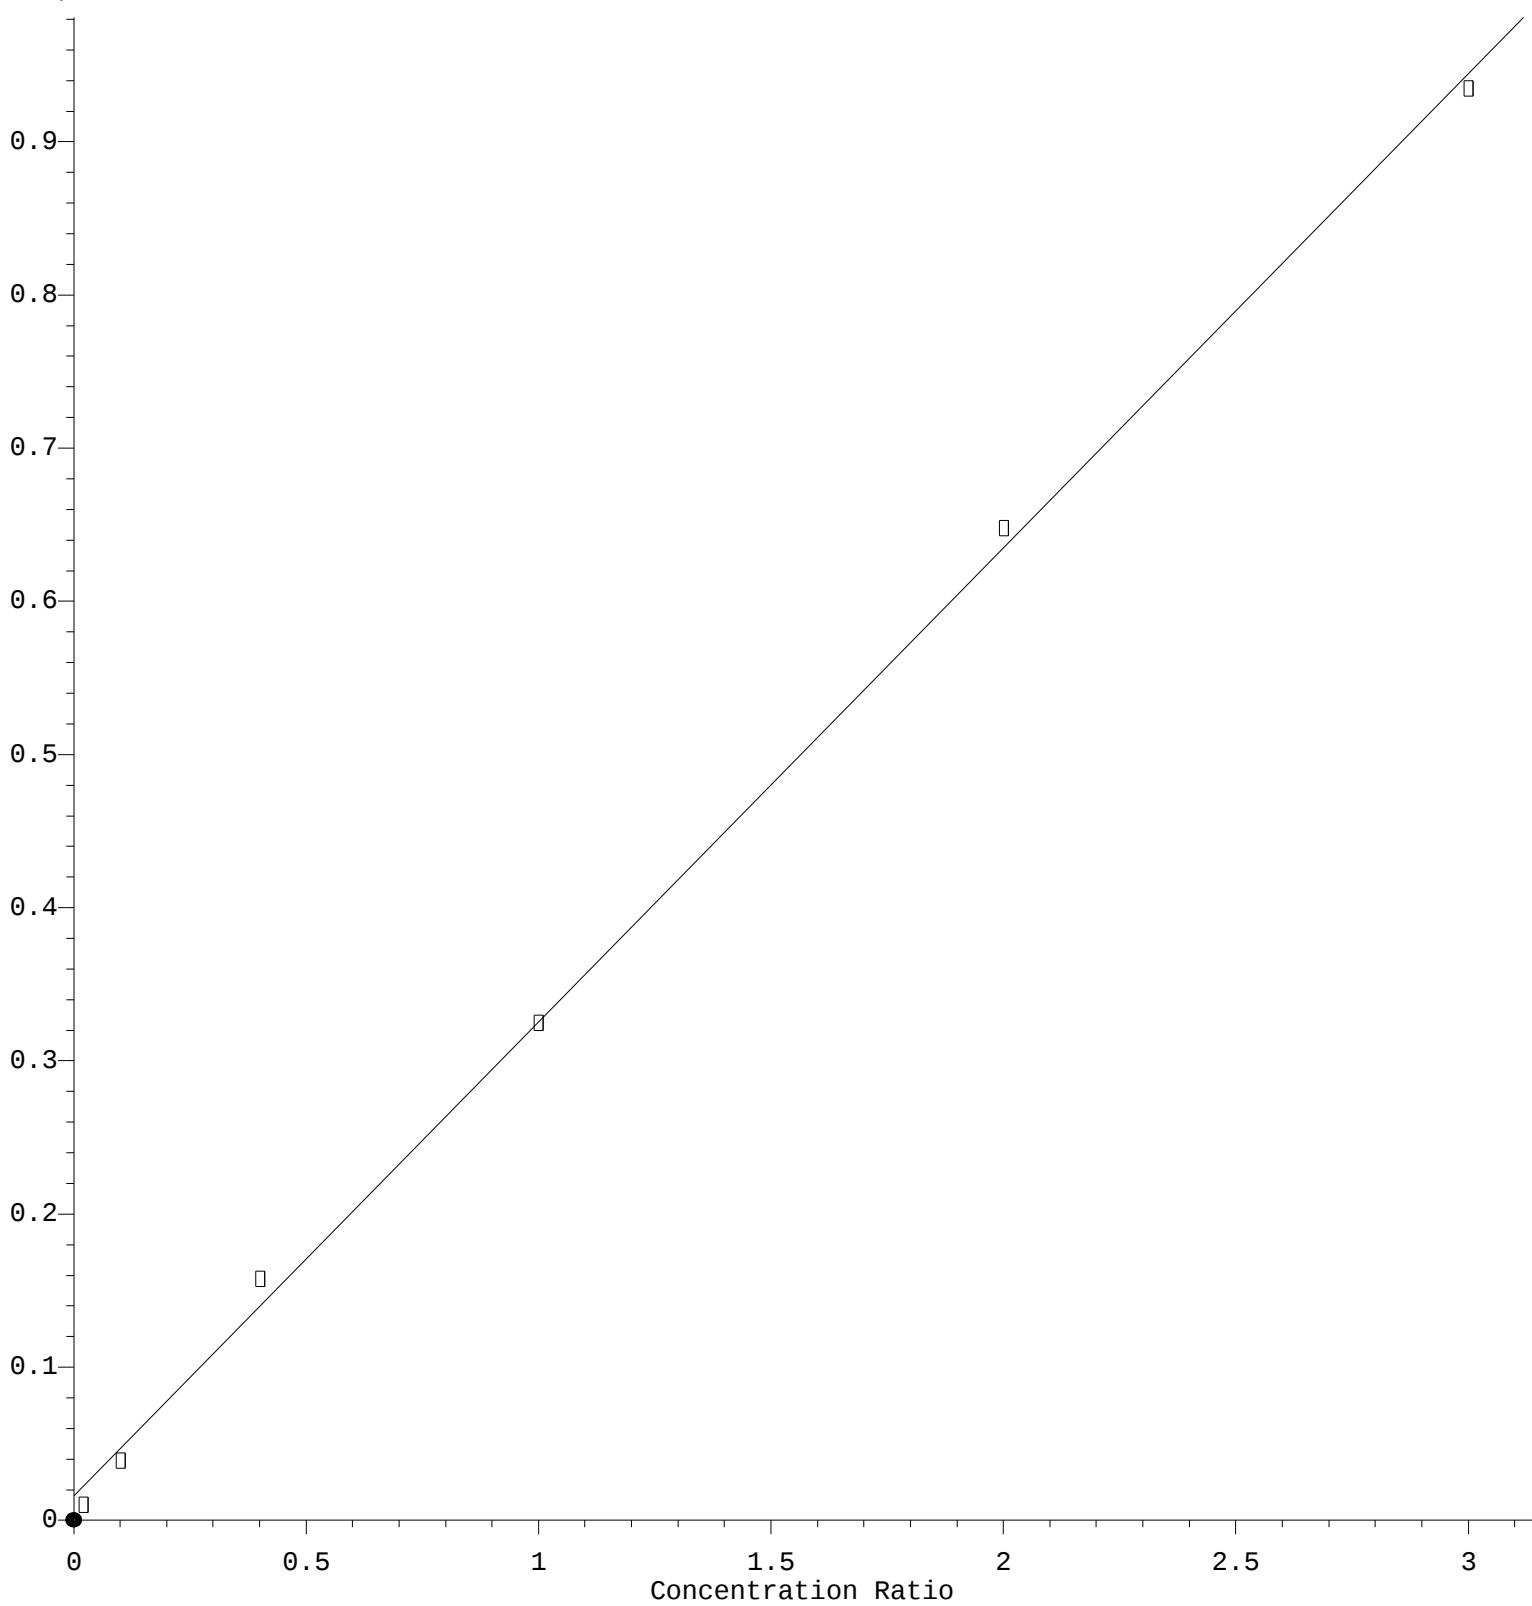

$$\text{Response} = 3.097\text{e-}001 * \text{Amt} + 1.570\text{e-}002$$


Coef of Det (r^2) = 0.998855 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M

Calibration Table Last Updated: Tue Apr 19 13:38:04 2022

Bromomethane

Response Ratio

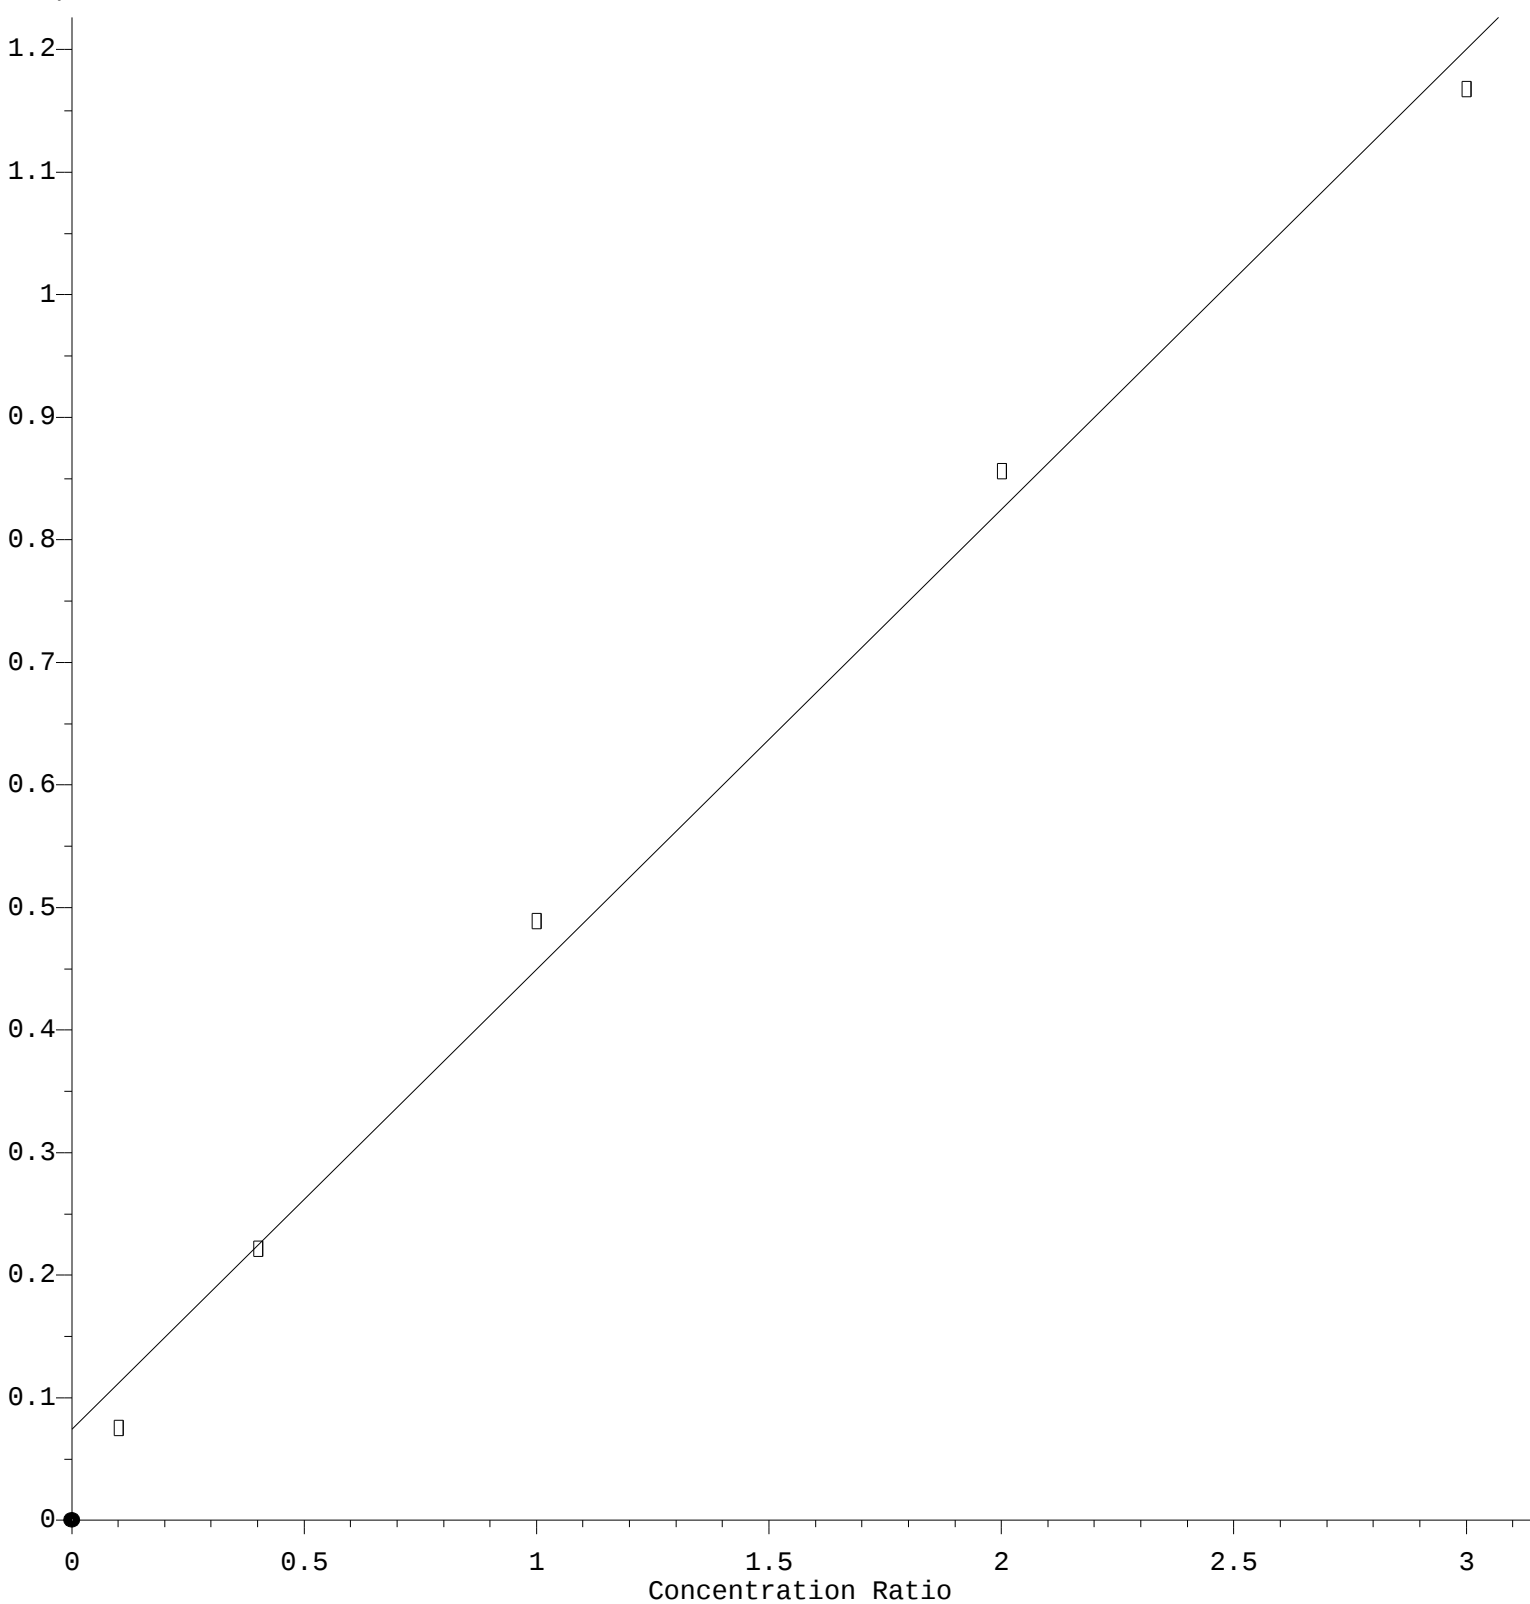

$$\text{Response} = 3.756\text{e-}001 * \text{Amt} + 7.351\text{e-}002$$


Coef of Det (r^2) = 0.993981 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M

Calibration Table Last Updated: Tue Apr 19 13:38:04 2022

Chloroethane

Response Ratio

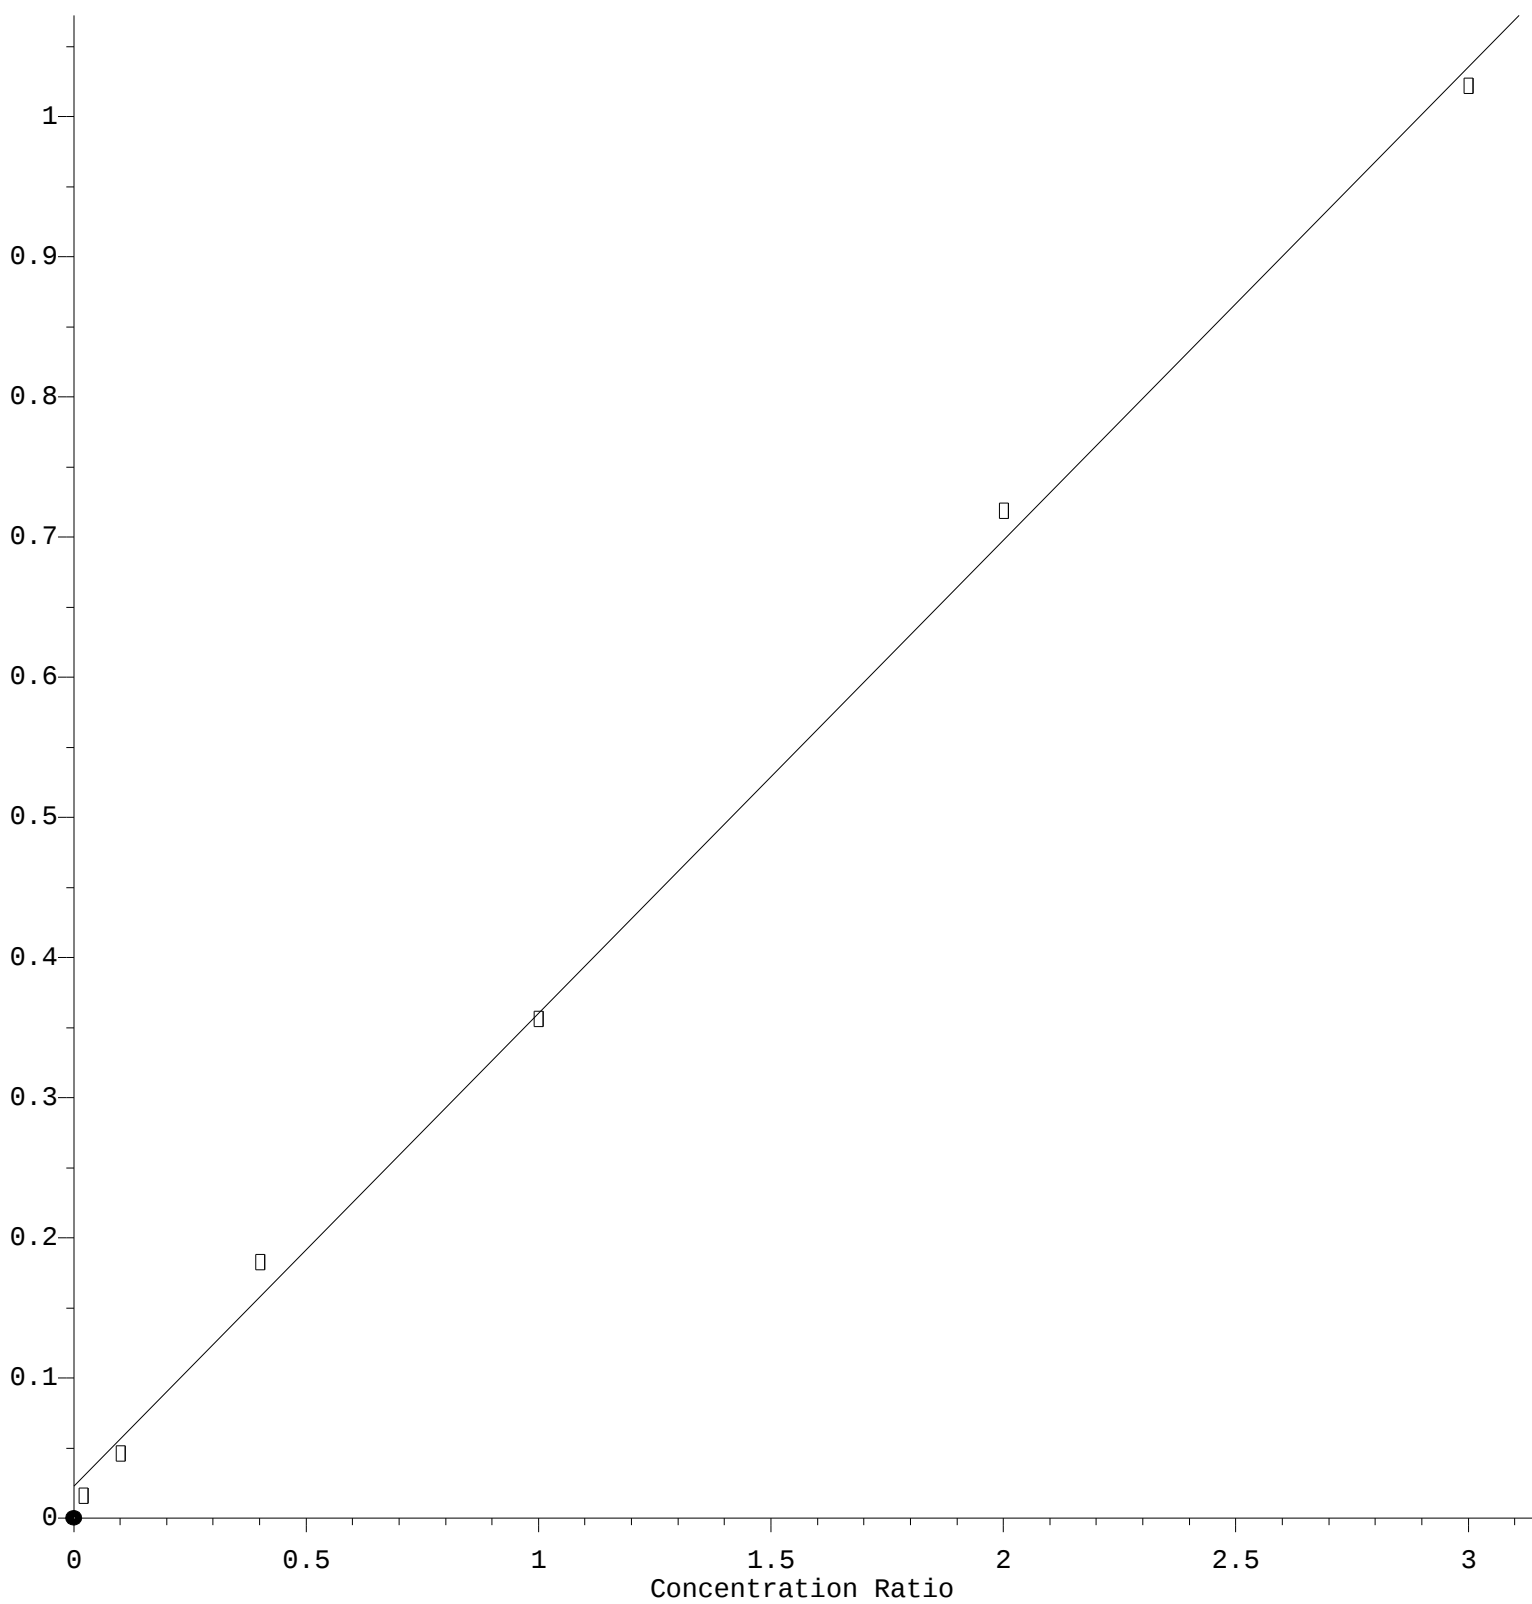

$$\text{Response} = 3.376\text{e-}001 * \text{Amt} + 2.329\text{e-}002$$


Coef of Det (r^2) = 0.998073 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M

Calibration Table Last Updated: Tue Apr 19 13:38:04 2022

Diethyl Ether

Response Ratio

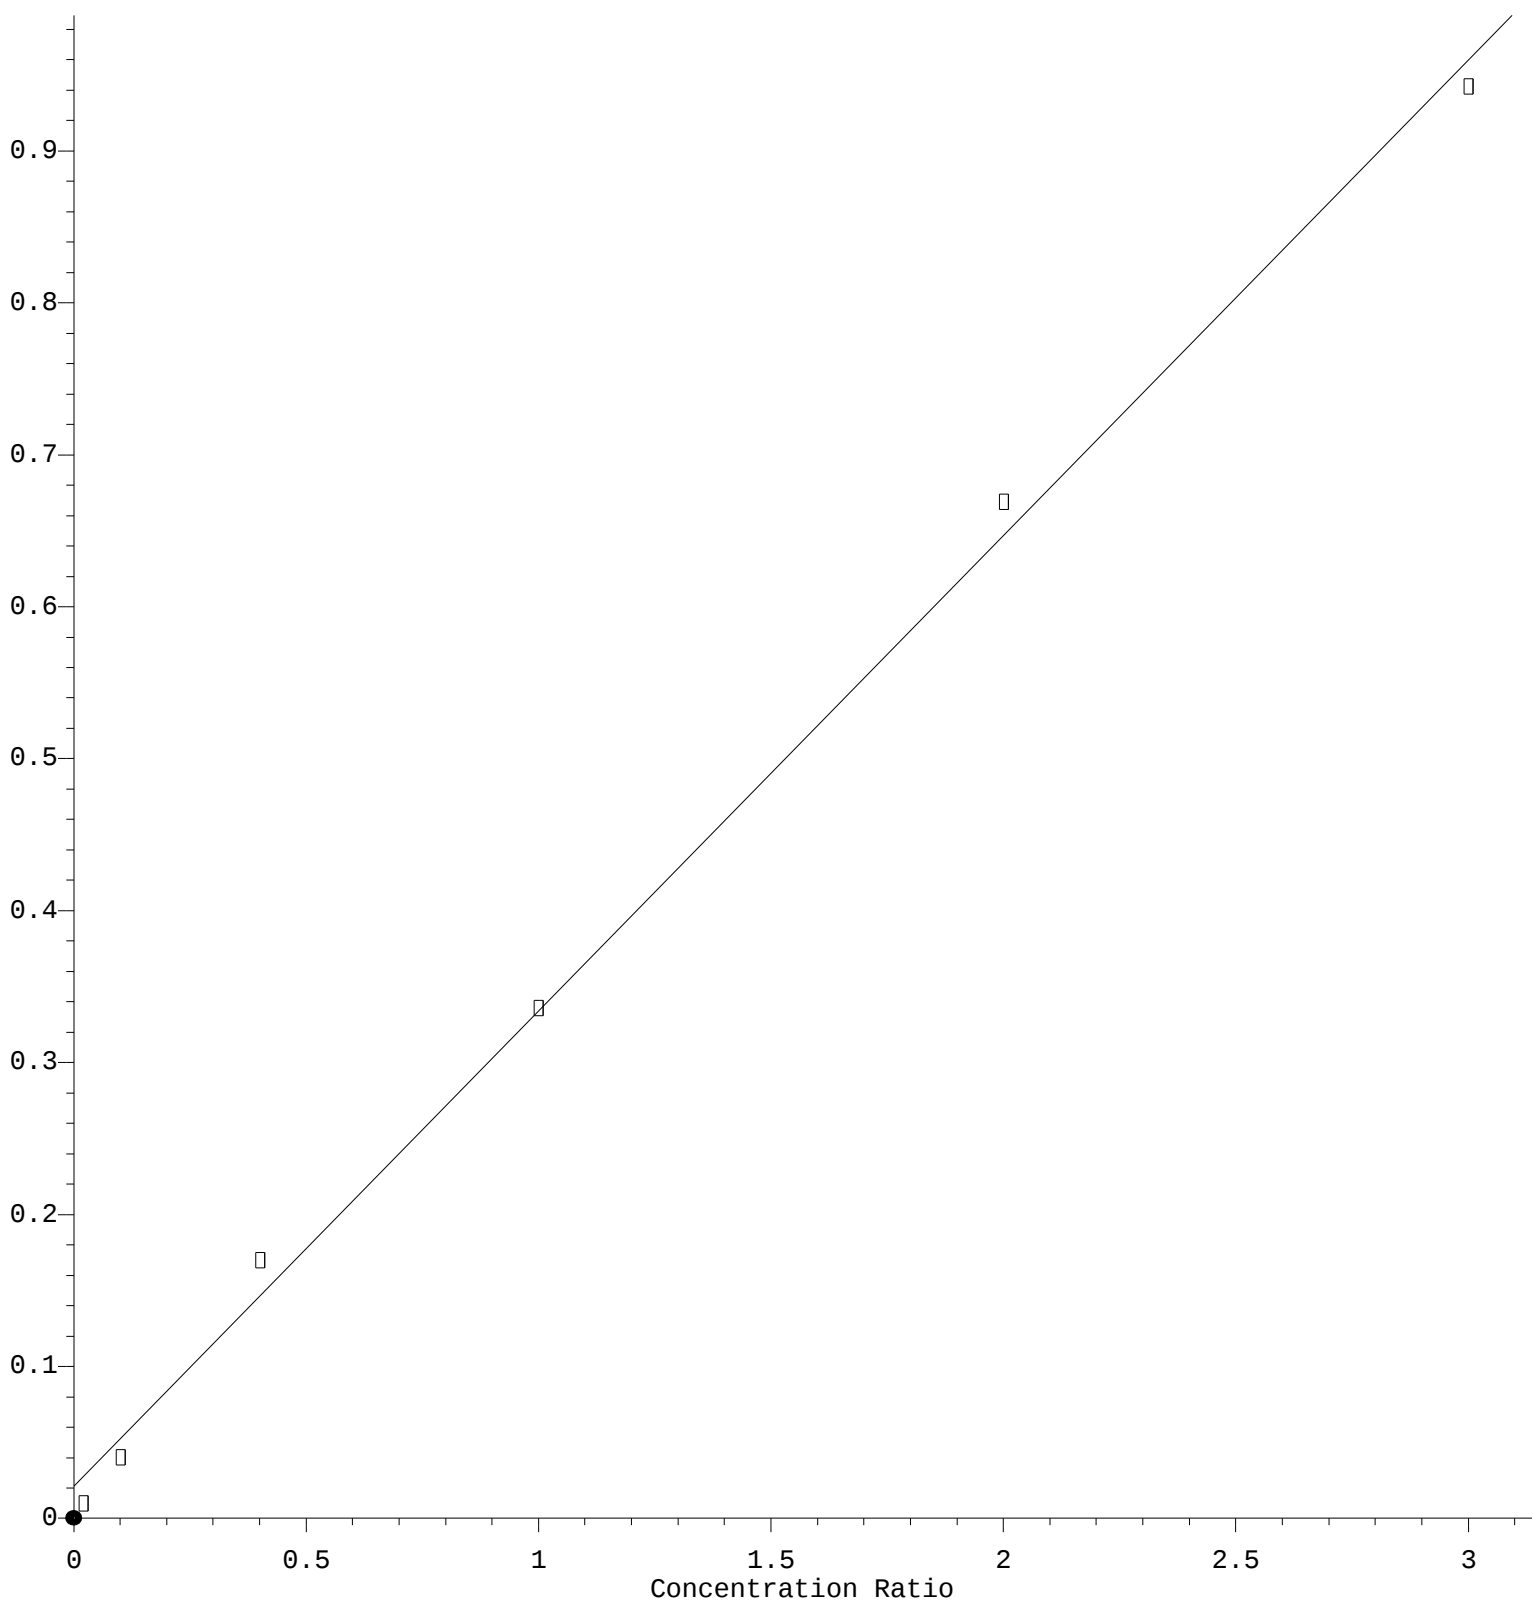

$$\text{Response} = 3.131\text{e-}001 * \text{Amt} + 2.082\text{e-}002$$


Coef of Det (r^2) = 0.997392 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M

Calibration Table Last Updated: Tue Apr 19 13:38:04 2022

Methyl Iodide

Response Ratio

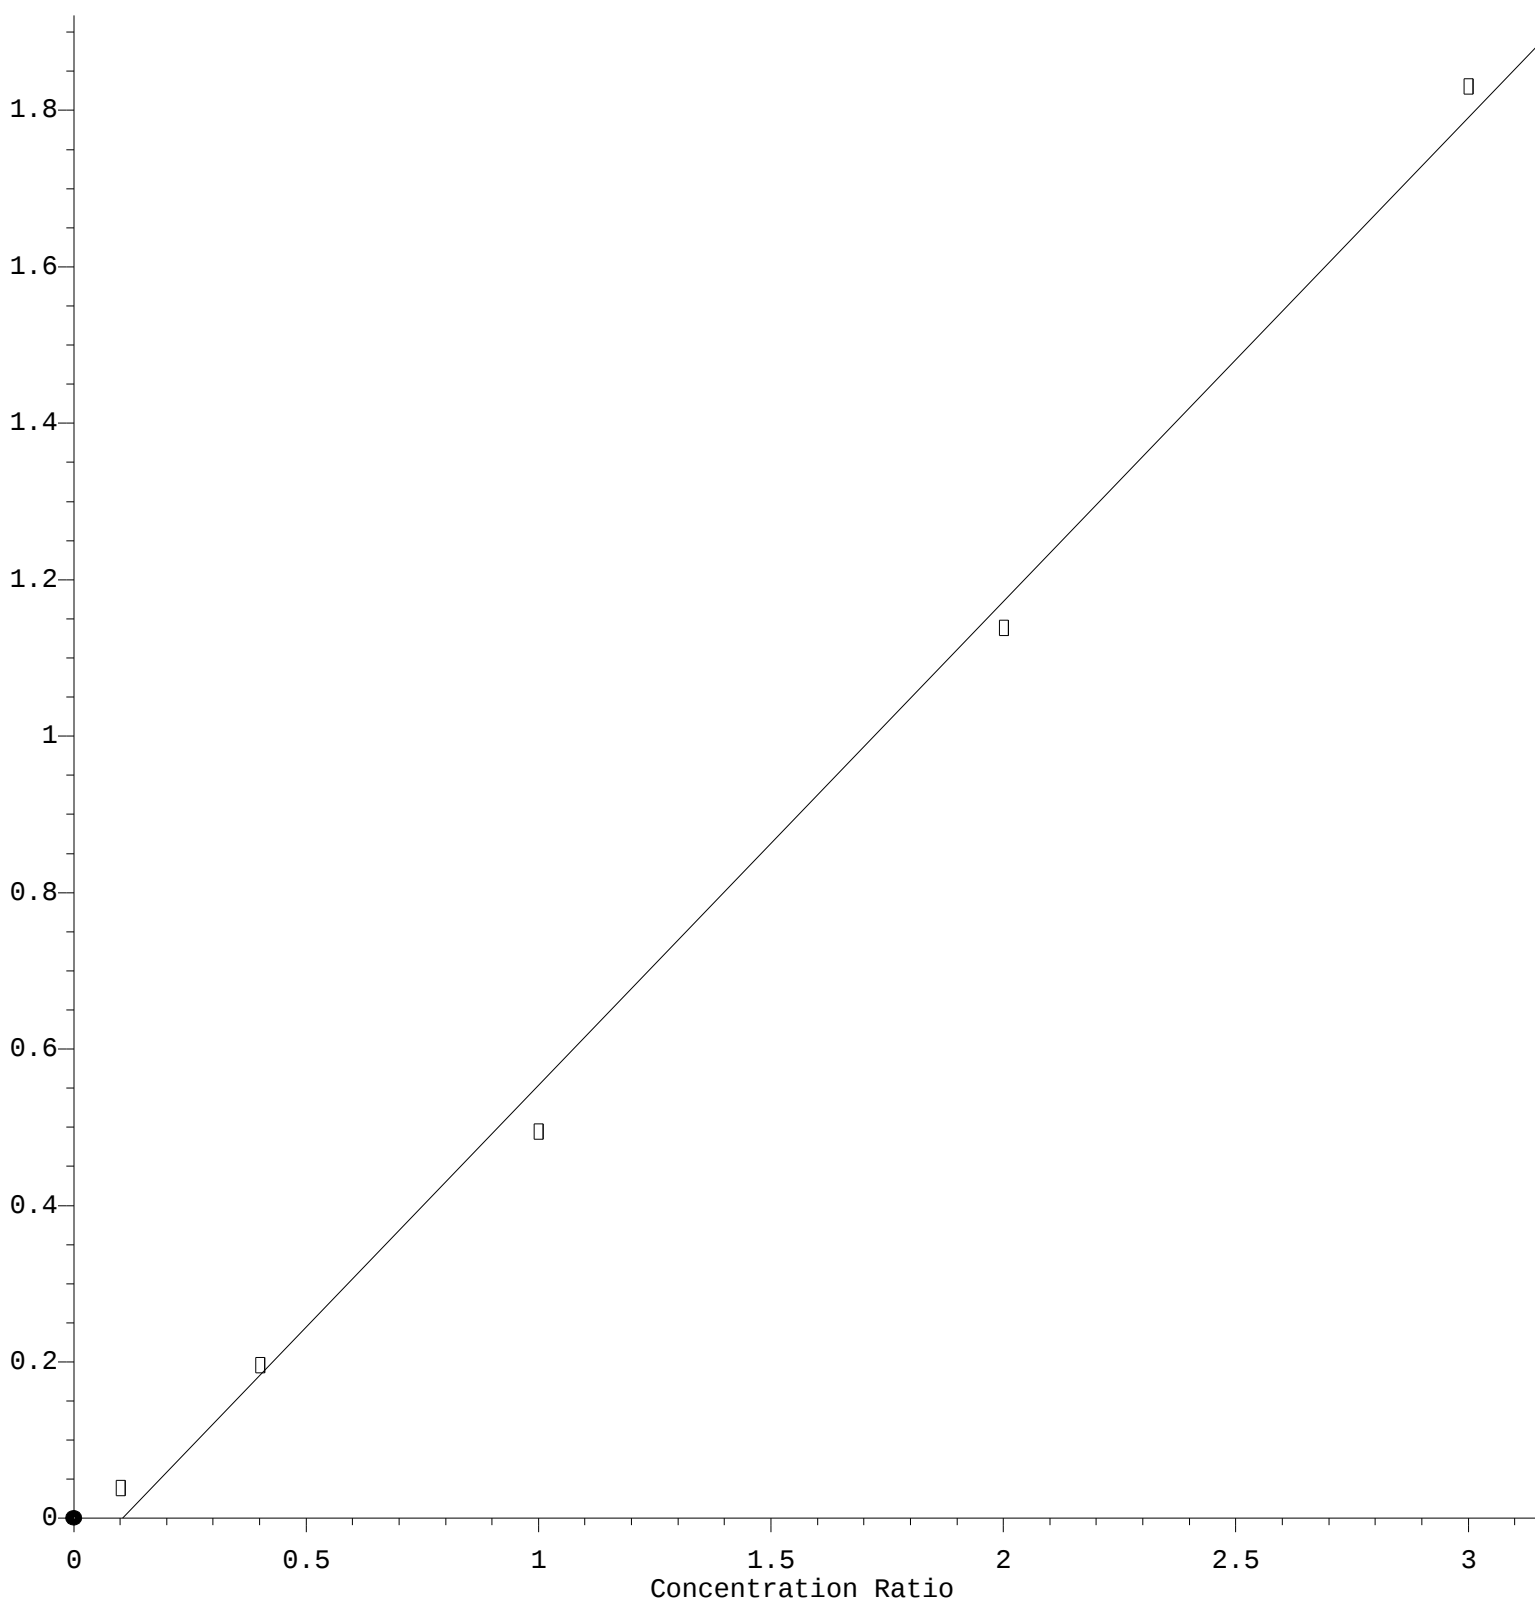

$$\text{Response} = 6.185\text{e-}001 * \text{Amt} - 6.475\text{e-}002$$


Coef of Det (r^2) = 0.996297 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M

Calibration Table Last Updated: Tue Apr 19 13:38:04 2022

Tert butylalcohol

Response Ratio

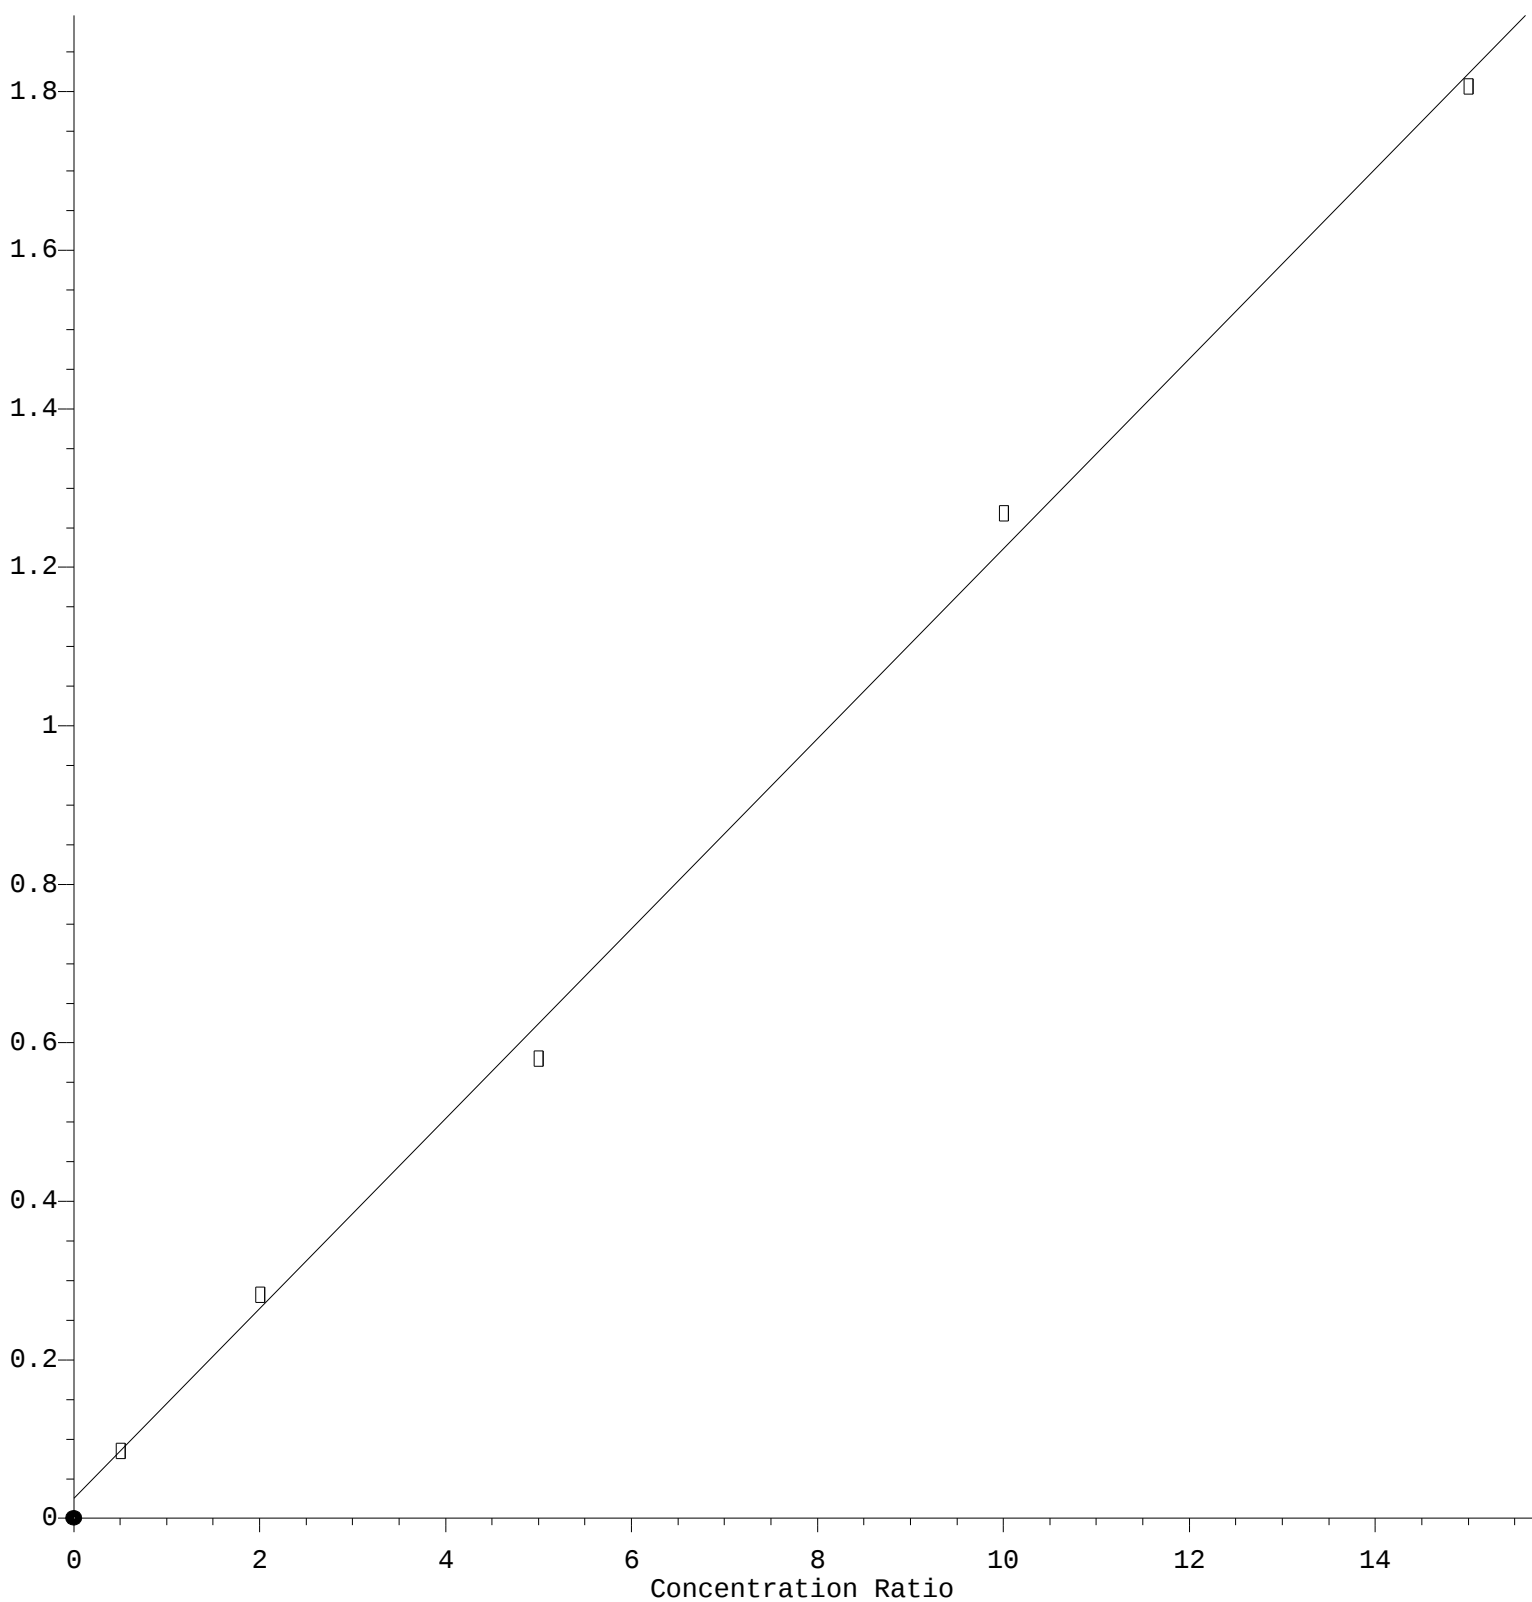

$$\text{Response} = 1.199\text{e-}001 * \text{Amt} + 2.481\text{e-}002$$


Coef of Det (r^2) = 0.997806 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M

Calibration Table Last Updated: Tue Apr 19 13:38:04 2022

Acetone

Response Ratio

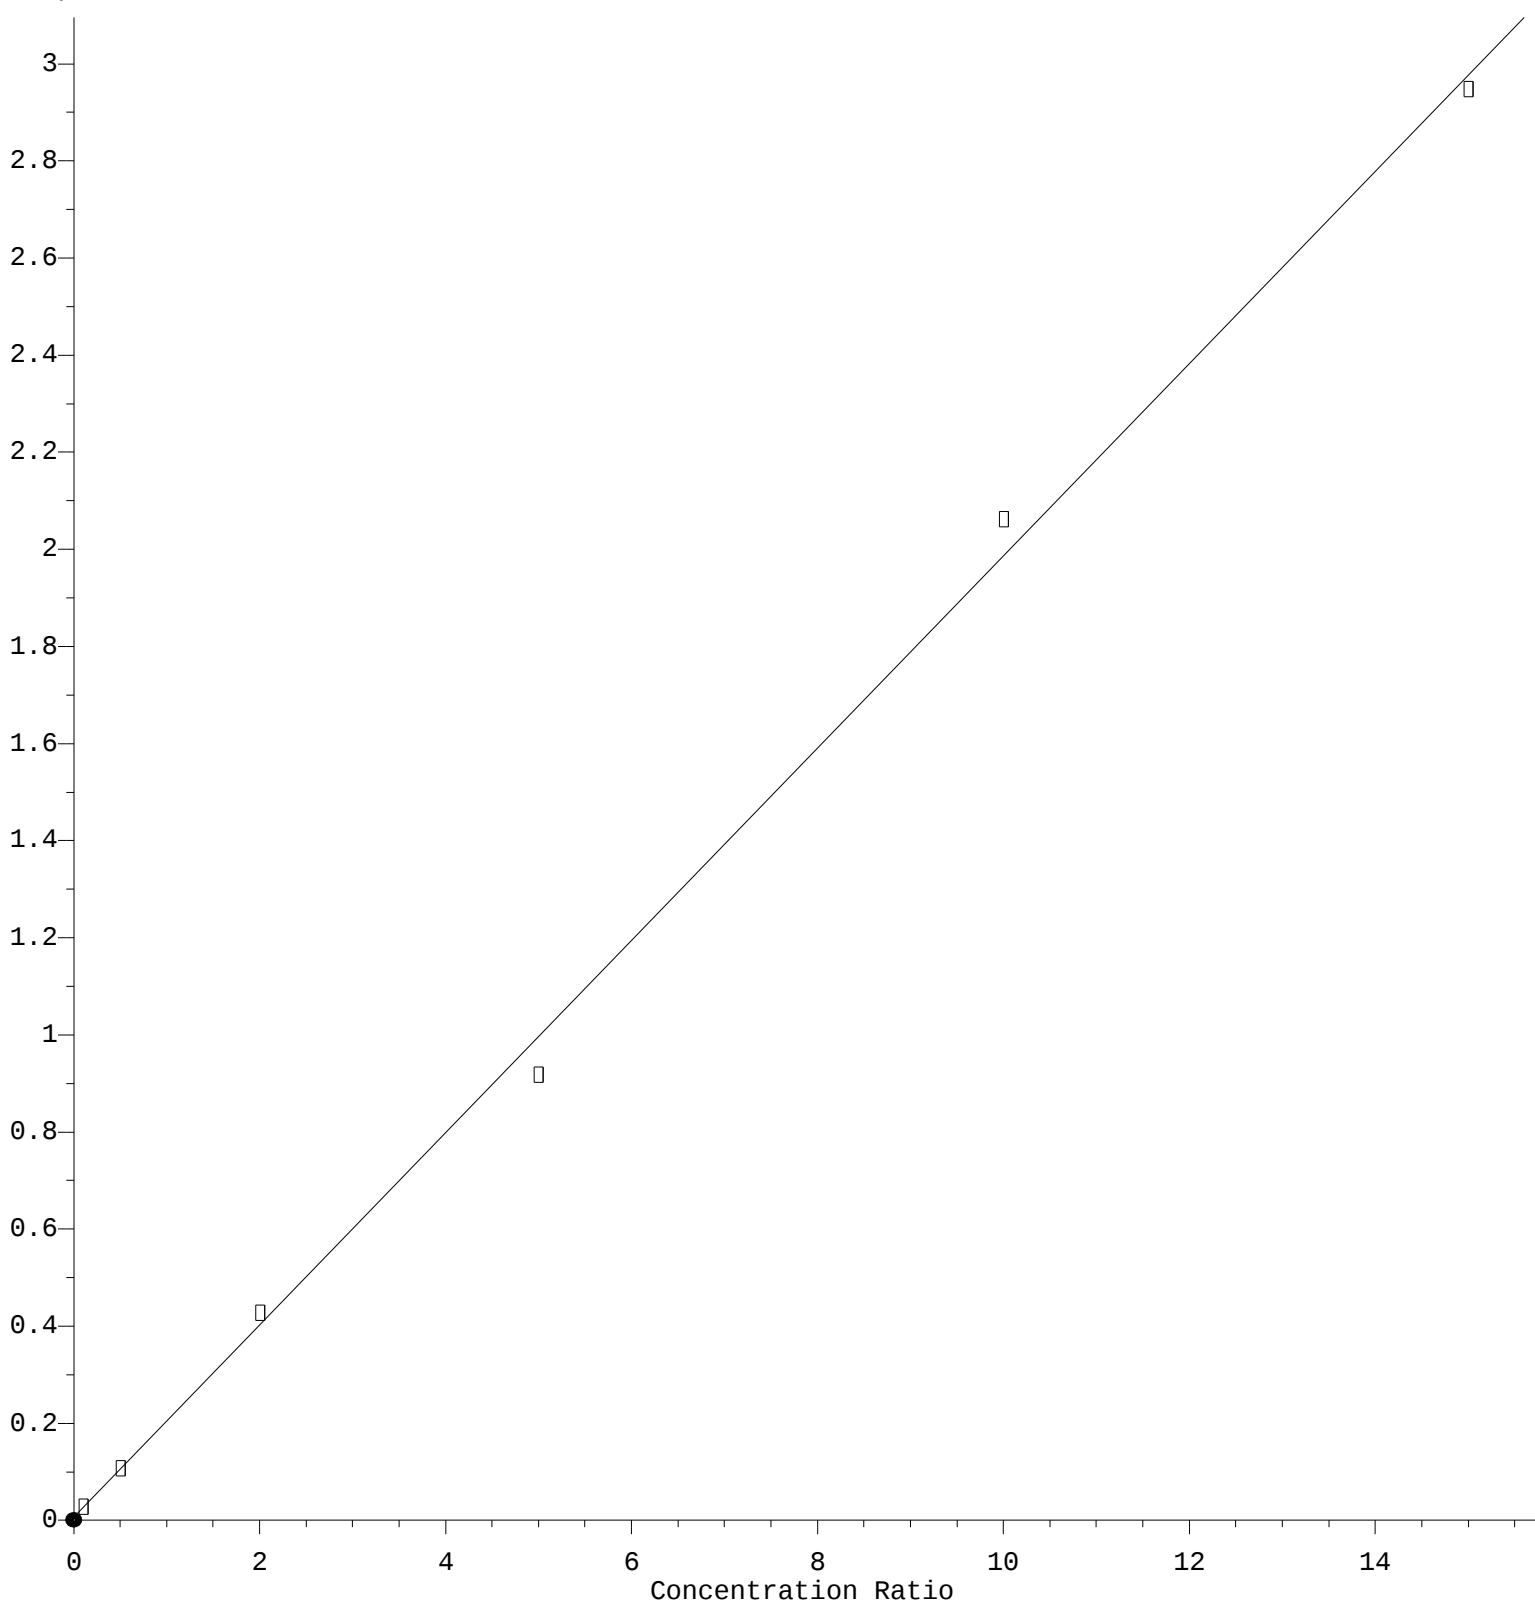

$$\text{Response} = 1.980\text{e-}001 * \text{Amt} + 5.560\text{e-}003$$


Coef of Det (r^2) = 0.998089 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M

Calibration Table Last Updated: Tue Apr 19 13:38:04 2022

Bromoform

Response Ratio

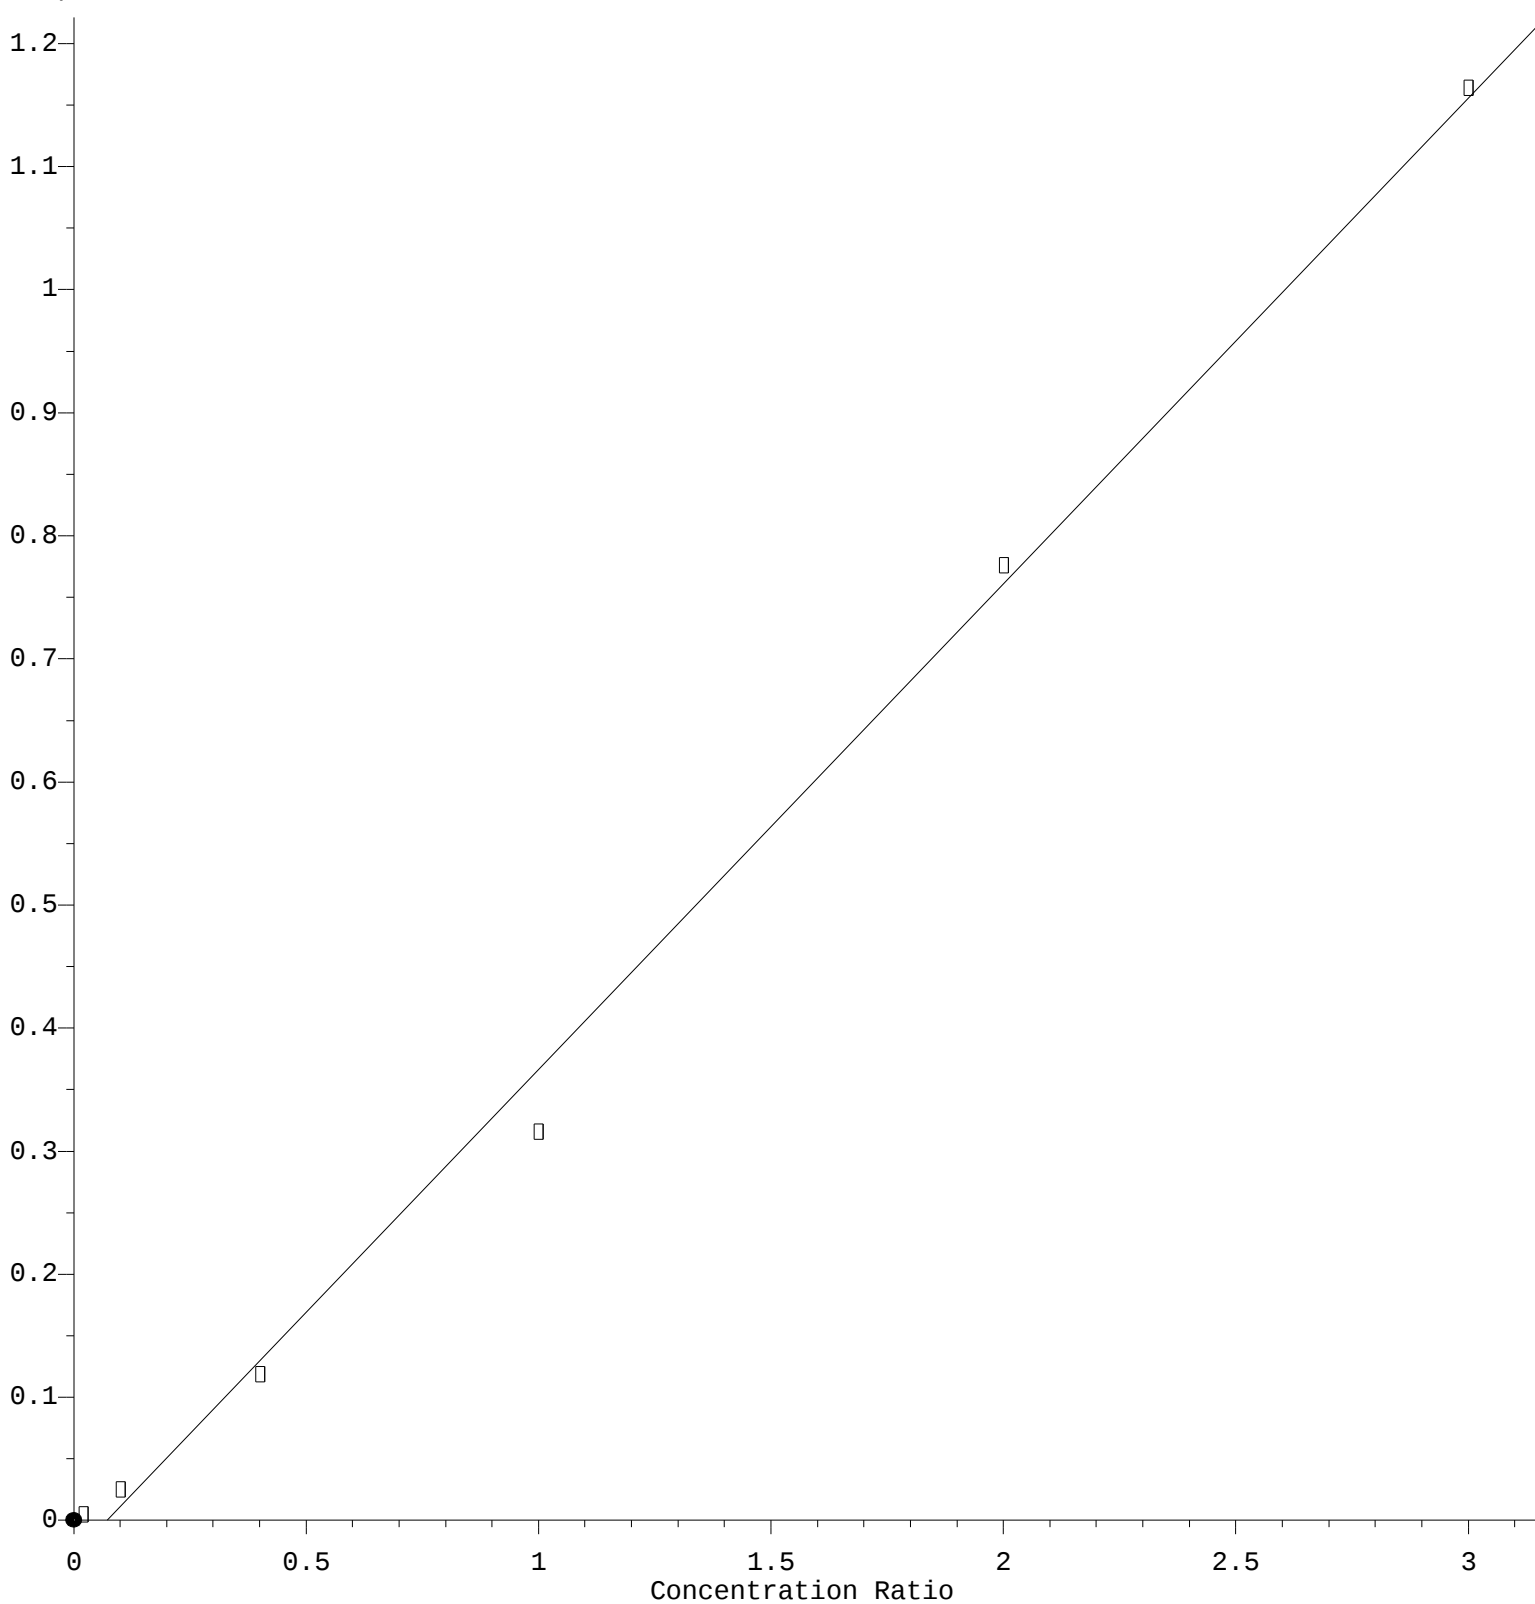

$$\text{Response} = 3.947\text{e-}001 * \text{Amt} - 2.822\text{e-}002$$


Coef of Det (r^2) = 0.996581 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M

Calibration Table Last Updated: Tue Apr 19 13:38:04 2022

Hexachloroethane

Response Ratio

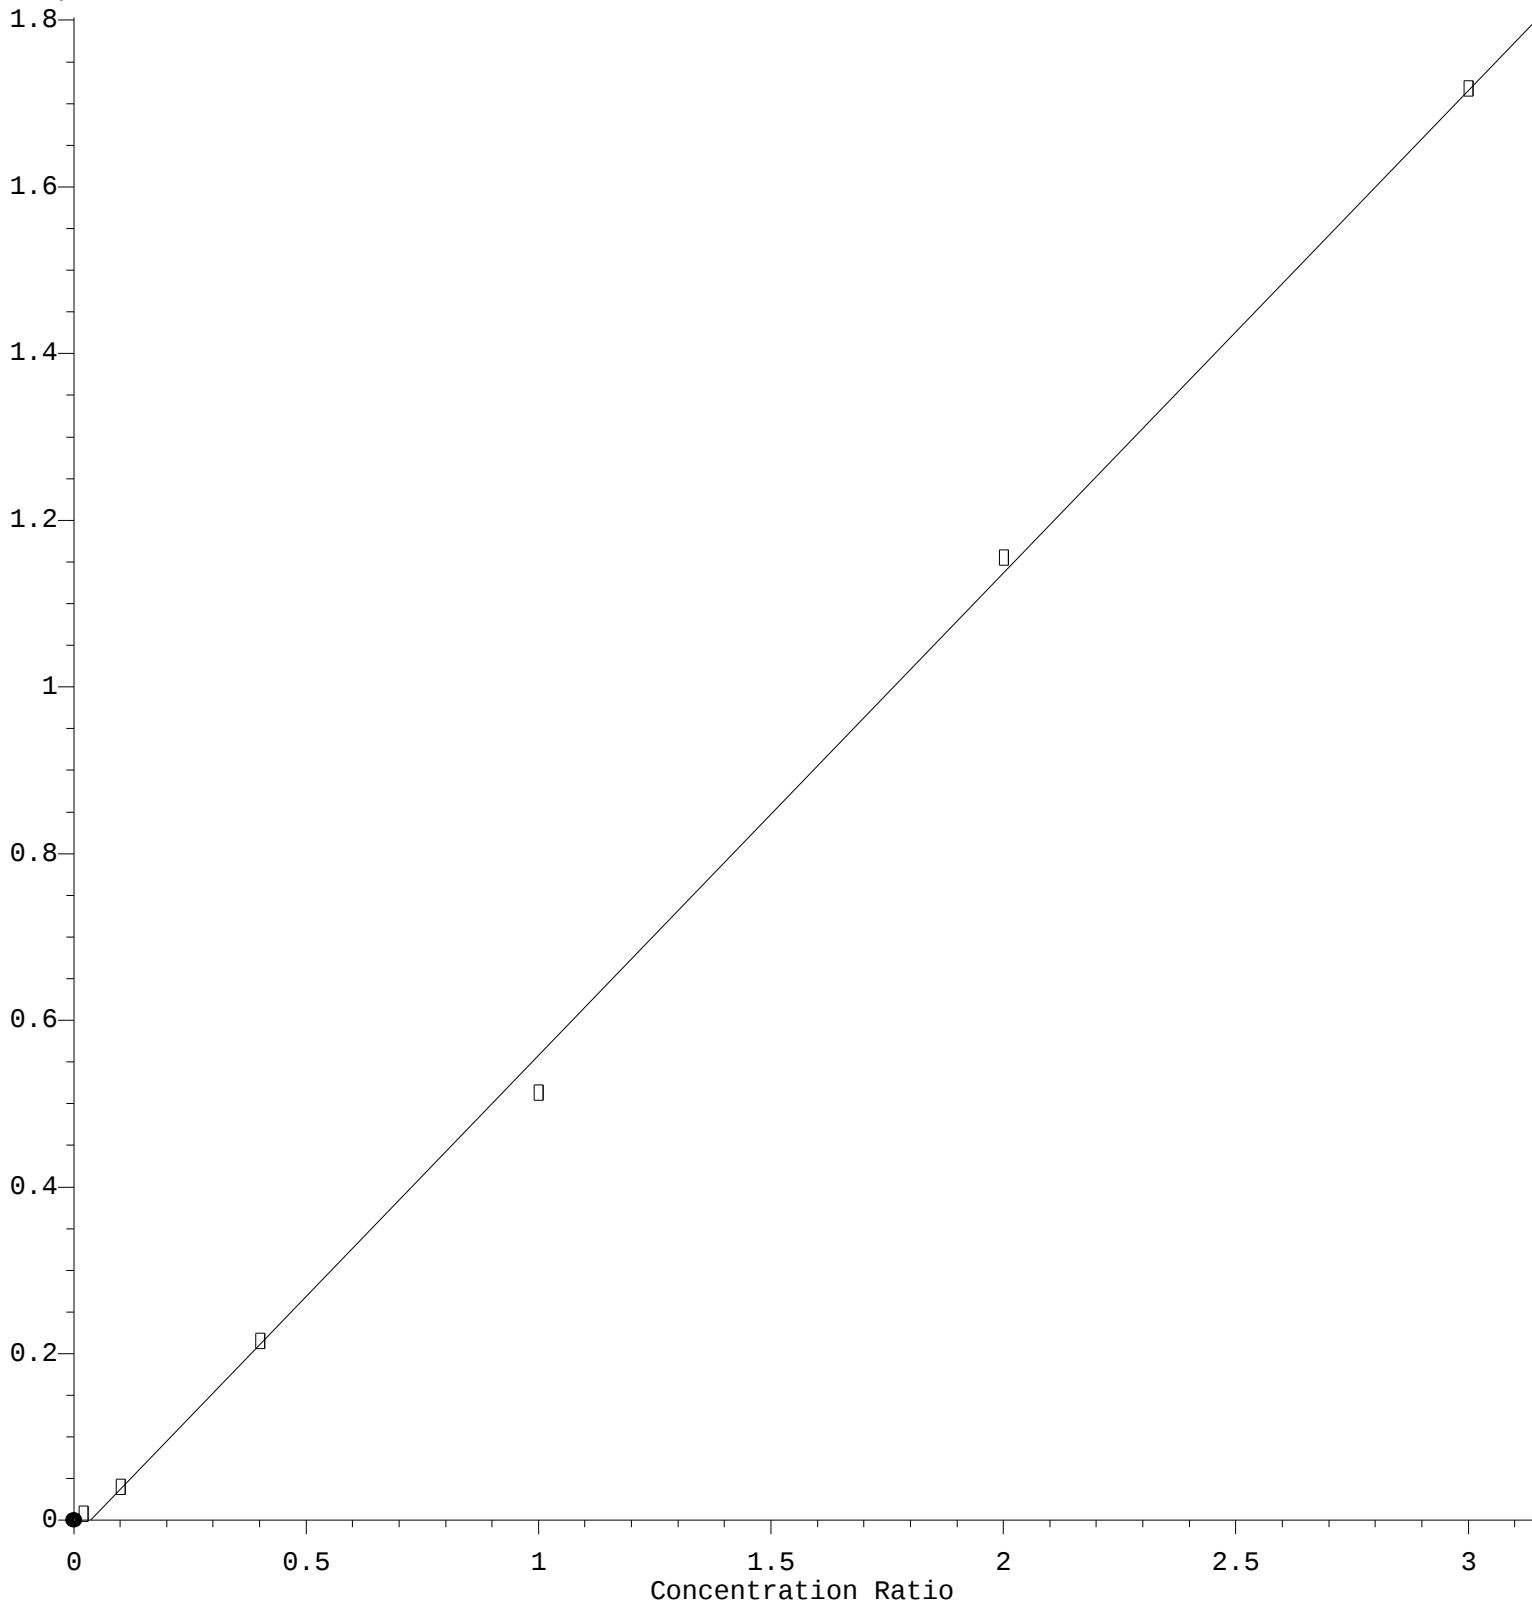

$$\text{Response} = 5.789\text{e-}001 * \text{Amt} - 2.100\text{e-}002$$

Coef of Det (r^2) = 0.998879 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M

Calibration Table Last Updated: Tue Apr 19 13:38:04 2022