

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041922\
 Data File : VX028173.D
 Acq On : 19 Apr 2022 20:53
 Operator : JC/MD
 Sample : PB144164ZHE#03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB144164ZHE#03

Quant Time: Apr 20 08:19:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 19 13:38:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	426511	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	729593	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	730257	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	343074	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	258129	46.416	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	92.840%
35) Dibromofluoromethane	5.385	113	238311	46.576	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	93.160%
50) Toluene-d8	8.653	98	872943	44.421	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	88.840%
62) 4-Bromofluorobenzene	11.079	95	333528	44.387	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	88.780%
Target Compounds						
					Qvalue	
16) Acetone	2.373	43	20923	10.983	ug/l	91
20) Methylene Chloride	2.788	84	205419	49.783	ug/l	99
43) Isopropyl Acetate	6.342	43	32304	2.931	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041922\
Data File : VX028173.D
Acq On : 19 Apr 2022 20:53
Operator : JC/MD
Sample : PB144164ZHE#03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB144164ZHE#03

Quant Time: Apr 20 08:19:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 19 13:38:04 2022
Response via : Initial Calibration




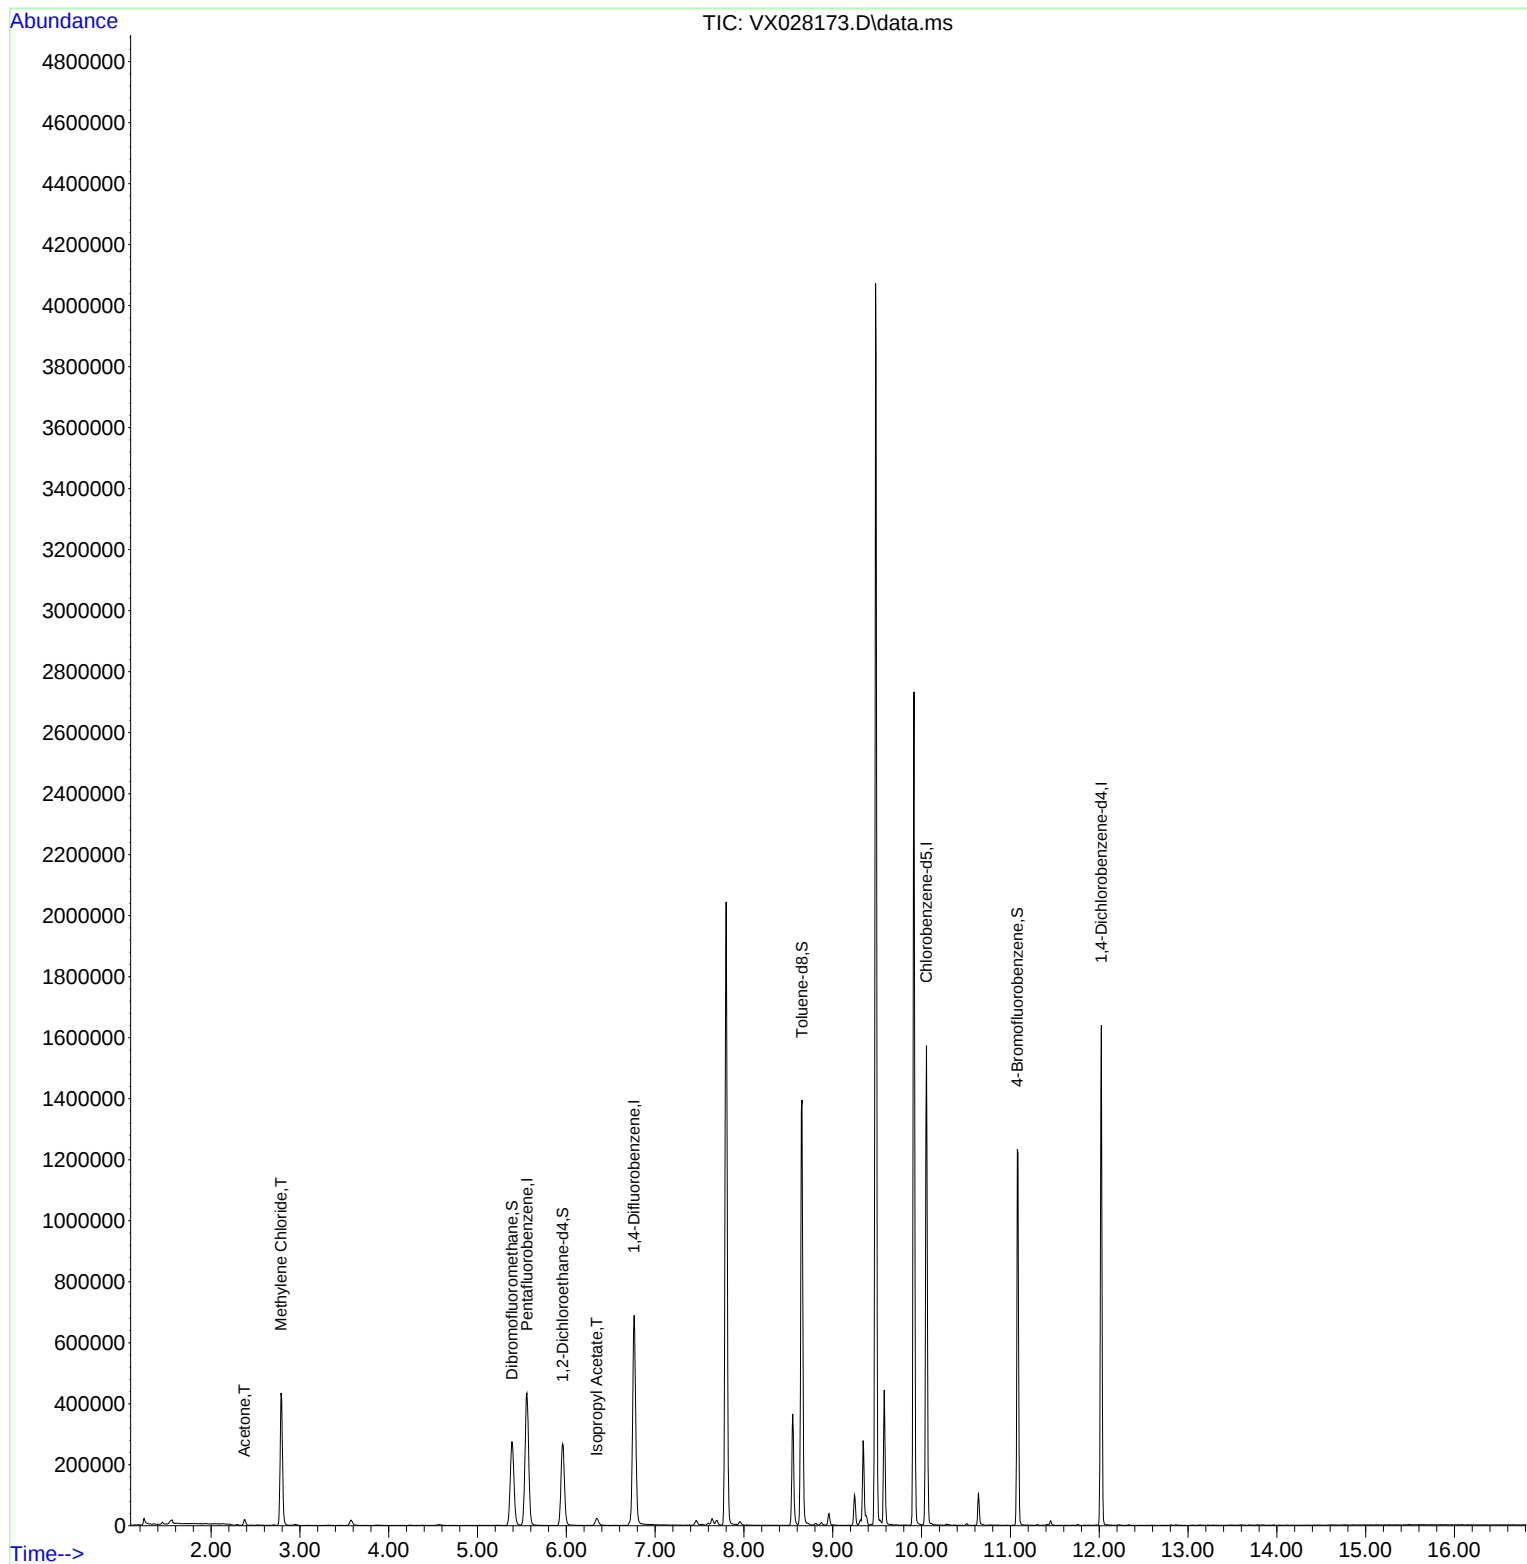




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX028173.D
Acq: 19 Apr 2022 20:53




Instrument :
MSVOA_X
ClientSampleId :
PB144164ZHE#03


Tgt Ion:168 Resp: 426511
Ion Ratio Lower Upper
168 100
99 56.6 41.7 62.5

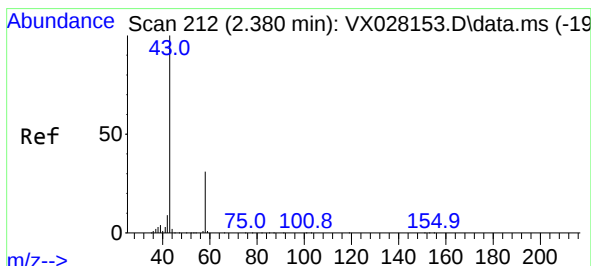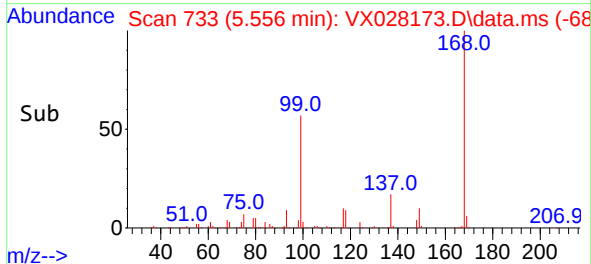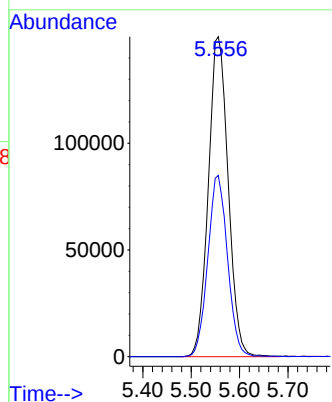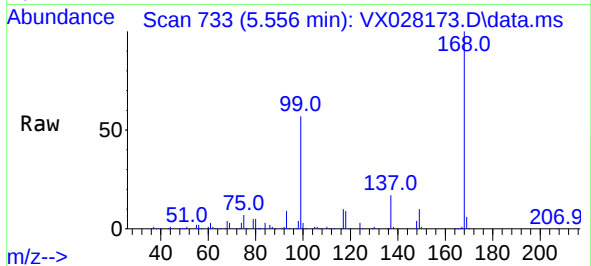

#16
Acetone
Concen: 10.983 ug/l
RT: 2.373 min Scan# 211
Delta R.T. -0.007 min
Lab File: VX028173.D
Acq: 19 Apr 2022 20:53


Tgt Ion: 43 Resp: 20923
Ion Ratio Lower Upper
43 100
58 30.6 28.8 43.2

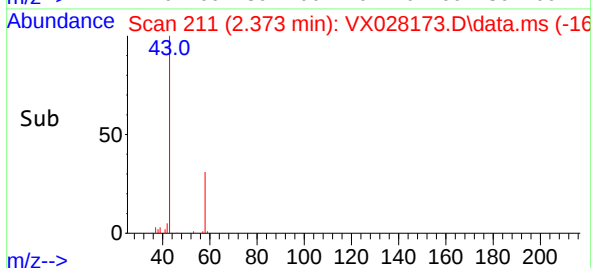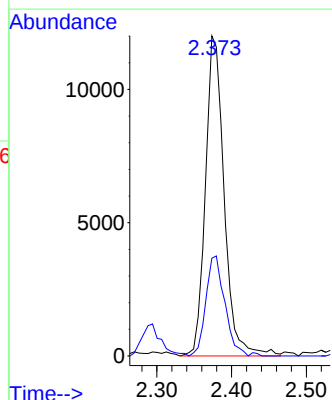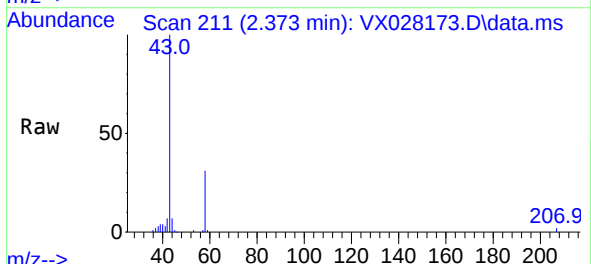

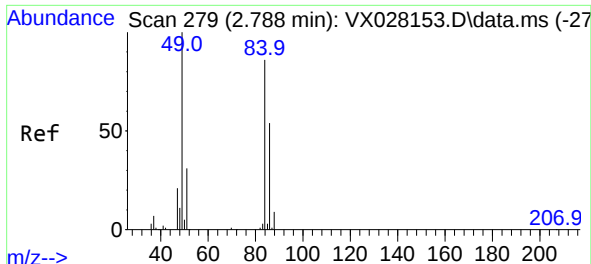




#20
Methylene Chloride
Concen: 49.783 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX028173.D
Acq: 19 Apr 2022 20:53

Instrument :
MSVOA_X
ClientSampleId :
PB144164ZHE#03

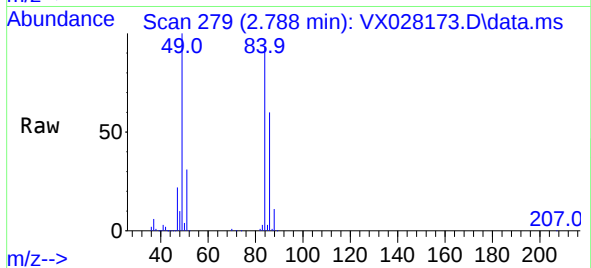

Tgt Ion: 84 Resp: 205419




Ion	Ratio	Lower	Upper
84	100		
49	107.4	85.5	128.3
51	32.8	26.6	39.8
86	64.0	51.5	77.3

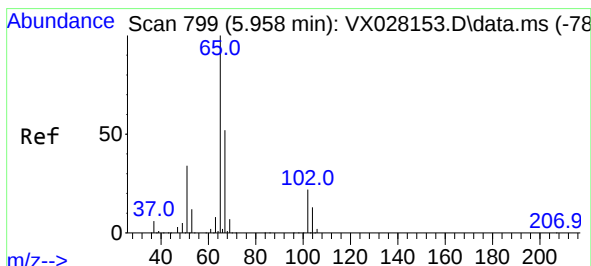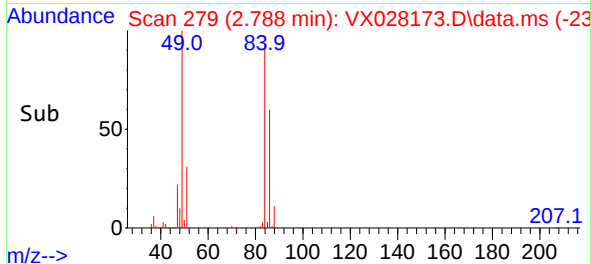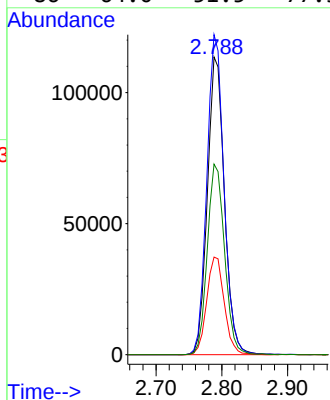

#33
1,2-Dichloroethane-d4
Concen: 46.416 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX028173.D
Acq: 19 Apr 2022 20:53

Tgt Ion: 65 Resp: 258129

Ion	Ratio	Lower	Upper
65	100		
67	52.0	0.0	107.4


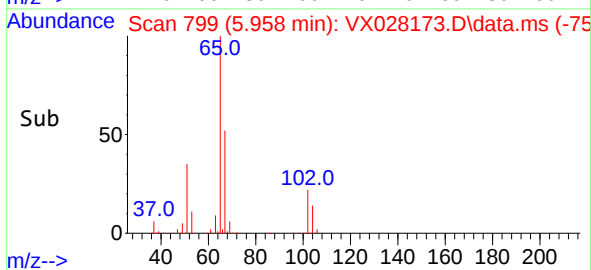
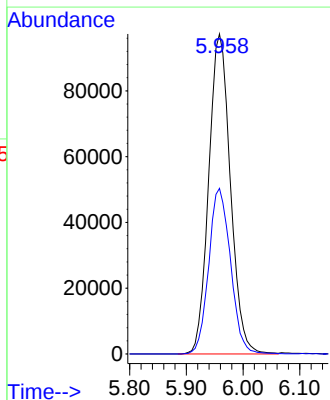
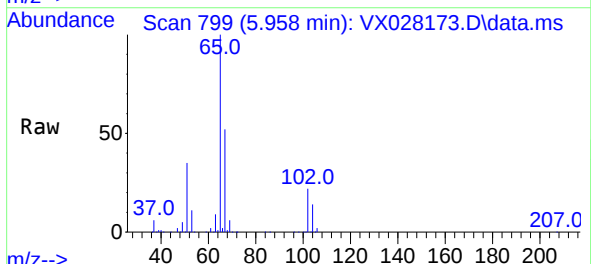




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX028173.D
Acq: 19 Apr 2022 20:53




Instrument :
MSVOA_X
ClientSampleId :
PB144164ZHE#03


Tgt Ion:114 Resp: 729593
Ion Ratio Lower Upper
114 100
63 18.4 0.0 36.8
88 15.1 0.0 32.4

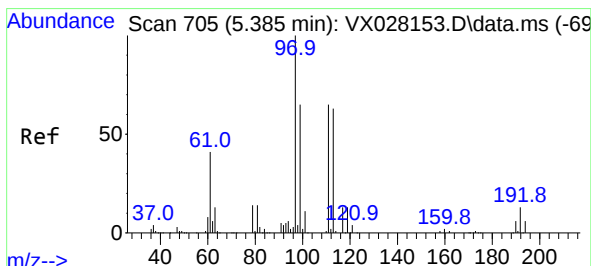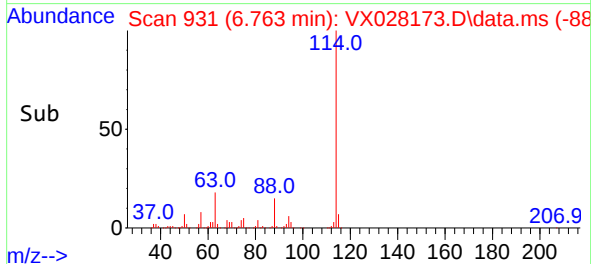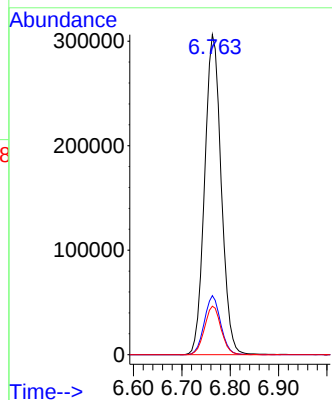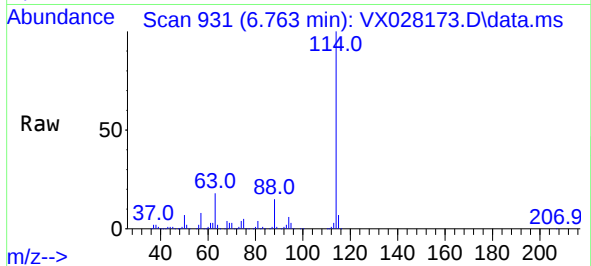

#35
Dibromofluoromethane
Concen: 46.576 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX028173.D
Acq: 19 Apr 2022 20:53

Tgt Ion:113 Resp: 238311
Ion Ratio Lower Upper
113 100
111 102.6 82.8 124.2
192 20.2 16.9 25.3


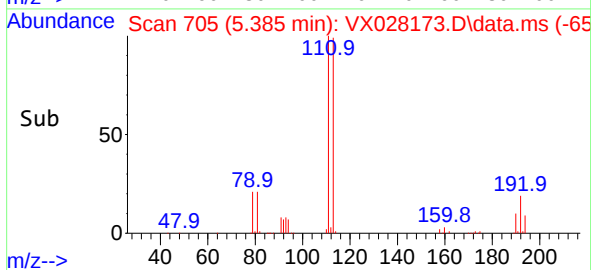
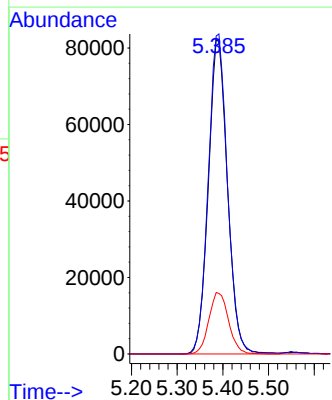
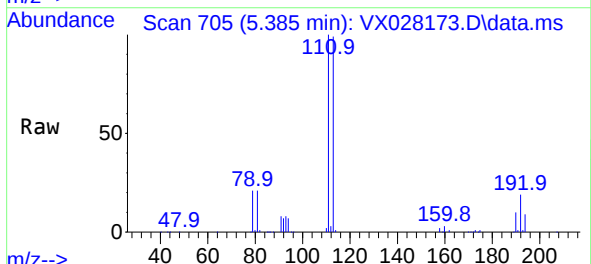


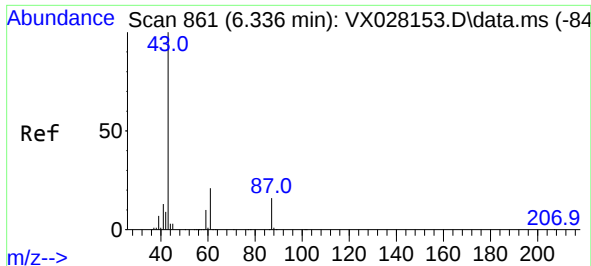

#43
Isopropyl Acetate
Concen: 2.931 ug/l
RT: 6.342 min Scan# 861
Delta R.T. 0.006 min
Lab File: VX028173.D
Acq: 19 Apr 2022 20:53




Instrument :
MSVOA_X
ClientSampleId :
PB144164ZHE#03


Tgt Ion: 43 Resp: 32304
Ion Ratio Lower Upper
43 100
61 22.4 18.5 27.7
87 16.6 13.0 19.6

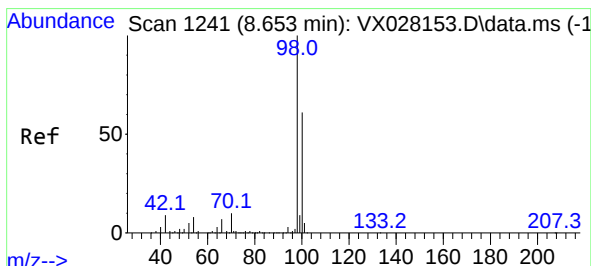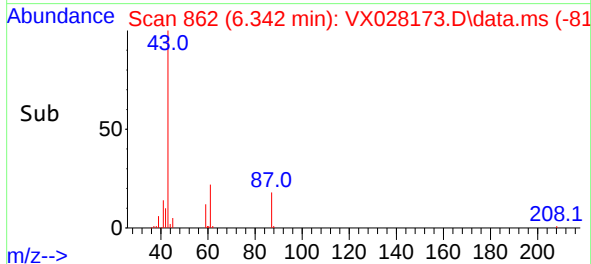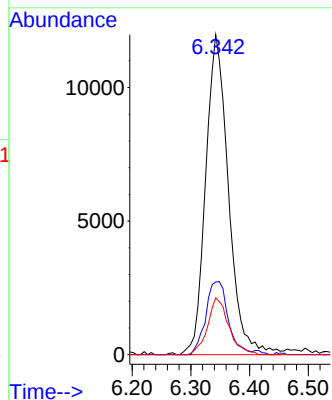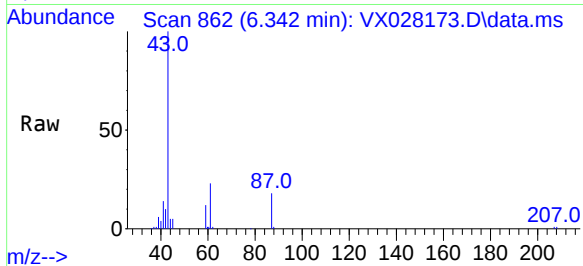

#50
Toluene-d8
Concen: 44.421 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX028173.D
Acq: 19 Apr 2022 20:53

Tgt Ion: 98 Resp: 872943
Ion Ratio Lower Upper
98 100
100 66.4 52.6 78.8


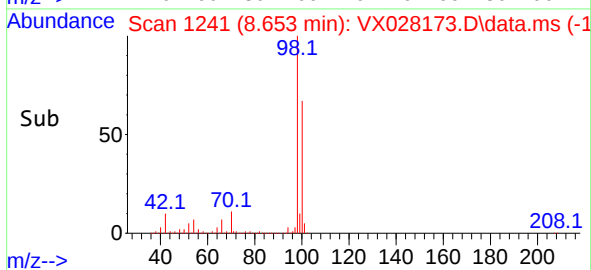
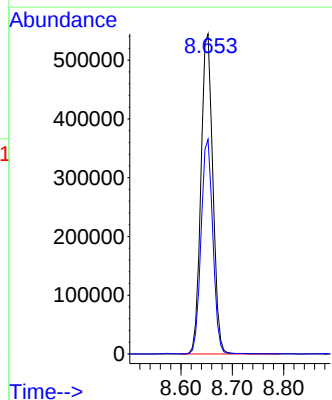
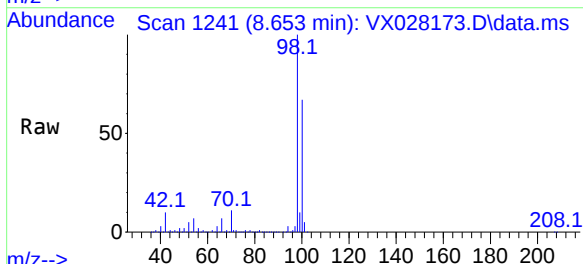


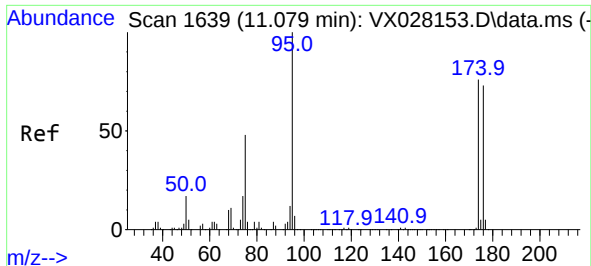

#62
4-Bromofluorobenzene
Concen: 44.387 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX028173.D
Acq: 19 Apr 2022 20:53




Instrument :
MSVOA_X
ClientSampleId :
PB144164ZHE#03


Tgt Ion: 95 Resp: 333528
Ion Ratio Lower Upper
95 100
174 83.7 0.0 163.0
176 81.4 0.0 155.0

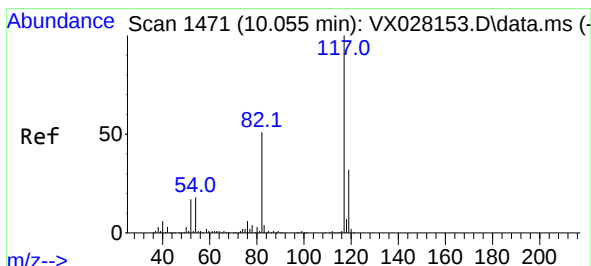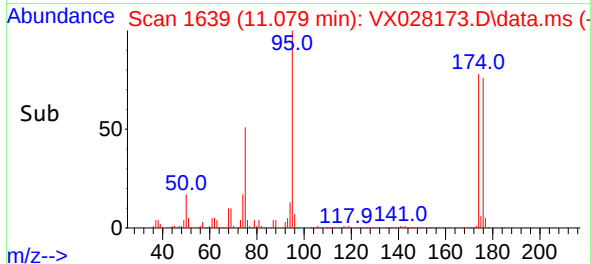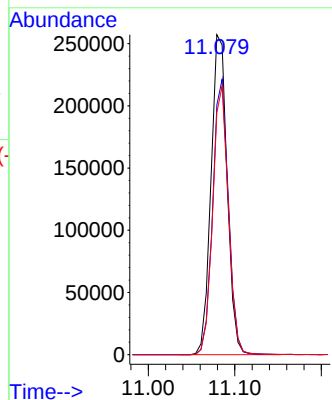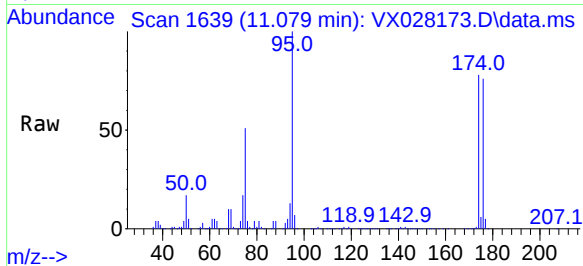

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX028173.D
Acq: 19 Apr 2022 20:53


Tgt Ion: 117 Resp: 730257
Ion Ratio Lower Upper
117 100
82 51.2 41.8 62.8
119 32.2 24.8 37.2

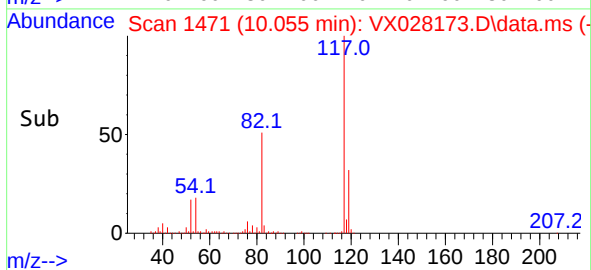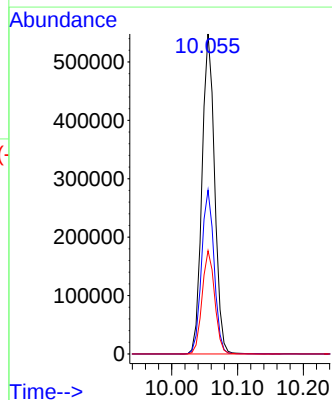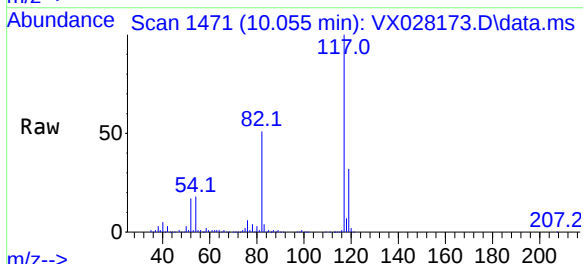

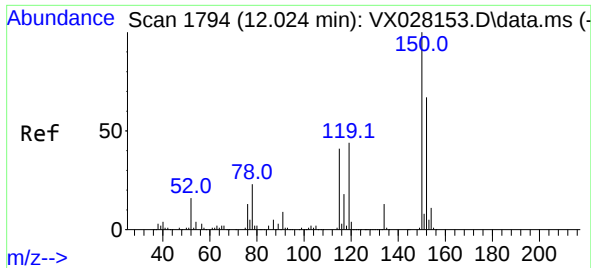

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX028173.D
 Acq: 19 Apr 2022 20:53

Instrument :
 MSVOA_X
 ClientSampleId :
 PB144164ZHE#03

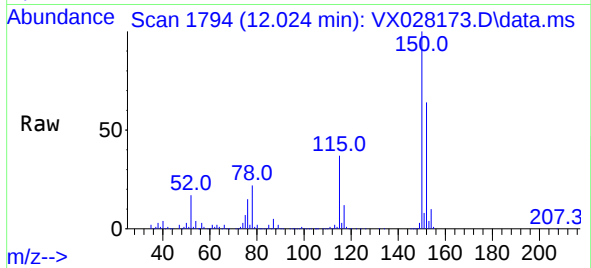

Tgt Ion:152 Resp: 343074
 Ion Ratio Lower Upper
 152 100
 115 58.4 37.5 112.7
 150 155.2 0.0 338.2

