
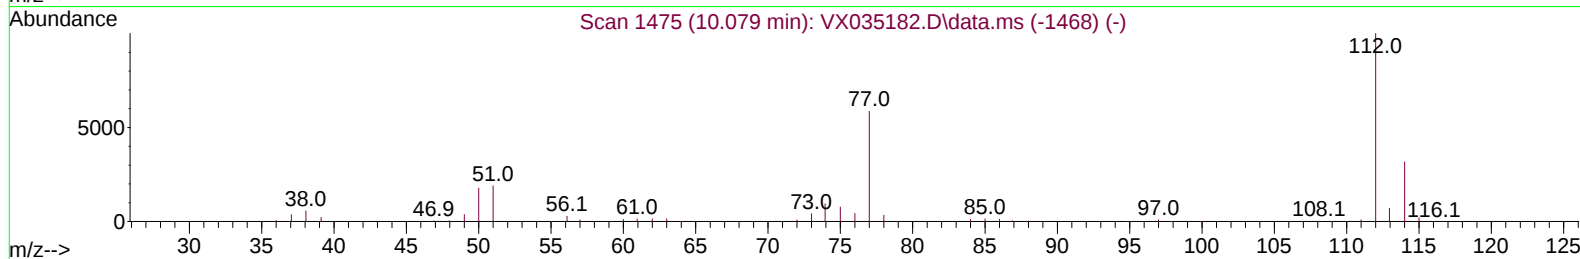
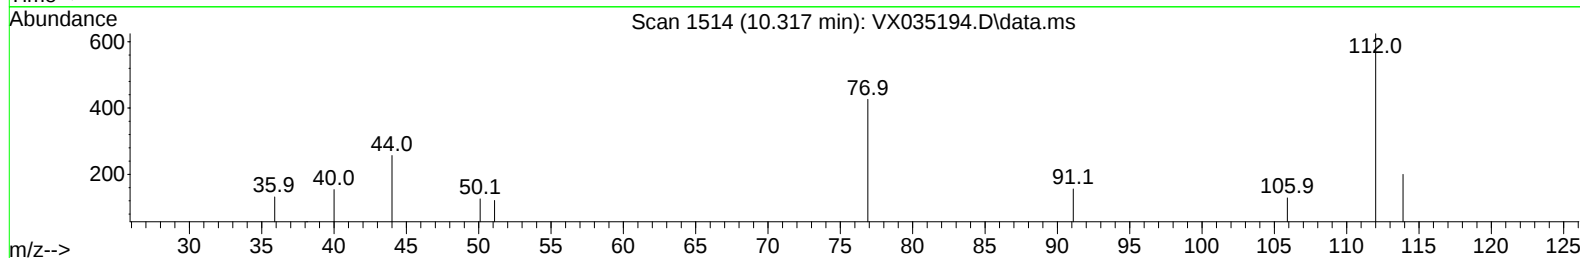


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035194.D
 Acq On : 20 Apr 2023 01:07
 Operator : JC/MD
 Sample : 02378-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 41 Sample Multiplier: 1

Quant Time: Apr 20 05:09:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041823WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 20 04:51:49 2023
 Response via : Initial Calibration

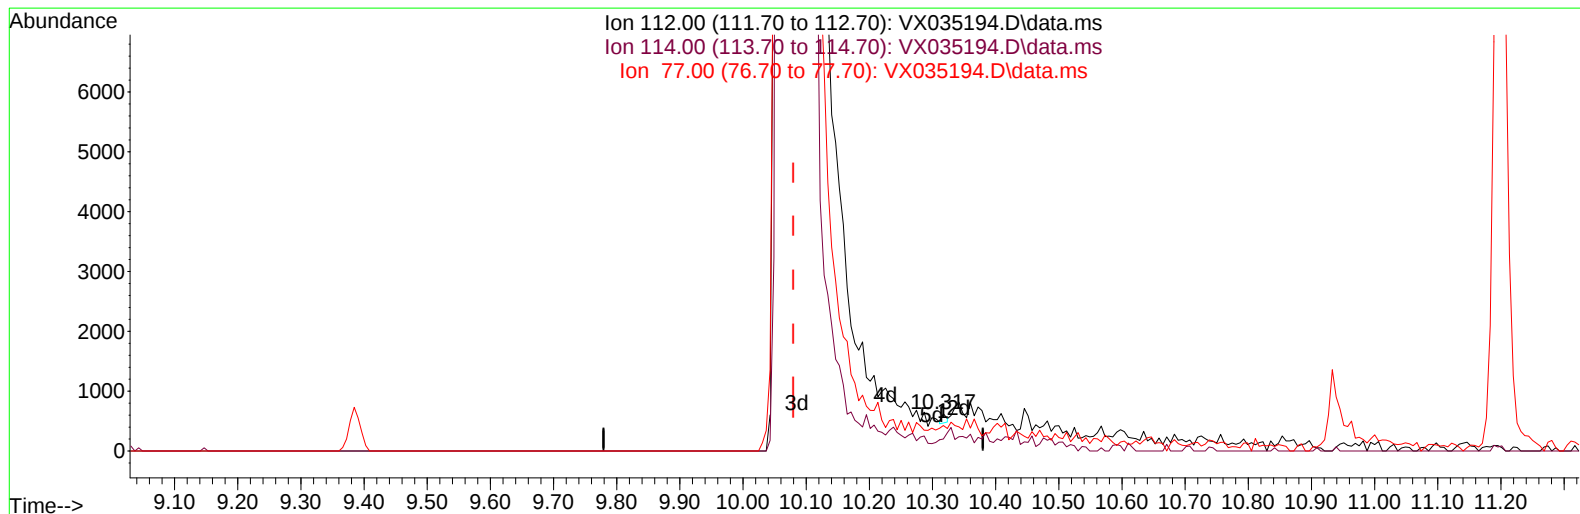

TIC: VX035194.D\data.ms

(51) Chlorobenzene (T)

10.317min (+ 0.238) 0.01 ug/L

response 82

Ion	Exp%	Act%
112.00	100.00	100.00
114.00	32.00	32.05
77.00	58.80	68.27
0.00	0.00	0.00