




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035201.D
Acq On : 20 Apr 2023 03:48
Operator : JC/MD
Sample : 02378-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COML2

Manual IntegrationsAPPROVED

Quant Time: Apr 20 05:11:48 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 20 04:51:49 2023
Response via : Initial Calibration

Reviewed By :John Carlone 04/20/2023
Supervised By :Mahesh Dadoda 04/21/2023

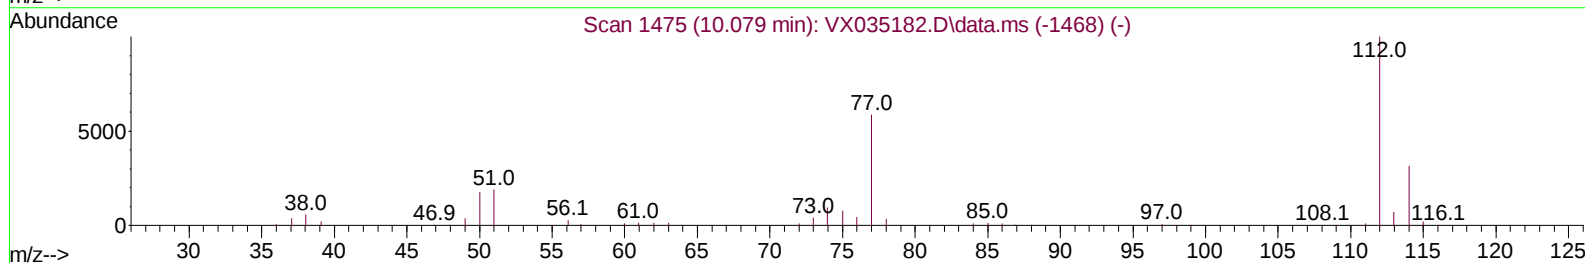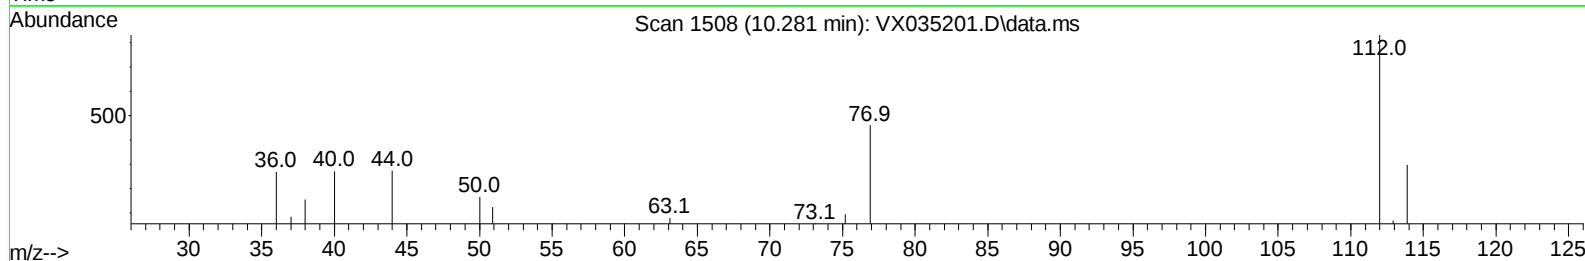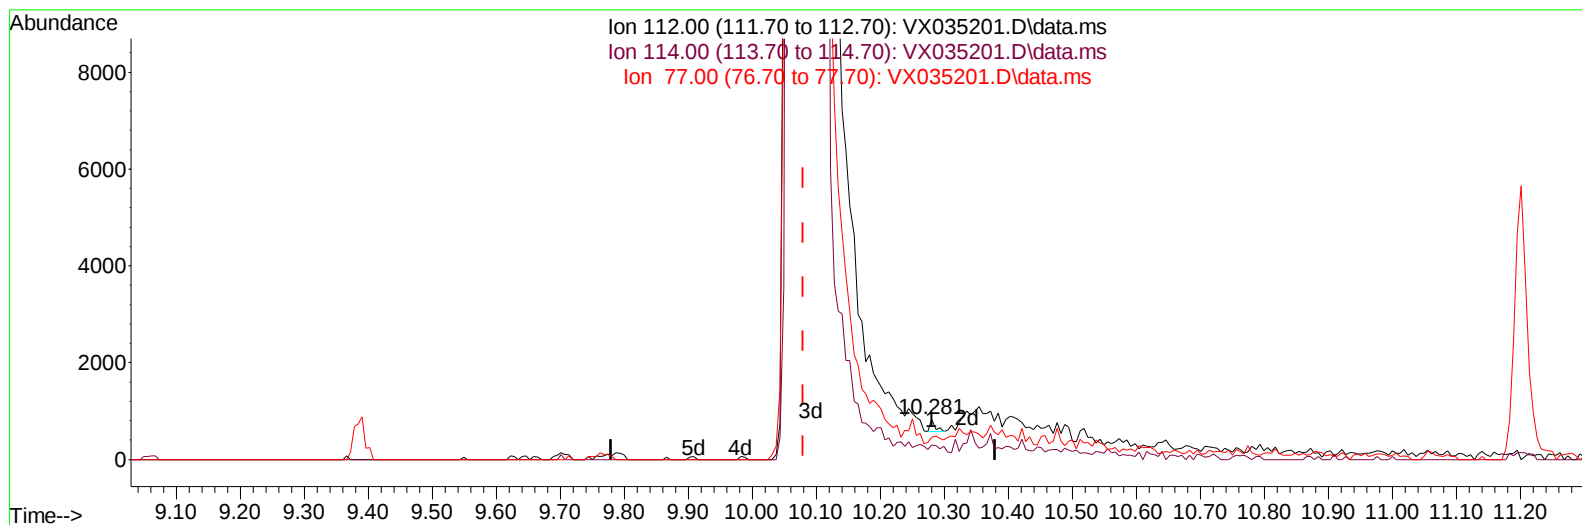

TIC: VX035201.D\data.ms

(51) Chlorobenzene (T)

10.281min (+ 0.201) 0.02 ug/L

response 139

Ion	Exp%	Act%
112.00	100.00	100.00
114.00	32.00	35.74
77.00	58.80	55.23
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035201.D
 Acq On : 20 Apr 2023 03:48
 Operator : JC/MD
 Sample : 02378-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML2

Manual IntegrationsAPPROVED

Quant Time: Apr 20 05:11:48 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 20 04:51:49 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 04/20/2023
 Supervised By :Mahesh Dadoda 04/21/2023

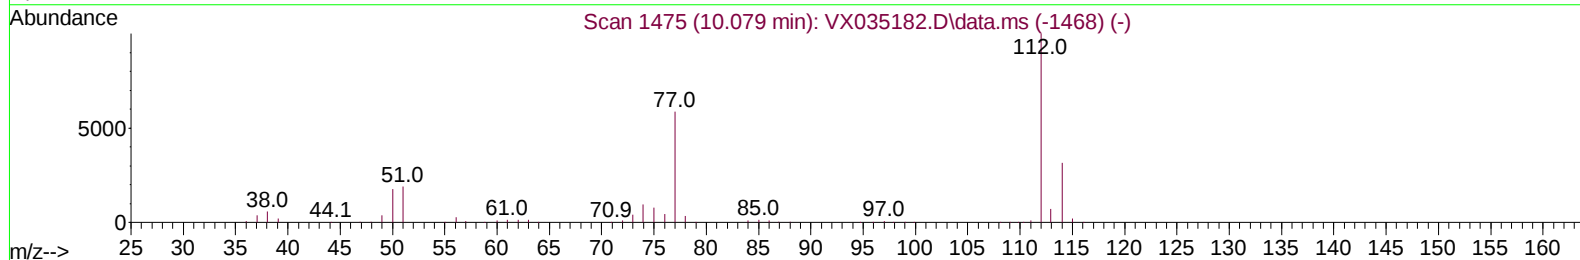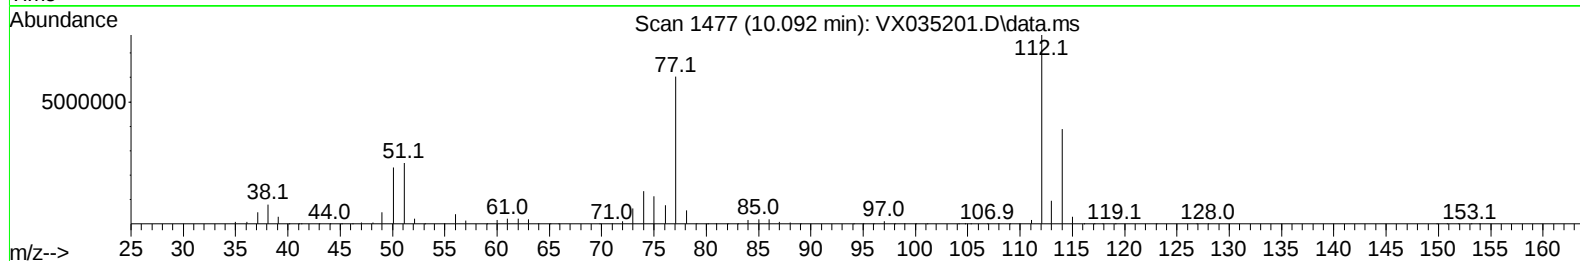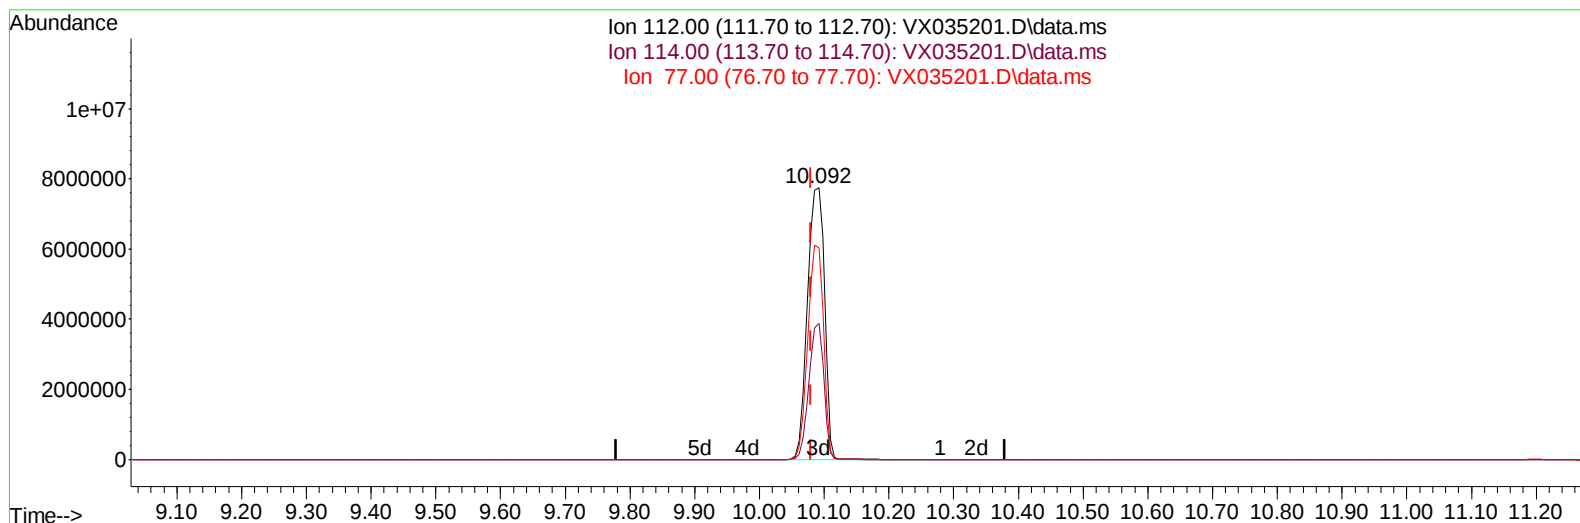

TIC: VX035201.D\data.ms

(51) Chlorobenzene (T)

10.092min (+ 0.012) 1777.40 ug/L m

response 14141151

Ion	Exp%	Act%
112.00	100.00	100.00
114.00	32.00	50.03#
77.00	58.80	77.96#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035201.D
 Acq On : 20 Apr 2023 03:48
 Operator : JC/MD
 Sample : 02378-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML2

Manual IntegrationsAPPROVED

Quant Time: Apr 20 05:11:48 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041823WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 20 04:51:49 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 04/20/2023
 Supervised By :Mahesh Dadoda 04/21/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	433871	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.061	117	384357	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	197230	50.000	ug/L	# 0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	115718	41.363	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	82.720%	
7) Chloroethane-d5	1.672	69	94409	46.702	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	93.400%	
11) 1,1-Dichloroethene-d2	2.306	65	61283	45.781	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	91.560%	
21) 2-Butanone-d5	4.458	46	208561	111.870	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	111.870%	
24) Chloroform-d	5.056	84	271992	51.627	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	103.260%	
26) 1,2-Dichloroethane-d4	5.958	65	184481	54.528	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	109.060%	
32) Benzene-d6	5.976	84	571681	51.778	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	103.560%	
36) 1,2-Dichloropropane-d6	7.305	67	178848	53.029	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	106.060%	
41) Toluene-d8	8.647	98	507671	50.310	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	100.620%	
43) trans-1,3-Dichloroprop...	8.951	79	69825	47.374	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	94.740%	
47) 2-Hexanone-d5	9.384	63	153519	113.351	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	113.350%	
56) 1,1,2,2-Tetrachloroeth...	11.189	84	225674	54.637	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	109.280%	
66) 1,2-Dichlorobenzene-d4	12.323	152	190452	49.829	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	99.660%	
Target Compounds						
						Qvalue
25) Chloroform	5.086	83	22703	4.352	ug/L	99
31) Carbon tetrachloride	5.678	117	16712	4.372	ug/L	100
33) Benzene	6.050	78	15947092	1370.053	ug/L	100
51) Chlorobenzene	10.092	112	14141151m	1777.401	ug/L	
64) 1,3-Dichlorobenzene	11.969	146	1139022	186.221	ug/L	100
65) 1,4-Dichlorobenzene	12.048	146	9530482	1522.731	ug/L #	83
67) 1,2-Dichlorobenzene	12.341	146	10491275	1691.636	ug/L #	81
70) 1,2,4-trichlorobenzene	13.591	180	1479334	417.811	ug/L	100
72) 1,2,3-Trichlorobenzene	13.963	180	310905	88.947	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035201.D
Acq On : 20 Apr 2023 03:48
Operator : JC/MD
Sample : 02378-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COML2

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/20/2023
Supervised By :Mahesh Dadoda 04/21/2023

Quant Time: Apr 20 05:11:48 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 20 04:51:49 2023
Response via : Initial Calibration

