

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035189.D
 Acq On : 19 Apr 2023 23:11
 Operator : JC/MD
 Sample : 02333-14 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMG9

Quant Time: Apr 20 05:08:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 20 04:51:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	497238	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	433866	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	201882	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	119285	37.205	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	74.400%
7) Chloroethane-d5	1.672	69	90679	39.140	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	78.280%
11) 1,1-Dichloroethene-d2	2.306	65	60483	39.426	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.860%
21) 2-Butanone-d5	4.459	46	210568	98.553	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	98.550%
24) Chloroform-d	5.056	84	264602	43.823	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.640%
26) 1,2-Dichloroethane-d4	5.958	65	180081	46.444	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.880%
32) Benzene-d6	5.970	84	560548	44.976	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.960%
36) 1,2-Dichloropropane-d6	7.306	67	177202	46.545	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	93.100%
41) Toluene-d8	8.647	98	497880	43.710	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.420%
43) trans-1,3-Dichloroprop...	8.952	79	65263	39.226	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.460%
47) 2-Hexanone-d5	9.384	63	148872	97.377	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	97.380%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	222877	47.803	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.600%
66) 1,2-Dichlorobenzene-d4	12.323	152	182671	46.692	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.380%
Target Compounds						
					Qvalue	
33) Benzene	6.038	78	13287	1.011	ug/L	100
51) Chlorobenzene	10.079	112	65947	7.343	ug/L	98
64) 1,3-Dichlorobenzene	11.969	146	53894	8.608	ug/L	99
65) 1,4-Dichlorobenzene	12.043	146	831420	129.779	ug/L	99
67) 1,2-Dichlorobenzene	12.335	146	214612	33.807	ug/L	99
70) 1,2,4-trichlorobenzene	13.591	180	42083	11.612	ug/L	99
72) 1,2,3-Trichlorobenzene	13.963	180	9492	2.653	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035189.D
Acq On : 19 Apr 2023 23:11
Operator : JC/MD
Sample : 02333-14 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMG9

Quant Time: Apr 20 05:08:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 20 04:51:49 2023
Response via : Initial Calibration




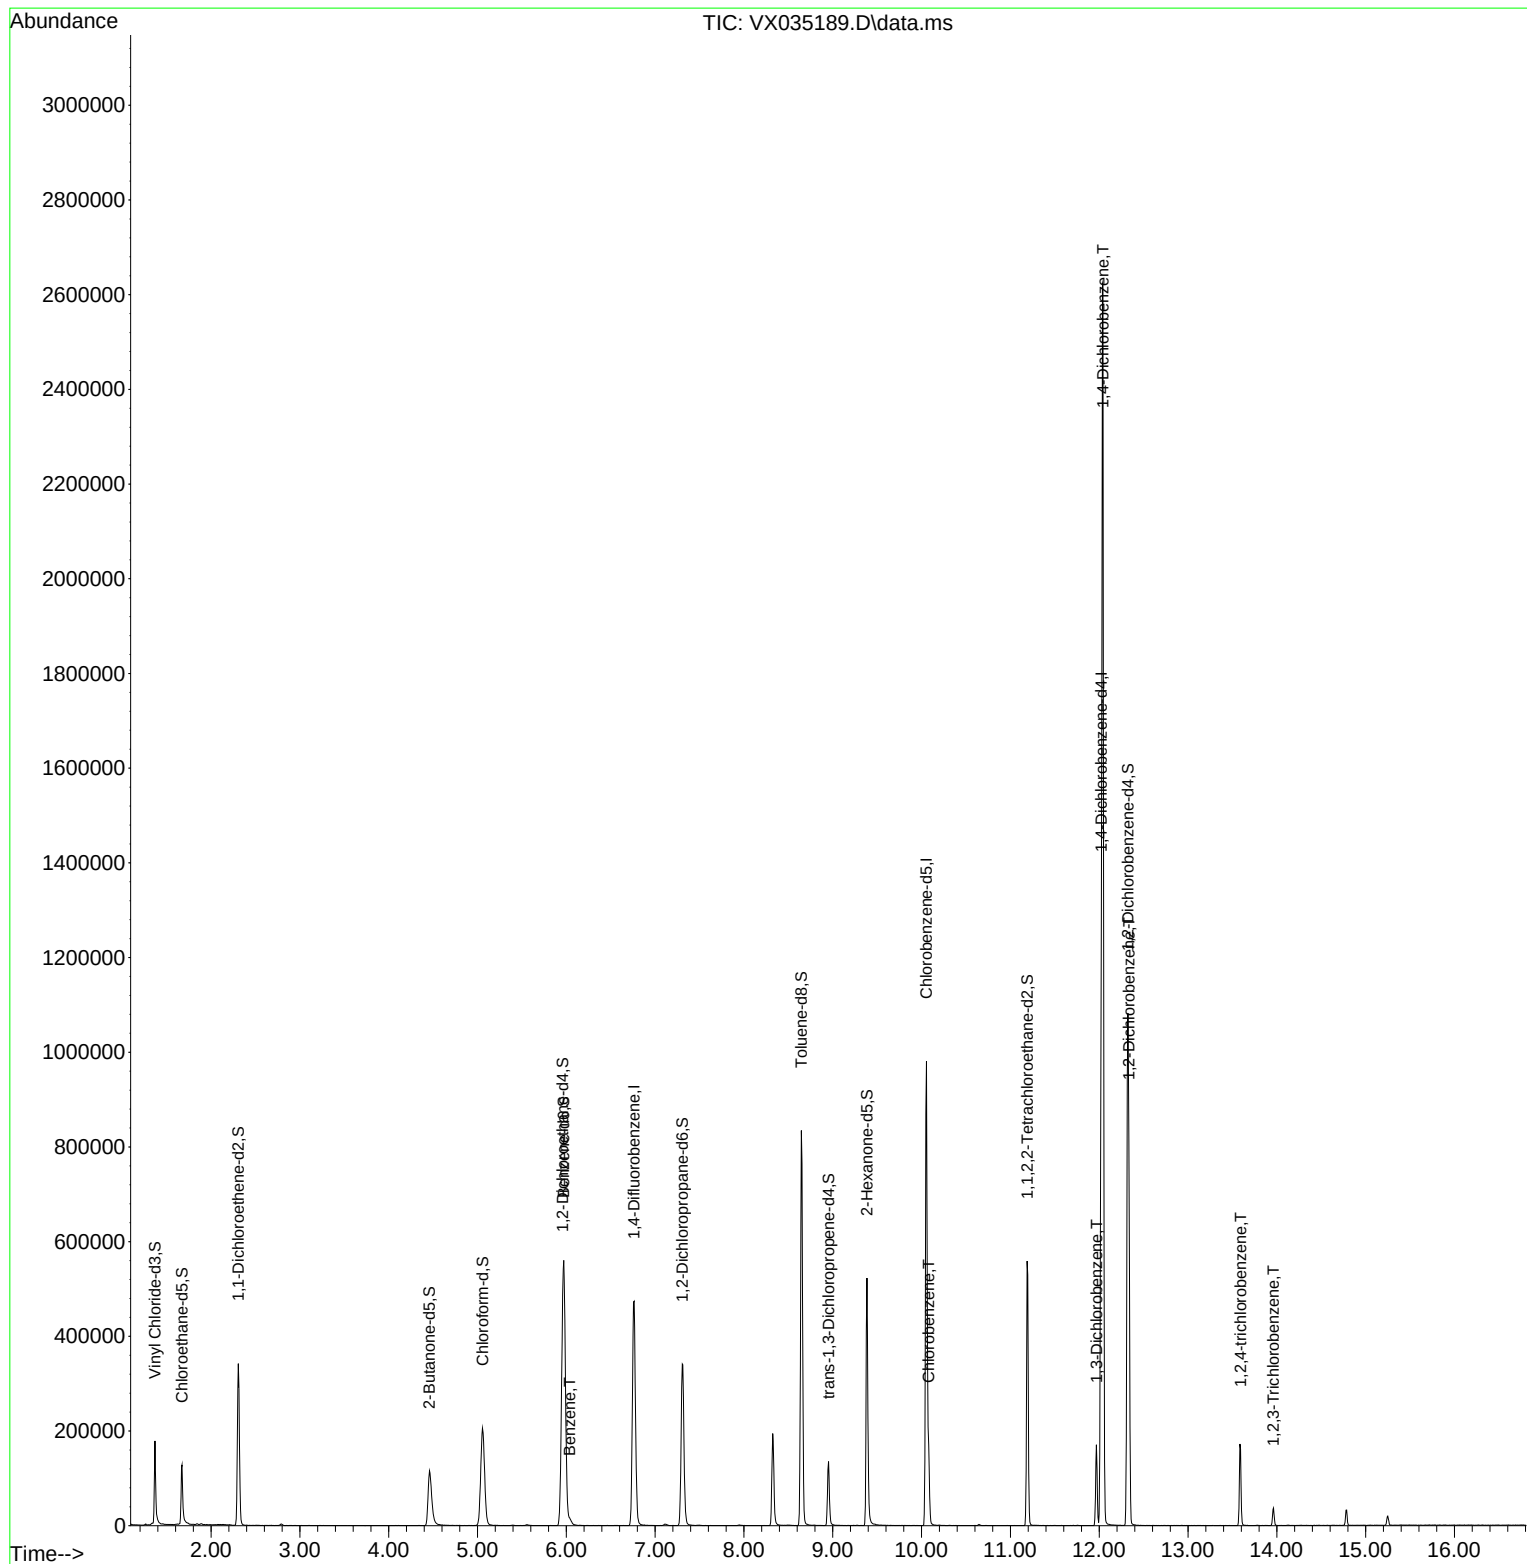


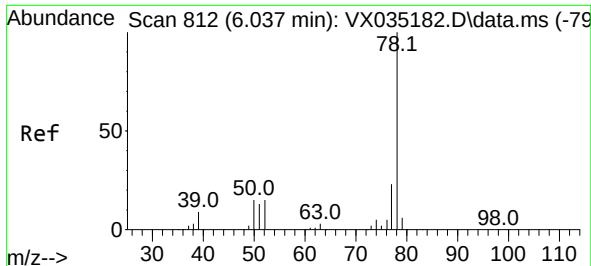

#33
Benzene
Concen: 1.011 ug/L
RT: 6.038 min Scan# 812
Delta R.T. 0.000 min
Lab File: VX035189.D
Acq: 19 Apr 2023 23:11




Instrument :
MSVOA_X
ClientSampleId :
COMG9


Tgt Ion: 78 Resp: 13287

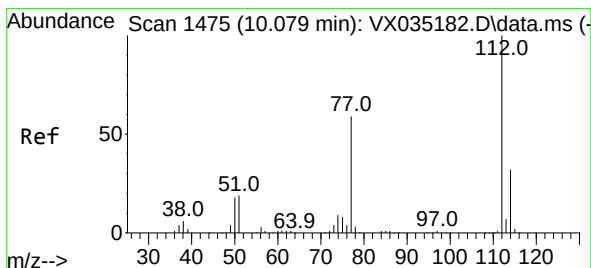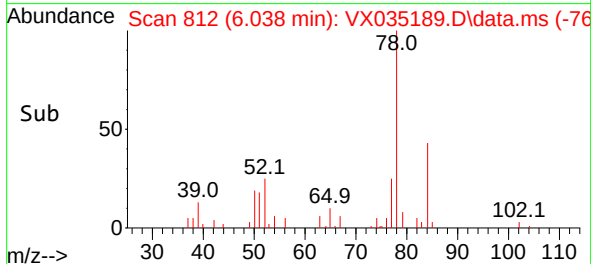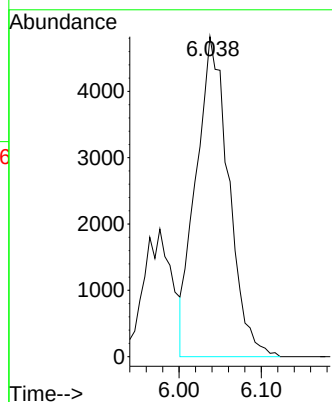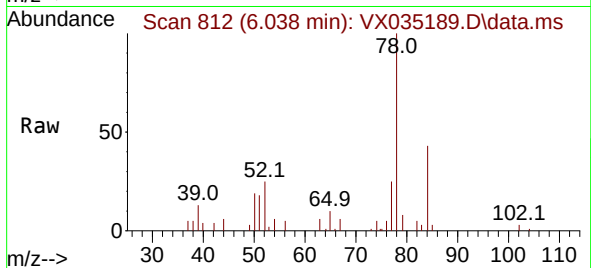

#51
Chlorobenzene
Concen: 7.343 ug/L
RT: 10.079 min Scan# 1475
Delta R.T. 0.000 min
Lab File: VX035189.D
Acq: 19 Apr 2023 23:11

Tgt Ion:112 Resp: 65947
Ion Ratio Lower Upper
112 100
114 33.4 22.4 41.6
77 57.5 47.0 70.6


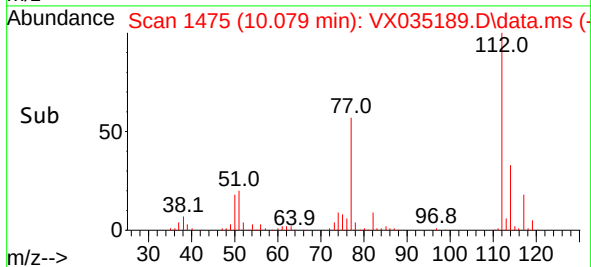
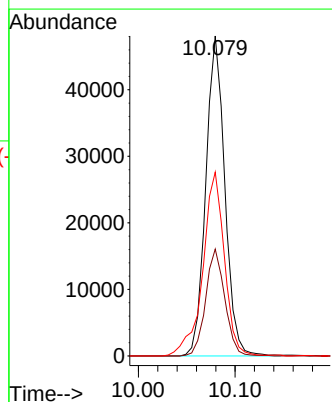
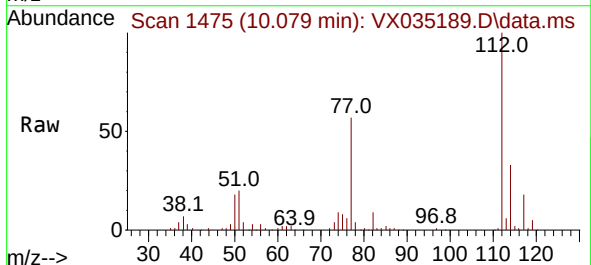


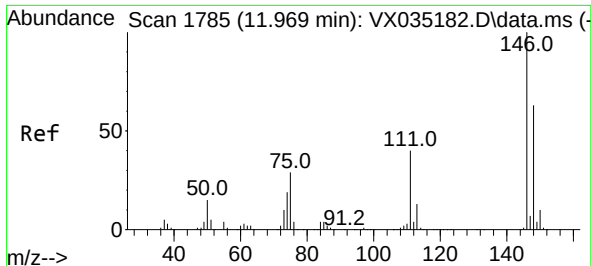

#64
 1,3-Dichlorobenzene
 Concen: 8.608 ug/L
 RT: 11.969 min Scan# 1785
 Delta R.T. 0.000 min
 Lab File: VX035189.D
 Acq: 19 Apr 2023 23:11




Instrument :
 MSVOA_X
 ClientSampleId :
 COMG9


Tgt Ion:146 Resp: 53894
 Ion Ratio Lower Upper
 146 100
 111 39.2 28.9 53.7
 148 63.5 44.3 82.3

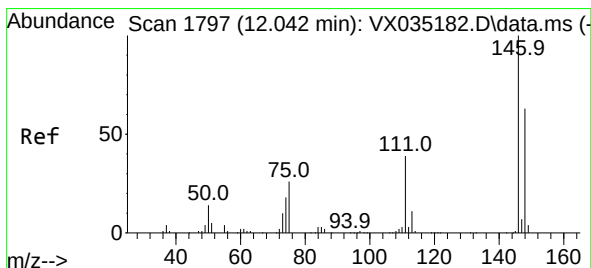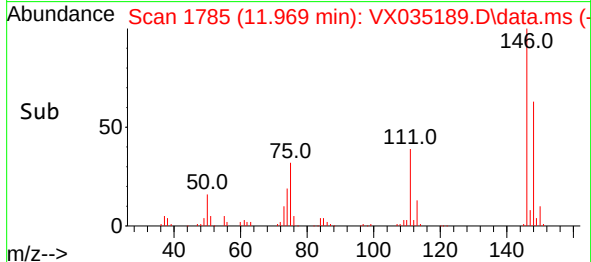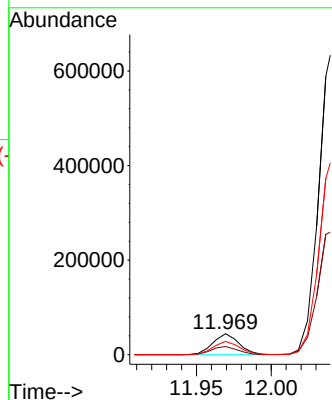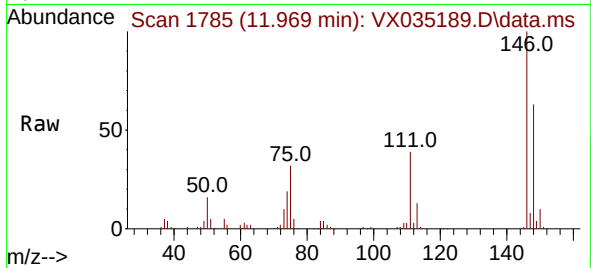

#65
 1,4-Dichlorobenzene
 Concen: 129.779 ug/L
 RT: 12.043 min Scan# 1797
 Delta R.T. 0.000 min
 Lab File: VX035189.D
 Acq: 19 Apr 2023 23:11

Tgt Ion:146 Resp: 831420
 Ion Ratio Lower Upper
 146 100
 111 39.0 27.9 51.7
 148 64.5 45.9 85.3

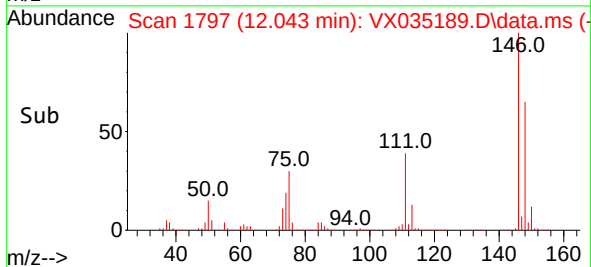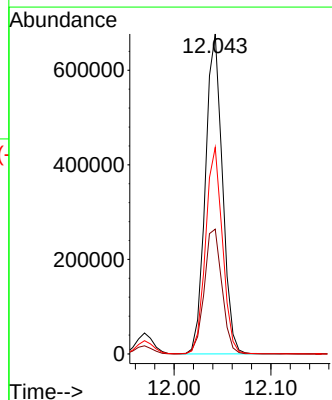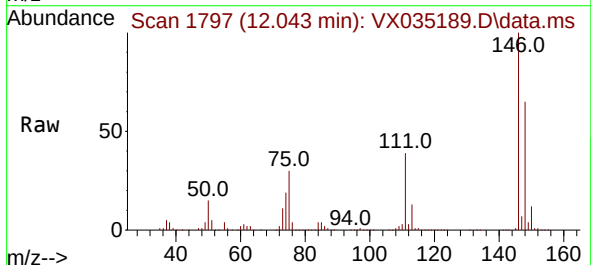

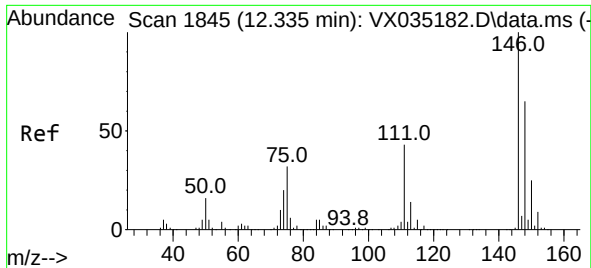

#67

1,2-Dichlorobenzene

Concen: 33.807 ug/L

RT: 12.335 min Scan# 1845

Delta R.T. 0.000 min

Lab File: VX035189.D

Acq: 19 Apr 2023 23:11

Instrument :

MSVOA_X

ClientSampleId :

COMG9





Tgt Ion:146 Resp: 214612

Ion Ratio Lower Upper

146 100

111 42.8 34.7 52.1

148 64.2 52.1 78.1

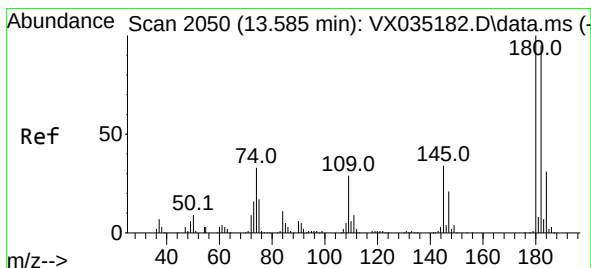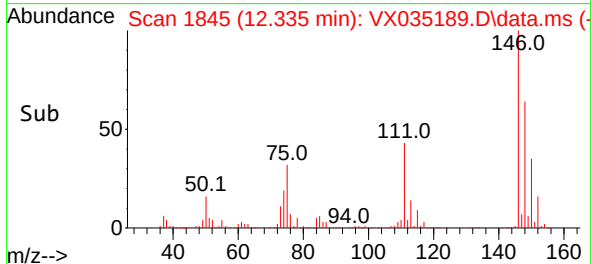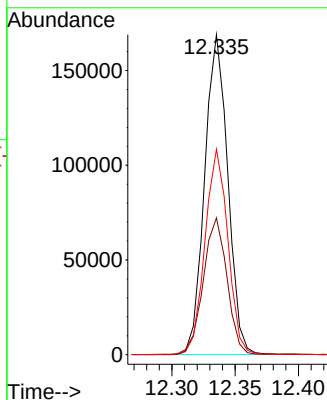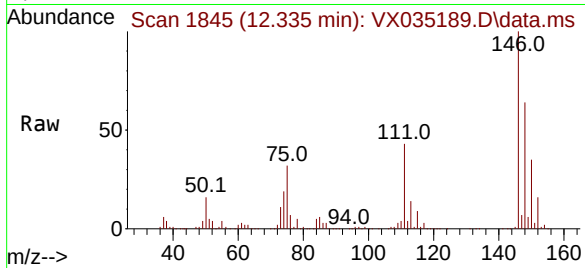

#70

1,2,4-trichlorobenzene

Concen: 11.612 ug/L

RT: 13.591 min Scan# 2051

Delta R.T. 0.006 min

Lab File: VX035189.D

Acq: 19 Apr 2023 23:11




Tgt Ion:180 Resp: 42083


Ion Ratio Lower Upper

180 100

182 96.1 76.6 114.8


145 33.7 26.2 39.4

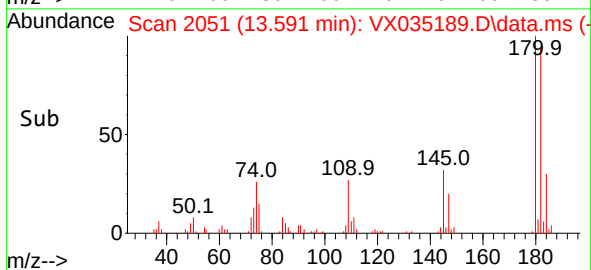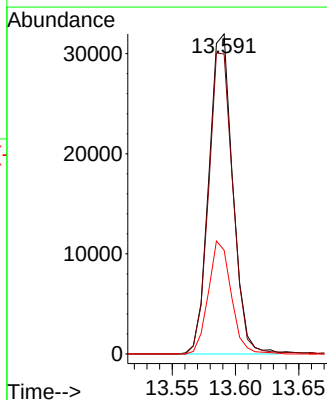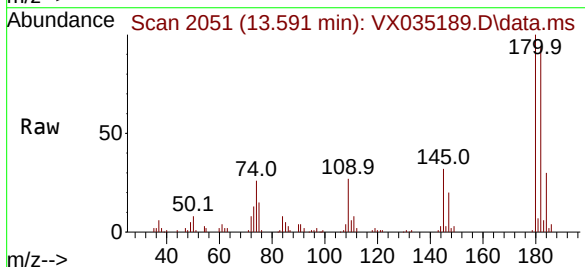

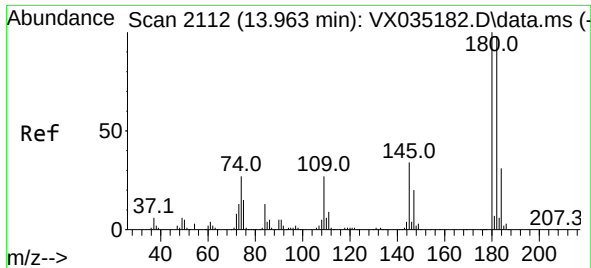

#72
 1,2,3-Trichlorobenzene
 Concen: 2.653 ug/L
 RT: 13.963 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VX035189.D
 Acq: 19 Apr 2023 23:11

Instrument :
 MSVOA_X
 ClientSampleId :
 C0MG9

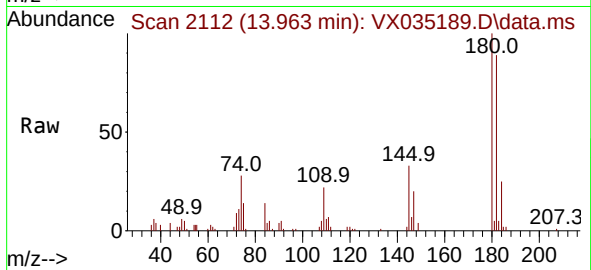

Tgt Ion:	180	Resp:	9492
Ion	Ratio	Lower	Upper
180	100		
182	92.8	75.0	112.6
145	32.5	27.1	40.7

