

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035158.D
 Acq On : 19 Apr 2023 10:46
 Operator : JC/MD
 Sample : VX0419WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK624

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035158.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	27	29	31	rBV3	1737	1685	0.09%	0.013%
2	1.368	42	46	57	rBV	209387	239062	13.37%	1.814%
3	1.673	91	96	110	rBV	158098	211997	11.85%	1.608%
4	2.307	194	200	211	rBV	402254	624333	34.91%	4.737%
5	2.520	230	235	238	rVB2	1213	1764	0.10%	0.013%
6	2.788	275	279	288	rVB4	2827	5485	0.31%	0.042%
7	3.002	312	314	315	rBV2	277	250	0.01%	0.002%
8	3.087	326	328	331	rBV3	726	973	0.05%	0.007%
9	3.215	347	349	353	rBV2	294	361	0.02%	0.003%
10	3.251	353	355	358	rVV2	189	206	0.01%	0.002%
11	3.306	363	364	366	rBV2	229	203	0.01%	0.002%
12	3.562	403	406	407	rBV	212	249	0.01%	0.002%
13	3.605	411	413	414	rBV	427	242	0.01%	0.002%
14	3.703	425	429	430	rBV2	191	254	0.01%	0.002%
15	3.739	432	435	437	rBV	233	220	0.01%	0.002%
16	3.800	444	445	448	rBV2	301	288	0.02%	0.002%
17	4.032	482	483	488	rVB2	404	445	0.02%	0.003%
18	4.111	494	496	499	rBV	331	299	0.02%	0.002%
19	4.294	525	526	528	rBV	250	200	0.01%	0.002%
20	4.331	531	532	535	rVB2	224	200	0.01%	0.002%
21	4.361	535	537	540	rBV2	208	255	0.01%	0.002%
22	4.465	543	554	574	rBV	106277	327231	18.30%	2.483%
23	4.721	594	596	599	rBV2	440	364	0.02%	0.003%
24	4.916	627	628	632	rVB2	298	218	0.01%	0.002%
25	4.971	634	637	639	rBV	162	217	0.01%	0.002%
26	5.056	639	651	670	rBV	219880	683799	38.23%	5.188%
27	5.263	682	685	686	rBV2	347	367	0.02%	0.003%
28	5.367	700	702	703	rBV	469	412	0.02%	0.003%
29	5.379	703	704	706	rBV	537	486	0.03%	0.004%
30	5.550	725	732	734	rBV3	2171	3997	0.22%	0.030%
31	5.751	764	765	768	rVB2	268	226	0.01%	0.002%
32	5.867	782	784	786	rBV2	239	221	0.01%	0.002%
33	5.964	788	800	819	rBV2	594275	1788539	100.00%	13.569%
34	6.318	856	858	861	rBV2	207	210	0.01%	0.002%
35	6.483	883	885	888	rBV3	309	390	0.02%	0.003%
36	6.690	916	919	921	rBV2	208	267	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035158.D
 Acq On : 19 Apr 2023 10:46
 Operator : JC/MD
 Sample : VX0419WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK624

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	6.757	921	930	946	rBV	482199	1163483	65.05%	8.827%
38	7.123	982	990	998	rBV5	4388	10775	0.60%	0.082%
39	7.226	1005	1007	1008	rBV2	332	263	0.01%	0.002%
40	7.306	1011	1020	1038	rBV	369803	807288	45.14%	6.125%
41	7.476	1045	1048	1050	rBV3	1108	1468	0.08%	0.011%
42	7.604	1066	1069	1070	rVV	193	200	0.01%	0.002%
43	7.647	1074	1076	1079	rVB2	203	206	0.01%	0.002%
44	7.757	1090	1094	1095	rBV	208	194	0.01%	0.001%
45	7.879	1112	1114	1116	rBV	290	240	0.01%	0.002%
46	7.915	1119	1120	1121	rBV	354	205	0.01%	0.002%
47	7.940	1122	1124	1126	rBV2	742	761	0.04%	0.006%
48	8.104	1148	1151	1154	rVB2	270	321	0.02%	0.002%
49	8.324	1181	1187	1209	rBV	227296	373193	20.87%	2.831%
50	8.580	1225	1229	1233	rBV4	408	602	0.03%	0.005%
51	8.647	1233	1240	1265	rBV	923949	1465838	81.96%	11.121%
52	8.891	1278	1280	1281	rBV2	263	203	0.01%	0.002%
53	8.952	1284	1290	1304	rBV	154079	234533	13.11%	1.779%
54	9.275	1339	1343	1347	rVB3	1268	1786	0.10%	0.014%
55	9.385	1355	1361	1381	rBV	493527	711700	39.79%	5.400%
56	9.653	1403	1405	1406	rBV2	349	189	0.01%	0.001%
57	9.823	1430	1433	1435	rVB	263	212	0.01%	0.002%
58	9.988	1458	1460	1463	rVB2	264	272	0.02%	0.002%
59	10.055	1465	1471	1490	rVV	925299	1313457	73.44%	9.965%
60	10.299	1509	1511	1512	rBV	463	292	0.02%	0.002%
61	10.403	1525	1528	1531	rBV	275	362	0.02%	0.003%
62	10.464	1537	1538	1541	rVB	329	249	0.01%	0.002%
63	10.488	1541	1542	1545	rBV2	274	244	0.01%	0.002%
64	10.647	1563	1568	1569	rBV3	767	788	0.04%	0.006%
65	10.744	1581	1584	1585	rBV	272	332	0.02%	0.003%
66	10.927	1610	1614	1616	rVB	257	281	0.02%	0.002%
67	10.964	1616	1620	1625	rBV2	1492	1489	0.08%	0.011%
68	11.018	1627	1629	1632	rBV2	200	197	0.01%	0.001%
69	11.092	1639	1641	1645	rBV2	436	533	0.03%	0.004%
70	11.189	1652	1657	1671	rVB	586633	757024	42.33%	5.743%
71	11.281	1671	1672	1677	rBV4	423	427	0.02%	0.003%
72	11.415	1690	1694	1695	rBV2	274	336	0.02%	0.003%
73	11.451	1697	1700	1704	rVB2	982	1239	0.07%	0.009%
74	11.713	1739	1743	1744	rVB3	704	592	0.03%	0.004%
75	11.756	1747	1750	1755	rVB3	816	1182	0.07%	0.009%
76	11.915	1773	1776	1777	rBV2	267	303	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035158.D
 Acq On : 19 Apr 2023 10:46
 Operator : JC/MD
 Sample : VX0419WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK624

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M

Title : VOC Analysis

77	11.976	1781	1786	1788	rBV3	2842	3757	0.21%	0.029%
78	12.018	1788	1793	1807	rVV	907664	1198158	66.99%	9.090%
79	12.317	1837	1842	1852	rBV	920726	1192674	66.68%	9.049%
80	12.518	1874	1875	1880	rVB2	323	408	0.02%	0.003%
81	12.597	1886	1888	1890	rVB2	342	237	0.01%	0.002%
82	12.628	1890	1893	1895	rBV2	281	322	0.02%	0.002%
83	12.707	1903	1906	1907	rBV	309	289	0.02%	0.002%
84	12.762	1913	1915	1920	rVB3	612	626	0.04%	0.005%
85	12.823	1924	1925	1928	rVB	386	338	0.02%	0.003%
86	12.902	1935	1938	1940	rBV2	370	332	0.02%	0.003%
87	13.061	1962	1964	1966	rVB	255	189	0.01%	0.001%
88	13.116	1969	1973	1978	rVB3	5457	6783	0.38%	0.051%
89	13.195	1983	1986	1987	rBV2	290	267	0.01%	0.002%
90	13.335	2004	2009	2010	rBV2	288	383	0.02%	0.003%
91	13.426	2022	2024	2026	rBV	215	188	0.01%	0.001%
92	13.591	2047	2051	2055	rBV2	11300	14262	0.80%	0.108%
93	13.780	2079	2082	2087	rVB	1915	2571	0.14%	0.020%
94	13.963	2108	2112	2118	rBV2	5027	6651	0.37%	0.050%
95	14.097	2130	2134	2135	rBV2	318	299	0.02%	0.002%
96	14.128	2137	2139	2144	rVB3	753	1092	0.06%	0.008%
97	14.280	2160	2164	2165	rBV2	506	540	0.03%	0.004%
98	14.371	2177	2179	2181	rVB2	360	249	0.01%	0.002%
99	15.073	2292	2294	2296	rBV	483	305	0.02%	0.002%
100	15.658	2388	2390	2392	rBV2	724	577	0.03%	0.004%




Sum of corrected areas: 13180671

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035158.D
Acq On : 19 Apr 2023 10:46
Operator : JC/MD
Sample : VX0419WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK624

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

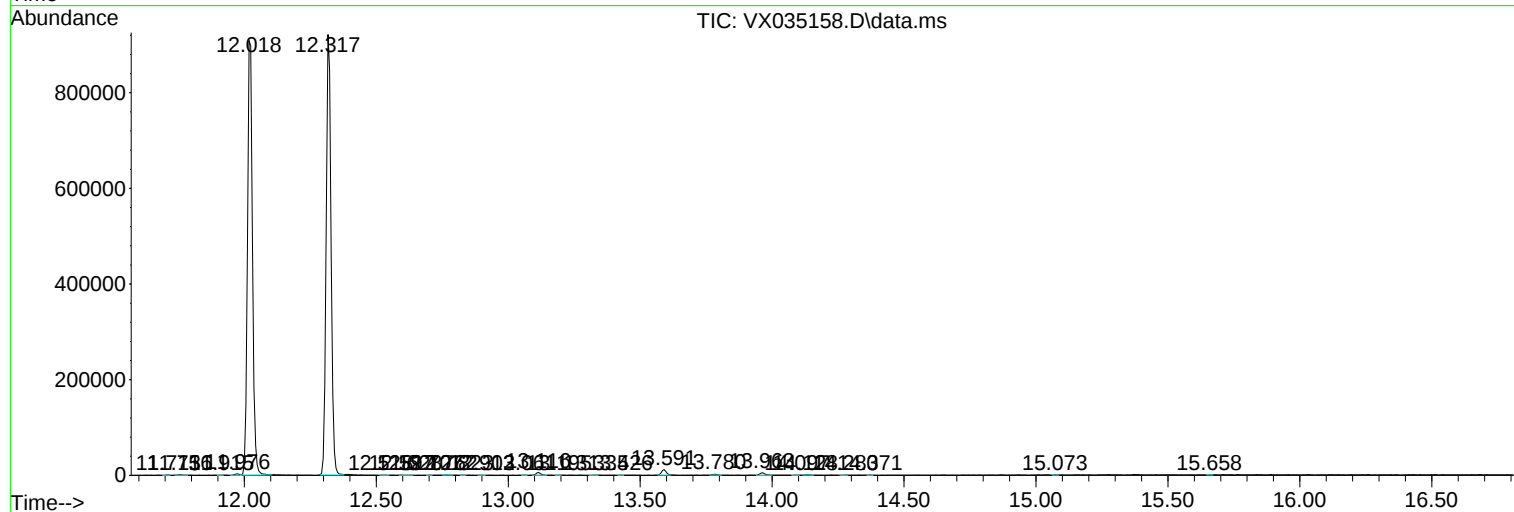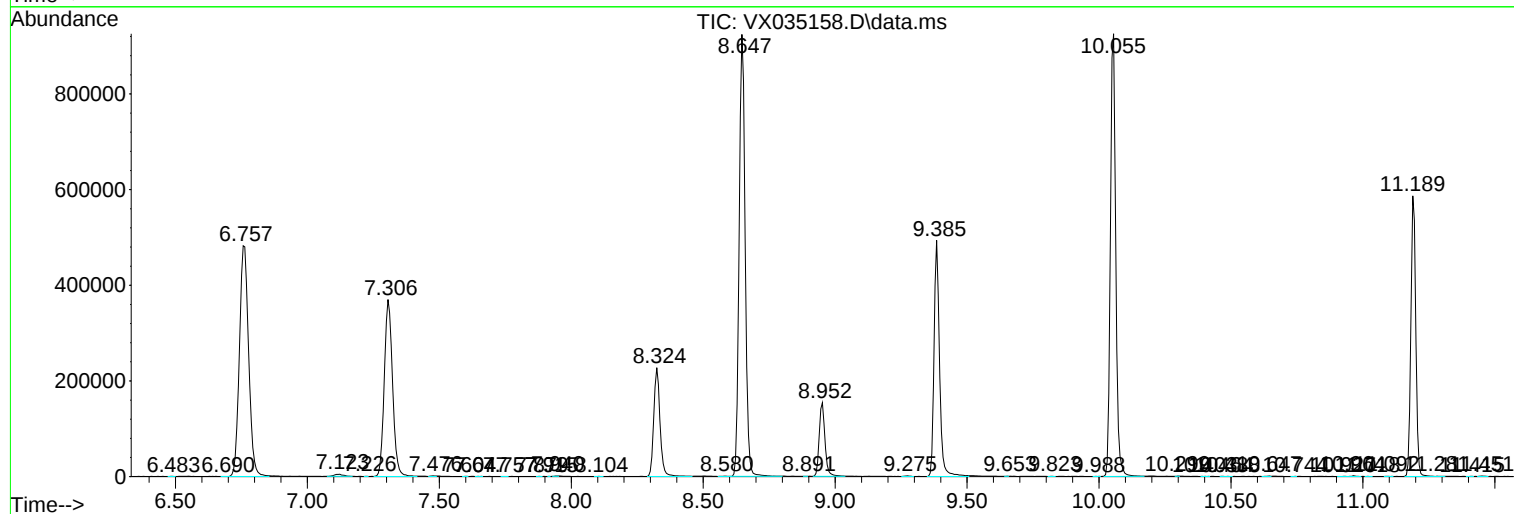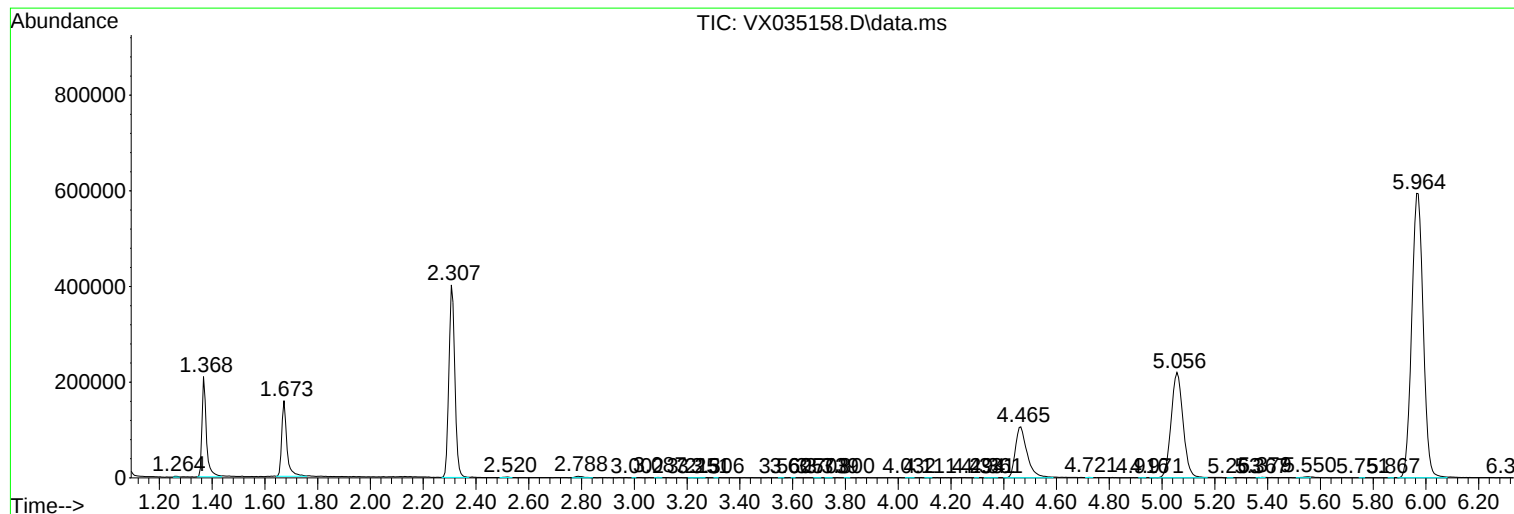

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035158.D
Acq On : 19 Apr 2023 10:46
Operator : JC/MD
Sample : VX0419WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK624

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035158.D
Acq On : 19 Apr 2023 10:46
Operator : JC/MD
Sample : VX0419WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK624

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc