

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035159.D
 Acq On : 19 Apr 2023 11:15
 Operator : JC/MD
 Sample : 02397-04DL 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035159.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	31	rBV2	1786	1996	0.08%	0.013%
2	1.367	42	46	58	rBV	213650	241027	9.49%	1.577%
3	1.672	91	96	108	rBV	162491	213274	8.40%	1.396%
4	2.306	194	200	213	rBV	405044	630137	24.81%	4.124%
5	2.593	244	247	249	rBV2	385	444	0.02%	0.003%
6	2.611	249	250	254	rBV	585	701	0.03%	0.005%
7	2.788	274	279	289	rVB3	3280	7039	0.28%	0.046%
8	2.873	289	293	296	rBV3	220	390	0.02%	0.003%
9	2.928	300	302	304	rBV2	443	460	0.02%	0.003%
10	3.032	317	319	321	rBV	282	270	0.01%	0.002%
11	3.093	325	329	331	rBV2	510	701	0.03%	0.005%
12	3.300	360	363	365	rBV2	297	222	0.01%	0.001%
13	3.452	384	388	390	rBV2	459	573	0.02%	0.004%
14	3.477	390	392	395	rVB3	240	222	0.01%	0.001%
15	3.526	399	400	403	rVB2	272	231	0.01%	0.002%
16	3.568	405	407	408	rBV	252	216	0.01%	0.001%
17	3.733	432	434	437	rVB2	274	283	0.01%	0.002%
18	3.867	454	456	459	rVB2	281	247	0.01%	0.002%
19	3.916	459	464	465	rBV2	313	371	0.01%	0.002%
20	4.099	490	494	495	rBV	215	257	0.01%	0.002%
21	4.391	540	542	545	rBV2	187	242	0.01%	0.002%
22	4.465	545	554	577	rBV	104210	333707	13.14%	2.184%
23	4.647	583	584	588	rBV3	523	411	0.02%	0.003%
24	4.946	629	633	634	rBV2	162	232	0.01%	0.002%
25	5.056	638	651	664	rBV	222488	704520	27.74%	4.611%
26	5.263	683	685	689	rVB3	390	361	0.01%	0.002%
27	5.324	693	695	698	rBV2	443	410	0.02%	0.003%
28	5.379	701	704	706	rBV3	399	518	0.02%	0.003%
29	5.550	725	732	737	rBV4	1847	4664	0.18%	0.031%
30	5.672	747	752	754	rBV3	852	1445	0.06%	0.009%
31	5.964	786	800	808	rBV2	614844	1867997	73.54%	12.225%
32	6.367	863	866	867	rBV2	214	232	0.01%	0.002%
33	6.464	876	882	883	rBV2	295	377	0.01%	0.002%
34	6.495	886	887	891	rBV3	225	306	0.01%	0.002%
35	6.537	892	894	897	rVV2	383	447	0.02%	0.003%
36	6.568	897	899	900	rVB2	383	236	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035159.D
 Acq On : 19 Apr 2023 11:15
 Operator : JC/MD
 Sample : 02397-04DL 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	6.757	920	930	951	rBV	444958	1063670	41.87%	6.961%
38	7.037	973	976	978	rBB	337	252	0.01%	0.002%
39	7.110	982	988	998	rVB5	3648	10128	0.40%	0.066%
40	7.232	1005	1008	1009	rBV	257	212	0.01%	0.001%

41	7.305	1011	1020	1038	rBV	382434	828369	32.61%	5.421%
42	7.476	1044	1048	1050	rBV4	742	1267	0.05%	0.008%
43	7.647	1071	1076	1078	rBV2	208	298	0.01%	0.002%
44	7.702	1083	1085	1088	rVV2	207	234	0.01%	0.002%
45	7.811	1100	1103	1107	rVB2	296	405	0.02%	0.003%

46	7.891	1114	1116	1117	rBV	359	229	0.01%	0.001%
47	7.946	1119	1125	1132	rBV4	1088	2539	0.10%	0.017%
48	8.049	1140	1142	1144	rVB	250	220	0.01%	0.001%
49	8.135	1153	1156	1157	rBV	267	218	0.01%	0.001%
50	8.196	1164	1166	1170	rVB2	165	207	0.01%	0.001%

51	8.257	1172	1176	1180	rVB4	984	1382	0.05%	0.009%
52	8.324	1180	1187	1200	rBV	233465	385956	15.19%	2.526%
53	8.494	1211	1215	1226	rBV6	876	2785	0.11%	0.018%
54	8.647	1233	1240	1255	rBV	948009	1507928	59.36%	9.868%
55	8.952	1284	1290	1301	rBV	157313	241506	9.51%	1.580%

56	9.275	1338	1343	1347	rBV2	1501	1973	0.08%	0.013%
57	9.384	1355	1361	1376	rBV	500435	724469	28.52%	4.741%
58	9.909	1444	1447	1451	rVV	315	306	0.01%	0.002%
59	10.055	1465	1471	1473	rBV	895530	1398082	55.04%	9.150%
60	10.238	1500	1501	1504	rVB	356	298	0.01%	0.002%

61	10.268	1504	1506	1509	rVB2	294	250	0.01%	0.002%
62	10.311	1509	1513	1519	rVB3	928	1447	0.06%	0.009%
63	10.396	1526	1527	1529	rBV2	360	215	0.01%	0.001%
64	10.488	1541	1542	1544	rBV	241	211	0.01%	0.001%
65	10.549	1550	1552	1555	rVB2	234	205	0.01%	0.001%

66	10.646	1566	1568	1569	rBV	555	520	0.02%	0.003%
67	10.969	1616	1621	1623	rVB2	520	765	0.03%	0.005%
68	11.091	1638	1641	1644	rVB3	471	603	0.02%	0.004%
69	11.128	1644	1647	1649	rVB	329	316	0.01%	0.002%
70	11.189	1652	1657	1670	rBV	586562	772675	30.42%	5.057%

71	11.311	1675	1677	1680	rVB3	713	723	0.03%	0.005%
72	11.457	1697	1701	1707	rBV4	810	1237	0.05%	0.008%
73	11.549	1714	1716	1718	rVB	281	251	0.01%	0.002%
74	11.573	1718	1720	1724	rVB3	246	266	0.01%	0.002%
75	11.622	1724	1728	1729	rBV2	197	217	0.01%	0.001%

76	11.640	1729	1731	1735	rVB3	206	279	0.01%	0.002%
----	--------	------	------	------	------	-----	-----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035159.D
 Acq On : 19 Apr 2023 11:15
 Operator : JC/MD
 Sample : 02397-04DL 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	11.713	1739	1743	1746	rVB4	1029	1210	0.05%	0.008%
78	11.756	1746	1750	1752	rBV3	834	864	0.03%	0.006%
79	11.969	1779	1785	1789	rBV	261977	324939	12.79%	2.127%
80	12.024	1789	1794	1795	rBV	989140	1233031	48.54%	8.069%
81	12.329	1837	1844	1854	rBV2	1345371	2540143	100.00%	16.624%
82	12.622	1890	1892	1895	rVB3	421	436	0.02%	0.003%
83	12.658	1896	1898	1901	rVV2	197	216	0.01%	0.001%
84	12.762	1909	1915	1919	rBV4	492	1035	0.04%	0.007%
85	12.926	1938	1942	1945	rVV5	1151	1358	0.05%	0.009%
86	12.987	1949	1952	1953	rBV	187	208	0.01%	0.001%
87	13.061	1962	1964	1967	rBV2	287	382	0.02%	0.002%
88	13.115	1969	1973	1977	rVB	2126	2285	0.09%	0.015%
89	13.201	1984	1987	1991	rVB2	614	826	0.03%	0.005%
90	13.506	2036	2037	2038	rBV	466	207	0.01%	0.001%
91	13.585	2045	2050	2059	rBV	106808	140667	5.54%	0.921%
92	13.701	2067	2069	2071	rBV2	230	206	0.01%	0.001%
93	13.780	2079	2082	2087	rVB2	1245	1840	0.07%	0.012%
94	13.963	2107	2112	2122	rVB	44410	58897	2.32%	0.385%
95	14.371	2178	2179	2182	rBV3	230	232	0.01%	0.002%
96	14.457	2191	2193	2195	rBV2	371	350	0.01%	0.002%
97	14.670	2226	2228	2232	rVB3	397	419	0.02%	0.003%
98	14.761	2241	2243	2244	rBV2	538	352	0.01%	0.002%
99	15.085	2294	2296	2297	rBV2	418	246	0.01%	0.002%
100	15.249	2321	2323	2329	rVB5	1591	1742	0.07%	0.011%




Sum of corrected areas: 15280370

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035159.D
Acq On : 19 Apr 2023 11:15
Operator : JC/MD
Sample : 02397-04DL 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COML6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

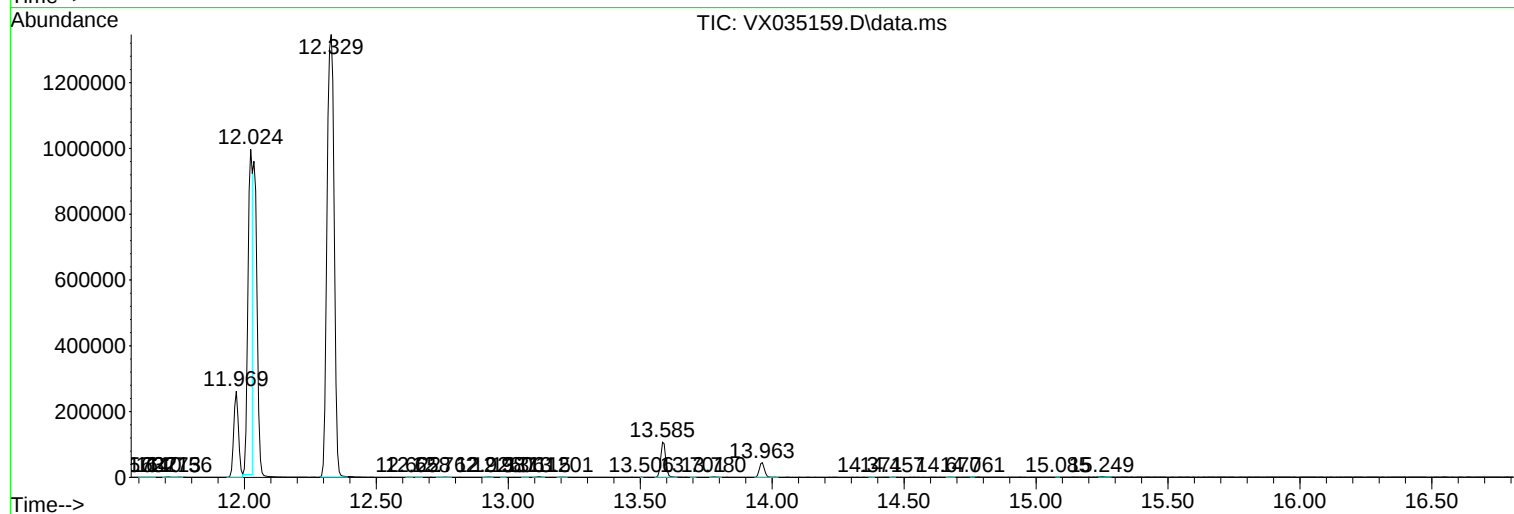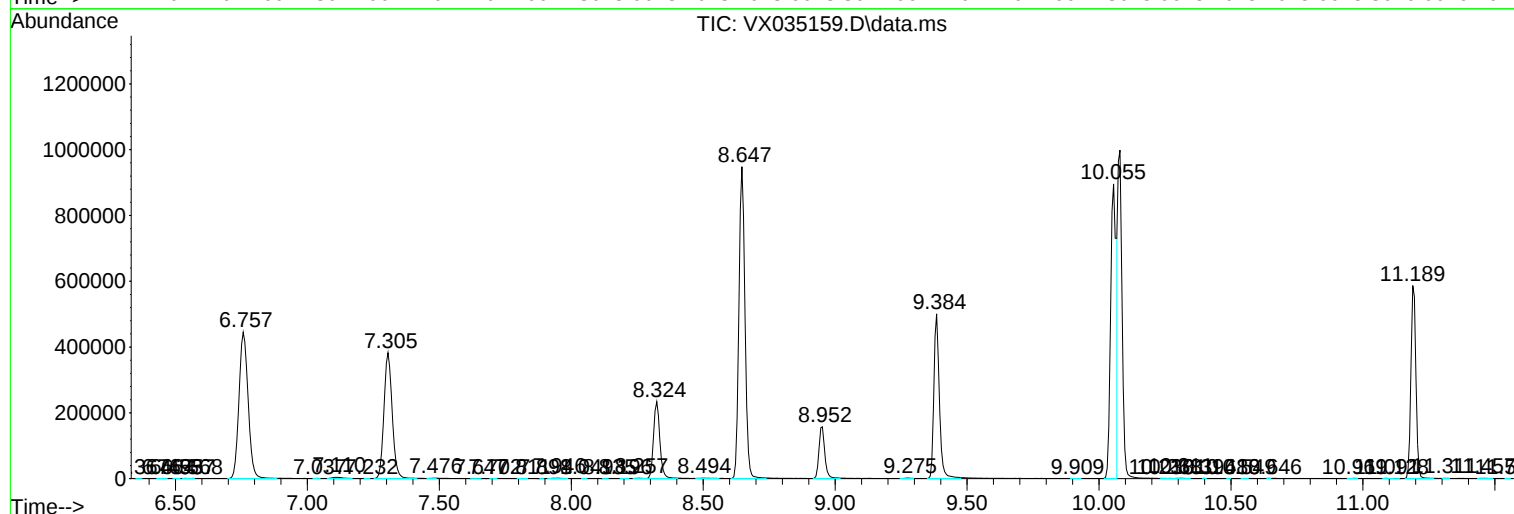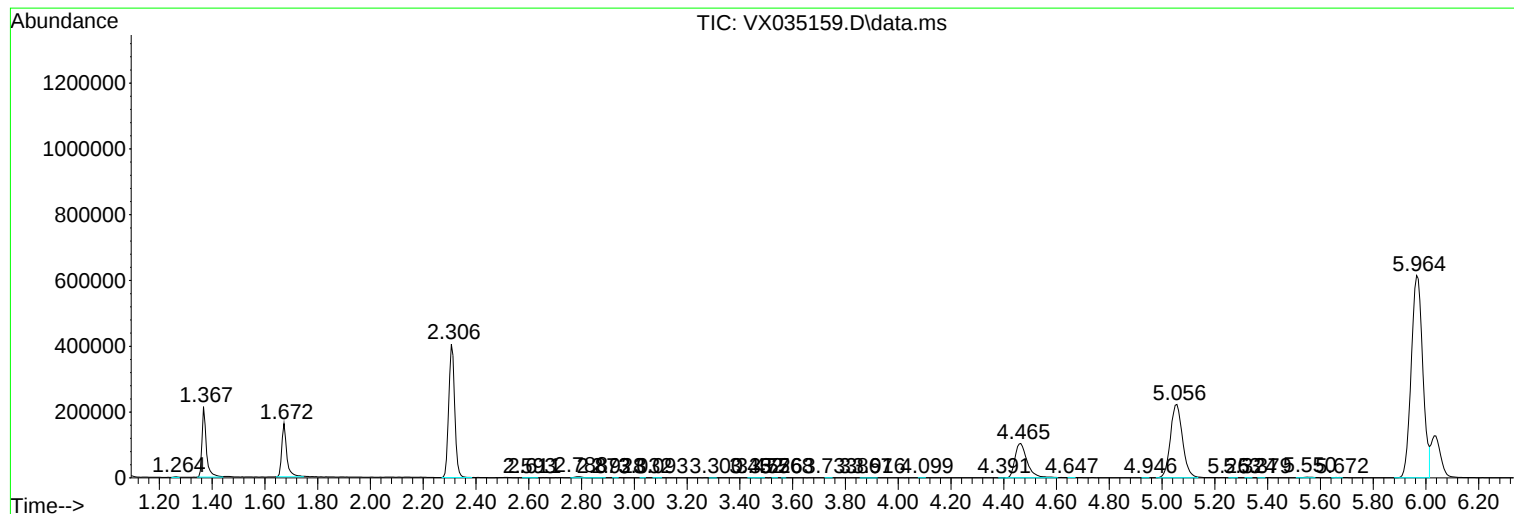

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035159.D
Acq On : 19 Apr 2023 11:15
Operator : JC/MD
Sample : 02397-04DL 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ML6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035159.D
Acq On : 19 Apr 2023 11:15
Operator : JC/MD
Sample : 02397-04DL 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ML6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------