

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035160.D
 Acq On : 19 Apr 2023 11:38
 Operator : JC/MD
 Sample : 02397-07DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035160.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	32	rBV4	1875	2242	0.09%	0.013%
2	1.368	42	46	59	rVB	215015	244695	9.59%	1.435%
3	1.672	92	96	118	rVB	164909	227353	8.91%	1.333%
4	2.307	193	200	212	rBV	416500	655467	25.68%	3.844%
5	2.514	231	234	241	rVB3	1012	1533	0.06%	0.009%
6	2.788	274	279	288	rVB3	3689	7251	0.28%	0.043%
7	2.941	301	304	305	rBV2	569	447	0.02%	0.003%
8	3.093	327	329	332	rVV2	312	376	0.01%	0.002%
9	3.166	339	341	343	rBV2	235	208	0.01%	0.001%
10	3.251	353	355	358	rVV2	276	271	0.01%	0.002%
11	3.288	358	361	363	rVV	245	247	0.01%	0.001%
12	3.312	363	365	369	rVV2	240	282	0.01%	0.002%
13	3.520	397	399	402	rVV	458	361	0.01%	0.002%
14	3.562	403	406	407	rVB3	225	204	0.01%	0.001%
15	3.587	407	410	413	rBV2	323	421	0.02%	0.002%
16	3.623	413	416	418	rBV2	268	263	0.01%	0.002%
17	3.873	453	457	459	rBV2	265	240	0.01%	0.001%
18	3.898	459	461	465	rVB2	249	285	0.01%	0.002%
19	3.946	467	469	471	rBV	156	205	0.01%	0.001%
20	4.020	480	481	484	rVB2	236	208	0.01%	0.001%
21	4.190	506	509	514	rVB3	258	368	0.01%	0.002%
22	4.385	538	541	545	rBV2	215	343	0.01%	0.002%
23	4.459	545	553	573	rBV	116819	365812	14.33%	2.146%
24	4.910	624	627	632	rVB4	424	799	0.03%	0.005%
25	4.946	632	633	634	rBV	319	199	0.01%	0.001%
26	5.056	638	651	669	rBV	233192	740449	29.01%	4.343%
27	5.233	678	680	682	rVB2	507	331	0.01%	0.002%
28	5.282	687	688	690	rVB	543	355	0.01%	0.002%
29	5.312	690	693	695	rBV2	338	291	0.01%	0.002%
30	5.361	700	701	703	rBV2	342	273	0.01%	0.002%
31	5.385	703	705	707	rBV2	455	589	0.02%	0.003%
32	5.556	726	733	743	rVB2	2074	5322	0.21%	0.031%
33	5.678	743	753	761	rBV5	1698	4299	0.17%	0.025%
34	5.739	761	763	766	rBV2	339	242	0.01%	0.001%
35	5.970	788	801	830	rVV2	637149	2007208	78.63%	11.773%
36	6.245	845	846	850	rVB2	385	372	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035160.D
 Acq On : 19 Apr 2023 11:38
 Operator : JC/MD
 Sample : 02397-07DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	6.275	850	851	853	rBV2	253	248	0.01%	0.001%
38	6.464	878	882	883	rBV	225	241	0.01%	0.001%
39	6.544	891	895	896	rBV2	314	375	0.01%	0.002%
40	6.611	903	906	910	rBV	360	466	0.02%	0.003%
41	6.757	921	930	947	rBV	462167	1106121	43.33%	6.488%
42	7.043	974	977	978	rVB3	232	212	0.01%	0.001%
43	7.117	981	989	997	rBV5	3745	9469	0.37%	0.056%
44	7.220	1003	1006	1008	rBV2	223	225	0.01%	0.001%
45	7.306	1008	1020	1039	rBV	395039	864209	33.85%	5.069%
46	7.556	1059	1061	1062	rBV	284	206	0.01%	0.001%
47	7.757	1091	1094	1098	rBV2	219	283	0.01%	0.002%
48	7.952	1121	1126	1131	rBV5	1342	2898	0.11%	0.017%
49	8.025	1136	1138	1142	rBV	216	249	0.01%	0.001%
50	8.153	1158	1159	1162	rVB2	343	276	0.01%	0.002%
51	8.190	1162	1165	1166	rBV	376	265	0.01%	0.002%
52	8.324	1180	1187	1201	rVV	242118	393055	15.40%	2.305%
53	8.488	1212	1214	1219	rBV3	705	1032	0.04%	0.006%
54	8.647	1234	1240	1256	rBV	1016767	1566878	61.38%	9.190%
55	8.952	1284	1290	1300	rBV	161251	248306	9.73%	1.456%
56	9.269	1337	1342	1346	rBV4	1224	1946	0.08%	0.011%
57	9.384	1355	1361	1376	rBV	553869	789230	30.92%	4.629%
58	9.744	1418	1420	1425	rBV2	283	420	0.02%	0.002%
59	9.787	1425	1427	1430	rBV4	269	264	0.01%	0.002%
60	9.903	1444	1446	1448	rBV	300	263	0.01%	0.002%
61	9.964	1452	1456	1457	rBV2	226	230	0.01%	0.001%
62	10.055	1465	1471	1473	rBV	922733	1393302	54.58%	8.172%
63	10.378	1522	1524	1526	rBV2	198	242	0.01%	0.001%
64	10.512	1541	1546	1548	rBV	373	574	0.02%	0.003%
65	10.561	1551	1554	1555	rVV3	248	232	0.01%	0.001%
66	10.646	1564	1568	1571	rBV3	503	973	0.04%	0.006%
67	10.793	1590	1592	1594	rBV	324	257	0.01%	0.002%
68	10.915	1608	1612	1615	rBV2	261	407	0.02%	0.002%
69	11.073	1636	1638	1641	rBV2	186	305	0.01%	0.002%
70	11.189	1652	1657	1670	rVB	650789	823339	32.25%	4.829%
71	11.409	1691	1693	1695	rBV2	301	257	0.01%	0.002%
72	11.463	1695	1702	1703	rVV2	401	535	0.02%	0.003%
73	11.530	1710	1713	1716	rVB3	232	306	0.01%	0.002%
74	11.561	1716	1718	1721	rBV	296	236	0.01%	0.001%
75	11.677	1735	1737	1739	rVB	403	242	0.01%	0.001%
76	11.713	1739	1743	1747	rBV2	744	841	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035160.D
 Acq On : 19 Apr 2023 11:38
 Operator : JC/MD
 Sample : 02397-07DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0ML9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	11.756	1747	1750	1754	rBV	505	403	0.02%	0.002%
78	11.969	1780	1785	1789	rBV	343556	422325	16.54%	2.477%
79	12.024	1789	1794	1807	rVB2	1003035	2125531	83.26%	12.467%
80	12.177	1818	1819	1824	rVB3	596	468	0.02%	0.003%
81	12.225	1824	1827	1832	rBV5	990	1423	0.06%	0.008%
82	12.323	1837	1843	1857	rVV2	1366187	2552793	100.00%	14.973%
83	12.756	1913	1914	1917	rVB3	376	309	0.01%	0.002%
84	12.859	1928	1931	1934	rBV3	344	472	0.02%	0.003%
85	12.920	1939	1941	1946	rVB3	846	1290	0.05%	0.008%
86	13.061	1963	1964	1966	rBV	470	380	0.01%	0.002%
87	13.116	1968	1973	1977	rVB2	1225	1466	0.06%	0.009%
88	13.384	2015	2017	2020	rVB2	227	209	0.01%	0.001%
89	13.439	2024	2026	2029	rBV3	229	215	0.01%	0.001%
90	13.585	2045	2050	2061	rBV	210239	278231	10.90%	1.632%
91	13.780	2079	2082	2089	rBV3	748	1623	0.06%	0.010%
92	13.841	2090	2092	2094	rVV	345	274	0.01%	0.002%
93	13.963	2107	2112	2125	rVV	119537	156728	6.14%	0.919%
94	14.054	2125	2127	2131	rVB2	356	307	0.01%	0.002%
95	14.713	2233	2235	2239	rBV	725	628	0.02%	0.004%
96	14.786	2241	2247	2250	rVV4	3124	5109	0.20%	0.030%
97	14.829	2252	2254	2258	rBV3	590	680	0.03%	0.004%
98	14.999	2280	2282	2285	rBV	641	696	0.03%	0.004%
99	15.249	2319	2323	2328	rBV2	13594	18162	0.71%	0.107%
100	16.030	2449	2451	2453	rBV2	699	582	0.02%	0.003%




Sum of corrected areas: 17049530

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035160.D
Acq On : 19 Apr 2023 11:38
Operator : JC/MD
Sample : 02397-07DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COML9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

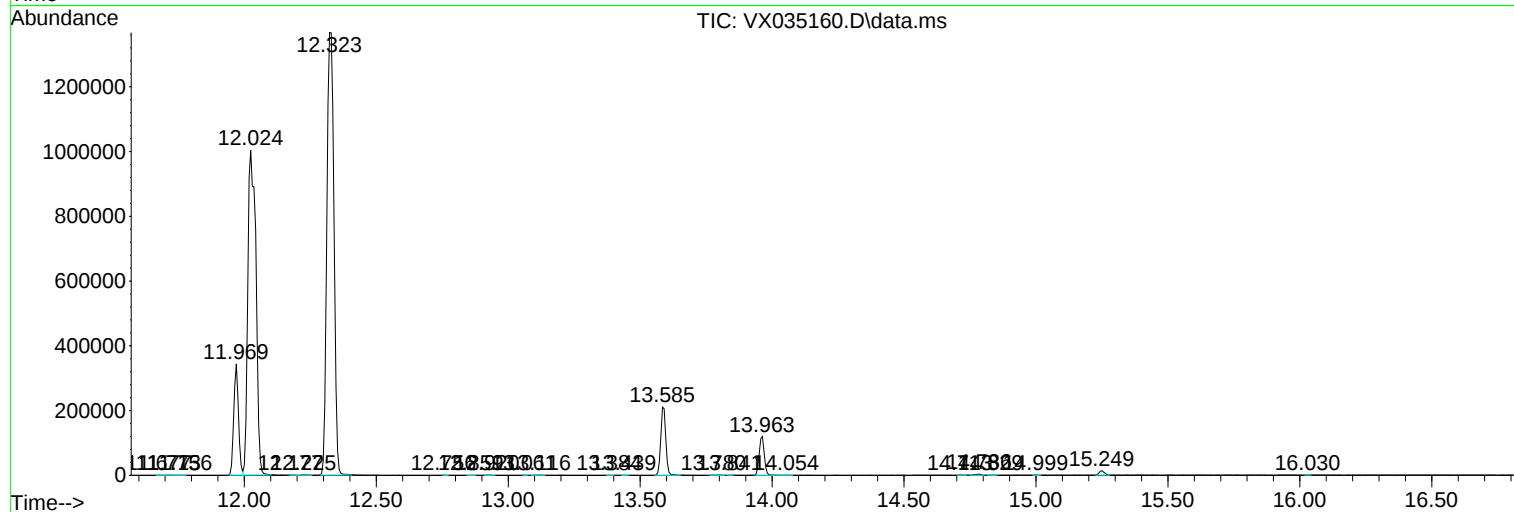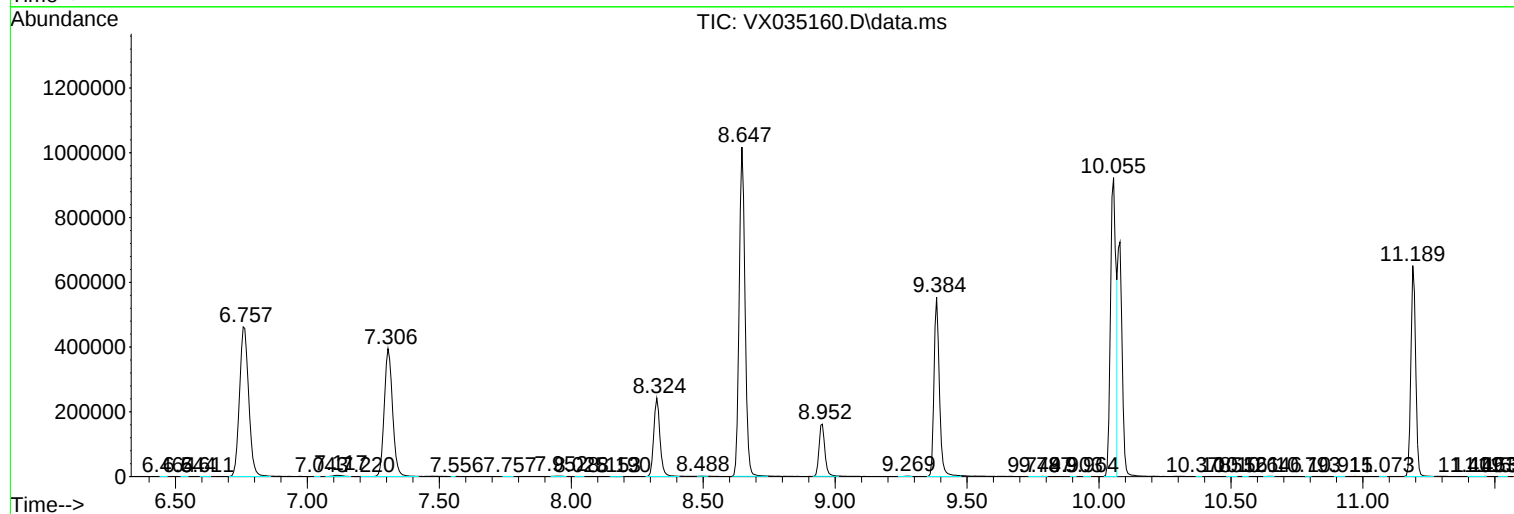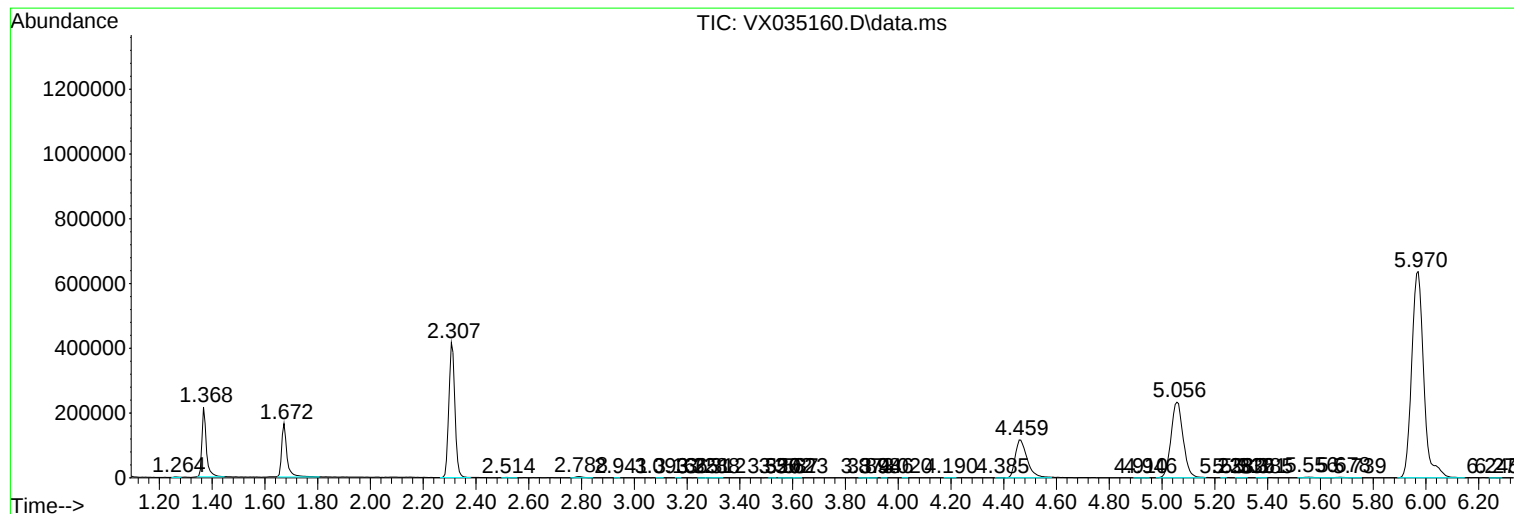

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035160.D
Acq On : 19 Apr 2023 11:38
Operator : JC/MD
Sample : 02397-07DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ML9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035160.D
Acq On : 19 Apr 2023 11:38
Operator : JC/MD
Sample : 02397-07DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ML9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------