

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035161.D
 Acq On : 19 Apr 2023 12:01
 Operator : JC/MD
 Sample : 02397-16DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035161.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	32	rBV3	2568	2946	0.08%	0.018%
2	1.368	42	46	56	rBV	237080	264340	7.47%	1.603%
3	1.672	91	96	109	rBV	180055	240627	6.80%	1.460%
4	2.306	194	200	211	rBV	450210	702550	19.84%	4.262%
5	2.508	232	233	236	rBV2	621	609	0.02%	0.004%
6	2.745	270	272	274	rBV2	216	209	0.01%	0.001%
7	2.788	274	279	283	rBV3	2066	3216	0.09%	0.020%
8	2.849	288	289	291	rBV	290	201	0.01%	0.001%
9	2.941	302	304	309	rVB3	336	578	0.02%	0.004%
10	3.008	313	315	318	rVB	238	205	0.01%	0.001%
11	3.160	336	340	341	rBV2	404	416	0.01%	0.003%
12	3.410	380	381	383	rBV	240	157	0.00%	0.001%
13	3.483	389	393	396	rBV2	240	360	0.01%	0.002%
14	3.544	400	403	404	rBV2	251	281	0.01%	0.002%
15	3.800	443	445	447	rVV2	248	222	0.01%	0.001%
16	3.837	449	451	453	rBV	163	143	0.00%	0.001%
17	3.946	468	469	471	rBV	293	263	0.01%	0.002%
18	3.971	471	473	476	rVV	378	448	0.01%	0.003%
19	4.014	478	480	481	rVV2	264	186	0.01%	0.001%
20	4.032	481	483	485	rVV	327	265	0.01%	0.002%
21	4.117	494	497	498	rBV2	244	214	0.01%	0.001%
22	4.148	501	502	504	rBV2	323	248	0.01%	0.002%
23	4.465	545	554	581	rBV	126534	396551	11.20%	2.405%
24	4.910	626	627	629	rBV	397	258	0.01%	0.002%
25	4.946	631	633	635	rBV3	213	168	0.00%	0.001%
26	5.056	639	651	672	rVV	264321	794389	22.44%	4.819%
27	5.367	700	702	704	rBV2	417	436	0.01%	0.003%
28	5.556	727	733	740	rBV5	2470	5220	0.15%	0.032%
29	5.684	753	754	759	rBV2	212	210	0.01%	0.001%
30	5.721	759	760	763	rVV2	213	195	0.01%	0.001%
31	5.970	788	801	820	rBV2	698655	2076708	58.65%	12.597%
32	6.355	861	864	865	rBV2	296	399	0.01%	0.002%
33	6.458	878	881	885	rBV2	328	541	0.02%	0.003%
34	6.525	890	892	893	rBV	219	156	0.00%	0.001%
35	6.605	903	905	907	rBV	231	184	0.01%	0.001%
36	6.647	910	912	914	rBV	198	186	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035161.D
 Acq On : 19 Apr 2023 12:01
 Operator : JC/MD
 Sample : 02397-16DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	6.696	918	920	921	rBV2	222	222	0.01%	0.001%
38	6.763	921	931	950	rBV	341355	820548	23.17%	4.977%
39	7.117	982	989	999	rVB5	4099	10325	0.29%	0.063%
40	7.208	1003	1004	1008	rBV4	374	376	0.01%	0.002%
41	7.306	1011	1020	1035	rBV	421276	937291	26.47%	5.686%
42	7.562	1060	1062	1064	rVB2	281	208	0.01%	0.001%
43	7.617	1069	1071	1073	rVV	257	267	0.01%	0.002%
44	7.665	1077	1079	1080	rBV	290	176	0.00%	0.001%
45	7.684	1080	1082	1083	rVB2	257	176	0.00%	0.001%
46	7.714	1086	1087	1092	rBV	223	286	0.01%	0.002%
47	7.751	1092	1093	1098	rVB	273	252	0.01%	0.002%
48	7.836	1104	1107	1109	rBV2	234	239	0.01%	0.001%
49	7.946	1121	1125	1128	rBV5	1486	2740	0.08%	0.017%
50	8.013	1135	1136	1138	rBV	316	184	0.01%	0.001%
51	8.037	1138	1140	1142	rVB	352	224	0.01%	0.001%
52	8.190	1163	1165	1168	rBV2	212	249	0.01%	0.002%
53	8.251	1171	1175	1180	rBV3	2143	3312	0.09%	0.020%
54	8.324	1181	1187	1200	rBV	261273	426983	12.06%	2.590%
55	8.647	1233	1240	1258	rBV	1084728	1702548	48.08%	10.328%
56	8.952	1284	1290	1304	rBV	177171	273112	7.71%	1.657%
57	9.122	1317	1318	1320	rBV2	432	378	0.01%	0.002%
58	9.214	1331	1333	1335	rBV2	407	311	0.01%	0.002%
59	9.238	1335	1337	1339	rBV2	258	181	0.01%	0.001%
60	9.281	1339	1344	1347	rVB5	1128	1602	0.05%	0.010%
61	9.311	1347	1349	1351	rBV2	266	294	0.01%	0.002%
62	9.384	1355	1361	1377	rBV	603799	856324	24.18%	5.194%
63	9.872	1438	1441	1442	rBV2	330	301	0.01%	0.002%
64	9.921	1447	1449	1452	rVB2	274	186	0.01%	0.001%
65	9.976	1456	1458	1459	rBV2	255	218	0.01%	0.001%
66	10.055	1465	1471	1473	rBV	690392	1000456	28.26%	6.069%
67	10.403	1526	1528	1530	rBV	298	157	0.00%	0.001%
68	10.433	1532	1533	1537	rVV2	329	258	0.01%	0.002%
69	10.500	1542	1544	1546	rBV	366	336	0.01%	0.002%
70	10.518	1546	1547	1549	rVV2	281	139	0.00%	0.001%
71	10.616	1560	1563	1564	rBV2	277	238	0.01%	0.001%
72	10.817	1593	1596	1598	rBV2	196	210	0.01%	0.001%
73	10.963	1619	1620	1622	rBV2	227	209	0.01%	0.001%
74	11.012	1626	1628	1631	rBV	315	322	0.01%	0.002%
75	11.067	1635	1637	1638	rBV	254	183	0.01%	0.001%
76	11.092	1639	1641	1642	rBV	286	144	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035161.D
 Acq On : 19 Apr 2023 12:01
 Operator : JC/MD
 Sample : 02397-16DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	11.189	1652	1657	1665	rBV	683999	882390	24.92%	5.353%
78	11.378	1686	1688	1689	rBV	329	284	0.01%	0.002%
79	11.652	1732	1733	1736	rBV2	325	275	0.01%	0.002%
80	11.713	1739	1743	1746	rVB4	702	977	0.03%	0.006%
81	11.823	1759	1761	1762	rBV2	212	167	0.00%	0.001%
82	11.890	1770	1772	1773	rBV2	241	183	0.01%	0.001%
83	11.969	1780	1785	1789	rBV	47532	60134	1.70%	0.365%
84	12.018	1789	1793	1807	rVB2	657422	1077910	30.44%	6.539%
85	12.329	1837	1844	1863	rBV2	2007736	3540784	100.00%	21.478%
86	12.927	1939	1942	1947	rVB4	1250	1767	0.05%	0.011%
87	13.048	1960	1962	1963	rBV2	273	221	0.01%	0.001%
88	13.116	1968	1973	1978	rBV4	779	1300	0.04%	0.008%
89	13.207	1984	1988	1990	rVB2	587	696	0.02%	0.004%
90	13.378	2014	2016	2017	rVB	290	162	0.00%	0.001%
91	13.585	2045	2050	2060	rBV	246249	317578	8.97%	1.926%
92	13.780	2079	2082	2089	rBV4	746	1249	0.04%	0.008%
93	13.963	2106	2112	2117	rBV	43295	55723	1.57%	0.338%
94	14.121	2137	2138	2141	rBV2	381	315	0.01%	0.002%
95	14.231	2154	2156	2159	rBV2	394	412	0.01%	0.002%
96	14.347	2173	2175	2176	rBV	359	173	0.00%	0.001%
97	14.591	2213	2215	2217	rBV2	464	578	0.02%	0.004%
98	14.786	2243	2247	2251	rVB3	1566	1996	0.06%	0.012%
99	15.255	2320	2324	2330	rVB5	2635	3295	0.09%	0.020%
100	16.572	2538	2540	2541	rBV	672	333	0.01%	0.002%




Sum of corrected areas: 16485352

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035161.D
Acq On : 19 Apr 2023 12:01
Operator : JC/MD
Sample : 02397-16DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

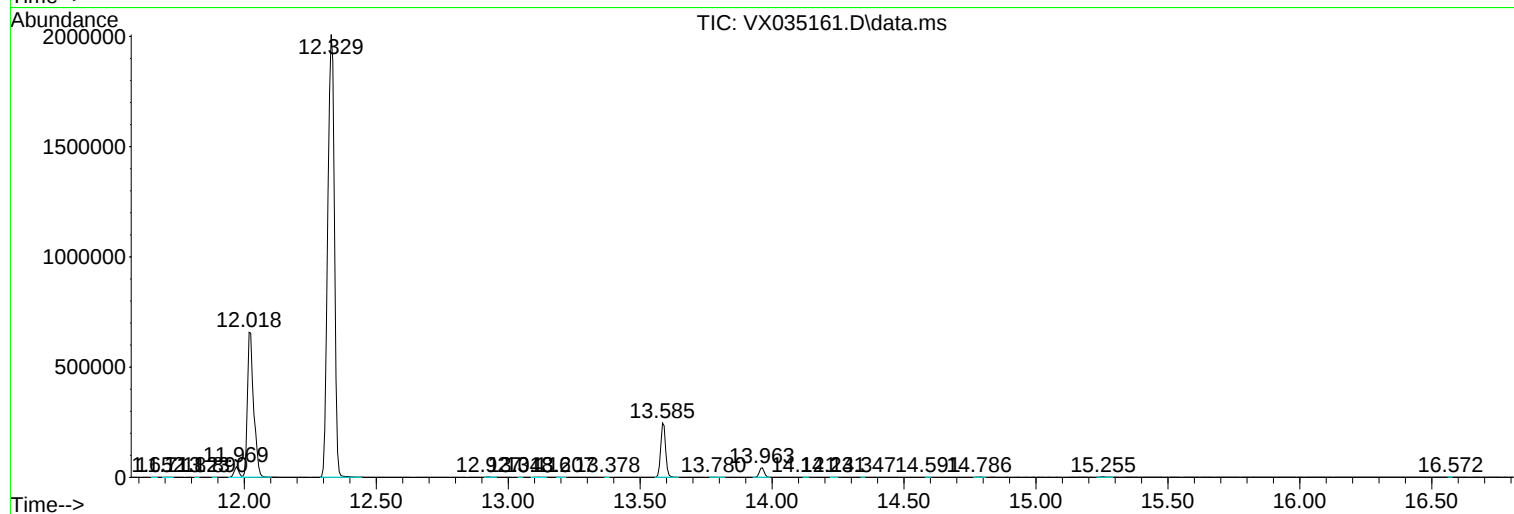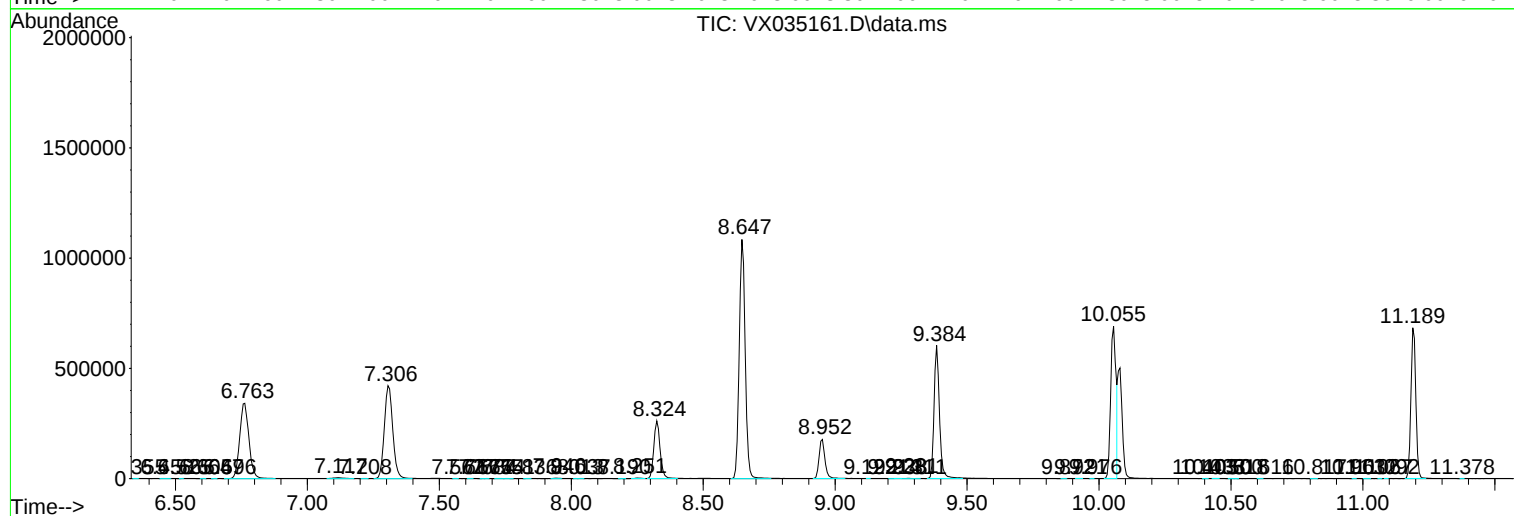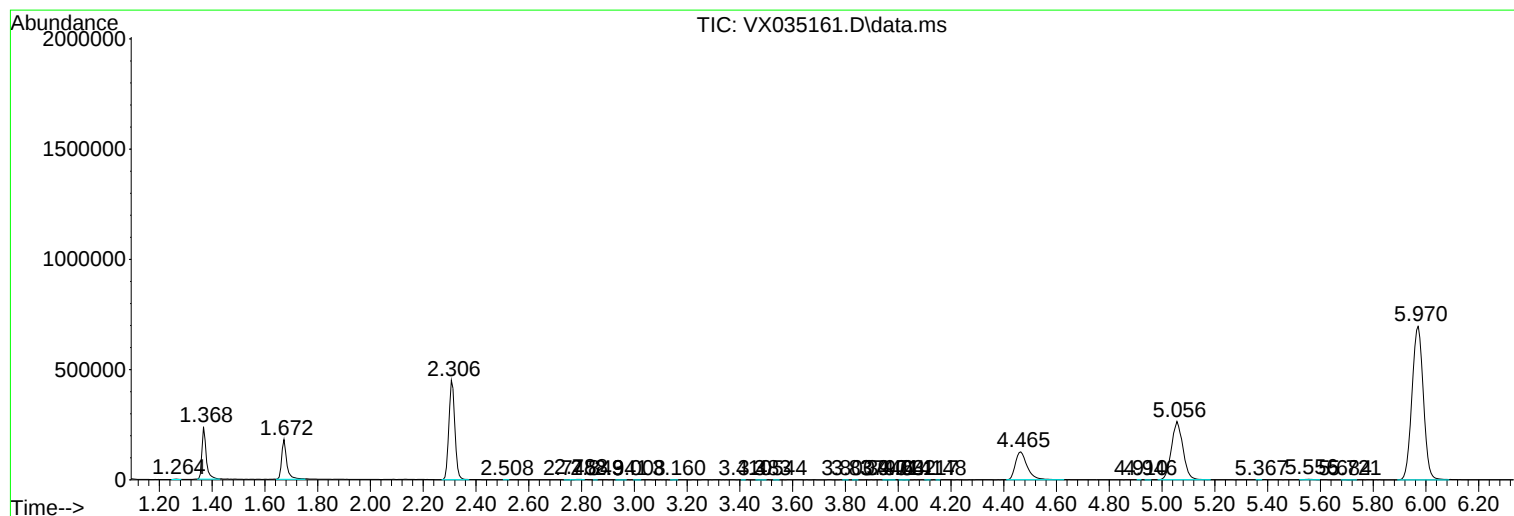

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035161.D
Acq On : 19 Apr 2023 12:01
Operator : JC/MD
Sample : 02397-16DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035161.D
Acq On : 19 Apr 2023 12:01
Operator : JC/MD
Sample : 02397-16DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------