

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035162.D
 Acq On : 19 Apr 2023 12:24
 Operator : JC/MD
 Sample : 02397-17DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035162.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	27	29	31	rBV3	2237	1840	0.05%	0.011%
2	1.368	42	46	58	rBV	211346	242566	6.90%	1.464%
3	1.672	91	96	108	rBV	168506	221847	6.31%	1.339%
4	2.306	194	200	211	rBV	405759	628384	17.89%	3.793%
5	2.520	230	235	237	rBV3	576	935	0.03%	0.006%
6	2.581	243	245	249	rBV	267	361	0.01%	0.002%
7	2.794	274	280	285	rBV	2713	5027	0.14%	0.030%
8	2.934	301	303	306	rVB2	459	475	0.01%	0.003%
9	2.965	306	308	312	rVV3	422	582	0.02%	0.004%
10	3.044	319	321	322	rVV	245	225	0.01%	0.001%
11	3.062	322	324	325	rVV	364	247	0.01%	0.001%
12	3.446	384	387	391	rBV2	314	432	0.01%	0.003%
13	3.568	405	407	409	rBV	177	217	0.01%	0.001%
14	3.800	443	445	446	rBV	290	215	0.01%	0.001%
15	3.983	472	475	476	rBV2	285	263	0.01%	0.002%
16	4.062	484	488	489	rBV2	260	222	0.01%	0.001%
17	4.245	517	518	521	rBV2	261	268	0.01%	0.002%
18	4.367	536	538	541	rBV3	270	233	0.01%	0.001%
19	4.465	545	554	580	rBV	109565	355615	10.12%	2.147%
20	4.897	623	625	627	rBV3	236	264	0.01%	0.002%
21	5.056	639	651	668	rBV	229296	710959	20.24%	4.292%
22	5.214	675	677	678	rBV	355	234	0.01%	0.001%
23	5.233	678	680	686	rVB4	837	1119	0.03%	0.007%
24	5.294	688	690	692	rBV	284	294	0.01%	0.002%
25	5.556	726	733	741	rBV3	1997	5051	0.14%	0.030%
26	5.696	753	756	757	rBV2	309	278	0.01%	0.002%
27	5.769	764	768	770	rBV2	157	215	0.01%	0.001%
28	5.842	777	780	781	rBV	339	269	0.01%	0.002%
29	5.970	788	801	821	rBV2	622383	1869086	53.20%	11.283%
30	6.263	846	849	852	rBV3	372	607	0.02%	0.004%
31	6.373	863	867	868	rBV3	212	248	0.01%	0.001%
32	6.440	877	878	880	rBV	338	210	0.01%	0.001%
33	6.757	921	930	954	rBV	477432	1161766	33.07%	7.013%
34	6.946	959	961	964	rBV3	227	269	0.01%	0.002%
35	7.013	970	972	973	rBV	643	302	0.01%	0.002%
36	7.123	982	990	995	rBV4	3299	7318	0.21%	0.044%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035162.D
 Acq On : 19 Apr 2023 12:24
 Operator : JC/MD
 Sample : 02397-17DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	7.305	1011	1020	1036	rBV	384188	842316	23.98%	5.085%
38	7.482	1045	1049	1053	rBV5	807	1521	0.04%	0.009%
39	7.647	1074	1076	1078	rBV	267	241	0.01%	0.001%
40	7.946	1120	1125	1126	rBV3	1287	1654	0.05%	0.010%
41	8.226	1168	1171	1174	rVB2	248	284	0.01%	0.002%
42	8.269	1174	1178	1180	rVB3	217	300	0.01%	0.002%
43	8.324	1181	1187	1201	rBV	229829	381732	10.87%	2.304%
44	8.647	1234	1240	1252	rBV	976961	1527388	43.47%	9.221%
45	8.952	1284	1290	1302	rBV	158695	241447	6.87%	1.458%
46	9.092	1311	1313	1316	rBV2	377	299	0.01%	0.002%
47	9.195	1329	1330	1335	rBV3	337	392	0.01%	0.002%
48	9.275	1339	1343	1348	rVB3	946	1595	0.05%	0.010%
49	9.317	1348	1350	1354	rBV2	326	537	0.02%	0.003%
50	9.384	1356	1361	1379	rBV	544464	766950	21.83%	4.630%
51	9.909	1444	1447	1452	rBV2	431	742	0.02%	0.004%
52	9.951	1452	1454	1457	rVB2	278	305	0.01%	0.002%
53	10.055	1465	1471	1473	rBV	971675	1377688	39.21%	8.317%
54	10.238	1498	1501	1503	rBV4	705	826	0.02%	0.005%
55	10.366	1518	1522	1523	rBV	326	412	0.01%	0.002%
56	10.384	1523	1525	1528	rVV2	266	381	0.01%	0.002%
57	10.494	1541	1543	1545	rVV	270	239	0.01%	0.001%
58	10.512	1545	1546	1548	rVV	296	279	0.01%	0.002%
59	10.549	1550	1552	1553	rVV	212	228	0.01%	0.001%
60	10.646	1563	1568	1570	rBV2	312	484	0.01%	0.003%
61	10.683	1570	1574	1577	rVB	238	341	0.01%	0.002%
62	11.030	1629	1631	1633	rVB	353	221	0.01%	0.001%
63	11.189	1652	1657	1672	rVV	616517	794215	22.61%	4.795%
64	11.451	1698	1700	1703	rVB	388	442	0.01%	0.003%
65	11.689	1737	1739	1741	rVV	318	264	0.01%	0.002%
66	11.713	1741	1743	1746	rVV	651	545	0.02%	0.003%
67	11.750	1747	1749	1754	rVB2	345	444	0.01%	0.003%
68	11.811	1757	1759	1762	rBV2	286	233	0.01%	0.001%
69	11.969	1780	1785	1789	rBV	46000	60136	1.71%	0.363%
70	12.024	1789	1794	1806	rVB2	941730	1423608	40.52%	8.594%
71	12.329	1837	1844	1860	rBV2	1989684	3513303	100.00%	21.209%
72	12.475	1864	1868	1871	rVV4	557	971	0.03%	0.006%
73	12.536	1874	1878	1879	rVB3	458	429	0.01%	0.003%
74	12.591	1884	1887	1888	rBV2	308	310	0.01%	0.002%
75	12.689	1901	1903	1904	rBV	267	210	0.01%	0.001%
76	12.750	1912	1913	1915	rBV2	305	250	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035162.D
 Acq On : 19 Apr 2023 12:24
 Operator : JC/MD
 Sample : 02397-17DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041823WMA.M
 Title : VOC Analysis

77	12.872	1929	1933	1935	rBV2	275	283	0.01%	0.002%
78	12.926	1939	1942	1946	rVB5	1587	2014	0.06%	0.012%
79	13.054	1959	1963	1964	rBV2	257	331	0.01%	0.002%
80	13.109	1970	1972	1977	rVV2	528	765	0.02%	0.005%
81	13.158	1978	1980	1983	rVB	345	252	0.01%	0.002%
82	13.195	1983	1986	1989	rBV3	666	731	0.02%	0.004%
83	13.390	2010	2018	2020	rVB2	341	711	0.02%	0.004%
84	13.475	2030	2032	2036	rVB2	353	406	0.01%	0.002%
85	13.585	2045	2050	2061	rBV	270363	333478	9.49%	2.013%
86	13.780	2079	2082	2085	rBV2	460	568	0.02%	0.003%
87	13.853	2092	2094	2097	rBV2	264	222	0.01%	0.001%
88	13.963	2107	2112	2119	rBV	40326	54480	1.55%	0.329%
89	14.304	2166	2168	2169	rVB	373	209	0.01%	0.001%
90	14.487	2196	2198	2200	rVB2	396	213	0.01%	0.001%
91	14.542	2206	2207	2210	rBV3	367	372	0.01%	0.002%
92	14.621	2218	2220	2223	rVV2	515	366	0.01%	0.002%
93	14.652	2223	2225	2228	rVB2	445	374	0.01%	0.002%
94	14.780	2244	2246	2250	rVB4	1663	2103	0.06%	0.013%
95	14.987	2277	2280	2282	rBV2	401	531	0.02%	0.003%
96	15.011	2282	2284	2285	rBV	511	327	0.01%	0.002%
97	15.109	2298	2300	2303	rBV2	641	668	0.02%	0.004%
98	15.255	2320	2324	2327	rBV4	1270	2102	0.06%	0.013%
99	15.371	2342	2343	2344	rBV	519	213	0.01%	0.001%
100	15.865	2422	2424	2426	rBV2	695	741	0.02%	0.004%




Sum of corrected areas: 16565065

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035162.D
Acq On : 19 Apr 2023 12:24
Operator : JC/MD
Sample : 02397-17DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

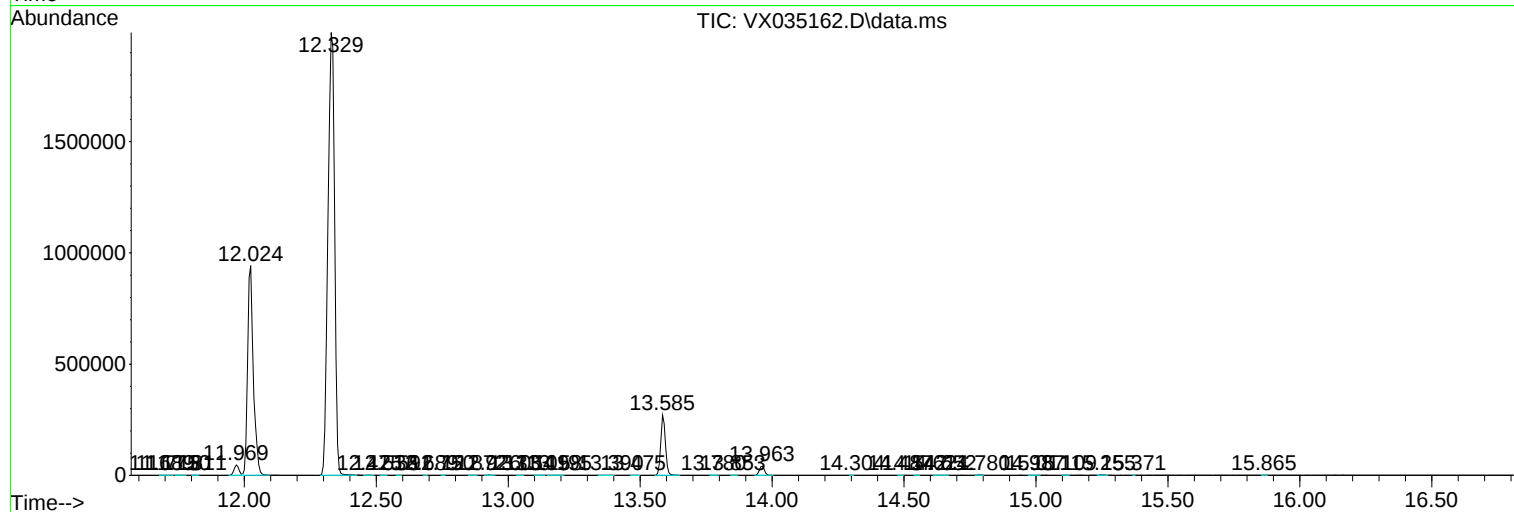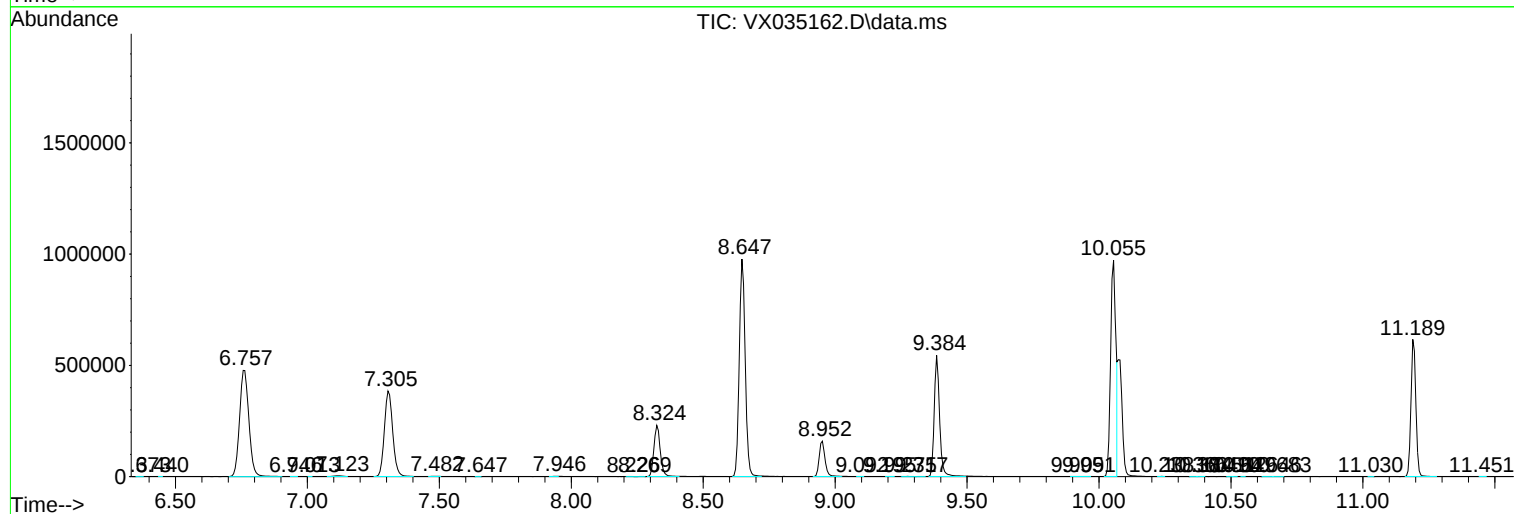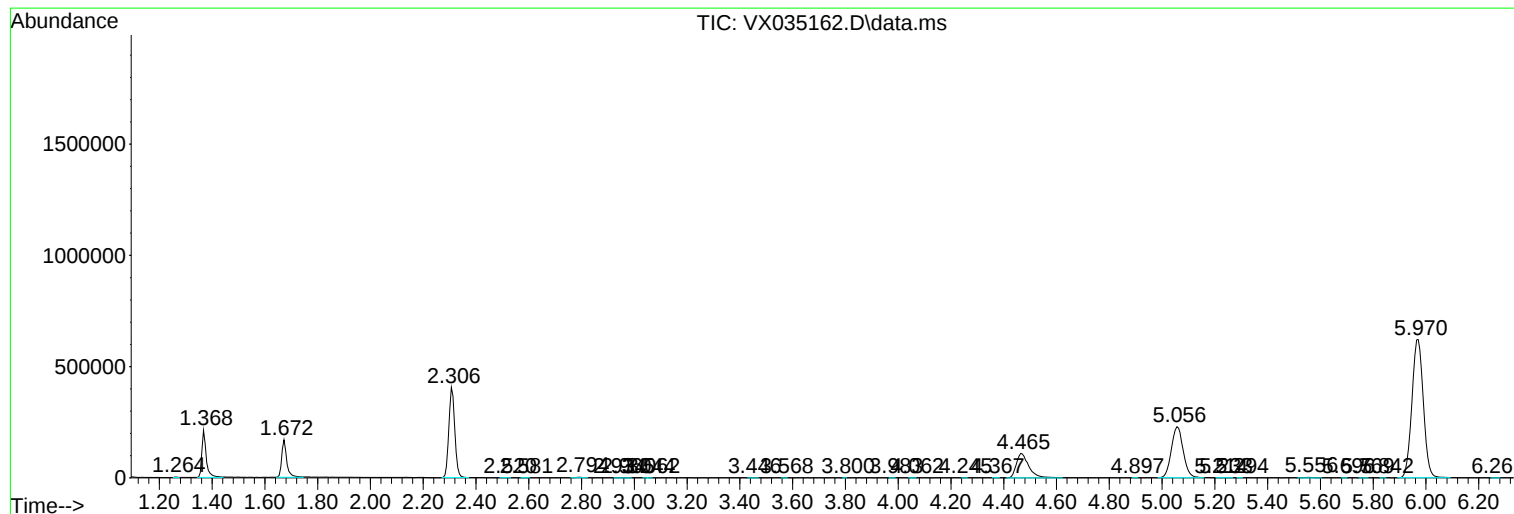

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035162.D
Acq On : 19 Apr 2023 12:24
Operator : JC/MD
Sample : 02397-17DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035162.D
Acq On : 19 Apr 2023 12:24
Operator : JC/MD
Sample : 02397-17DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc