

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035164.D
 Acq On : 19 Apr 2023 13:10
 Operator : JC/MD
 Sample : 02397-09DL 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M

Title : VOC Analysis

Signal : TIC: VX035164.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	33	rBV3	2221	2854	0.12%	0.019%
2	1.368	42	46	58	rVB	198018	223814	9.15%	1.478%
3	1.672	92	96	109	rBV	155777	205526	8.40%	1.357%
4	2.307	194	200	212	rBV	381259	598589	24.47%	3.952%
5	2.502	230	232	234	rBV2	433	391	0.02%	0.003%
6	2.794	275	280	287	rVB3	2748	4574	0.19%	0.030%
7	3.008	312	315	316	rBV2	269	249	0.01%	0.002%
8	3.081	325	327	329	rBV	268	253	0.01%	0.002%
9	3.099	329	330	332	rVV	447	274	0.01%	0.002%
10	3.130	332	335	338	rVV3	490	542	0.02%	0.004%
11	3.197	345	346	349	rBV2	327	321	0.01%	0.002%
12	3.227	349	351	354	rVV2	272	298	0.01%	0.002%
13	3.251	354	355	359	rVB2	316	294	0.01%	0.002%
14	3.337	367	369	370	rBV2	305	266	0.01%	0.002%
15	3.447	384	387	389	rVB3	335	348	0.01%	0.002%
16	3.477	389	392	393	rBV	299	263	0.01%	0.002%
17	3.501	393	396	398	rVV2	275	300	0.01%	0.002%
18	3.898	457	461	462	rBV2	228	262	0.01%	0.002%
19	3.934	465	467	468	rVB	379	256	0.01%	0.002%
20	3.959	468	471	472	rBV	344	221	0.01%	0.001%
21	3.971	472	473	476	rBV2	234	230	0.01%	0.002%
22	3.995	476	477	480	rBV2	308	273	0.01%	0.002%
23	4.129	495	499	502	rVB2	220	330	0.01%	0.002%
24	4.160	502	504	506	rBV2	305	352	0.01%	0.002%
25	4.465	544	554	579	rBV	106850	337291	13.79%	2.227%
26	4.946	630	633	634	rBV2	223	264	0.01%	0.002%
27	5.056	637	651	671	rBV	224744	680835	27.83%	4.495%
28	5.367	699	702	703	rBV2	467	496	0.02%	0.003%
29	5.385	703	705	707	rBV2	539	594	0.02%	0.004%
30	5.477	718	720	721	rBV	310	250	0.01%	0.002%
31	5.495	721	723	726	rVV2	435	500	0.02%	0.003%
32	5.562	729	734	741	rVB5	2141	5219	0.21%	0.034%
33	5.727	759	761	763	rBV3	270	300	0.01%	0.002%
34	5.830	774	778	779	rBV2	214	224	0.01%	0.001%
35	5.970	788	801	822	rBV2	594648	1792408	73.27%	11.835%
36	6.202	838	839	843	rVB2	391	317	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035164.D
 Acq On : 19 Apr 2023 13:10
 Operator : JC/MD
 Sample : 02397-09DL 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	6.239	843	845	847	rBV2	260	266	0.01%	0.002%
38	6.464	880	882	885	rVB	356	243	0.01%	0.002%
39	6.550	893	896	897	rVV2	387	407	0.02%	0.003%
40	6.763	919	931	951	rBV	461273	1119229	45.75%	7.390%
41	7.043	975	977	980	rBV2	278	331	0.01%	0.002%
42	7.117	982	989	996	rBV4	3266	8083	0.33%	0.053%
43	7.226	1004	1007	1010	rVB	420	509	0.02%	0.003%
44	7.306	1010	1020	1036	rBV	358666	804933	32.91%	5.315%
45	7.665	1077	1079	1083	rVB2	253	311	0.01%	0.002%
46	7.824	1103	1105	1109	rVB2	428	409	0.02%	0.003%
47	7.860	1109	1111	1114	rBV3	356	400	0.02%	0.003%
48	7.940	1121	1124	1128	rBV3	1011	1515	0.06%	0.010%
49	8.263	1174	1177	1181	rVB2	323	459	0.02%	0.003%
50	8.324	1181	1187	1205	rBV	216082	364939	14.92%	2.410%
51	8.452	1207	1208	1212	rBV3	444	446	0.02%	0.003%
52	8.488	1212	1214	1215	rBV2	578	536	0.02%	0.004%
53	8.647	1234	1240	1257	rBV	910875	1450759	59.31%	9.579%
54	8.909	1282	1283	1284	rBV	431	237	0.01%	0.002%
55	8.952	1284	1290	1307	rVV	148791	227948	9.32%	1.505%
56	9.153	1322	1323	1325	rBV2	296	258	0.01%	0.002%
57	9.275	1341	1343	1344	rBV	447	305	0.01%	0.002%
58	9.336	1351	1353	1356	rBV2	360	391	0.02%	0.003%
59	9.385	1356	1361	1380	rBV	511545	725903	29.67%	4.793%
60	10.055	1465	1471	1474	rBV	915829	1459887	59.68%	9.639%
61	10.360	1519	1521	1522	rBV2	297	235	0.01%	0.002%
62	10.372	1522	1523	1524	rVB	657	244	0.01%	0.002%
63	10.390	1524	1526	1530	rBV2	435	443	0.02%	0.003%
64	10.604	1558	1561	1564	rBV2	293	449	0.02%	0.003%
65	10.653	1566	1569	1572	rVB	381	389	0.02%	0.003%
66	10.689	1572	1575	1576	rBV	250	268	0.01%	0.002%
67	10.707	1576	1578	1581	rVB2	281	252	0.01%	0.002%
68	10.750	1581	1585	1587	rBV2	339	397	0.02%	0.003%
69	10.970	1618	1621	1623	rBV2	260	288	0.01%	0.002%
70	11.049	1631	1634	1636	rVB3	236	277	0.01%	0.002%
71	11.189	1652	1657	1670	rBV	594460	756835	30.94%	4.997%
72	11.433	1694	1697	1698	rBV2	203	223	0.01%	0.001%
73	11.567	1717	1719	1720	rBV	351	344	0.01%	0.002%
74	11.762	1748	1751	1753	rVB	344	312	0.01%	0.002%
75	11.829	1760	1762	1765	rVB2	339	254	0.01%	0.002%
76	11.969	1780	1785	1789	rBV	41847	52938	2.16%	0.350%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035164.D
 Acq On : 19 Apr 2023 13:10
 Operator : JC/MD
 Sample : 02397-09DL 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	12.024	1789	1794	1809	rVB2	918069	1395926	57.07%	9.217%
78	12.213	1823	1825	1827	rBV	331	337	0.01%	0.002%
79	12.268	1832	1834	1837	rBV2	347	356	0.01%	0.002%
80	12.329	1837	1844	1860	rBV2	1296083	2446199	100.00%	16.152%
81	12.658	1895	1898	1900	rBV2	539	557	0.02%	0.004%
82	12.927	1937	1942	1949	rVB3	2310	3340	0.14%	0.022%
83	12.988	1949	1952	1954	rBV2	380	357	0.01%	0.002%
84	13.055	1961	1963	1968	rBV2	551	662	0.03%	0.004%
85	13.201	1983	1987	1991	rVB4	1141	1765	0.07%	0.012%
86	13.244	1991	1994	1996	rBV2	279	356	0.01%	0.002%
87	13.439	2023	2026	2027	rBV2	327	353	0.01%	0.002%
88	13.524	2036	2040	2042	rBV2	373	533	0.02%	0.004%
89	13.585	2045	2050	2062	rVV	290063	354042	14.47%	2.338%
90	13.872	2095	2097	2098	rBV	335	309	0.01%	0.002%
91	13.890	2098	2100	2101	rVB	374	233	0.01%	0.002%
92	13.963	2107	2112	2118	rBV	58911	75999	3.11%	0.502%
93	14.128	2137	2139	2142	rBV3	389	387	0.02%	0.003%
94	14.207	2150	2152	2155	rBV	308	379	0.02%	0.003%
95	14.603	2216	2217	2219	rBV2	374	251	0.01%	0.002%
96	14.786	2243	2247	2251	rVB	3095	3625	0.15%	0.024%
97	15.249	2319	2323	2329	rBV2	10221	14516	0.59%	0.096%
98	15.670	2389	2392	2394	rVB2	603	520	0.02%	0.003%
99	16.316	2496	2498	2502	rBV3	854	1015	0.04%	0.007%
100	16.377	2506	2508	2510	rVV2	584	331	0.01%	0.002%




Sum of corrected areas: 15144978

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035164.D
Acq On : 19 Apr 2023 13:10
Operator : JC/MD
Sample : 02397-09DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

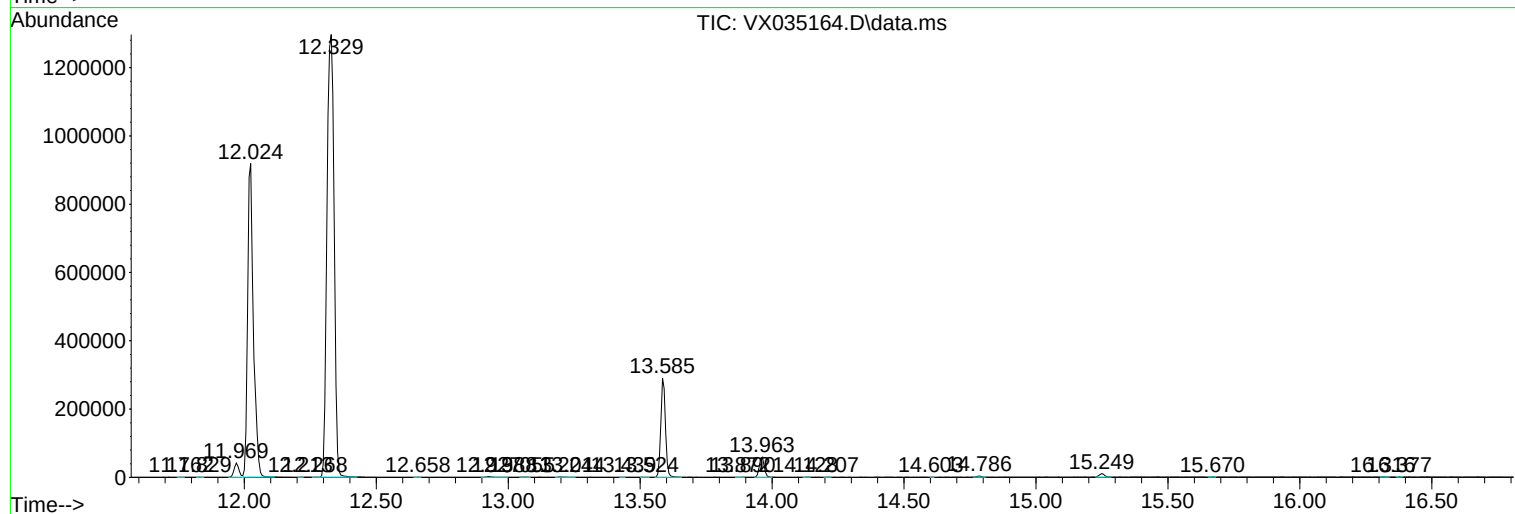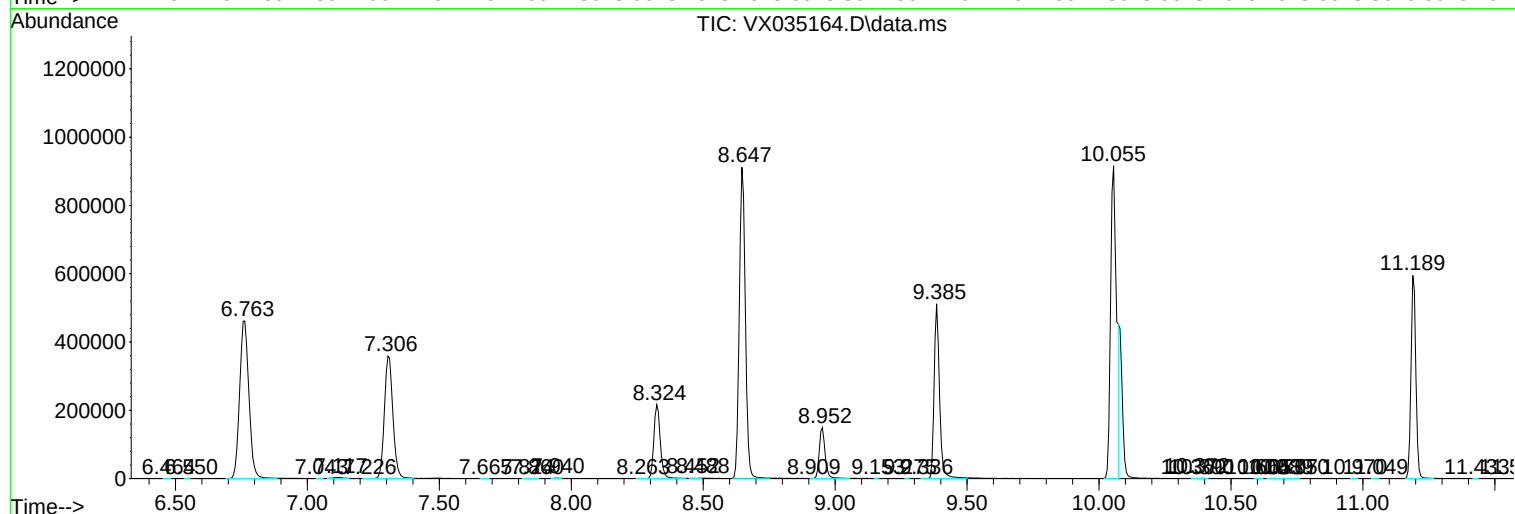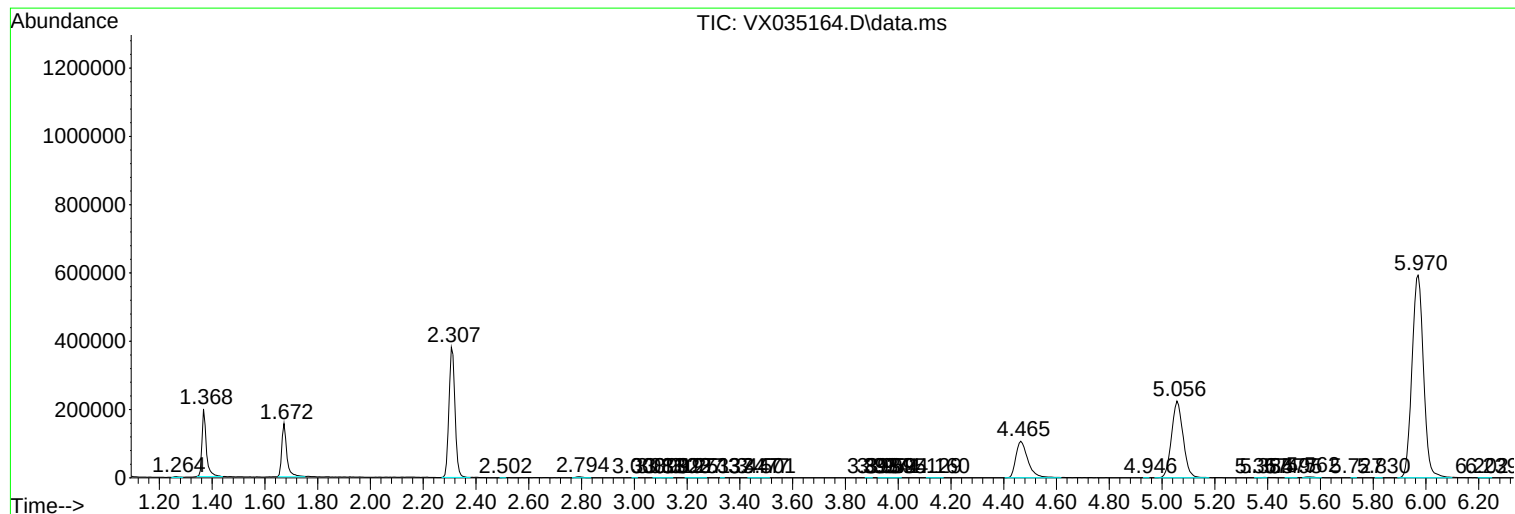

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035164.D
Acq On : 19 Apr 2023 13:10
Operator : JC/MD
Sample : 02397-09DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035164.D
Acq On : 19 Apr 2023 13:10
Operator : JC/MD
Sample : 02397-09DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------