

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035165.D
 Acq On : 19 Apr 2023 13:33
 Operator : JC/MD
 Sample : 02397-14DL 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035165.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	31	rBV2	2527	2525	0.09%	0.013%
2	1.368	42	46	62	rBV	201233	231721	8.08%	1.168%
3	1.673	91	96	111	rBV	159898	213331	7.44%	1.076%
4	2.307	194	200	213	rBV	396404	607534	21.19%	3.063%
5	2.788	275	279	285	rVB4	1527	3191	0.11%	0.016%
6	2.849	287	289	294	rVB2	487	489	0.02%	0.002%
7	2.904	296	298	299	rBV2	409	184	0.01%	0.001%
8	2.941	302	304	306	rBV2	212	177	0.01%	0.001%
9	3.111	331	332	335	rVV3	252	241	0.01%	0.001%
10	3.398	375	379	380	rVB2	247	274	0.01%	0.001%
11	3.483	390	393	394	rVV	458	315	0.01%	0.002%
12	3.611	411	414	415	rBV2	221	241	0.01%	0.001%
13	3.648	419	420	422	rBV	213	188	0.01%	0.001%
14	3.709	427	430	431	rVB3	270	196	0.01%	0.001%
15	3.739	431	435	436	rBV	183	181	0.01%	0.001%
16	3.819	446	448	451	rVB	257	212	0.01%	0.001%
17	3.855	451	454	459	rBV2	398	530	0.02%	0.003%
18	3.922	463	465	467	rVB	253	176	0.01%	0.001%
19	4.001	476	478	480	rVB2	303	227	0.01%	0.001%
20	4.117	493	497	498	rBV2	203	230	0.01%	0.001%
21	4.154	501	503	507	rBV	187	206	0.01%	0.001%
22	4.300	524	527	528	rBV2	662	842	0.03%	0.004%
23	4.355	534	536	538	rVB	301	236	0.01%	0.001%
24	4.385	540	541	544	rVB2	221	176	0.01%	0.001%
25	4.465	546	554	576	rBV	105550	345770	12.06%	1.743%
26	4.910	625	627	628	rVB2	336	210	0.01%	0.001%
27	4.928	628	630	633	rVB2	546	537	0.02%	0.003%
28	4.971	633	637	638	rBV2	338	416	0.01%	0.002%
29	5.056	638	651	668	rBV	221788	689595	24.05%	3.477%
30	5.391	700	706	708	rBV4	858	1900	0.07%	0.010%
31	5.556	726	733	741	rVB4	2502	6548	0.23%	0.033%
32	5.611	741	742	746	rVB2	276	247	0.01%	0.001%
33	5.678	746	753	761	rBV3	906	2080	0.07%	0.010%
34	5.830	775	778	779	rVB2	306	278	0.01%	0.001%
35	5.971	788	801	807	rBV2	609626	1818319	63.42%	9.169%
36	6.367	863	866	868	rVB	391	326	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035165.D
 Acq On : 19 Apr 2023 13:33
 Operator : JC/MD
 Sample : 02397-14DL 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	6.391	868	870	873	rVB	208	172	0.01%	0.001%
38	6.452	878	880	882	rBV	334	308	0.01%	0.002%
39	6.477	882	884	886	rBV3	211	180	0.01%	0.001%
40	6.653	909	913	914	rBV2	256	267	0.01%	0.001%
41	6.757	921	930	947	rBV	458619	1112048	38.79%	5.607%
42	7.117	983	989	995	rBV4	3494	7756	0.27%	0.039%
43	7.245	1007	1010	1011	rVV3	292	282	0.01%	0.001%
44	7.306	1011	1020	1042	rVV	367269	811464	28.30%	4.092%
45	7.482	1045	1049	1053	rBV4	1099	1793	0.06%	0.009%
46	7.568	1060	1063	1065	rVB2	313	345	0.01%	0.002%
47	7.604	1068	1069	1072	rBV2	214	241	0.01%	0.001%
48	7.940	1121	1124	1135	rBV3	858	2392	0.08%	0.012%
49	8.184	1162	1164	1167	rVB2	201	171	0.01%	0.001%
50	8.324	1180	1187	1201	rBV	226250	370150	12.91%	1.866%
51	8.482	1211	1213	1215	rBV2	627	644	0.02%	0.003%
52	8.525	1218	1220	1223	rVB3	644	453	0.02%	0.002%
53	8.647	1234	1240	1257	rBV	951406	1475304	51.46%	7.439%
54	8.952	1284	1290	1299	rBV	151846	230669	8.05%	1.163%
55	9.147	1320	1322	1325	rVB	427	324	0.01%	0.002%
56	9.275	1340	1343	1347	rBV	756	899	0.03%	0.005%
57	9.336	1352	1353	1355	rBV	233	193	0.01%	0.001%
58	9.385	1356	1361	1372	rBV	527106	738402	25.76%	3.723%
59	9.586	1392	1394	1395	rBV2	529	403	0.01%	0.002%
60	9.622	1399	1400	1402	rBV	476	303	0.01%	0.002%
61	9.647	1402	1404	1406	rVB2	313	218	0.01%	0.001%
62	9.750	1420	1421	1424	rBV	336	253	0.01%	0.001%
63	9.897	1444	1445	1448	rVB2	203	168	0.01%	0.001%
64	10.006	1461	1463	1465	rVB	292	232	0.01%	0.001%
65	10.055	1465	1471	1472	rBV	980278	1281617	44.70%	6.462%
66	10.080	1472	1475	1492	rVB	2065041	2760354	96.28%	13.919%
67	10.458	1535	1537	1539	rBV2	249	229	0.01%	0.001%
68	10.604	1559	1561	1564	rVB3	312	334	0.01%	0.002%
69	10.659	1567	1570	1572	rBV	160	183	0.01%	0.001%
70	10.884	1605	1607	1609	rBV	352	255	0.01%	0.001%
71	10.915	1609	1612	1614	rVV2	239	333	0.01%	0.002%
72	11.006	1625	1627	1629	rBV	296	251	0.01%	0.001%
73	11.098	1641	1642	1645	rBV	223	181	0.01%	0.001%
74	11.189	1652	1657	1666	rBV	594280	769218	26.83%	3.879%
75	11.427	1693	1696	1697	rBV2	231	219	0.01%	0.001%
76	11.561	1717	1718	1721	rVB2	325	279	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035165.D
 Acq On : 19 Apr 2023 13:33
 Operator : JC/MD
 Sample : 02397-14DL 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041823WMA.M
 Title : VOC Analysis

77	11.591	1721	1723	1727	rBV2	224	199	0.01%	0.001%
78	11.652	1730	1733	1734	rBV2	188	196	0.01%	0.001%
79	11.665	1734	1735	1738	rBV2	277	313	0.01%	0.002%
80	11.713	1740	1743	1746	rVB	862	859	0.03%	0.004%
81	11.811	1757	1759	1760	rBV2	217	181	0.01%	0.001%
82	11.915	1774	1776	1779	rVB2	243	239	0.01%	0.001%
83	11.969	1779	1785	1789	rBV	86939	108830	3.80%	0.549%
84	12.037	1789	1796	1811	rVB2	1437595	2866920	100.00%	14.456%
85	12.329	1837	1844	1865	rVB2	1329728	2464982	85.98%	12.429%
86	12.616	1890	1891	1894	rBV	272	242	0.01%	0.001%
87	12.927	1938	1942	1950	rVB3	6401	8373	0.29%	0.042%
88	13.055	1960	1963	1970	rVB3	1776	3301	0.12%	0.017%
89	13.110	1970	1972	1977	rBV2	1486	1621	0.06%	0.008%
90	13.195	1982	1986	1991	rBV5	3740	5113	0.18%	0.026%
91	13.347	2009	2011	2013	rVB2	311	229	0.01%	0.001%
92	13.366	2013	2014	2016	rBV2	262	221	0.01%	0.001%
93	13.384	2016	2017	2019	rVB	397	188	0.01%	0.001%
94	13.585	2045	2050	2062	rBV	531859	667143	23.27%	3.364%
95	13.920	2103	2105	2106	rBV	507	364	0.01%	0.002%
96	13.957	2106	2111	2124	rVV	128536	171637	5.99%	0.865%
97	14.432	2188	2189	2191	rVB	521	264	0.01%	0.001%
98	14.780	2241	2246	2251	rBV3	5671	7996	0.28%	0.040%
99	15.103	2297	2299	2300	rBV2	529	400	0.01%	0.002%
100	15.249	2318	2323	2330	rVB2	15820	22868	0.80%	0.115%


Sum of corrected areas: 19832015

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035165.D
Acq On : 19 Apr 2023 13:33
Operator : JC/MD
Sample : 02397-14DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

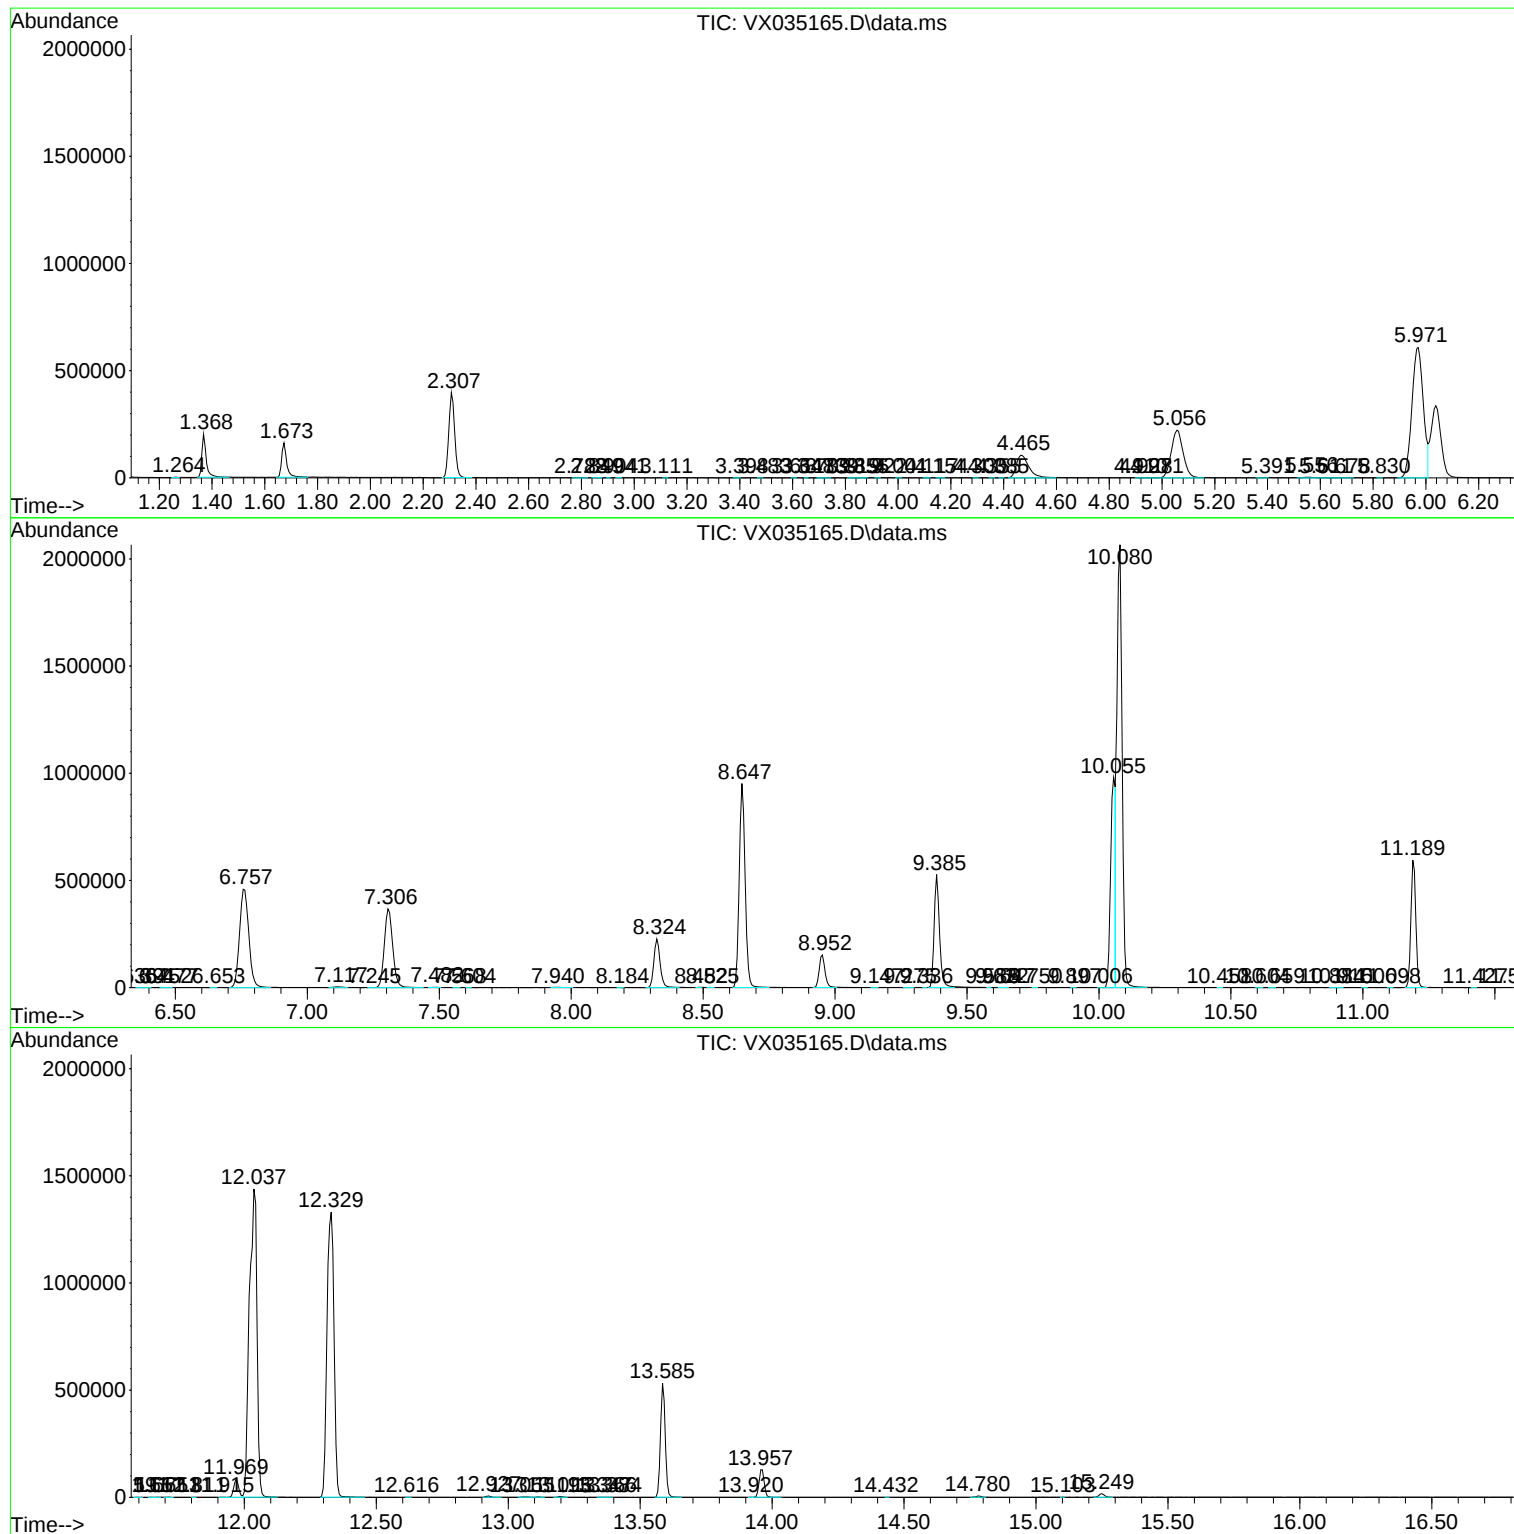

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035165.D
Acq On : 19 Apr 2023 13:33
Operator : JC/MD
Sample : 02397-14DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035165.D
Acq On : 19 Apr 2023 13:33
Operator : JC/MD
Sample : 02397-14DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------