

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035167.D
 Acq On : 19 Apr 2023 14:19
 Operator : JC/MD
 Sample : 02397-06DL 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035167.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	32	rBV2	2326	2383	0.06%	0.013%
2	1.368	42	46	62	rBV	202326	231118	5.65%	1.281%
3	1.672	91	96	110	rBV	154428	206762	5.06%	1.146%
4	2.307	194	200	213	rVB	392762	608632	14.88%	3.374%
5	2.550	239	240	243	rBV	264	277	0.01%	0.002%
6	2.788	274	279	286	rBV3	3091	5768	0.14%	0.032%
7	2.947	302	305	308	rBV2	333	530	0.01%	0.003%
8	2.995	311	313	314	rBV2	224	170	0.00%	0.001%
9	3.154	337	339	341	rVB	275	204	0.00%	0.001%
10	3.191	341	345	350	rBV3	351	668	0.02%	0.004%
11	3.282	357	360	361	rBV	312	232	0.01%	0.001%
12	3.373	373	375	377	rVB	239	210	0.01%	0.001%
13	3.398	377	379	382	rBV2	187	237	0.01%	0.001%
14	3.477	391	392	394	rBV	240	229	0.01%	0.001%
15	3.514	396	398	402	rVB2	317	347	0.01%	0.002%
16	3.556	402	405	406	rBV	442	270	0.01%	0.001%
17	3.617	411	415	416	rVV	456	358	0.01%	0.002%
18	3.636	416	418	422	rVV2	193	249	0.01%	0.001%
19	3.703	427	429	433	rVB2	247	211	0.01%	0.001%
20	3.861	453	455	458	rVB3	222	243	0.01%	0.001%
21	3.916	460	464	466	rBV2	262	362	0.01%	0.002%
22	4.032	481	483	485	rBV3	249	173	0.00%	0.001%
23	4.300	524	527	530	rBV3	368	406	0.01%	0.002%
24	4.324	530	531	535	rVB3	416	448	0.01%	0.002%
25	4.367	535	538	539	rBV2	153	175	0.00%	0.001%
26	4.465	545	554	584	rBV	107315	347027	8.49%	1.924%
27	4.690	589	591	594	rBV3	313	391	0.01%	0.002%
28	4.818	608	612	615	rVB2	341	464	0.01%	0.003%
29	5.056	639	651	668	rBV2	221887	694184	16.98%	3.848%
30	5.294	689	690	693	rBV3	286	317	0.01%	0.002%
31	5.397	699	707	714	rBV5	1378	4283	0.10%	0.024%
32	5.446	714	715	717	rBV	226	188	0.00%	0.001%
33	5.562	725	734	740	rBV5	3370	9608	0.23%	0.053%
34	5.678	746	753	759	rBV4	806	1936	0.05%	0.011%
35	5.751	761	765	767	rBV3	285	350	0.01%	0.002%
36	5.794	770	772	775	rBV2	185	219	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035167.D
 Acq On : 19 Apr 2023 14:19
 Operator : JC/MD
 Sample : 02397-06DL 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	5.971	788	801	806	rBV2	620625	1817631	44.45%	10.075%
38	6.452	878	880	881	rBV	276	223	0.01%	0.001%
39	6.763	921	931	950	rVV	478653	1147039	28.05%	6.358%
40	7.111	983	988	996	rVB3	3499	7532	0.18%	0.042%
41	7.220	1003	1006	1009	rBV	341	543	0.01%	0.003%
42	7.306	1011	1020	1033	rBV	377362	818377	20.01%	4.536%
43	7.696	1083	1084	1086	rBV	206	188	0.00%	0.001%
44	7.720	1086	1088	1092	rVB2	303	313	0.01%	0.002%
45	7.848	1108	1109	1112	rVB2	260	192	0.00%	0.001%
46	7.946	1121	1125	1129	rBV4	1249	2425	0.06%	0.013%
47	8.098	1147	1150	1151	rBV2	327	300	0.01%	0.002%
48	8.184	1162	1164	1167	rBV	248	285	0.01%	0.002%
49	8.226	1170	1171	1173	rBV	275	205	0.01%	0.001%
50	8.324	1181	1187	1199	rBV	223606	365545	8.94%	2.026%
51	8.647	1233	1240	1259	rVV	943255	1487521	36.37%	8.245%
52	8.909	1281	1283	1284	rVB2	415	222	0.01%	0.001%
53	8.952	1284	1290	1302	rBV	153682	233383	5.71%	1.294%
54	9.061	1306	1308	1313	rVB2	599	716	0.02%	0.004%
55	9.244	1335	1338	1340	rBV2	215	217	0.01%	0.001%
56	9.330	1350	1352	1353	rBV	371	224	0.01%	0.001%
57	9.385	1356	1361	1382	rVV	529701	752344	18.40%	4.170%
58	9.744	1419	1420	1422	rBV2	300	180	0.00%	0.001%
59	9.805	1428	1430	1432	rBV2	226	177	0.00%	0.001%
60	9.909	1445	1447	1449	rBV	217	218	0.01%	0.001%
61	10.080	1465	1475	1491	rBV2	2098550	4089436	100.00%	22.667%
62	10.427	1530	1532	1533	rVB	489	274	0.01%	0.002%
63	10.458	1533	1537	1539	rBV2	396	491	0.01%	0.003%
64	10.567	1553	1555	1557	rVB	299	242	0.01%	0.001%
65	10.592	1557	1559	1561	rVB2	234	218	0.01%	0.001%
66	10.738	1581	1583	1584	rVB	416	246	0.01%	0.001%
67	11.049	1632	1634	1637	rVB3	231	200	0.00%	0.001%
68	11.189	1652	1657	1670	rBV	579281	776972	19.00%	4.307%
69	11.634	1726	1730	1732	rVB	192	252	0.01%	0.001%
70	11.707	1739	1742	1745	rVB2	600	623	0.02%	0.003%
71	11.787	1753	1755	1757	rBV2	201	173	0.00%	0.001%
72	11.969	1780	1785	1789	rBV	47926	61023	1.49%	0.338%
73	12.024	1789	1794	1811	rVB2	1043695	2198018	53.75%	12.183%
74	12.256	1831	1832	1837	rBV2	418	395	0.01%	0.002%
75	12.323	1837	1843	1861	rBV2	1096858	1979354	48.40%	10.971%
76	12.567	1881	1883	1886	rBV2	255	227	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035167.D
 Acq On : 19 Apr 2023 14:19
 Operator : JC/MD
 Sample : 02397-06DL 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041823WMA.M
 Title : VOC Analysis

77	12.640	1893	1895	1896	rVB	349	227	0.01%	0.001%
78	12.664	1896	1899	1900	rBV	174	208	0.01%	0.001%
79	12.756	1912	1914	1917	rVB	504	406	0.01%	0.002%
80	12.792	1917	1920	1922	rBV2	246	256	0.01%	0.001%
81	12.939	1941	1944	1949	rBV2	261	404	0.01%	0.002%
82	12.975	1949	1950	1952	rVB2	406	216	0.01%	0.001%
83	13.006	1952	1955	1956	rBV2	232	263	0.01%	0.001%
84	13.109	1968	1972	1975	rBV2	1309	1542	0.04%	0.009%
85	13.195	1983	1986	1987	rBV2	259	215	0.01%	0.001%
86	13.268	1996	1998	1999	rBV2	306	201	0.00%	0.001%
87	13.359	2010	2013	2015	rBV	249	345	0.01%	0.002%
88	13.487	2033	2034	2036	rVB	388	172	0.00%	0.001%
89	13.518	2036	2039	2041	rBV	365	282	0.01%	0.002%
90	13.585	2045	2050	2062	rVV2	95734	129432	3.17%	0.717%
91	13.683	2065	2066	2067	rVV	583	258	0.01%	0.001%
92	13.701	2067	2069	2072	rVB2	336	301	0.01%	0.002%
93	13.780	2077	2082	2084	rBV3	308	654	0.02%	0.004%
94	13.841	2091	2092	2095	rBV2	291	268	0.01%	0.001%
95	13.963	2107	2112	2118	rVB2	14841	19718	0.48%	0.109%
96	14.134	2134	2140	2143	rBV3	595	1011	0.02%	0.006%
97	14.250	2157	2159	2164	rVB2	294	320	0.01%	0.002%
98	14.554	2207	2209	2212	rBV2	416	490	0.01%	0.003%
99	14.847	2256	2257	2260	rVB2	577	284	0.01%	0.002%
100	15.249	2318	2323	2328	rVB2	14838	20083	0.49%	0.111%




Sum of corrected areas: 18041329

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035167.D
Acq On : 19 Apr 2023 14:19
Operator : JC/MD
Sample : 02397-06DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COML8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

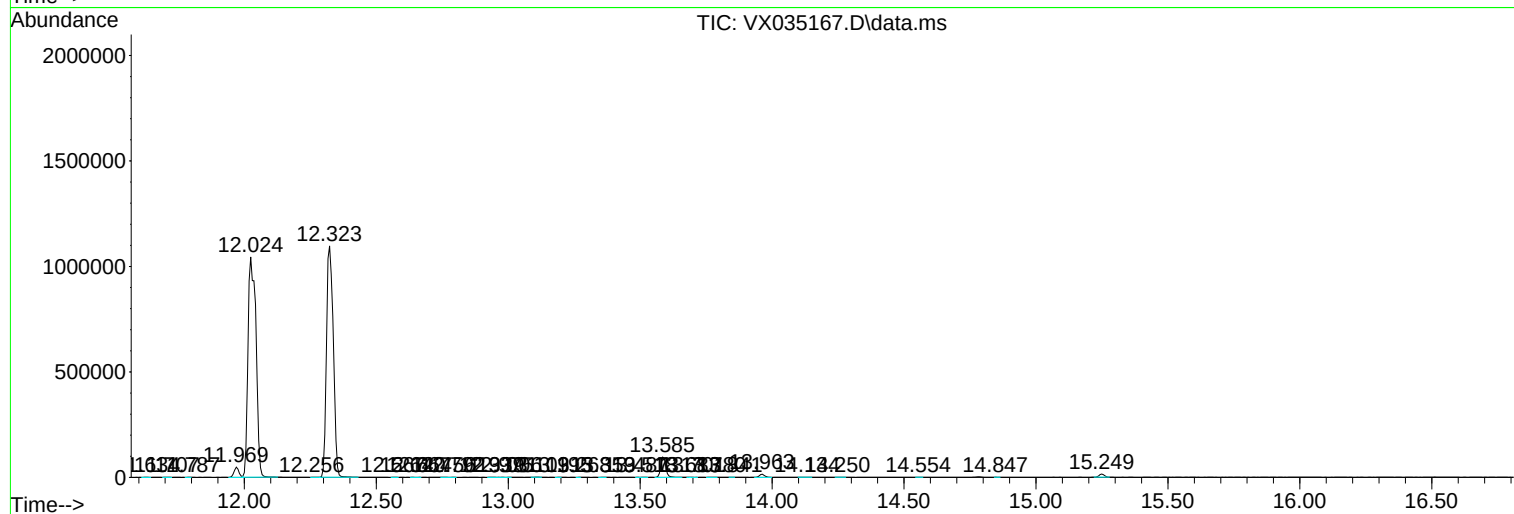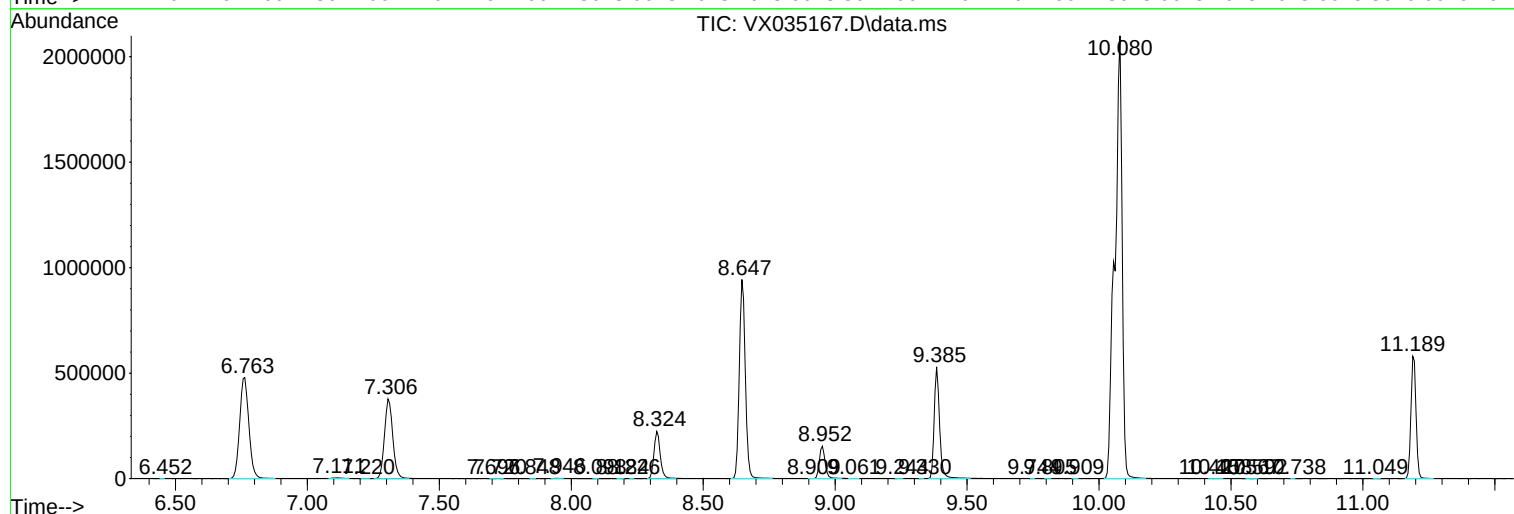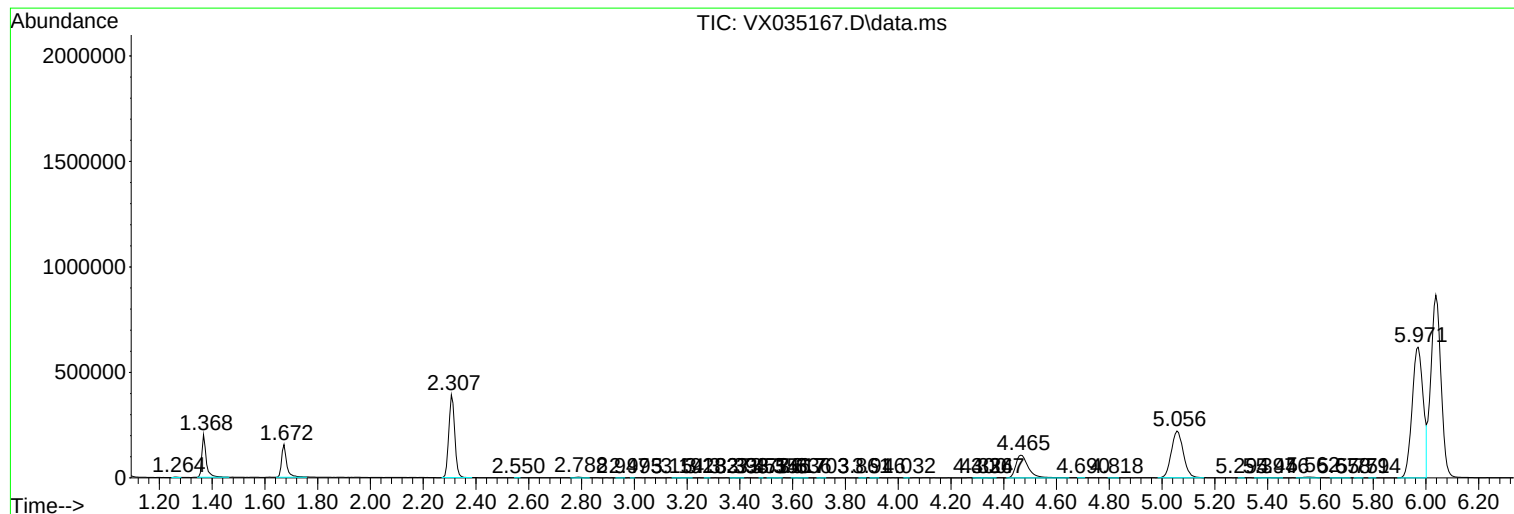

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035167.D
Acq On : 19 Apr 2023 14:19
Operator : JC/MD
Sample : 02397-06DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ML8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035167.D
Acq On : 19 Apr 2023 14:19
Operator : JC/MD
Sample : 02397-06DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ML8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------