

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035168.D
 Acq On : 19 Apr 2023 14:43
 Operator : JC/MD
 Sample : 02397-10DL 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035168.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	32	rBV2	2338	2445	0.05%	0.012%
2	1.368	42	46	60	rBV	203711	229455	4.94%	1.159%
3	1.673	91	96	108	rBV	154941	207783	4.47%	1.050%
4	2.307	194	200	210	rBV	393879	606403	13.06%	3.064%
5	2.453	222	224	226	rBV2	389	236	0.01%	0.001%
6	2.715	265	267	270	rVB3	601	615	0.01%	0.003%
7	2.758	270	274	275	rBV3	305	440	0.01%	0.002%
8	2.788	275	279	287	rVB3	2482	4548	0.10%	0.023%
9	2.922	299	301	303	rBV2	255	235	0.01%	0.001%
10	3.111	329	332	334	rVV2	296	330	0.01%	0.002%
11	3.142	334	337	340	rVV2	187	242	0.01%	0.001%
12	3.203	344	347	348	rBV2	292	290	0.01%	0.001%
13	3.313	360	365	366	rBV2	295	422	0.01%	0.002%
14	3.489	392	394	396	rBV	275	232	0.00%	0.001%
15	3.520	396	399	400	rBV2	205	222	0.00%	0.001%
16	3.630	416	417	420	rBV2	235	233	0.01%	0.001%
17	3.812	445	447	450	rVB	303	319	0.01%	0.002%
18	3.849	450	453	455	rBV3	277	316	0.01%	0.002%
19	3.873	455	457	460	rVB2	289	270	0.01%	0.001%
20	4.032	482	483	486	rBV2	355	309	0.01%	0.002%
21	4.105	492	495	496	rBV	254	214	0.00%	0.001%
22	4.294	523	526	533	rBV4	658	1624	0.03%	0.008%
23	4.465	545	554	579	rBV	113894	371193	7.99%	1.876%
24	4.745	598	600	601	rBV	348	299	0.01%	0.002%
25	5.056	638	651	671	rBV	233149	696759	15.01%	3.521%
26	5.330	694	696	697	rVB	412	259	0.01%	0.001%
27	5.349	697	699	700	rBV	328	215	0.00%	0.001%
28	5.385	700	705	710	rBV4	1116	2213	0.05%	0.011%
29	5.471	717	719	724	rVB4	497	639	0.01%	0.003%
30	5.556	725	733	742	rVB3	2523	6616	0.14%	0.033%
31	5.678	751	753	755	rVV	244	249	0.01%	0.001%
32	5.971	787	801	809	rBV2	606148	1853250	39.91%	9.365%
33	6.153	829	831	833	rBV2	495	362	0.01%	0.002%
34	6.245	844	846	848	rBV	263	229	0.00%	0.001%
35	6.410	870	873	876	rBV2	254	247	0.01%	0.001%
36	6.452	876	880	881	rBV	281	247	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035168.D
 Acq On : 19 Apr 2023 14:43
 Operator : JC/MD
 Sample : 02397-10DL 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	6.470	881	883	885	rVB2	401	304	0.01%	0.002%
38	6.531	892	893	896	rBV3	273	265	0.01%	0.001%
39	6.763	921	931	950	rBV	467351	1128210	24.30%	5.701%
40	7.111	983	988	998	rVB4	3330	8026	0.17%	0.041%
41	7.196	1000	1002	1003	rVB	457	255	0.01%	0.001%
42	7.306	1011	1020	1039	rBV	369671	819343	17.65%	4.140%
43	7.482	1046	1049	1053	rVB5	942	1587	0.03%	0.008%
44	7.586	1064	1066	1068	rVB2	317	241	0.01%	0.001%
45	7.793	1097	1100	1103	rVV2	151	270	0.01%	0.001%
46	7.818	1103	1104	1107	rVV2	293	268	0.01%	0.001%
47	7.909	1115	1119	1120	rBV2	308	324	0.01%	0.002%
48	7.952	1120	1126	1130	rVV3	1093	2492	0.05%	0.013%
49	8.019	1134	1137	1139	rBV2	349	410	0.01%	0.002%
50	8.037	1139	1140	1142	rBV	239	247	0.01%	0.001%
51	8.086	1145	1148	1152	rBV	209	260	0.01%	0.001%
52	8.117	1152	1153	1157	rBV3	172	280	0.01%	0.001%
53	8.257	1174	1176	1177	rBV	246	238	0.01%	0.001%
54	8.324	1181	1187	1207	rBV	228089	367286	7.91%	1.856%
55	8.495	1213	1215	1218	rBV2	739	904	0.02%	0.005%
56	8.647	1234	1240	1258	rBV	948897	1488260	32.05%	7.520%
57	8.952	1284	1290	1304	rBV	154984	233297	5.02%	1.179%
58	9.196	1326	1330	1332	rBV	606	664	0.01%	0.003%
59	9.385	1356	1361	1382	rBV	554025	793031	17.08%	4.007%
60	9.732	1415	1418	1420	rBV2	412	458	0.01%	0.002%
61	9.787	1425	1427	1430	rVB2	293	285	0.01%	0.001%
62	9.830	1432	1434	1435	rBV	320	230	0.00%	0.001%
63	10.080	1465	1475	1496	rBV2	2490797	4643391	100.00%	23.463%
64	10.342	1515	1518	1520	rBV3	465	434	0.01%	0.002%
65	10.384	1523	1525	1527	rBV3	280	300	0.01%	0.002%
66	10.451	1534	1536	1539	rBV3	477	436	0.01%	0.002%
67	10.549	1550	1552	1555	rBV2	282	342	0.01%	0.002%
68	10.573	1555	1556	1559	rVV2	276	291	0.01%	0.001%
69	10.750	1583	1585	1589	rVB2	278	402	0.01%	0.002%
70	10.799	1589	1593	1595	rBV2	432	507	0.01%	0.003%
71	11.098	1640	1642	1644	rBV	478	234	0.01%	0.001%
72	11.189	1652	1657	1671	rBV	602731	788784	16.99%	3.986%
73	11.360	1683	1685	1689	rVB2	382	464	0.01%	0.002%
74	11.433	1695	1697	1699	rBV	245	221	0.00%	0.001%
75	11.543	1709	1715	1717	rBV3	267	636	0.01%	0.003%
76	11.671	1734	1736	1739	rBV2	254	239	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035168.D
 Acq On : 19 Apr 2023 14:43
 Operator : JC/MD
 Sample : 02397-10DL 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	11.707	1739	1742	1748	rVB5	746	1025	0.02%	0.005%
78	11.969	1779	1785	1789	rBV	183626	223281	4.81%	1.128%
79	12.024	1789	1794	1795	rBV	1057174	1332883	28.70%	6.735%
80	12.329	1837	1844	1858	rBV2	1876739	3341115	71.95%	16.883%
81	12.713	1904	1907	1911	rBV3	308	463	0.01%	0.002%
82	12.927	1939	1942	1947	rVB4	1334	1819	0.04%	0.009%
83	13.067	1963	1965	1969	rVB2	316	263	0.01%	0.001%
84	13.116	1971	1973	1976	rVB2	566	378	0.01%	0.002%
85	13.207	1984	1988	1991	rBV2	806	772	0.02%	0.004%
86	13.268	1995	1998	2000	rBV2	269	329	0.01%	0.002%
87	13.299	2001	2003	2004	rVB	395	221	0.00%	0.001%
88	13.317	2005	2006	2009	rBV	313	306	0.01%	0.002%
89	13.384	2013	2017	2022	rVB2	240	495	0.01%	0.003%
90	13.530	2039	2041	2043	rBV	252	272	0.01%	0.001%
91	13.585	2045	2050	2064	rBV	353890	446310	9.61%	2.255%
92	13.847	2092	2093	2095	rBV	411	248	0.01%	0.001%
93	13.963	2106	2112	2119	rBV	105898	139883	3.01%	0.707%
94	14.115	2136	2137	2139	rBV2	351	314	0.01%	0.002%
95	14.280	2160	2164	2167	rVB2	548	776	0.02%	0.004%
96	14.463	2191	2194	2196	rBV	462	503	0.01%	0.003%
97	14.640	2221	2223	2225	rBV	342	266	0.01%	0.001%
98	14.786	2242	2247	2252	rVB3	3872	5340	0.12%	0.027%
99	15.249	2318	2323	2328	rBV2	13611	18386	0.40%	0.093%
100	15.682	2393	2394	2397	rVB3	616	395	0.01%	0.002%




Sum of corrected areas: 19790119

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035168.D
Acq On : 19 Apr 2023 14:43
Operator : JC/MD
Sample : 02397-10DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

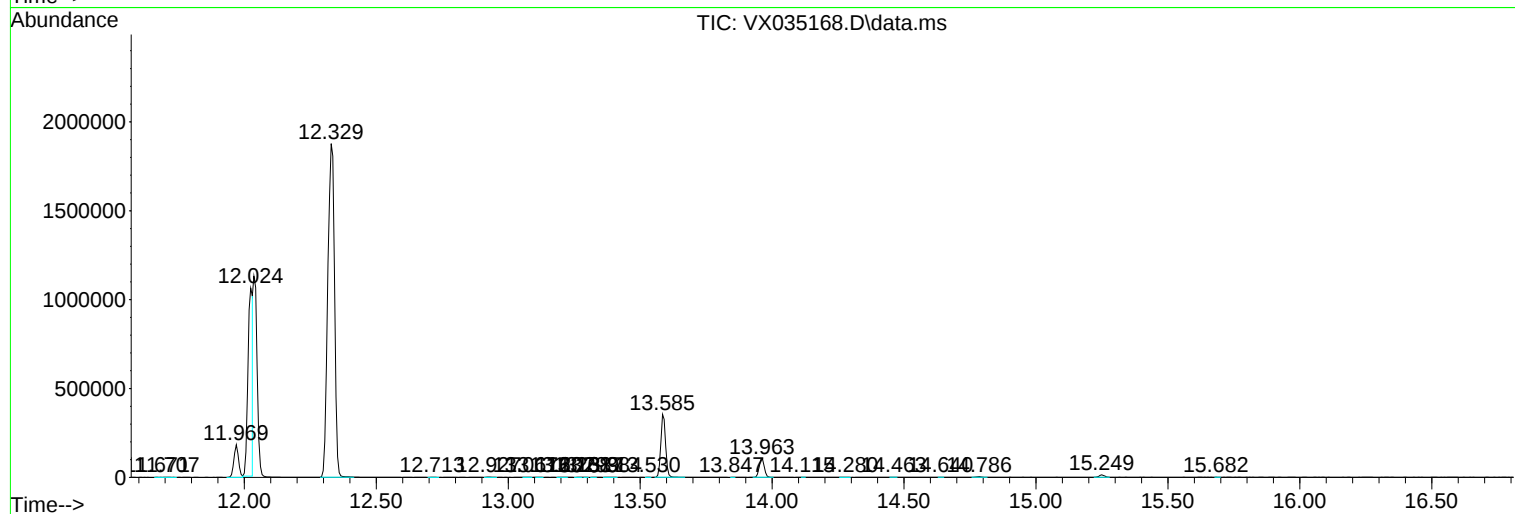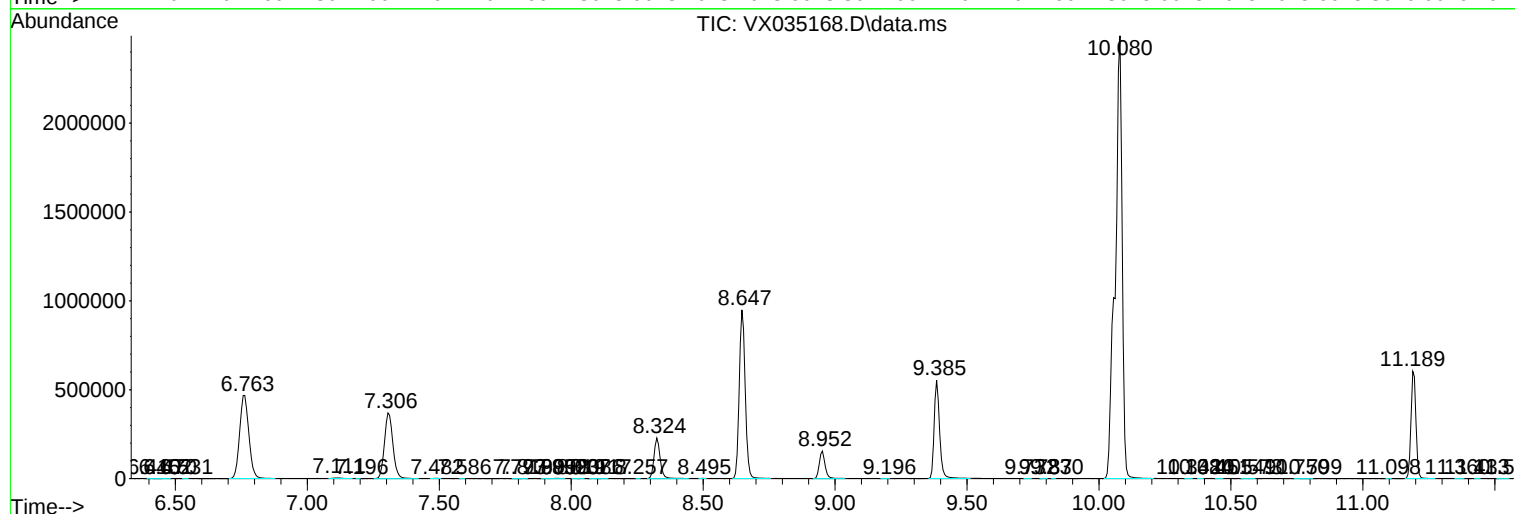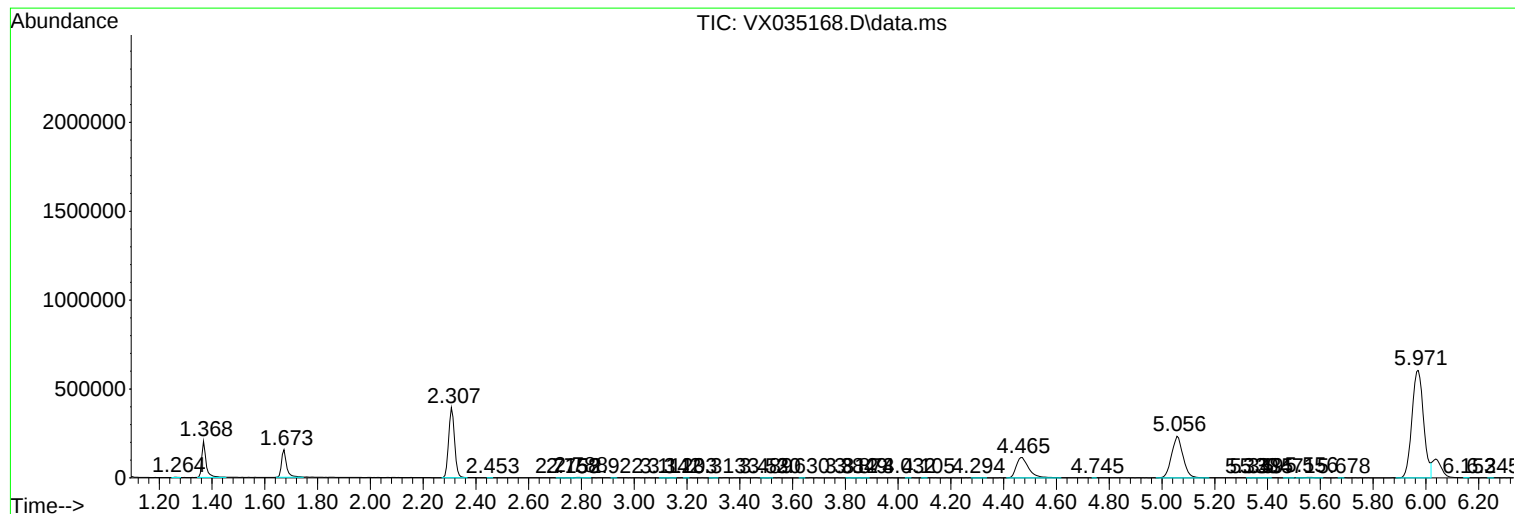

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035168.D
Acq On : 19 Apr 2023 14:43
Operator : JC/MD
Sample : 02397-10DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035168.D
Acq On : 19 Apr 2023 14:43
Operator : JC/MD
Sample : 02397-10DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------