

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035169.D
 Acq On : 19 Apr 2023 15:06
 Operator : JC/MD
 Sample : 02397-05DL 400X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035169.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	35	rBV3	3309	4471	0.09%	0.022%
2	1.368	42	46	59	rBV	197812	224016	4.30%	1.082%
3	1.672	91	96	111	rBV	157591	211056	4.05%	1.019%
4	2.306	194	200	210	rBV	386224	600681	11.52%	2.901%
5	2.514	232	234	237	rBV2	708	555	0.01%	0.003%
6	2.788	275	279	287	rVB3	2596	4662	0.09%	0.023%
7	3.087	325	328	329	rVB2	291	273	0.01%	0.001%
8	3.111	329	332	334	rBV2	221	262	0.01%	0.001%
9	3.129	334	335	337	rBV2	294	202	0.00%	0.001%
10	3.361	372	373	375	rBV	264	212	0.00%	0.001%
11	3.392	375	378	379	rVB2	207	191	0.00%	0.001%
12	3.568	405	407	409	rBV	192	189	0.00%	0.001%
13	3.599	410	412	413	rVB2	367	211	0.00%	0.001%
14	3.641	415	419	420	rVB2	215	250	0.00%	0.001%
15	3.666	420	423	424	rBV3	214	223	0.00%	0.001%
16	3.733	431	434	436	rBV2	268	255	0.00%	0.001%
17	3.812	444	447	449	rVV2	261	236	0.00%	0.001%
18	3.946	466	469	470	rBV2	211	251	0.00%	0.001%
19	3.989	474	476	477	rBV2	327	222	0.00%	0.001%
20	4.007	477	479	482	rVB2	353	285	0.01%	0.001%
21	4.044	482	485	486	rBV	308	290	0.01%	0.001%
22	4.257	517	520	521	rBV2	267	268	0.01%	0.001%
23	4.288	524	525	528	rVB	435	230	0.00%	0.001%
24	4.397	540	543	544	rBV	447	402	0.01%	0.002%
25	4.465	545	554	578	rBV	109325	356707	6.84%	1.723%
26	4.800	607	609	613	rBV3	324	416	0.01%	0.002%
27	4.946	631	633	638	rVB2	395	441	0.01%	0.002%
28	5.056	638	651	668	rBV	216187	676427	12.98%	3.267%
29	5.196	672	674	675	rBV	438	231	0.00%	0.001%
30	5.342	696	698	699	rBV	238	212	0.00%	0.001%
31	5.391	699	706	711	rVV4	1161	2569	0.05%	0.012%
32	5.544	724	731	732	rBV2	2597	3258	0.06%	0.016%
33	5.629	743	745	748	rVB3	326	237	0.00%	0.001%
34	5.653	748	749	752	rBV	222	251	0.00%	0.001%
35	5.714	757	759	760	rBV	375	251	0.00%	0.001%
36	5.970	788	801	825	rBV2	605165	1800273	34.53%	8.694%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035169.D
 Acq On : 19 Apr 2023 15:06
 Operator : JC/MD
 Sample : 02397-05DL 400X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	6.232	842	844	848	rBV3	285	339	0.01%	0.002%
38	6.361	863	865	867	rBV2	263	271	0.01%	0.001%
39	6.452	877	880	881	rBV2	383	329	0.01%	0.002%
40	6.513	889	890	892	rBV	231	200	0.00%	0.001%
41	6.531	892	893	894	rVV	332	211	0.00%	0.001%
42	6.568	898	899	904	rVB2	263	431	0.01%	0.002%
43	6.763	921	931	952	rBV	474760	1127895	21.64%	5.447%
44	6.970	963	965	969	rVB	439	269	0.01%	0.001%
45	7.116	982	989	996	rBV5	3792	9016	0.17%	0.044%
46	7.305	1011	1020	1039	rBV	369235	810043	15.54%	3.912%
47	7.482	1044	1049	1062	rVB5	1125	3666	0.07%	0.018%
48	7.732	1089	1090	1092	rVB	400	203	0.00%	0.001%
49	7.818	1101	1104	1107	rBV2	199	272	0.01%	0.001%
50	7.860	1107	1111	1113	rVV	164	236	0.00%	0.001%
51	7.946	1120	1125	1135	rVV5	1372	3367	0.06%	0.016%
52	8.068	1143	1145	1147	rVB	281	234	0.00%	0.001%
53	8.116	1151	1153	1154	rVB	379	195	0.00%	0.001%
54	8.220	1168	1170	1173	rBV2	191	234	0.00%	0.001%
55	8.324	1180	1187	1201	rBV	218648	360728	6.92%	1.742%
56	8.494	1214	1215	1216	rBV	486	247	0.00%	0.001%
57	8.580	1226	1229	1233	rBV4	324	350	0.01%	0.002%
58	8.647	1234	1240	1260	rVV	918172	1465222	28.11%	7.076%
59	8.952	1284	1290	1300	rBV	152718	223803	4.29%	1.081%
60	9.201	1328	1331	1332	rBV2	290	322	0.01%	0.002%
61	9.226	1332	1335	1337	rBV3	199	233	0.00%	0.001%
62	9.275	1342	1343	1345	rBV	409	296	0.01%	0.001%
63	9.384	1356	1361	1384	rVV	554000	777052	14.91%	3.753%
64	9.695	1410	1412	1415	rBV2	433	453	0.01%	0.002%
65	9.756	1420	1422	1424	rVV2	388	285	0.01%	0.001%
66	9.823	1430	1433	1437	rBV3	251	376	0.01%	0.002%
67	10.079	1465	1475	1494	rBV2	2923853	5213207	100.00%	25.177%
68	10.287	1508	1509	1510	rVB	547	200	0.00%	0.001%
69	10.372	1521	1523	1526	rVB2	455	423	0.01%	0.002%
70	10.396	1526	1527	1529	rBV	336	279	0.01%	0.001%
71	10.640	1565	1567	1568	rVV	405	277	0.01%	0.001%
72	10.823	1595	1597	1598	rVB	489	206	0.00%	0.001%
73	11.043	1630	1633	1636	rBV2	264	292	0.01%	0.001%
74	11.097	1640	1642	1643	rBV2	344	229	0.00%	0.001%
75	11.116	1643	1645	1648	rVB2	285	290	0.01%	0.001%
76	11.189	1652	1657	1670	rBV	585936	767326	14.72%	3.706%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035169.D
 Acq On : 19 Apr 2023 15:06
 Operator : JC/MD
 Sample : 02397-05DL 400X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0ML7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	11.360	1683	1685	1687	rBV	502	415	0.01%	0.002%
78	11.384	1687	1689	1692	rVV	187	206	0.00%	0.001%
79	11.567	1717	1719	1721	rBV2	490	456	0.01%	0.002%
80	11.713	1739	1743	1744	rBV2	332	388	0.01%	0.002%
81	11.969	1780	1785	1789	rBV	90565	111910	2.15%	0.540%
82	12.024	1789	1794	1811	rVB2	958184	1683899	32.30%	8.132%
83	12.329	1837	1844	1852	rBV2	2229484	3794913	72.79%	18.327%
84	12.792	1918	1920	1922	rBV	334	234	0.00%	0.001%
85	12.926	1935	1942	1945	rBV4	2410	3592	0.07%	0.017%
86	13.164	1980	1981	1984	rVB	358	324	0.01%	0.002%
87	13.201	1984	1987	1992	rBV5	1425	2366	0.05%	0.011%
88	13.445	2025	2027	2029	rBV2	221	217	0.00%	0.001%
89	13.585	2045	2050	2060	rBV	283742	359790	6.90%	1.738%
90	13.695	2066	2068	2069	rBV	322	246	0.00%	0.001%
91	13.963	2106	2112	2120	rVB	52895	67940	1.30%	0.328%
92	14.225	2152	2155	2158	rVB2	532	482	0.01%	0.002%
93	14.475	2194	2196	2199	rVB2	453	452	0.01%	0.002%
94	14.505	2199	2201	2202	rBV	396	344	0.01%	0.002%
95	14.786	2244	2247	2252	rVB5	2161	2933	0.06%	0.014%
96	14.822	2252	2253	2256	rBV2	487	441	0.01%	0.002%
97	14.853	2256	2258	2262	rVB2	600	535	0.01%	0.003%
98	15.133	2302	2304	2306	rBV3	481	611	0.01%	0.003%
99	15.249	2319	2323	2329	rVB2	9352	12698	0.24%	0.061%
100	16.030	2449	2451	2453	rBV2	720	469	0.01%	0.002%




Sum of corrected areas: 20706534

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035169.D
Acq On : 19 Apr 2023 15:06
Operator : JC/MD
Sample : 02397-05DL 400X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COML7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

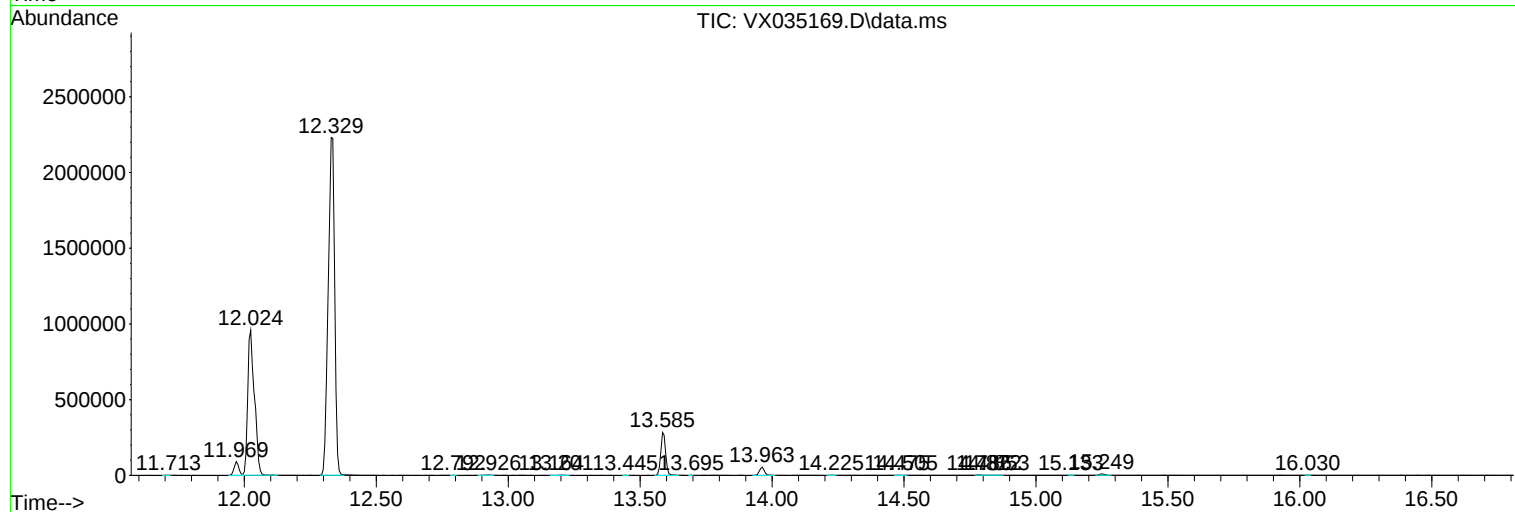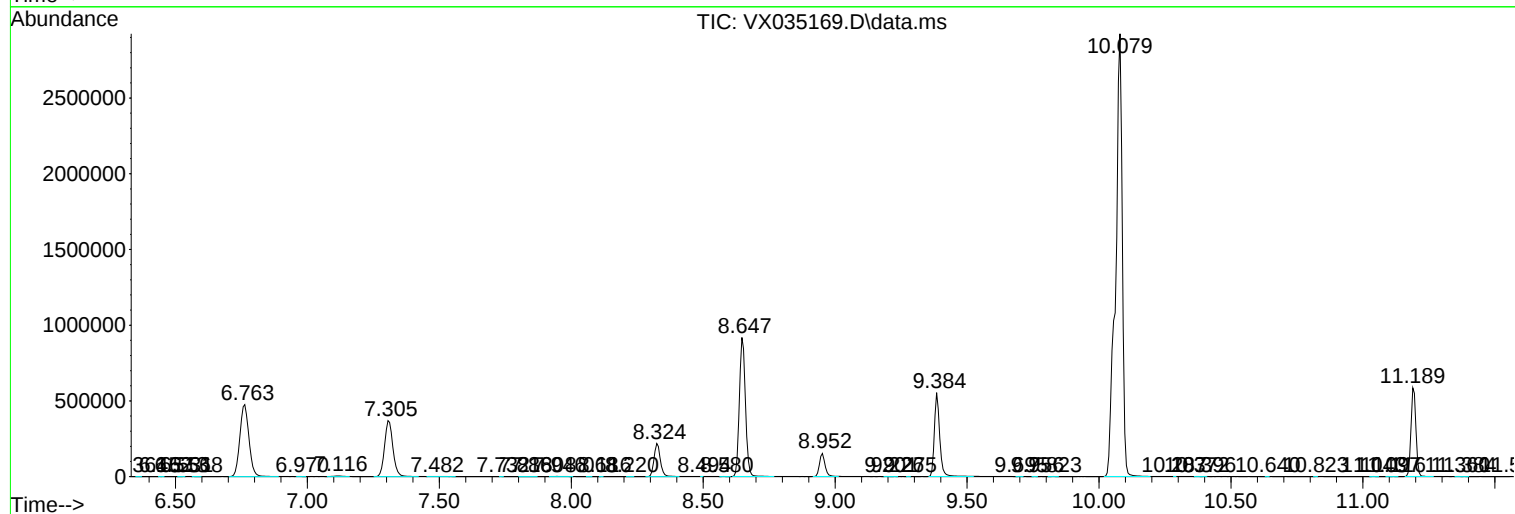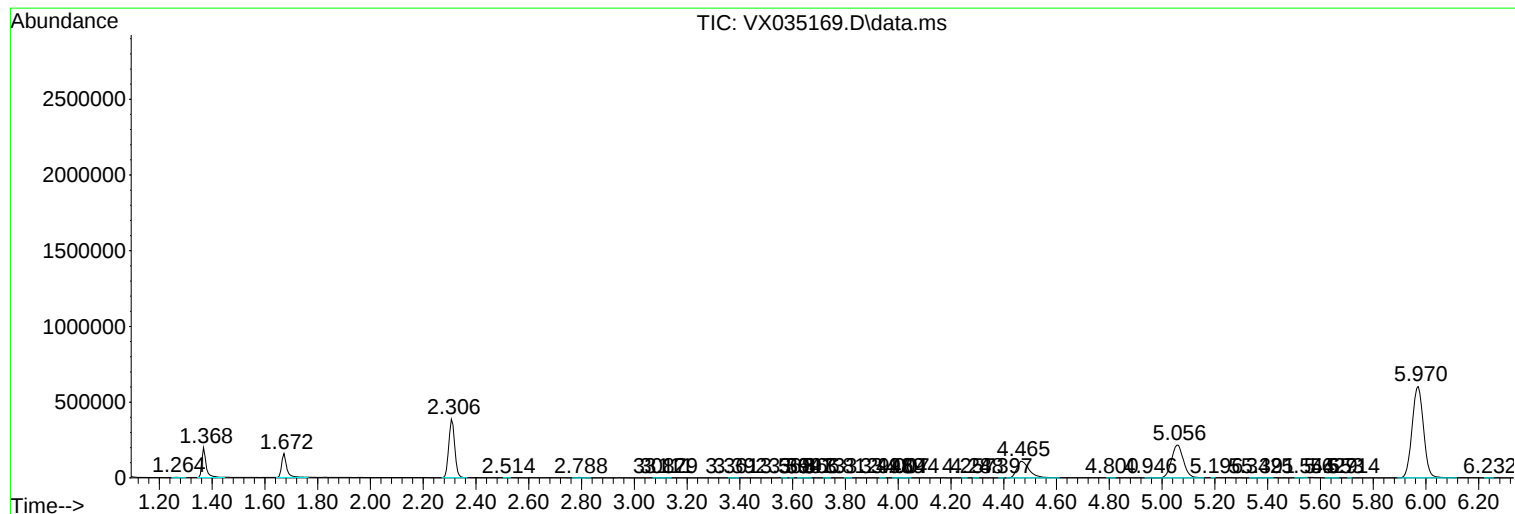

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035169.D
Acq On : 19 Apr 2023 15:06
Operator : JC/MD
Sample : 02397-05DL 400X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ML7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035169.D
Acq On : 19 Apr 2023 15:06
Operator : JC/MD
Sample : 02397-05DL 400X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ML7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------