

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035170.D
 Acq On : 19 Apr 2023 15:29
 Operator : JC/MD
 Sample : 02397-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035170.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	32	rBV2	2516	2900	0.16%	0.023%
2	1.368	42	46	58	rVB	200457	220009	12.30%	1.728%
3	1.672	91	96	115	rVB	147740	202048	11.29%	1.587%
4	2.307	194	200	210	rBV	383018	592270	33.10%	4.653%
5	2.575	241	244	245	rBV2	343	355	0.02%	0.003%
6	2.630	252	253	255	rVB	543	230	0.01%	0.002%
7	2.782	276	278	280	rBV3	660	537	0.03%	0.004%
8	3.373	373	375	376	rBV	402	272	0.02%	0.002%
9	3.398	376	379	383	rVB2	239	363	0.02%	0.003%
10	3.764	437	439	443	rBV2	300	381	0.02%	0.003%
11	3.831	448	450	452	rVV2	244	241	0.01%	0.002%
12	3.946	467	469	472	rVB2	186	228	0.01%	0.002%
13	3.983	472	475	477	rBV	254	271	0.02%	0.002%
14	4.184	505	508	509	rBV2	196	241	0.01%	0.002%
15	4.282	521	524	527	rBV	262	304	0.02%	0.002%
16	4.465	544	554	571	rBV2	112128	345574	19.32%	2.715%
17	4.940	630	632	635	rVB2	410	272	0.02%	0.002%
18	5.056	638	651	673	rVV	222028	709788	39.67%	5.576%
19	5.373	699	703	704	rBV2	959	1317	0.07%	0.010%
20	5.550	725	732	733	rBV4	3943	6075	0.34%	0.048%
21	5.879	785	786	789	rBV3	308	300	0.02%	0.002%
22	5.970	789	801	819	rBV2	597434	1789117	100.00%	14.055%
23	6.245	844	846	848	rVB2	308	279	0.02%	0.002%
24	6.294	852	854	856	rBV2	342	264	0.01%	0.002%
25	6.336	859	861	863	rBV3	222	217	0.01%	0.002%
26	6.379	867	868	871	rBV2	481	314	0.02%	0.002%
27	6.403	871	872	876	rBV2	264	298	0.02%	0.002%
28	6.464	881	882	885	rVB2	365	272	0.02%	0.002%
29	6.617	905	907	909	rBV2	316	309	0.02%	0.002%
30	6.763	921	931	949	rBV	419551	1017572	56.88%	7.994%
31	7.050	976	978	981	rBV3	341	402	0.02%	0.003%
32	7.117	981	989	998	rVV4	4381	10593	0.59%	0.083%
33	7.306	1011	1020	1034	rVV	362764	799446	44.68%	6.280%
34	7.464	1044	1046	1047	rBV2	547	313	0.02%	0.002%
35	7.592	1065	1067	1069	rBV2	287	328	0.02%	0.003%
36	7.854	1106	1110	1114	rVV4	932	1491	0.08%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035170.D
 Acq On : 19 Apr 2023 15:29
 Operator : JC/MD
 Sample : 02397-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	7.897	1114	1117	1118	rVV2	337	300	0.02%	0.002%
38	7.946	1121	1125	1132	rVB5	1142	2208	0.12%	0.017%
39	8.068	1143	1145	1149	rVB3	259	257	0.01%	0.002%
40	8.123	1151	1154	1157	rBV2	351	387	0.02%	0.003%
41	8.147	1157	1158	1161	rBV	352	234	0.01%	0.002%
42	8.202	1164	1167	1170	rBV	303	263	0.01%	0.002%
43	8.324	1181	1187	1200	rBV	216403	359364	20.09%	2.823%
44	8.574	1226	1228	1233	rVB4	408	493	0.03%	0.004%
45	8.647	1233	1240	1253	rBV	913354	1443445	80.68%	11.339%
46	8.872	1276	1277	1279	rBV2	388	304	0.02%	0.002%
47	8.952	1284	1290	1301	rBV	155665	228428	12.77%	1.794%
48	9.159	1322	1324	1326	rVB	573	410	0.02%	0.003%
49	9.281	1341	1344	1348	rVB3	978	1179	0.07%	0.009%
50	9.385	1356	1361	1378	rBV	548147	761028	42.54%	5.978%
51	9.878	1441	1442	1446	rVB3	331	250	0.01%	0.002%
52	10.055	1465	1471	1486	rBV	828547	1144731	63.98%	8.993%
53	10.232	1498	1500	1502	rBV	332	268	0.01%	0.002%
54	10.275	1506	1507	1510	rBV	434	458	0.03%	0.004%
55	10.360	1519	1521	1524	rVB2	428	372	0.02%	0.003%
56	10.390	1524	1526	1528	rVV2	211	210	0.01%	0.002%
57	10.579	1555	1557	1559	rVV2	267	270	0.02%	0.002%
58	10.604	1559	1561	1563	rVV	328	229	0.01%	0.002%
59	10.628	1563	1565	1567	rVV	377	231	0.01%	0.002%
60	10.714	1576	1579	1580	rBV2	316	347	0.02%	0.003%
61	10.756	1583	1586	1588	rVV3	273	330	0.02%	0.003%
62	10.793	1590	1592	1597	rVB	530	535	0.03%	0.004%
63	10.866	1601	1604	1610	rBV3	612	892	0.05%	0.007%
64	10.951	1615	1618	1619	rBV	296	271	0.02%	0.002%
65	11.043	1631	1633	1637	rVB2	209	220	0.01%	0.002%
66	11.189	1652	1657	1667	rBV	589635	781310	43.67%	6.138%
67	11.384	1688	1689	1691	rBV	275	218	0.01%	0.002%
68	11.616	1726	1727	1730	rBV2	209	232	0.01%	0.002%
69	11.689	1735	1739	1740	rBV2	289	399	0.02%	0.003%
70	11.707	1740	1742	1746	rVB3	506	428	0.02%	0.003%
71	11.762	1749	1751	1752	rBV2	637	342	0.02%	0.003%
72	11.841	1762	1764	1765	rVB	465	284	0.02%	0.002%
73	11.933	1772	1779	1782	rBV2	653	1010	0.06%	0.008%
74	11.976	1782	1786	1788	rBV4	1621	2081	0.12%	0.016%
75	12.024	1788	1794	1803	rBV	800274	1029288	57.53%	8.086%
76	12.219	1822	1826	1837	rBV2	11175	18825	1.05%	0.148%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035170.D
 Acq On : 19 Apr 2023 15:29
 Operator : JC/MD
 Sample : 02397-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1855	rVB	891102	1201555	67.16%	9.439%
78	12.555	1879	1881	1882	rBV	349	282	0.02%	0.002%
79	12.634	1893	1894	1896	rVB2	322	228	0.01%	0.002%
80	12.658	1896	1898	1901	rBV2	332	339	0.02%	0.003%
81	12.823	1921	1925	1927	rBV3	454	450	0.03%	0.004%
82	12.860	1927	1931	1938	rVB3	4347	5750	0.32%	0.045%
83	13.097	1969	1970	1973	rVV	228	241	0.01%	0.002%
84	13.512	2037	2038	2041	rBV2	328	347	0.02%	0.003%
85	13.591	2046	2051	2060	rVB2	16173	22056	1.23%	0.173%
86	13.847	2091	2093	2094	rBV2	309	276	0.02%	0.002%
87	13.865	2094	2096	2101	rVB3	572	790	0.04%	0.006%
88	13.963	2108	2112	2117	rBV3	2785	3350	0.19%	0.026%
89	14.103	2130	2135	2136	rBV2	449	522	0.03%	0.004%
90	14.201	2149	2151	2153	rVB	430	352	0.02%	0.003%
91	14.225	2153	2155	2158	rBV3	336	495	0.03%	0.004%
92	14.475	2192	2196	2200	rVB2	516	721	0.04%	0.006%
93	14.701	2231	2233	2236	rBV3	498	576	0.03%	0.005%
94	14.865	2256	2260	2262	rBV3	577	791	0.04%	0.006%
95	14.902	2265	2266	2267	rBV	599	330	0.02%	0.003%
96	15.060	2291	2292	2293	rBV	533	259	0.01%	0.002%
97	15.304	2330	2332	2334	rBV2	558	619	0.03%	0.005%
98	15.798	2410	2413	2415	rBV3	827	890	0.05%	0.007%
99	16.475	2522	2524	2525	rBV	689	362	0.02%	0.003%
100	16.536	2532	2534	2537	rVB2	786	567	0.03%	0.004%


Sum of corrected areas: 12729670

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035170.D
Acq On : 19 Apr 2023 15:29
Operator : JC/MD
Sample : 02397-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

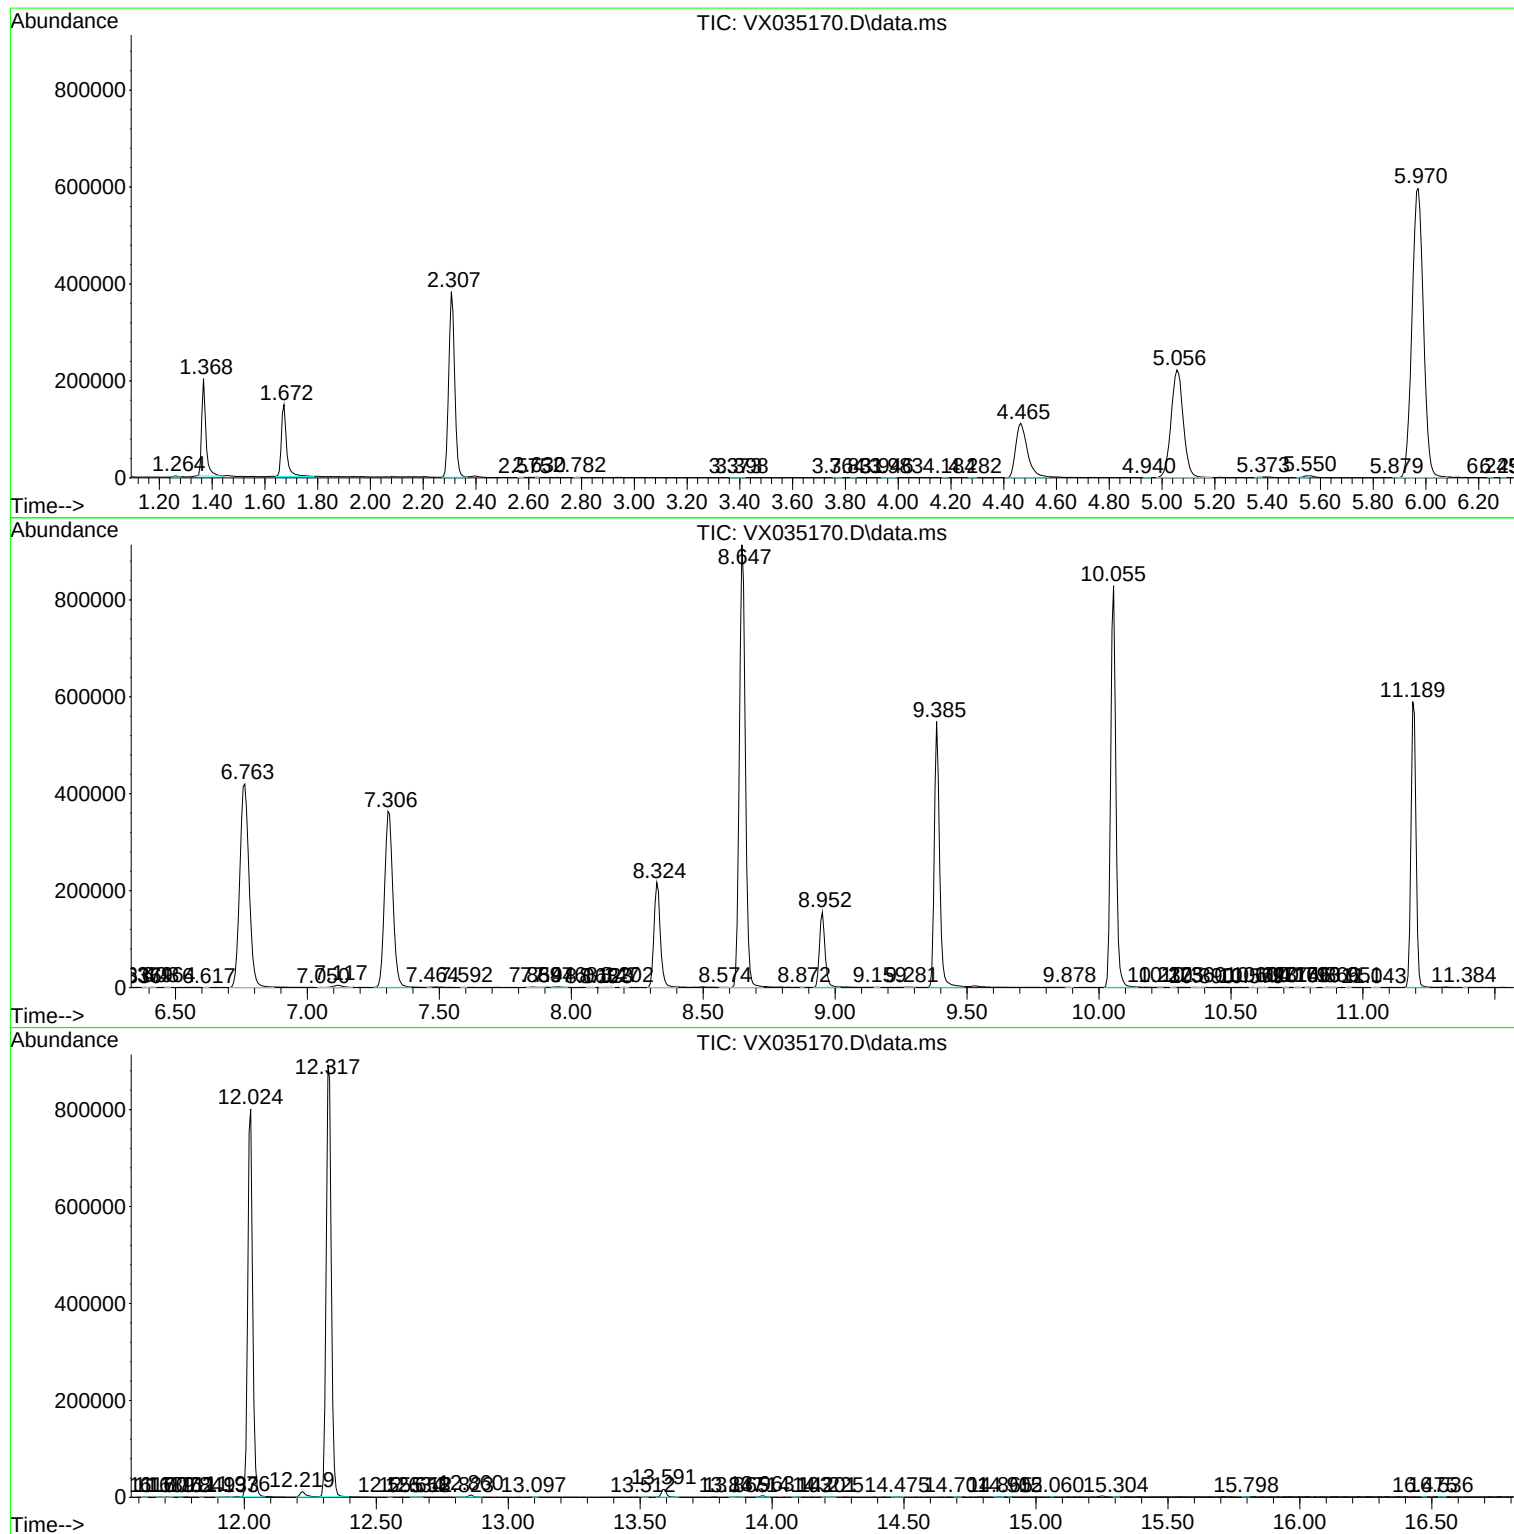

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035170.D
Acq On : 19 Apr 2023 15:29
Operator : JC/MD
Sample : 02397-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035170.D
Acq On : 19 Apr 2023 15:29
Operator : JC/MD
Sample : 02397-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------