

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035171.D
 Acq On : 19 Apr 2023 15:52
 Operator : JC/MD
 Sample : 02397-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035171.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	17	rBV2	19235	18531	0.65%	0.103%
2	1.264	26	29	32	rBV2	6709	5391	0.19%	0.030%
3	1.367	42	46	54	rBV	232429	262548	9.19%	1.453%
4	1.672	92	96	105	rVB	160166	203185	7.11%	1.125%
5	2.306	194	200	210	rBV	399480	626829	21.95%	3.469%
6	2.520	230	235	237	rBV3	1237	2010	0.07%	0.011%
7	2.715	263	267	269	rBV3	678	984	0.03%	0.005%
8	2.788	275	279	280	rBV3	1120	1299	0.05%	0.007%
9	3.099	327	330	333	rBV3	908	1266	0.04%	0.007%
10	3.160	338	340	343	rBV2	206	273	0.01%	0.002%
11	3.355	370	372	374	rBV2	309	398	0.01%	0.002%
12	3.446	382	387	396	rVB4	1447	2933	0.10%	0.016%
13	3.593	408	411	412	rBV	366	353	0.01%	0.002%
14	3.666	421	423	427	rVB2	242	319	0.01%	0.002%
15	3.946	465	469	476	rBV3	399	721	0.03%	0.004%
16	4.129	496	499	502	rBV2	210	376	0.01%	0.002%
17	4.196	507	510	512	rBV2	336	356	0.01%	0.002%
18	4.227	512	515	518	rVB	316	282	0.01%	0.002%
19	4.464	545	554	578	rBV	117958	368781	12.91%	2.041%
20	4.922	627	629	631	rVB2	353	339	0.01%	0.002%
21	4.958	631	635	638	rBV2	292	544	0.02%	0.003%
22	5.056	639	651	670	rBV	226761	706743	24.75%	3.912%
23	5.257	682	684	688	rVB2	502	371	0.01%	0.002%
24	5.385	700	705	706	rBV2	971	1365	0.05%	0.008%
25	5.464	715	718	719	rBV	380	316	0.01%	0.002%
26	5.483	719	721	723	rVV2	345	251	0.01%	0.001%
27	5.556	723	733	744	rVB2	3381	8970	0.31%	0.050%
28	5.635	744	746	747	rBV2	326	285	0.01%	0.002%
29	5.830	776	778	782	rVB3	436	492	0.02%	0.003%
30	5.970	788	801	828	rBV2	627949	1890080	66.18%	10.461%
31	6.342	860	862	864	rBV	293	248	0.01%	0.001%
32	6.367	864	866	869	rVV3	391	403	0.01%	0.002%
33	6.556	892	897	899	rBV	355	569	0.02%	0.003%
34	6.763	920	931	951	rBV	467383	1123602	39.34%	6.219%
35	6.891	951	952	954	rVB2	634	297	0.01%	0.002%
36	6.946	959	961	965	rVB2	502	546	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035171.D
 Acq On : 19 Apr 2023 15:52
 Operator : JC/MD
 Sample : 02397-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	7.116	980	989	996	rVV5	1943	4812	0.17%	0.027%
38	7.184	998	1000	1003	rVB2	322	309	0.01%	0.002%
39	7.305	1011	1020	1039	rBV	382234	840539	29.43%	4.652%
40	7.482	1044	1049	1050	rBV2	831	1046	0.04%	0.006%
41	7.939	1120	1124	1126	rBV2	1555	2181	0.08%	0.012%
42	8.043	1138	1141	1142	rBV2	240	266	0.01%	0.001%
43	8.074	1142	1146	1147	rBV	245	245	0.01%	0.001%
44	8.269	1176	1178	1181	rVB2	294	254	0.01%	0.001%
45	8.324	1181	1187	1203	rBV	230315	376210	13.17%	2.082%
46	8.488	1212	1214	1215	rBV2	697	512	0.02%	0.003%
47	8.592	1229	1231	1233	rBV2	281	322	0.01%	0.002%
48	8.647	1233	1240	1258	rVV	973862	1520461	53.24%	8.415%
49	8.951	1283	1290	1304	rBV	161434	242565	8.49%	1.342%
50	9.275	1338	1343	1346	rBV3	811	1124	0.04%	0.006%
51	9.384	1356	1361	1374	rBV	565810	802606	28.10%	4.442%
52	9.653	1402	1405	1409	rVV4	470	756	0.03%	0.004%
53	9.872	1438	1441	1443	rVB2	417	432	0.02%	0.002%
54	9.933	1448	1451	1456	rVV2	175	305	0.01%	0.002%
55	10.055	1465	1471	1473	rBV	963951	1375562	48.16%	7.613%
56	10.238	1498	1501	1505	rBV3	644	916	0.03%	0.005%
57	10.354	1518	1520	1523	rBV2	261	294	0.01%	0.002%
58	10.409	1526	1529	1531	rVB2	312	287	0.01%	0.002%
59	10.457	1535	1537	1539	rVB	522	253	0.01%	0.001%
60	10.482	1539	1541	1544	rBV2	296	253	0.01%	0.001%
61	10.591	1556	1559	1562	rBV	242	286	0.01%	0.002%
62	10.707	1575	1578	1580	rVV2	258	296	0.01%	0.002%
63	10.799	1590	1593	1596	rBV2	316	325	0.01%	0.002%
64	10.939	1615	1616	1619	rBV2	256	293	0.01%	0.002%
65	11.024	1627	1630	1631	rBV2	298	252	0.01%	0.001%
66	11.116	1643	1645	1647	rVB2	267	258	0.01%	0.001%
67	11.146	1647	1650	1652	rBV2	250	328	0.01%	0.002%
68	11.189	1652	1657	1671	rVV	619399	819860	28.71%	4.538%
69	11.305	1674	1676	1681	rVV4	720	990	0.03%	0.005%
70	11.366	1681	1686	1691	rVV	5145	6569	0.23%	0.036%
71	11.433	1691	1697	1698	rVV4	421	825	0.03%	0.005%
72	11.463	1698	1702	1709	rVB2	2311	3112	0.11%	0.017%
73	11.713	1739	1743	1745	rBV2	776	620	0.02%	0.003%
74	11.756	1749	1750	1753	rVB2	416	343	0.01%	0.002%
75	11.792	1753	1756	1757	rBV	342	242	0.01%	0.001%
76	11.969	1779	1785	1789	rBV	508268	620836	21.74%	3.436%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035171.D
 Acq On : 19 Apr 2023 15:52
 Operator : JC/MD
 Sample : 02397-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	12.036	1789	1796	1809	rVB2	1416081	2856023	100.00%	15.807%
78	12.219	1822	1826	1834	rBV2	9835	17273	0.60%	0.096%
79	12.323	1837	1843	1855	rVV3	1077833	1755873	61.48%	9.718%
80	12.536	1875	1878	1879	rVV2	408	409	0.01%	0.002%
81	12.554	1879	1881	1883	rVV2	322	304	0.01%	0.002%
82	12.579	1883	1885	1887	rVV2	464	372	0.01%	0.002%
83	12.676	1899	1901	1902	rBV	449	256	0.01%	0.001%
84	12.707	1904	1906	1909	rVB2	820	766	0.03%	0.004%
85	12.920	1937	1941	1950	rVB2	7553	10705	0.37%	0.059%
86	13.067	1959	1965	1969	rVV3	12144	23419	0.82%	0.130%
87	13.115	1969	1973	1979	rVV2	12583	15863	0.56%	0.088%
88	13.201	1983	1987	1990	rVV3	2234	3387	0.12%	0.019%
89	13.384	2013	2017	2022	rVB4	1382	2011	0.07%	0.011%
90	13.432	2022	2025	2026	rBV2	315	298	0.01%	0.002%
91	13.585	2045	2050	2062	rVV	976017	1191900	41.73%	6.597%
92	13.749	2075	2077	2079	rBV	276	255	0.01%	0.001%
93	13.774	2079	2081	2083	rBV	484	403	0.01%	0.002%
94	13.963	2106	2112	2121	rVV	198812	259699	9.09%	1.437%
95	14.103	2131	2135	2137	rBV2	280	449	0.02%	0.002%
96	14.743	2239	2240	2241	rBV	589	426	0.01%	0.002%
97	14.780	2241	2246	2253	rVB2	12922	19361	0.68%	0.107%
98	14.914	2266	2268	2271	rBV3	460	414	0.01%	0.002%
99	15.249	2318	2323	2330	rBV	33682	47592	1.67%	0.263%
100	15.517	2365	2367	2369	rBV4	674	515	0.02%	0.003%




Sum of corrected areas: 18068174

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035171.D
Acq On : 19 Apr 2023 15:52
Operator : JC/MD
Sample : 02397-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

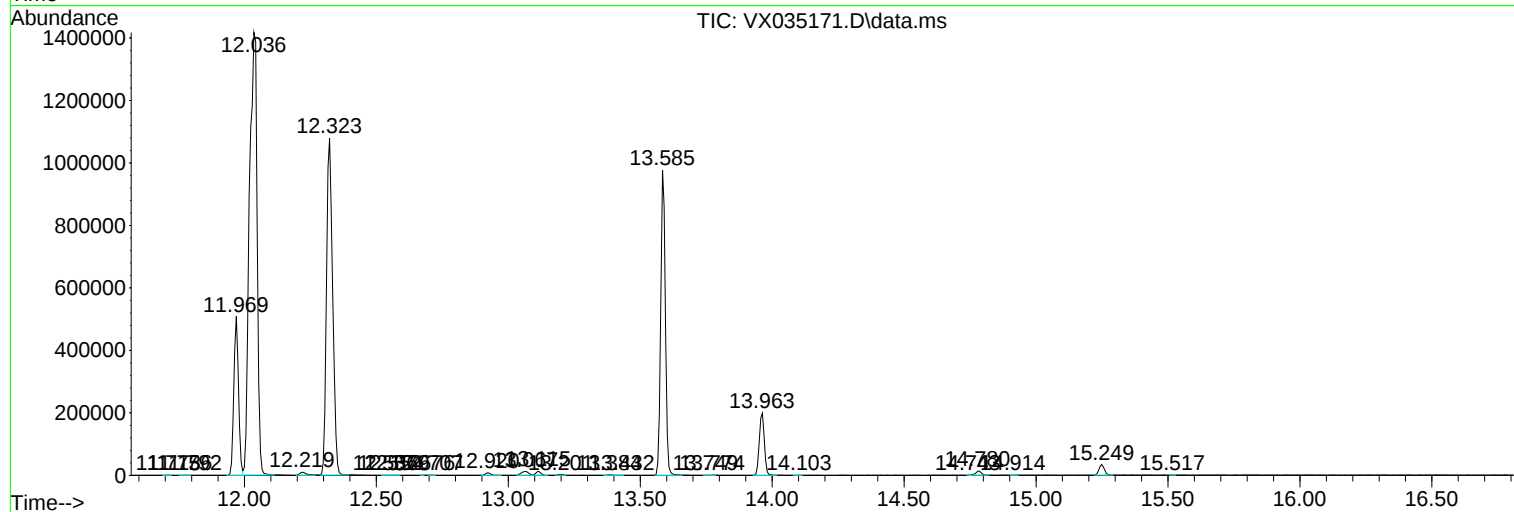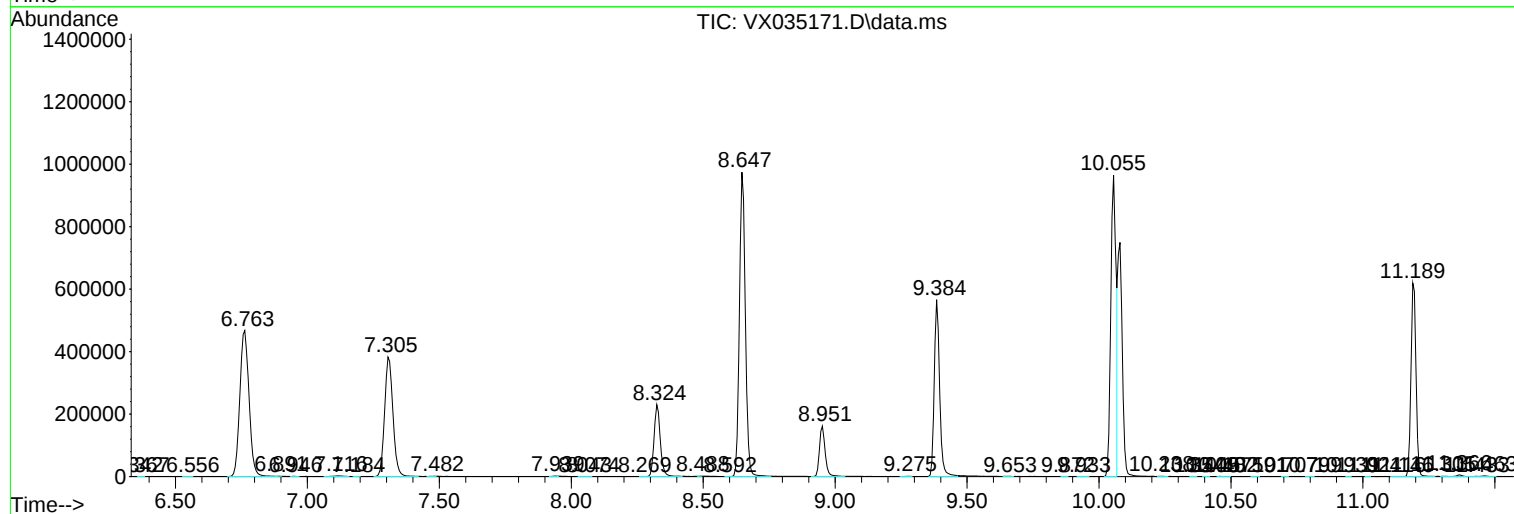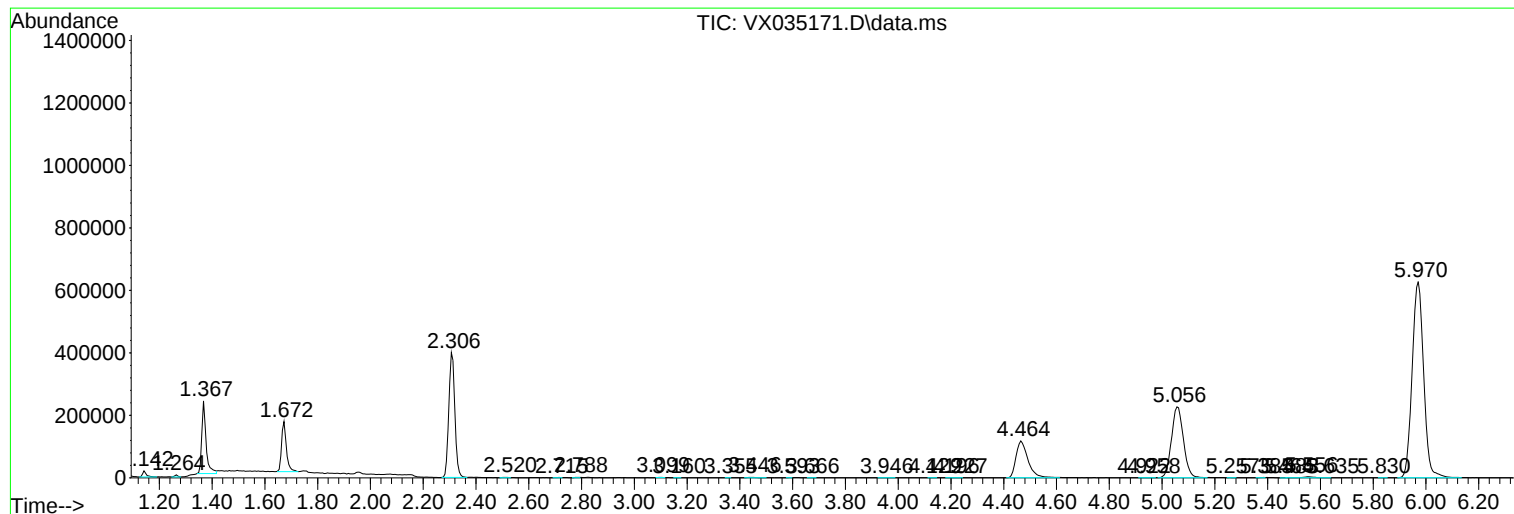

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035171.D
Acq On : 19 Apr 2023 15:52
Operator : JC/MD
Sample : 02397-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035171.D
Acq On : 19 Apr 2023 15:52
Operator : JC/MD
Sample : 02397-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------