

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035183.D
 Acq On : 19 Apr 2023 20:52
 Operator : JC/MD
 Sample : VX0419WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK625

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035183.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.325	34	39	42	rBV	8158	16411	0.99%	0.136%
2	1.368	43	46	57	rVB	195307	216310	12.99%	1.789%
3	1.672	92	96	110	rBV	139103	187745	11.27%	1.552%
4	2.306	194	200	211	rBV	371619	576806	34.64%	4.769%
5	2.520	229	235	241	rVB3	1592	2495	0.15%	0.021%
6	2.562	241	242	244	rBV2	417	245	0.01%	0.002%
7	2.629	251	253	255	rBV2	343	326	0.02%	0.003%
8	2.788	273	279	288	rVV	4521	8032	0.48%	0.066%
9	2.959	305	307	308	rVB	390	258	0.02%	0.002%
10	3.007	311	315	316	rBV2	161	222	0.01%	0.002%
11	3.081	323	327	328	rBV3	560	528	0.03%	0.004%
12	3.349	370	371	374	rVB	421	290	0.02%	0.002%
13	3.416	381	382	386	rVB2	406	287	0.02%	0.002%
14	3.666	421	423	428	rVV2	198	266	0.02%	0.002%
15	3.721	430	432	433	rBV2	318	229	0.01%	0.002%
16	3.794	440	444	447	rBV3	243	406	0.02%	0.003%
17	3.995	474	477	478	rBV	318	381	0.02%	0.003%
18	4.044	483	485	487	rVV	417	362	0.02%	0.003%
19	4.074	487	490	492	rVB3	330	350	0.02%	0.003%
20	4.105	492	495	496	rBV2	258	327	0.02%	0.003%
21	4.148	500	502	505	rVB	237	298	0.02%	0.002%
22	4.465	545	554	579	rBV	100333	330665	19.86%	2.734%
23	4.794	607	608	612	rBV3	328	327	0.02%	0.003%
24	5.056	639	651	670	rBV	203888	627473	37.68%	5.188%
25	5.288	688	689	692	rVV2	262	280	0.02%	0.002%
26	5.330	694	696	699	rVB2	255	311	0.02%	0.003%
27	5.397	699	707	714	rBV5	1131	2887	0.17%	0.024%
28	5.562	727	734	741	rVV3	1938	4975	0.30%	0.041%
29	5.970	787	801	820	rBV2	558761	1665377	100.00%	13.770%
30	6.172	833	834	836	rVB2	375	230	0.01%	0.002%
31	6.379	867	868	872	rVB3	291	341	0.02%	0.003%
32	6.428	875	876	879	rVB2	322	286	0.02%	0.002%
33	6.464	879	882	883	rBV2	297	366	0.02%	0.003%
34	6.647	909	912	914	rBV2	272	345	0.02%	0.003%
35	6.763	921	931	948	rBV	425591	1029989	61.85%	8.516%
36	7.001	966	970	971	rBV	364	346	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035183.D
 Acq On : 19 Apr 2023 20:52
 Operator : JC/MD
 Sample : VX0419WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK625

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	7.049	977	978	981	rVB2	501	356	0.02%	0.003%
38	7.110	981	988	998	rBV7	3443	9307	0.56%	0.077%
39	7.305	1011	1020	1038	rBV	335691	752211	45.17%	6.219%
40	7.464	1044	1046	1047	rBV	487	358	0.02%	0.003%
41	7.476	1047	1048	1051	rVV3	730	705	0.04%	0.006%
42	7.568	1061	1063	1065	rBV2	264	229	0.01%	0.002%
43	7.738	1089	1091	1096	rBV2	231	260	0.02%	0.002%
44	7.940	1122	1124	1125	rBV	670	523	0.03%	0.004%
45	8.049	1140	1142	1144	rVB2	301	282	0.02%	0.002%
46	8.281	1178	1180	1181	rBV2	324	232	0.01%	0.002%
47	8.324	1181	1187	1199	rBV	197695	322957	19.39%	2.670%
48	8.647	1233	1240	1260	rBV	874576	1361356	81.74%	11.256%
49	8.952	1284	1290	1302	rBV	135539	204980	12.31%	1.695%
50	9.122	1316	1318	1321	rBV2	421	528	0.03%	0.004%
51	9.275	1339	1343	1348	rVB3	1058	1382	0.08%	0.011%
52	9.384	1356	1361	1374	rBV	499841	697621	41.89%	5.768%
53	9.714	1413	1415	1418	rVV3	276	403	0.02%	0.003%
54	9.768	1422	1424	1426	rVV2	333	240	0.01%	0.002%
55	10.012	1461	1464	1465	rBV2	325	315	0.02%	0.003%
56	10.055	1465	1471	1483	rBV	829608	1155265	69.37%	9.552%
57	10.299	1509	1511	1519	rVB4	919	1619	0.10%	0.013%
58	10.457	1536	1537	1539	rBV	245	214	0.01%	0.002%
59	10.640	1565	1567	1569	rBV2	705	618	0.04%	0.005%
60	10.817	1593	1596	1598	rBV2	356	295	0.02%	0.002%
61	10.860	1600	1603	1604	rBV2	245	223	0.01%	0.002%
62	10.963	1617	1620	1625	rVB2	838	992	0.06%	0.008%
63	11.049	1632	1634	1636	rVB2	293	256	0.02%	0.002%
64	11.189	1652	1657	1672	rBV	555715	724623	43.51%	5.991%
65	11.414	1692	1694	1695	rBV	598	318	0.02%	0.003%
66	11.451	1697	1700	1704	rVB2	909	1233	0.07%	0.010%
67	11.634	1727	1730	1732	rBV2	297	324	0.02%	0.003%
68	11.689	1735	1739	1741	rBV2	214	251	0.02%	0.002%
69	11.707	1741	1742	1747	rVV3	567	623	0.04%	0.005%
70	11.756	1747	1750	1755	rVB3	1225	1530	0.09%	0.013%
71	11.805	1755	1758	1761	rVB2	345	498	0.03%	0.004%
72	11.835	1761	1763	1765	rBV	211	264	0.02%	0.002%
73	11.969	1780	1785	1788	rBV3	1846	2468	0.15%	0.020%
74	12.024	1788	1794	1810	rVV	793979	1045598	62.78%	8.645%
75	12.317	1837	1842	1859	rVB	845632	1098754	65.98%	9.085%
76	12.512	1872	1874	1875	rBV	316	215	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035183.D
 Acq On : 19 Apr 2023 20:52
 Operator : JC/MD
 Sample : VX0419WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK625

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	12.579	1882	1885	1889	rBV3	391	612	0.04%	0.005%
78	12.689	1901	1903	1905	rVB2	296	226	0.01%	0.002%
79	12.707	1905	1906	1909	rBV2	276	249	0.01%	0.002%
80	12.762	1911	1915	1920	rVV2	624	885	0.05%	0.007%
81	12.841	1925	1928	1930	rBV2	274	348	0.02%	0.003%
82	13.079	1964	1967	1968	rBV2	296	345	0.02%	0.003%
83	13.115	1969	1973	1977	rVV5	3718	5338	0.32%	0.044%
84	13.176	1980	1983	1985	rBV2	269	380	0.02%	0.003%
85	13.304	2003	2004	2008	rVV	253	245	0.01%	0.002%
86	13.335	2008	2009	2012	rVB2	343	230	0.01%	0.002%
87	13.365	2012	2014	2015	rBV	290	225	0.01%	0.002%
88	13.390	2017	2018	2021	rVB2	401	299	0.02%	0.002%
89	13.591	2047	2051	2058	rVB2	5794	7799	0.47%	0.064%
90	13.786	2079	2083	2087	rBV2	1265	1616	0.10%	0.013%
91	13.926	2104	2106	2109	rBV2	294	318	0.02%	0.003%
92	13.963	2109	2112	2118	rVB4	3444	4181	0.25%	0.035%
93	14.048	2125	2126	2128	rBV	402	244	0.01%	0.002%
94	14.127	2136	2139	2141	rBV2	846	900	0.05%	0.007%
95	14.292	2165	2166	2170	rBV2	487	543	0.03%	0.004%
96	14.426	2187	2188	2192	rBV2	332	334	0.02%	0.003%
97	14.566	2209	2211	2213	rBV2	255	242	0.01%	0.002%
98	14.981	2277	2279	2280	rBV2	598	500	0.03%	0.004%
99	15.786	2409	2411	2413	rBV2	902	732	0.04%	0.006%
100	16.755	2568	2570	2571	rBV	756	408	0.02%	0.003%




Sum of corrected areas: 12094397

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035183.D
Acq On : 19 Apr 2023 20:52
Operator : JC/MD
Sample : VX0419WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK625

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

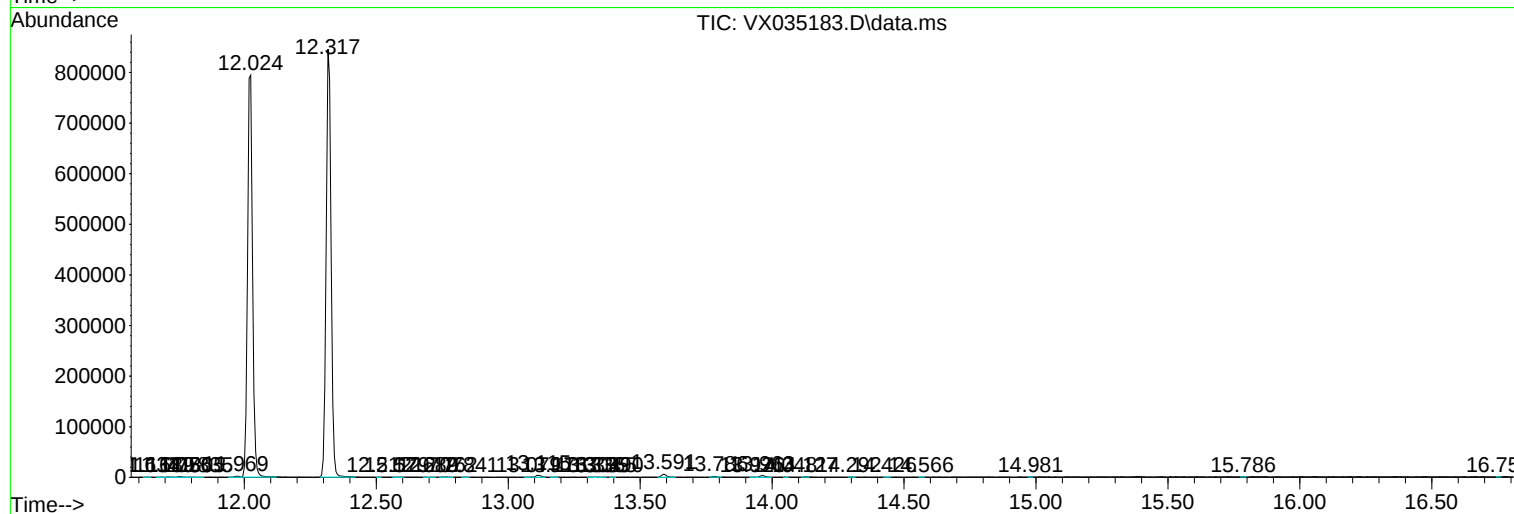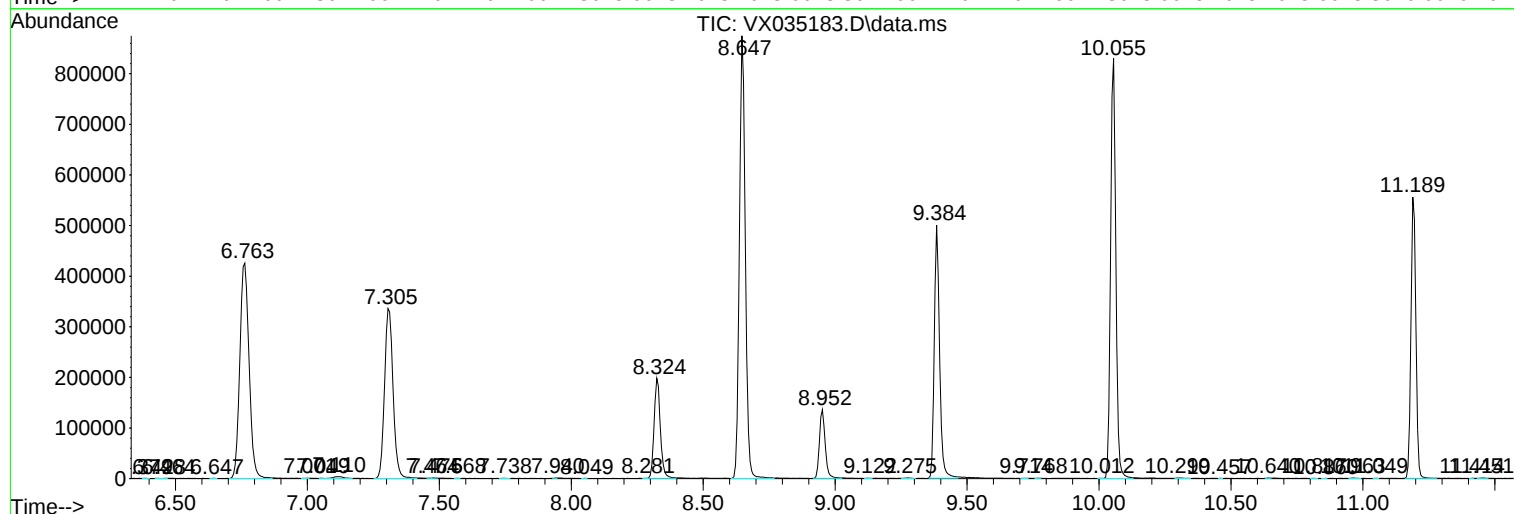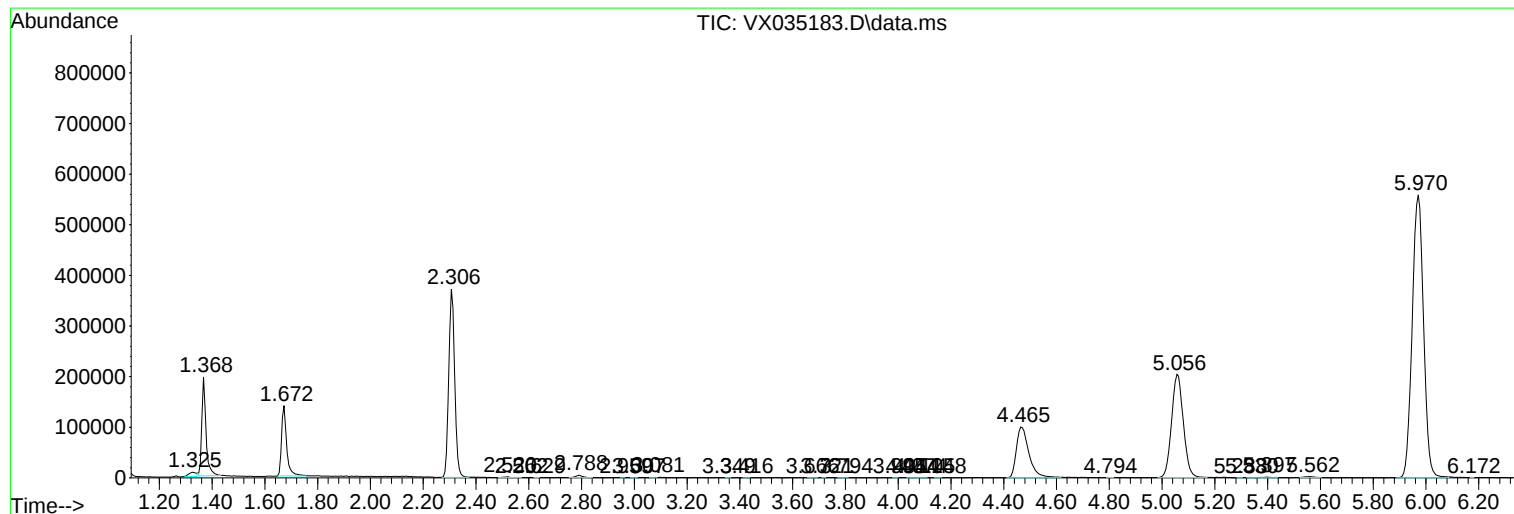

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035183.D
Acq On : 19 Apr 2023 20:52
Operator : JC/MD
Sample : VX0419WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK625

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035183.D
Acq On : 19 Apr 2023 20:52
Operator : JC/MD
Sample : VX0419WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK625

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc