

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035185.D
 Acq On : 19 Apr 2023 21:39
 Operator : JC/MD
 Sample : 02333-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M

Title : VOC Analysis

Signal : TIC: VX035185.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	31	rBV2	2691	2988	0.17%	0.023%
2	1.313	31	37	42	rVV	15092	38671	2.20%	0.297%
3	1.367	43	46	60	rVB	192428	217688	12.39%	1.669%
4	1.672	92	96	113	rVB	148552	194230	11.05%	1.489%
5	2.306	194	200	211	rBV	363194	563648	32.07%	4.322%
6	2.514	231	234	236	rBV2	758	847	0.05%	0.006%
7	2.617	250	251	252	rBV	370	211	0.01%	0.002%
8	2.666	256	259	261	rBV2	355	414	0.02%	0.003%
9	2.690	261	263	264	rBV2	331	280	0.02%	0.002%
10	2.873	291	293	298	rBV3	220	365	0.02%	0.003%
11	2.922	298	301	302	rBV2	257	282	0.02%	0.002%
12	2.946	302	305	307	rVB2	435	514	0.03%	0.004%
13	3.026	316	318	321	rBV2	418	581	0.03%	0.004%
14	3.081	325	327	329	rBV2	301	321	0.02%	0.002%
15	3.135	334	336	339	rBV2	347	399	0.02%	0.003%
16	3.239	350	353	355	rBV2	335	305	0.02%	0.002%
17	3.270	357	358	361	rBV2	286	233	0.01%	0.002%
18	3.855	452	454	458	rVB3	179	202	0.01%	0.002%
19	4.105	492	495	500	rVB2	234	368	0.02%	0.003%
20	4.154	500	503	506	rBV2	245	319	0.02%	0.002%
21	4.397	539	543	544	rVB2	270	291	0.02%	0.002%
22	4.464	546	554	573	rBV	116318	372630	21.20%	2.857%
23	4.702	592	593	594	rBV	567	228	0.01%	0.002%
24	4.891	622	624	627	rVB2	368	374	0.02%	0.003%
25	5.056	638	651	672	rBV	231684	713696	40.61%	5.472%
26	5.312	692	693	696	rVB2	298	200	0.01%	0.002%
27	5.367	700	702	703	rBV	417	308	0.02%	0.002%
28	5.397	703	707	717	rVB4	942	2297	0.13%	0.018%
29	5.470	718	719	725	rVB2	137	219	0.01%	0.002%
30	5.519	725	727	728	rBV	381	327	0.02%	0.003%
31	5.550	728	732	742	rVB4	2067	4982	0.28%	0.038%
32	5.720	758	760	762	rBV	265	192	0.01%	0.001%
33	5.787	769	771	774	rVB2	239	239	0.01%	0.002%
34	5.970	787	801	829	rBV2	596888	1757517	100.00%	13.475%
35	6.226	841	843	845	rBV2	226	206	0.01%	0.002%
36	6.403	868	872	873	rVB2	176	192	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035185.D
 Acq On : 19 Apr 2023 21:39
 Operator : JC/MD
 Sample : 02333-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	6.440	873	878	879	rBV2	435	378	0.02%	0.003%
38	6.458	879	881	882	rBV	255	187	0.01%	0.001%
39	6.610	904	906	907	rBV	273	216	0.01%	0.002%
40	6.671	915	916	920	rBV	258	276	0.02%	0.002%
41	6.763	920	931	946	rBV	466544	1126846	64.12%	8.640%
42	7.116	981	989	997	rVB5	3643	9095	0.52%	0.070%
43	7.190	997	1001	1002	rVB2	335	339	0.02%	0.003%
44	7.208	1002	1004	1007	rBV	248	317	0.02%	0.002%
45	7.312	1012	1021	1035	rBV	356234	802330	45.65%	6.152%
46	7.738	1089	1091	1094	rVB3	242	245	0.01%	0.002%
47	7.848	1106	1109	1114	rVB2	840	1308	0.07%	0.010%
48	7.903	1114	1118	1120	rBV3	411	682	0.04%	0.005%
49	7.946	1120	1125	1129	rBV4	1407	2812	0.16%	0.022%
50	8.031	1136	1139	1142	rVB3	210	277	0.02%	0.002%
51	8.183	1160	1164	1167	rVB2	330	344	0.02%	0.003%
52	8.324	1180	1187	1200	rBV	214290	351289	19.99%	2.693%
53	8.494	1211	1215	1220	rBV6	1186	2091	0.12%	0.016%
54	8.647	1233	1240	1260	rBV	868620	1399157	79.61%	10.728%
55	8.951	1284	1290	1301	rBV	146055	220149	12.53%	1.688%
56	9.275	1339	1343	1347	rBV2	1585	2130	0.12%	0.016%
57	9.384	1356	1361	1374	rBV	562840	805744	45.85%	6.178%
58	9.829	1430	1434	1438	rBV2	434	742	0.04%	0.006%
59	9.909	1446	1447	1451	rVB2	216	199	0.01%	0.002%
60	9.945	1451	1453	1456	rBV3	193	285	0.02%	0.002%
61	10.055	1465	1471	1489	rBV	938742	1268885	72.20%	9.729%
62	10.232	1498	1500	1501	rVB2	448	242	0.01%	0.002%
63	10.384	1524	1525	1528	rVB	332	208	0.01%	0.002%
64	10.738	1581	1583	1585	rVB	300	199	0.01%	0.002%
65	10.963	1618	1620	1625	rBV2	309	403	0.02%	0.003%
66	11.091	1639	1641	1644	rBV2	257	287	0.02%	0.002%
67	11.189	1652	1657	1669	rBV	597640	804634	45.78%	6.169%
68	11.451	1697	1700	1703	rBV2	443	746	0.04%	0.006%
69	11.536	1713	1714	1717	rBV2	202	211	0.01%	0.002%
70	11.603	1723	1725	1728	rBV2	271	279	0.02%	0.002%
71	11.707	1739	1742	1744	rVB3	483	442	0.03%	0.003%
72	11.768	1748	1752	1756	rVB4	783	1462	0.08%	0.011%
73	11.811	1756	1759	1762	rBV3	565	816	0.05%	0.006%
74	11.878	1767	1770	1771	rBV	402	387	0.02%	0.003%
75	11.975	1781	1786	1788	rBV2	1044	1450	0.08%	0.011%
76	12.024	1788	1794	1803	rBV	885387	1146464	65.23%	8.790%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035185.D
 Acq On : 19 Apr 2023 21:39
 Operator : JC/MD
 Sample : 02333-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	12.219	1821	1826	1835	rBV2	6835	11662	0.66%	0.089%
78	12.317	1837	1842	1853	rVV	909333	1181701	67.24%	9.060%
79	12.682	1898	1902	1904	rBV3	270	386	0.02%	0.003%
80	12.768	1911	1916	1918	rBV3	532	648	0.04%	0.005%
81	12.817	1922	1924	1925	rBV	619	339	0.02%	0.003%
82	12.859	1925	1931	1935	rVB4	3372	4790	0.27%	0.037%
83	12.890	1935	1936	1937	rBV	595	219	0.01%	0.002%
84	12.914	1937	1940	1941	rBV	424	253	0.01%	0.002%
85	12.939	1942	1944	1945	rVB	360	193	0.01%	0.001%
86	12.957	1945	1947	1948	rBV	493	339	0.02%	0.003%
87	13.060	1962	1964	1967	rBV2	313	315	0.02%	0.002%
88	13.115	1970	1973	1978	rBV2	678	745	0.04%	0.006%
89	13.274	1997	1999	2001	rBV2	270	266	0.02%	0.002%
90	13.347	2009	2011	2013	rBV2	298	351	0.02%	0.003%
91	13.384	2015	2017	2018	rVV2	321	207	0.01%	0.002%
92	13.420	2022	2023	2025	rVB	394	216	0.01%	0.002%
93	13.591	2047	2051	2056	rBV2	3362	3999	0.23%	0.031%
94	13.743	2074	2076	2077	rVB2	368	206	0.01%	0.002%
95	13.877	2092	2098	2102	rVB4	550	1236	0.07%	0.009%
96	13.963	2107	2112	2115	rBV3	862	1379	0.08%	0.011%
97	14.310	2167	2169	2172	rVB2	357	278	0.02%	0.002%
98	14.572	2211	2212	2215	rBV2	461	401	0.02%	0.003%
99	14.804	2247	2250	2254	rVB4	536	675	0.04%	0.005%
100	15.005	2282	2283	2284	rBV	482	281	0.02%	0.002%




Sum of corrected areas: 13042402

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035185.D
Acq On : 19 Apr 2023 21:39
Operator : JC/MD
Sample : 02333-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMG1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

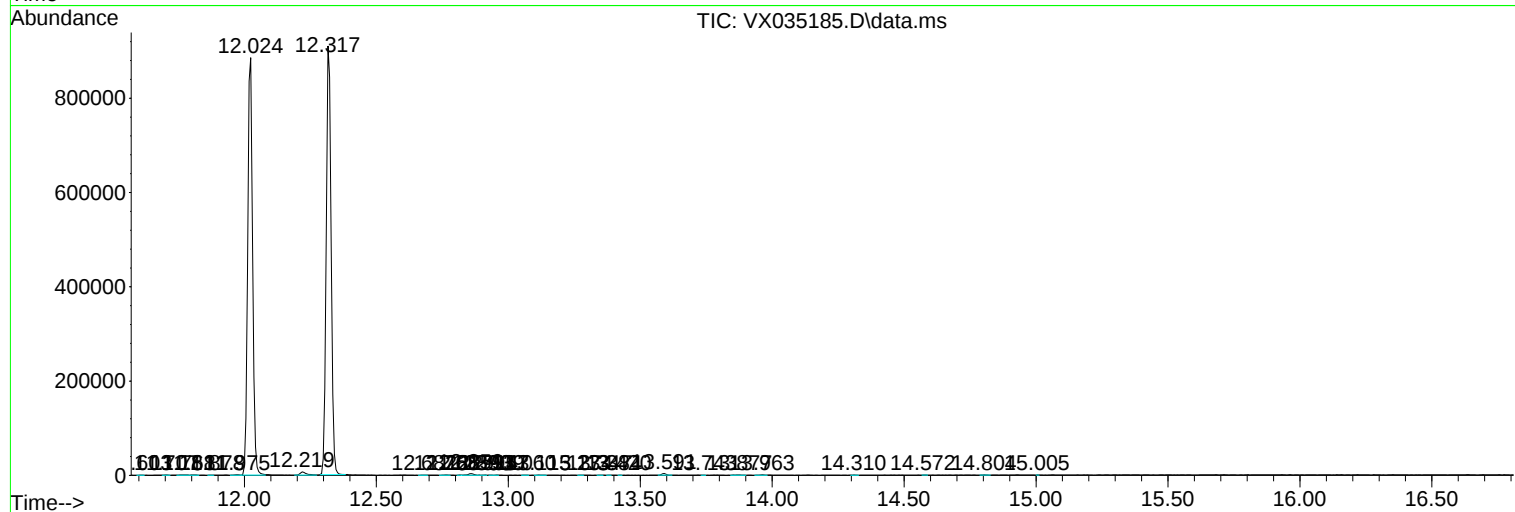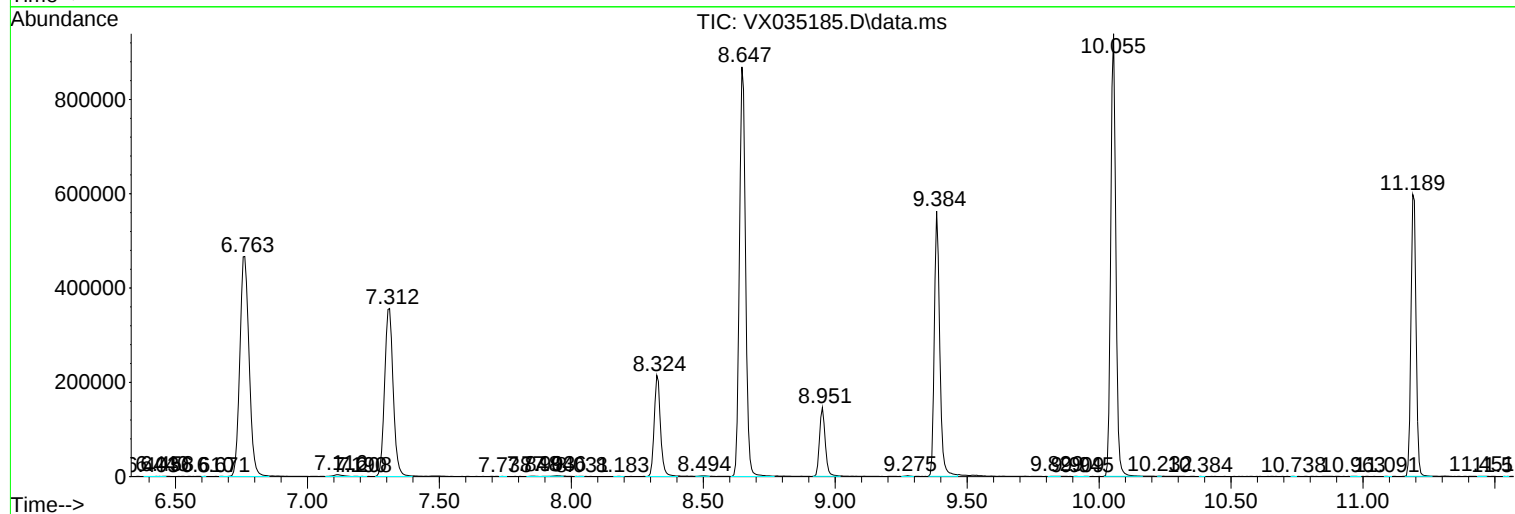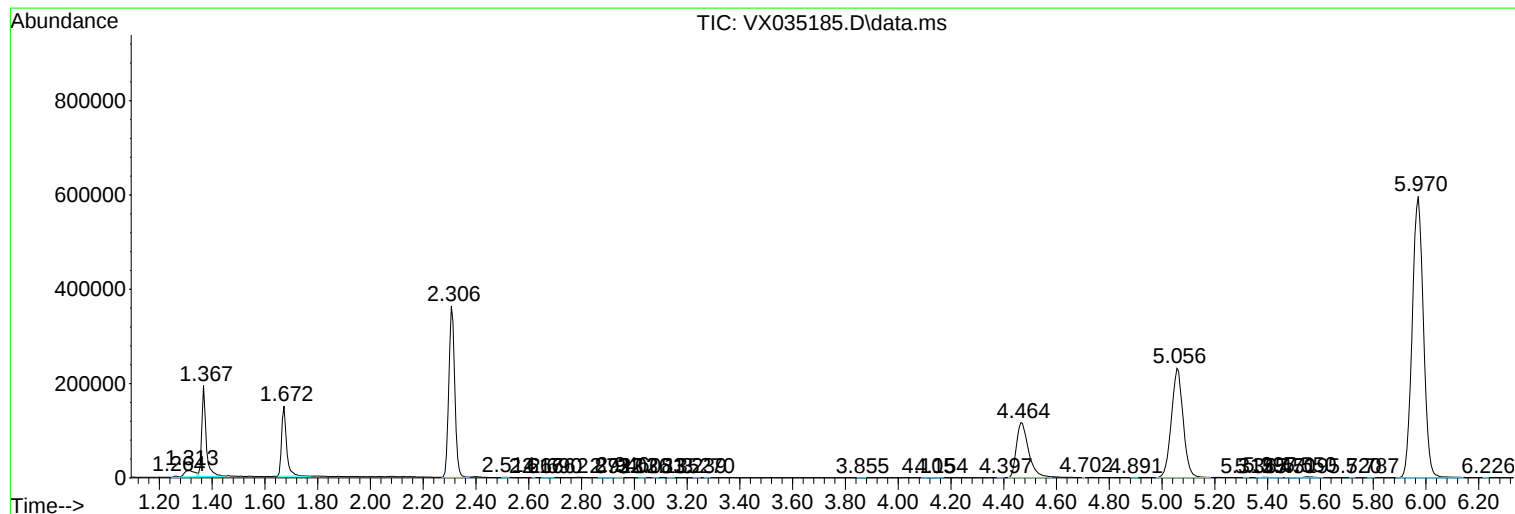

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035185.D
Acq On : 19 Apr 2023 21:39
Operator : JC/MD
Sample : 02333-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0MG1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035185.D
Acq On : 19 Apr 2023 21:39
Operator : JC/MD
Sample : 02333-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0MG1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc