

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035187.D
 Acq On : 19 Apr 2023 22:25
 Operator : JC/MD
 Sample : 02333-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035187.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	31	rBV3	2250	2222	0.13%	0.017%
2	1.313	31	37	42	rBV	11363	28912	1.66%	0.225%
3	1.368	42	46	59	rVB	195161	217388	12.49%	1.693%
4	1.672	91	96	109	rBV	143605	190461	10.94%	1.483%
5	2.307	194	200	211	rBV	357507	553236	31.78%	4.307%
6	2.660	257	258	261	rVB	459	312	0.02%	0.002%
7	2.691	261	263	264	rBV	274	157	0.01%	0.001%
8	2.916	298	300	301	rBV	306	215	0.01%	0.002%
9	2.941	302	304	305	rVB	438	236	0.01%	0.002%
10	3.008	312	315	319	rBV3	209	295	0.02%	0.002%
11	3.197	343	346	347	rBV	315	323	0.02%	0.003%
12	3.258	354	356	357	rVB2	220	142	0.01%	0.001%
13	3.276	357	359	361	rBV2	330	386	0.02%	0.003%
14	3.312	363	365	367	rVV	203	144	0.01%	0.001%
15	3.349	370	371	375	rVB2	324	287	0.02%	0.002%
16	3.410	378	381	383	rBV	182	172	0.01%	0.001%
17	3.568	406	407	409	rBV	211	157	0.01%	0.001%
18	3.678	423	425	426	rVB	394	182	0.01%	0.001%
19	3.697	426	428	429	rBV	337	151	0.01%	0.001%
20	3.764	437	439	441	rBV2	301	228	0.01%	0.002%
21	3.843	450	452	455	rVB	181	223	0.01%	0.002%
22	3.886	458	459	461	rVB	265	163	0.01%	0.001%
23	3.971	469	473	474	rVV2	204	161	0.01%	0.001%
24	4.007	474	479	481	rVV	213	330	0.02%	0.003%
25	4.056	484	487	489	rBV2	245	189	0.01%	0.001%
26	4.178	505	507	512	rBV2	205	245	0.01%	0.002%
27	4.257	515	520	522	rBV2	266	495	0.03%	0.004%
28	4.349	533	535	537	rBV2	286	276	0.02%	0.002%
29	4.465	545	554	575	rBV	116872	360042	20.68%	2.803%
30	5.056	639	651	674	rBV	216054	668200	38.39%	5.203%
31	5.355	698	700	701	rBV	360	221	0.01%	0.002%
32	5.495	722	723	724	rVB	393	144	0.01%	0.001%
33	5.556	724	733	743	rBV4	2448	6751	0.39%	0.053%
34	5.647	747	748	750	rBV2	139	141	0.01%	0.001%
35	5.836	776	779	780	rBV	190	199	0.01%	0.002%
36	5.971	787	801	823	rBV2	584099	1740730	100.00%	13.553%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035187.D
 Acq On : 19 Apr 2023 22:25
 Operator : JC/MD
 Sample : 02333-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	6.147	829	830	831	rVB	513	188	0.01%	0.001%
38	6.458	876	881	884	rBV2	409	526	0.03%	0.004%
39	6.519	888	891	892	rBV2	251	202	0.01%	0.002%
40	6.531	892	893	896	rBV2	328	401	0.02%	0.003%
41	6.763	921	931	948	rBV	482751	1154723	66.34%	8.991%
42	7.068	979	981	983	rBV2	261	213	0.01%	0.002%
43	7.111	983	988	997	rVV6	3288	7878	0.45%	0.061%
44	7.226	1003	1007	1008	rBV	312	334	0.02%	0.003%
45	7.306	1011	1020	1036	rBV	357146	789612	45.36%	6.148%
46	7.574	1061	1064	1067	rBV2	277	441	0.03%	0.003%
47	7.610	1069	1070	1071	rVV	267	151	0.01%	0.001%
48	7.647	1074	1076	1079	rVV2	257	254	0.01%	0.002%
49	7.696	1082	1084	1085	rBV2	224	168	0.01%	0.001%
50	7.842	1107	1108	1110	rBV2	373	209	0.01%	0.002%
51	7.940	1120	1124	1130	rBV3	1558	2779	0.16%	0.022%
52	8.257	1171	1176	1181	rBV2	247	476	0.03%	0.004%
53	8.324	1181	1187	1207	rBV	207226	344933	19.82%	2.686%
54	8.647	1234	1240	1254	rBV	874568	1373116	78.88%	10.691%
55	8.952	1284	1290	1302	rBV	144260	215513	12.38%	1.678%
56	9.232	1335	1336	1339	rVB	252	168	0.01%	0.001%
57	9.275	1339	1343	1348	rVB3	1230	2034	0.12%	0.016%
58	9.385	1356	1361	1383	rBV	542376	779317	44.77%	6.068%
59	9.647	1402	1404	1405	rVB2	501	243	0.01%	0.002%
60	9.860	1437	1439	1440	rBV	327	150	0.01%	0.001%
61	10.055	1465	1471	1482	rBV	923907	1280217	73.54%	9.968%
62	10.226	1497	1499	1501	rVB2	317	151	0.01%	0.001%
63	10.311	1510	1513	1515	rBV2	404	477	0.03%	0.004%
64	10.372	1519	1523	1526	rBV2	377	387	0.02%	0.003%
65	10.421	1530	1531	1534	rVB2	236	159	0.01%	0.001%
66	10.518	1545	1547	1548	rVV	299	176	0.01%	0.001%
67	10.549	1550	1552	1558	rVB2	197	320	0.02%	0.002%
68	10.683	1570	1574	1578	rBV3	242	272	0.02%	0.002%
69	10.927	1613	1614	1616	rBV	345	192	0.01%	0.001%
70	10.951	1616	1618	1619	rBV2	307	227	0.01%	0.002%
71	11.146	1646	1650	1652	rBV2	282	294	0.02%	0.002%
72	11.189	1652	1657	1670	rBV	621030	794624	45.65%	6.187%
73	11.311	1675	1677	1682	rVB2	1073	1593	0.09%	0.012%
74	11.415	1693	1694	1697	rBV2	291	178	0.01%	0.001%
75	11.445	1697	1699	1701	rBV	198	165	0.01%	0.001%
76	11.518	1709	1711	1713	rBV	214	216	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035187.D
 Acq On : 19 Apr 2023 22:25
 Operator : JC/MD
 Sample : 02333-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041823WMA.M
 Title : VOC Analysis

77	11.537	1713	1714	1721	rVB2	375	349	0.02%	0.003%
78	11.659	1732	1734	1736	rBV2	260	278	0.02%	0.002%
79	11.713	1740	1743	1748	rVB2	654	911	0.05%	0.007%
80	11.933	1777	1779	1782	rVV	297	352	0.02%	0.003%
81	11.969	1783	1785	1788	rVV	846	666	0.04%	0.005%
82	12.018	1788	1793	1808	rVV	870904	1153901	66.29%	8.984%
83	12.219	1823	1826	1831	rVB4	1794	2406	0.14%	0.019%
84	12.317	1837	1842	1853	rBV	892370	1148041	65.95%	8.938%
85	12.475	1867	1868	1872	rVV2	546	434	0.02%	0.003%
86	12.506	1872	1873	1876	rVB2	579	396	0.02%	0.003%
87	12.707	1904	1906	1909	rVB	253	173	0.01%	0.001%
88	12.768	1911	1916	1921	rBV4	619	1082	0.06%	0.008%
89	12.835	1925	1927	1928	rVB	241	153	0.01%	0.001%
90	12.975	1949	1950	1955	rBV2	241	422	0.02%	0.003%
91	13.134	1974	1976	1978	rBV2	257	282	0.02%	0.002%
92	13.213	1987	1989	1993	rBV2	244	312	0.02%	0.002%
93	13.414	2020	2022	2024	rVB2	296	155	0.01%	0.001%
94	13.591	2048	2051	2058	rVB3	2420	2935	0.17%	0.023%
95	13.841	2091	2092	2095	rBV2	334	244	0.01%	0.002%
96	13.914	2101	2104	2107	rBV3	326	487	0.03%	0.004%
97	14.000	2115	2118	2123	rBV3	462	785	0.05%	0.006%
98	14.268	2160	2162	2163	rBV2	368	224	0.01%	0.002%
99	15.127	2302	2303	2306	rBV2	549	499	0.03%	0.004%
100	16.426	2514	2516	2518	rBV	650	520	0.03%	0.004%


Sum of corrected areas: 12843800

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035187.D
Acq On : 19 Apr 2023 22:25
Operator : JC/MD
Sample : 02333-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

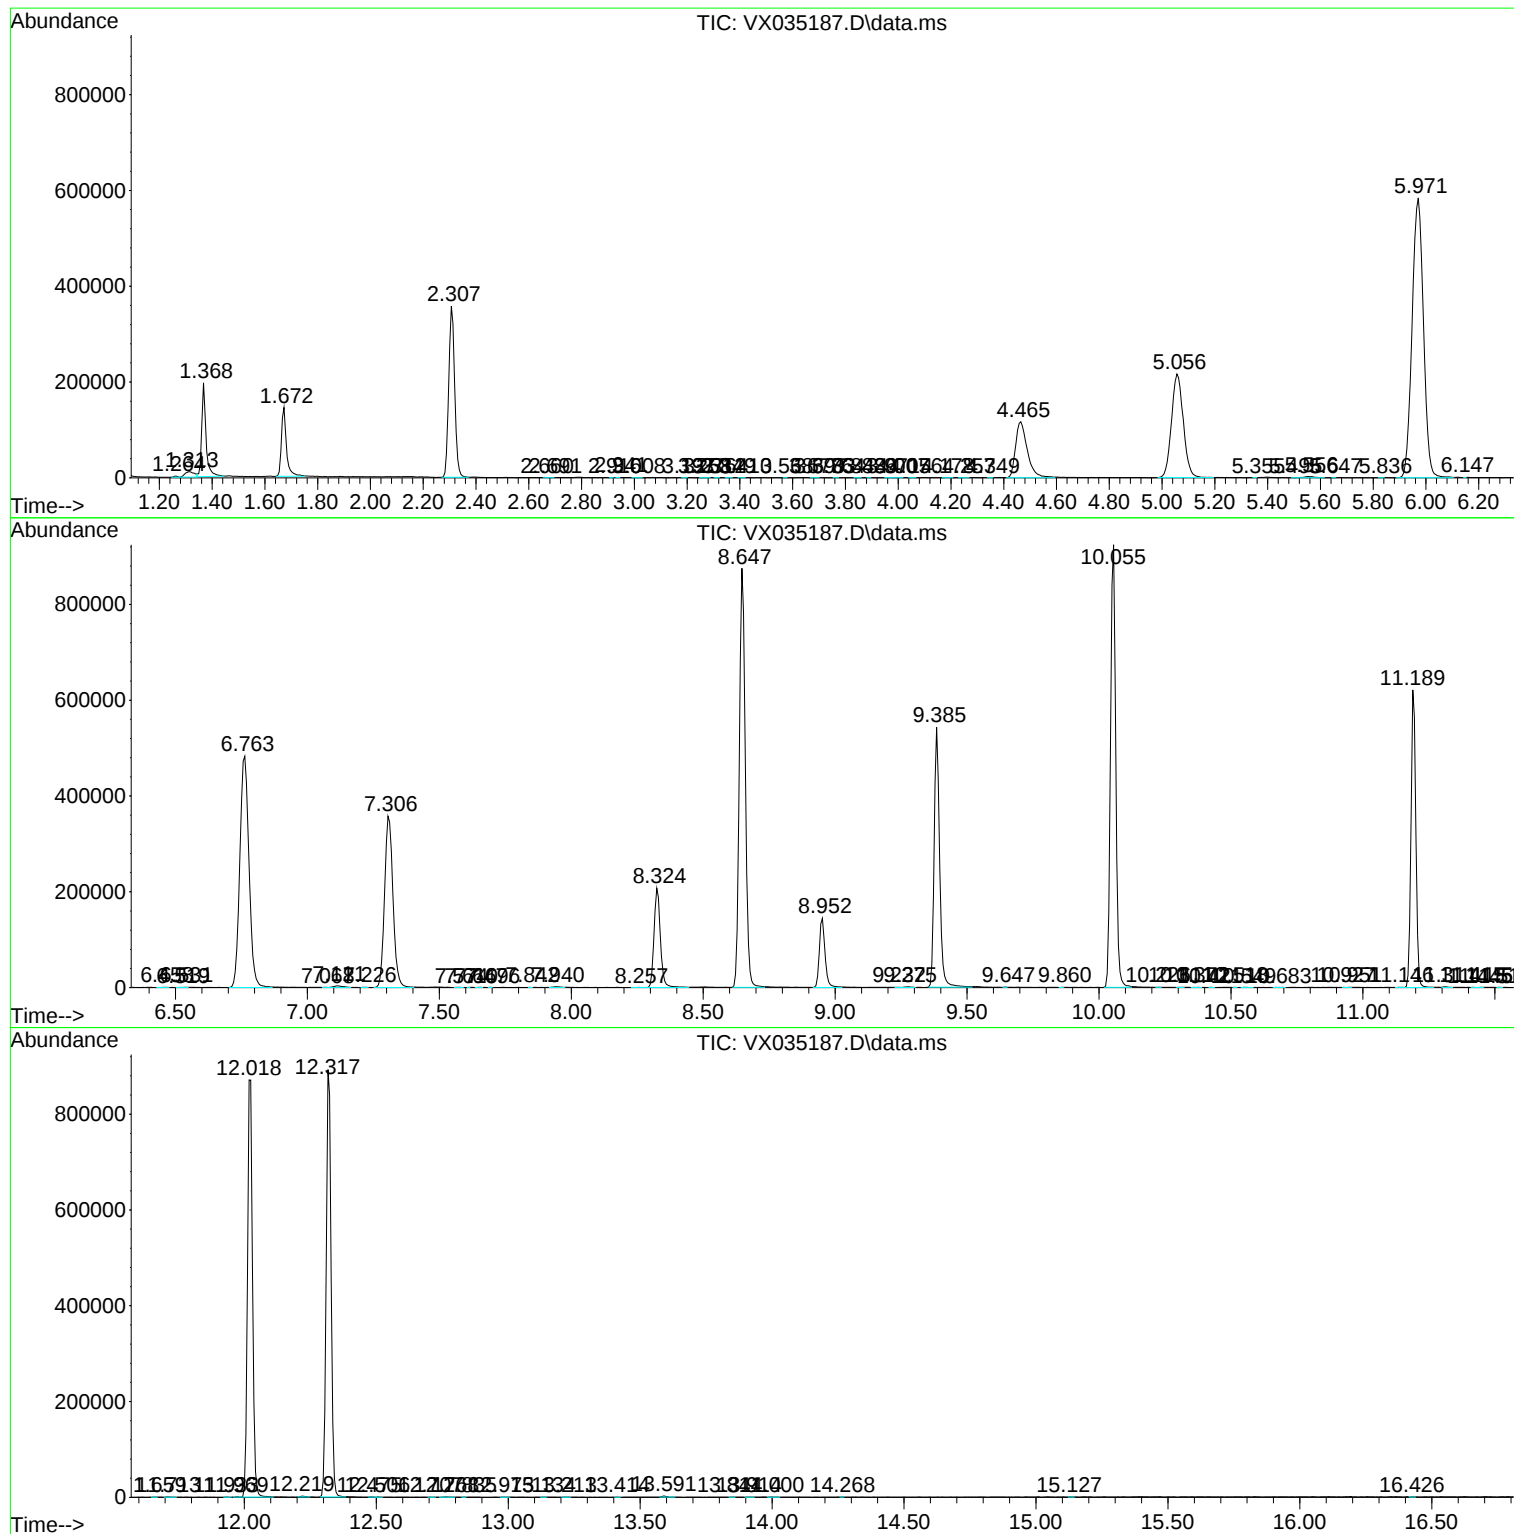

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035187.D
Acq On : 19 Apr 2023 22:25
Operator : JC/MD
Sample : 02333-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0MG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035187.D
Acq On : 19 Apr 2023 22:25
Operator : JC/MD
Sample : 02333-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0MG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------