

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035188.D
 Acq On : 19 Apr 2023 22:48
 Operator : JC/MD
 Sample : 02333-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035188.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	31	rBV2	2727	2393	0.14%	0.019%
2	1.313	32	37	42	rVV	8518	22334	1.29%	0.174%
3	1.368	42	46	60	rVB	186022	211778	12.21%	1.648%
4	1.672	91	96	110	rBV	142003	190595	10.98%	1.483%
5	2.306	194	200	210	rBV	352145	550065	31.70%	4.281%
6	2.776	276	277	278	rBV	540	327	0.02%	0.003%
7	2.965	304	308	310	rVB3	340	337	0.02%	0.003%
8	2.995	310	313	315	rBV2	209	222	0.01%	0.002%
9	3.014	315	316	320	rBV2	253	286	0.02%	0.002%
10	3.318	365	366	367	rBV	480	198	0.01%	0.002%
11	3.513	396	398	400	rBV2	398	321	0.02%	0.002%
12	3.550	402	404	405	rVB2	432	225	0.01%	0.002%
13	3.574	405	408	409	rBV	298	202	0.01%	0.002%
14	3.733	432	434	435	rBV	283	204	0.01%	0.002%
15	3.873	452	457	460	rBV2	260	304	0.02%	0.002%
16	3.995	474	477	480	rVV2	283	339	0.02%	0.003%
17	4.074	488	490	491	rVB2	347	218	0.01%	0.002%
18	4.117	494	497	500	rBV2	221	380	0.02%	0.003%
19	4.178	504	507	508	rBV2	235	206	0.01%	0.002%
20	4.465	545	554	575	rBV	116512	352609	20.32%	2.744%
21	4.782	604	606	611	rVB3	350	346	0.02%	0.003%
22	4.934	629	631	633	rBV2	283	204	0.01%	0.002%
23	5.056	639	651	671	rBV	215194	665433	38.35%	5.179%
24	5.300	688	691	693	rBV2	304	324	0.02%	0.003%
25	5.336	695	697	700	rVB2	293	201	0.01%	0.002%
26	5.452	714	716	718	rVB2	425	341	0.02%	0.003%
27	5.562	726	734	742	rVV4	2747	6754	0.39%	0.053%
28	5.885	785	787	789	rBV2	202	224	0.01%	0.002%
29	5.970	789	801	819	rBV2	576261	1735131	100.00%	13.504%
30	6.202	838	839	841	rBV	337	220	0.01%	0.002%
31	6.300	853	855	856	rBV	330	235	0.01%	0.002%
32	6.763	921	931	948	rBV	466166	1124281	64.80%	8.750%
33	7.062	977	980	981	rBV2	206	207	0.01%	0.002%
34	7.116	983	989	996	rVV5	3565	8047	0.46%	0.063%
35	7.305	1011	1020	1039	rBV	355919	786216	45.31%	6.119%
36	7.488	1046	1050	1055	rBV4	785	1481	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035188.D
 Acq On : 19 Apr 2023 22:48
 Operator : JC/MD
 Sample : 02333-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	7.574	1062	1064	1066	rVB2	376	213	0.01%	0.002%
38	7.610	1066	1070	1072	rVB	205	217	0.01%	0.002%
39	7.641	1072	1075	1076	rBV2	347	315	0.02%	0.002%
40	7.769	1095	1096	1099	rBV2	262	260	0.01%	0.002%
41	7.842	1106	1108	1111	rBV2	202	225	0.01%	0.002%
42	7.940	1119	1124	1129	rBV4	1378	2961	0.17%	0.023%
43	8.074	1144	1146	1151	rVB	270	312	0.02%	0.002%
44	8.129	1151	1155	1156	rBV2	164	198	0.01%	0.002%
45	8.324	1181	1187	1203	rBV	203275	339464	19.56%	2.642%
46	8.494	1211	1215	1223	rVB5	859	1814	0.10%	0.014%
47	8.586	1229	1230	1232	rBV	282	221	0.01%	0.002%
48	8.647	1234	1240	1250	rBV	872347	1372242	79.09%	10.680%
49	8.952	1284	1290	1302	rBV	141829	215694	12.43%	1.679%
50	9.147	1321	1322	1324	rBV	314	202	0.01%	0.002%
51	9.171	1324	1326	1327	rBV	396	198	0.01%	0.002%
52	9.275	1340	1343	1348	rVB2	1050	1604	0.09%	0.012%
53	9.384	1356	1361	1375	rBV	541318	767352	44.22%	5.972%
54	9.829	1433	1434	1437	rBV2	246	263	0.02%	0.002%
55	9.884	1440	1443	1445	rVB2	393	480	0.03%	0.004%
56	9.903	1445	1446	1449	rBV2	423	423	0.02%	0.003%
57	9.951	1452	1454	1456	rVV	328	211	0.01%	0.002%
58	10.055	1465	1471	1482	rBV	917091	1269493	73.16%	9.880%
59	10.439	1532	1534	1536	rVB2	321	290	0.02%	0.002%
60	10.512	1543	1546	1547	rBV2	247	215	0.01%	0.002%
61	10.543	1549	1551	1554	rBV	219	277	0.02%	0.002%
62	10.671	1570	1572	1573	rBV	357	306	0.02%	0.002%
63	11.128	1645	1647	1649	rBV2	259	292	0.02%	0.002%
64	11.189	1652	1657	1672	rVV	591188	787597	45.39%	6.130%
65	11.317	1674	1678	1681	rVV3	1155	1872	0.11%	0.015%
66	11.372	1685	1687	1691	rVB2	313	355	0.02%	0.003%
67	11.402	1691	1692	1694	rBV	233	217	0.01%	0.002%
68	11.451	1698	1700	1703	rBV2	268	308	0.02%	0.002%
69	11.658	1732	1734	1737	rVB	337	282	0.02%	0.002%
70	11.756	1747	1750	1751	rVB2	325	299	0.02%	0.002%
71	11.805	1756	1758	1759	rBV	239	197	0.01%	0.002%
72	11.933	1777	1779	1780	rBV	257	231	0.01%	0.002%
73	11.969	1782	1785	1788	rVV2	4621	5526	0.32%	0.043%
74	12.024	1788	1794	1805	rVB	900339	1228821	70.82%	9.564%
75	12.219	1823	1826	1833	rVB3	2355	3762	0.22%	0.029%
76	12.317	1837	1842	1854	rVV	883134	1164231	67.10%	9.061%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035188.D
 Acq On : 19 Apr 2023 22:48
 Operator : JC/MD
 Sample : 02333-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	12.591	1885	1887	1889	rBV2	303	225	0.01%	0.002%
78	12.689	1901	1903	1905	rBV2	226	229	0.01%	0.002%
79	12.762	1913	1915	1916	rBV	460	306	0.02%	0.002%
80	12.817	1922	1924	1926	rBV2	277	334	0.02%	0.003%
81	12.969	1947	1949	1952	rVB2	291	288	0.02%	0.002%
82	13.012	1953	1956	1958	rBV	291	256	0.01%	0.002%
83	13.182	1980	1984	1985	rBV3	294	334	0.02%	0.003%
84	13.213	1988	1989	1993	rVB3	336	252	0.01%	0.002%
85	13.250	1993	1995	1998	rBV2	278	262	0.02%	0.002%
86	13.298	2001	2003	2004	rBV	378	250	0.01%	0.002%
87	13.512	2037	2038	2040	rBV2	268	219	0.01%	0.002%
88	13.591	2048	2051	2057	rVB3	5275	6937	0.40%	0.054%
89	13.640	2057	2059	2062	rBV2	252	235	0.01%	0.002%
90	13.877	2096	2098	2099	rBV	311	228	0.01%	0.002%
91	13.963	2110	2112	2117	rVB3	1260	1524	0.09%	0.012%
92	14.024	2120	2122	2123	rBV	479	313	0.02%	0.002%
93	14.134	2138	2140	2145	rVB2	495	720	0.04%	0.006%
94	14.170	2145	2146	2149	rBV	514	380	0.02%	0.003%
95	14.201	2149	2151	2153	rBV	316	266	0.02%	0.002%
96	14.280	2163	2164	2166	rBV	473	249	0.01%	0.002%
97	14.396	2181	2183	2187	rVB2	458	484	0.03%	0.004%
98	14.591	2211	2215	2216	rBV2	421	448	0.03%	0.003%
99	14.957	2273	2275	2277	rBV2	466	386	0.02%	0.003%
100	15.158	2306	2308	2312	rVB4	663	892	0.05%	0.007%

Sum of corrected areas: 12848645




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035188.D
Acq On : 19 Apr 2023 22:48
Operator : JC/MD
Sample : 02333-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

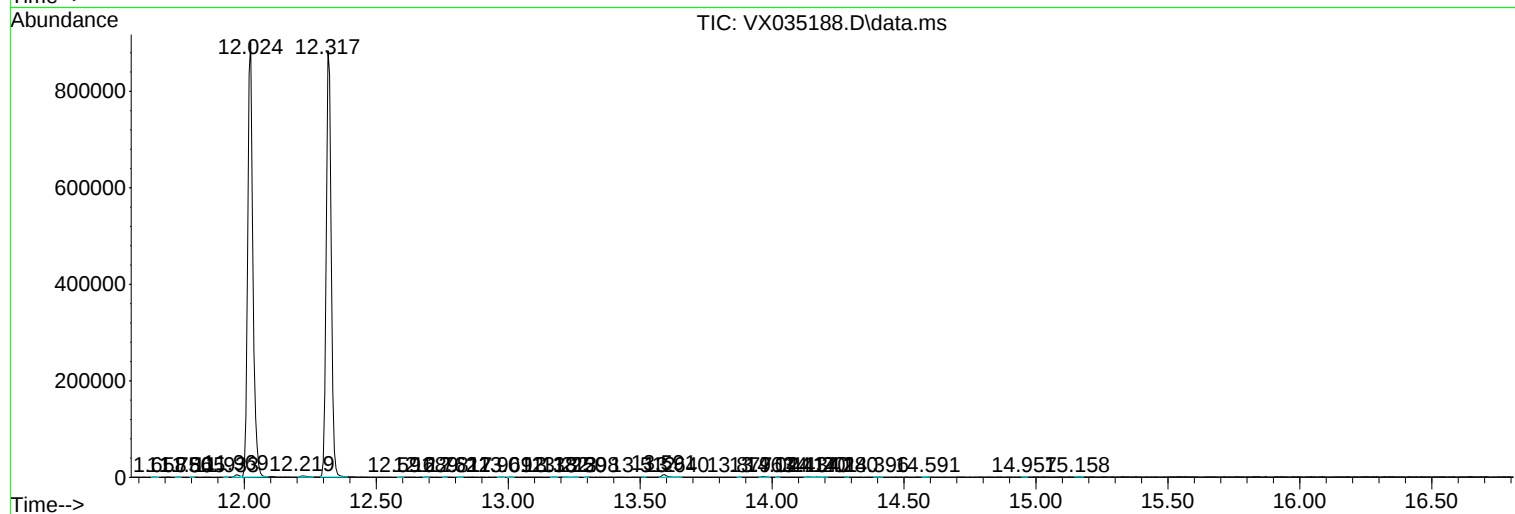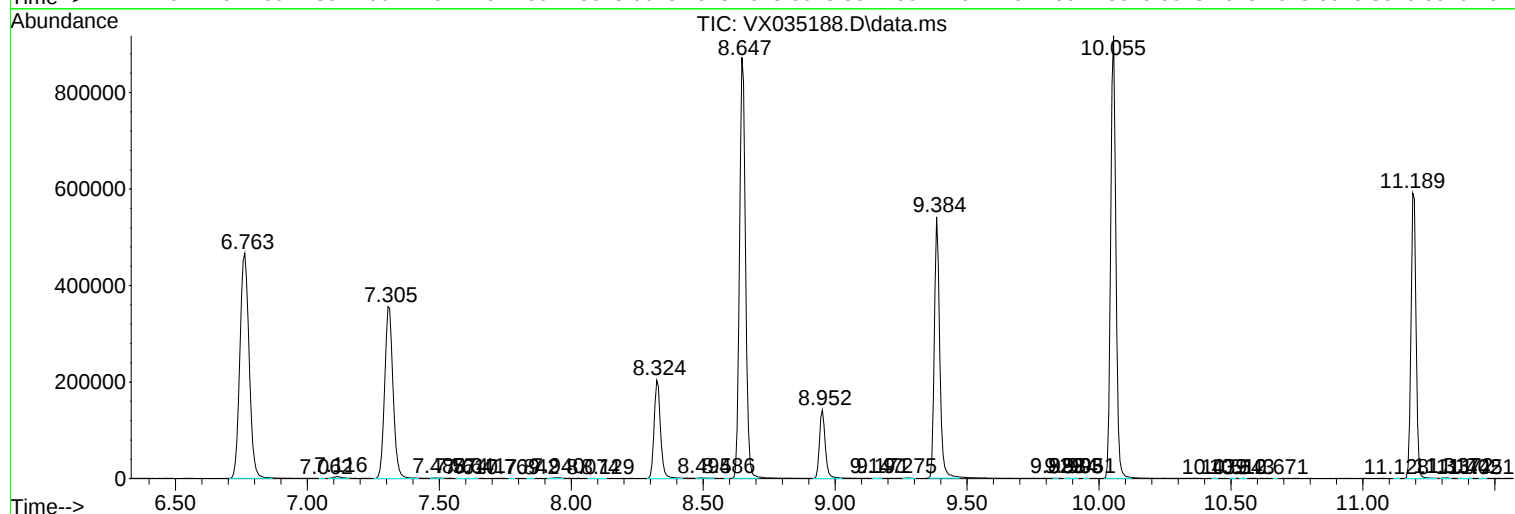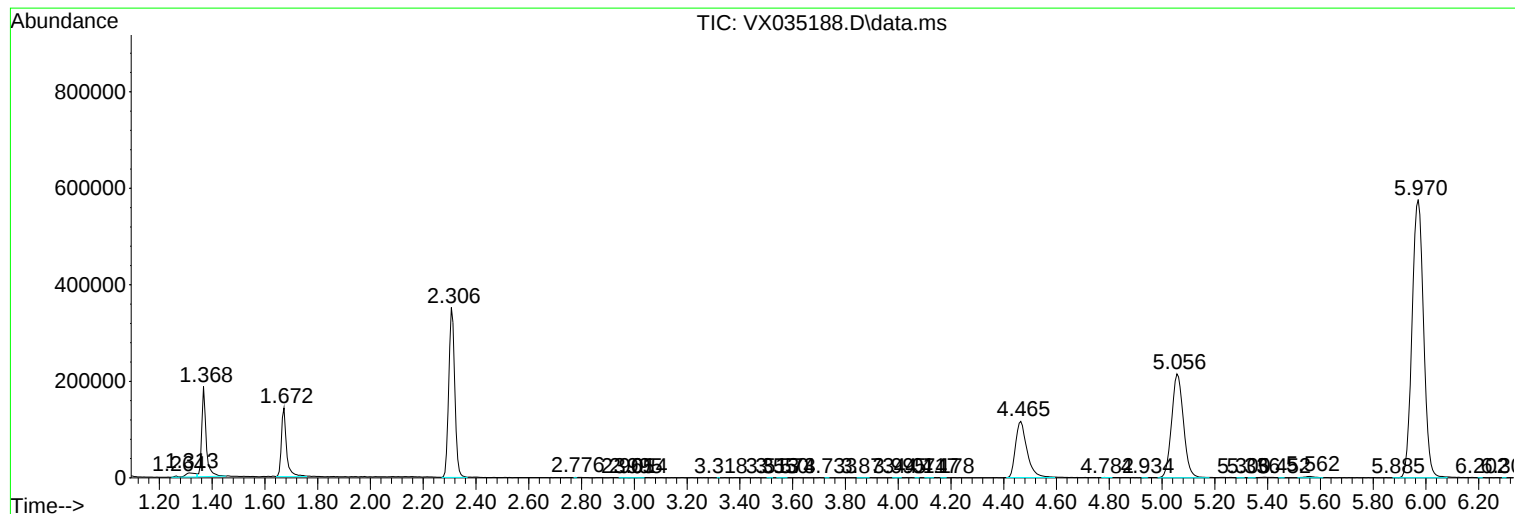

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035188.D
Acq On : 19 Apr 2023 22:48
Operator : JC/MD
Sample : 02333-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035188.D
Acq On : 19 Apr 2023 22:48
Operator : JC/MD
Sample : 02333-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0MH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc