

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035190.D
 Acq On : 19 Apr 2023 23:34
 Operator : JC/MD
 Sample : 02333-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M

Title : VOC Analysis

Signal : TIC: VX035190.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	31	rBV3	2382	2345	0.14%	0.019%
2	1.368	42	46	65	rVB	184522	211899	12.24%	1.693%
3	1.672	91	96	106	rBV	147029	192105	11.09%	1.535%
4	2.306	194	200	210	rBV	365959	555164	32.06%	4.436%
5	2.404	211	216	223	rVB2	3424	7752	0.45%	0.062%
6	2.587	245	246	248	rBV2	321	282	0.02%	0.002%
7	2.691	262	263	267	rVB3	561	361	0.02%	0.003%
8	2.788	277	279	283	rVB4	992	1135	0.07%	0.009%
9	2.898	294	297	300	rBV	366	376	0.02%	0.003%
10	2.934	300	303	308	rBV2	422	650	0.04%	0.005%
11	3.300	361	363	367	rBV2	394	419	0.02%	0.003%
12	3.367	370	374	377	rVV	282	326	0.02%	0.003%
13	3.678	423	425	427	rBV2	253	263	0.02%	0.002%
14	3.812	446	447	451	rVB	217	259	0.01%	0.002%
15	3.861	451	455	457	rBV2	248	226	0.01%	0.002%
16	3.898	459	461	464	rVV2	265	211	0.01%	0.002%
17	4.001	475	478	481	rBV	392	364	0.02%	0.003%
18	4.123	496	498	502	rVB3	252	360	0.02%	0.003%
19	4.276	521	523	525	rVB2	310	242	0.01%	0.002%
20	4.318	525	530	531	rBV2	203	286	0.02%	0.002%
21	4.373	537	539	542	rBV2	356	268	0.02%	0.002%
22	4.465	545	554	576	rBV	117047	368117	21.26%	2.941%
23	4.672	587	588	590	rVB2	575	289	0.02%	0.002%
24	4.739	596	599	602	rBV3	481	446	0.03%	0.004%
25	4.952	632	634	637	rVB3	414	399	0.02%	0.003%
26	5.056	637	651	666	rBV	215526	673074	38.87%	5.378%
27	5.391	704	706	707	rBV2	377	326	0.02%	0.003%
28	5.471	716	719	721	rVB	302	351	0.02%	0.003%
29	5.538	724	730	731	rBV3	734	1105	0.06%	0.009%
30	5.763	764	767	771	rVB2	333	380	0.02%	0.003%
31	5.800	771	773	774	rBV	318	223	0.01%	0.002%
32	5.970	789	801	815	rBV2	579563	1731704	100.00%	13.836%
33	6.196	836	838	841	rBV3	427	397	0.02%	0.003%
34	6.300	852	855	858	rBV2	373	484	0.03%	0.004%
35	6.324	858	859	862	rBV2	354	303	0.02%	0.002%
36	6.470	881	883	886	rBV2	225	332	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035190.D
 Acq On : 19 Apr 2023 23:34
 Operator : JC/MD
 Sample : 02333-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	6.763	921	931	946	rBV	425266	1010252	58.34%	8.071%
38	6.964	963	964	967	rVB	333	208	0.01%	0.002%
39	7.043	973	977	980	rVB3	450	755	0.04%	0.006%
40	7.117	983	989	996	rVB5	2851	6321	0.37%	0.051%
41	7.306	1011	1020	1033	rBV	354458	793445	45.82%	6.339%
42	7.488	1044	1050	1051	rBV4	679	1122	0.06%	0.009%
43	7.641	1074	1075	1078	rBV2	259	223	0.01%	0.002%
44	7.793	1099	1100	1104	rVB	288	271	0.02%	0.002%
45	7.952	1121	1126	1132	rBV4	1105	2620	0.15%	0.021%
46	8.092	1146	1149	1150	rVV	180	219	0.01%	0.002%
47	8.251	1173	1175	1178	rBV	365	360	0.02%	0.003%
48	8.324	1181	1187	1202	rBV	202256	340438	19.66%	2.720%
49	8.494	1211	1215	1216	rBV3	831	1060	0.06%	0.008%
50	8.647	1233	1240	1253	rBV	901097	1383371	79.88%	11.053%
51	8.866	1275	1276	1280	rVB3	370	331	0.02%	0.003%
52	8.897	1280	1281	1283	rBV	424	290	0.02%	0.002%
53	8.952	1284	1290	1305	rVV	145088	213415	12.32%	1.705%
54	9.281	1341	1344	1348	rVB2	1070	1301	0.08%	0.010%
55	9.384	1356	1361	1378	rBV	559633	799688	46.18%	6.389%
56	9.689	1409	1411	1415	rVB4	348	509	0.03%	0.004%
57	9.726	1415	1417	1420	rVB3	296	234	0.01%	0.002%
58	9.769	1423	1424	1426	rBV2	278	229	0.01%	0.002%
59	9.927	1448	1450	1455	rVB2	277	368	0.02%	0.003%
60	10.055	1465	1471	1490	rBV	832509	1143007	66.00%	9.132%
61	10.305	1509	1512	1516	rBV2	505	712	0.04%	0.006%
62	10.360	1519	1521	1523	rBV2	270	236	0.01%	0.002%
63	10.451	1535	1536	1538	rBV2	263	215	0.01%	0.002%
64	10.506	1544	1545	1547	rBV2	231	210	0.01%	0.002%
65	10.537	1548	1550	1556	rVB3	424	555	0.03%	0.004%
66	10.616	1558	1563	1566	rBV2	311	652	0.04%	0.005%
67	10.677	1572	1573	1574	rBV	573	273	0.02%	0.002%
68	10.713	1577	1579	1582	rVV2	284	346	0.02%	0.003%
69	10.744	1582	1584	1587	rVV	265	303	0.02%	0.002%
70	10.927	1611	1614	1618	rBV2	284	408	0.02%	0.003%
71	11.061	1633	1636	1637	rBV	297	234	0.01%	0.002%
72	11.189	1652	1657	1673	rVV	626697	802537	46.34%	6.412%
73	11.317	1673	1678	1682	rVV3	950	1427	0.08%	0.011%
74	11.360	1683	1685	1688	rVB2	327	280	0.02%	0.002%
75	11.482	1702	1705	1707	rBV	279	329	0.02%	0.003%
76	11.573	1717	1720	1722	rBV2	223	282	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035190.D
 Acq On : 19 Apr 2023 23:34
 Operator : JC/MD
 Sample : 02333-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	11.634	1727	1730	1734	rVB2	273	324	0.02%	0.003%
78	11.665	1734	1735	1737	rBV	309	269	0.02%	0.002%
79	11.707	1740	1742	1747	rVB2	455	513	0.03%	0.004%
80	11.969	1782	1785	1788	rBV3	1627	1976	0.11%	0.016%
81	12.018	1788	1793	1805	rVV	781827	1050712	60.68%	8.395%
82	12.219	1822	1826	1833	rBV4	3435	5443	0.31%	0.043%
83	12.317	1837	1842	1855	rVV	897103	1174716	67.84%	9.385%
84	12.555	1879	1881	1883	rBV	301	225	0.01%	0.002%
85	12.762	1913	1915	1920	rVB2	539	521	0.03%	0.004%
86	12.805	1920	1922	1925	rBV	312	305	0.02%	0.002%
87	12.878	1932	1934	1936	rBV2	363	285	0.02%	0.002%
88	12.926	1938	1942	1945	rBV2	284	468	0.03%	0.004%
89	12.975	1948	1950	1954	rVB	336	260	0.02%	0.002%
90	13.018	1954	1957	1961	rBV3	307	539	0.03%	0.004%
91	13.067	1964	1965	1970	rVB	366	411	0.02%	0.003%
92	13.213	1987	1989	1992	rBV2	276	359	0.02%	0.003%
93	13.457	2026	2029	2034	rVB2	292	401	0.02%	0.003%
94	13.591	2047	2051	2060	rVB2	7298	10157	0.59%	0.081%
95	13.963	2107	2112	2115	rBV4	1735	2105	0.12%	0.017%
96	14.030	2121	2123	2125	rBV	474	381	0.02%	0.003%
97	14.127	2137	2139	2141	rVB2	374	226	0.01%	0.002%
98	14.536	2203	2206	2207	rBV3	495	422	0.02%	0.003%
99	14.749	2238	2241	2243	rBV3	569	703	0.04%	0.006%
100	14.786	2243	2247	2251	rBV2	1681	2343	0.14%	0.019%


Sum of corrected areas: 12516323

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035190.D
Acq On : 19 Apr 2023 23:34
Operator : JC/MD
Sample : 02333-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

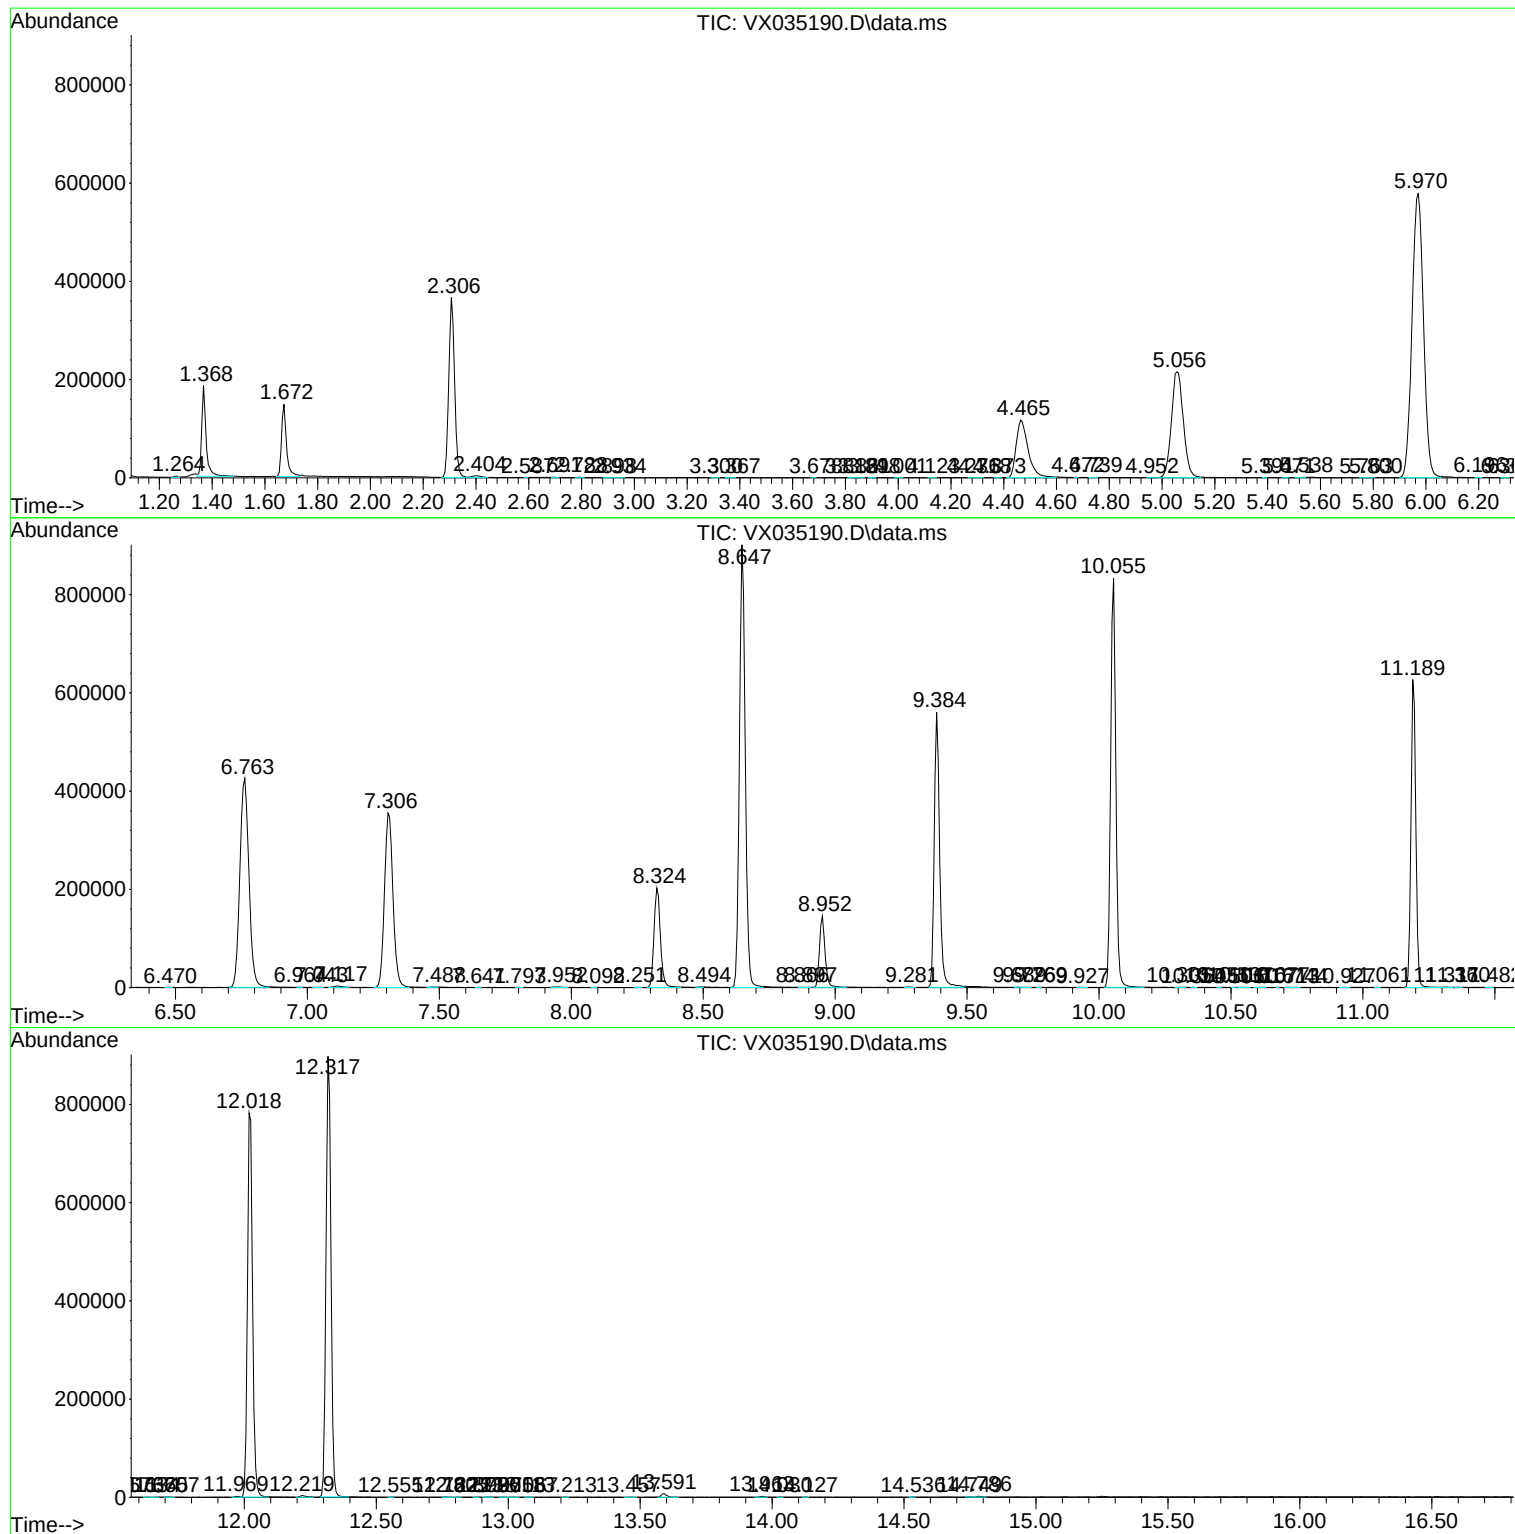

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035190.D
Acq On : 19 Apr 2023 23:34
Operator : JC/MD
Sample : 02333-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035190.D
Acq On : 19 Apr 2023 23:34
Operator : JC/MD
Sample : 02333-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0MF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc