

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035191.D
 Acq On : 19 Apr 2023 23:58
 Operator : JC/MD
 Sample : VIBLK625
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK625

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035191.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	32	rBV3	2391	2351	0.14%	0.019%
2	1.367	42	46	58	rBV	189842	205181	11.89%	1.617%
3	1.672	91	96	109	rBV	143306	192260	11.14%	1.515%
4	2.306	194	200	211	rVB	363263	553980	32.11%	4.366%
5	2.593	244	247	250	rVB2	355	275	0.02%	0.002%
6	2.623	250	252	254	rBV2	355	357	0.02%	0.003%
7	2.788	273	279	286	rVB3	5282	9785	0.57%	0.077%
8	2.849	286	289	290	rBV	268	233	0.01%	0.002%
9	3.026	316	318	322	rVB	355	395	0.02%	0.003%
10	3.556	401	405	406	rBV2	290	381	0.02%	0.003%
11	3.983	472	475	476	rBV	194	238	0.01%	0.002%
12	3.995	476	477	479	rVV	308	213	0.01%	0.002%
13	4.062	484	488	490	rVB3	304	498	0.03%	0.004%
14	4.080	490	491	494	rBV	381	447	0.03%	0.004%
15	4.141	499	501	503	rVB2	242	204	0.01%	0.002%
16	4.160	503	504	507	rBV2	182	198	0.01%	0.002%
17	4.379	537	540	541	rBV	278	207	0.01%	0.002%
18	4.464	543	554	577	rBV	118235	361215	20.93%	2.847%
19	4.769	601	604	605	rVB	301	252	0.01%	0.002%
20	4.794	605	608	609	rBV2	317	341	0.02%	0.003%
21	4.861	617	619	621	rVB2	297	264	0.02%	0.002%
22	5.056	638	651	668	rBV	210346	657088	38.08%	5.178%
23	5.233	678	680	681	rVB2	540	318	0.02%	0.003%
24	5.355	698	700	701	rBV	228	198	0.01%	0.002%
25	5.379	703	704	707	rVV3	453	427	0.02%	0.003%
26	5.403	707	708	709	rVV	549	268	0.02%	0.002%
27	5.422	709	711	712	rVV	354	221	0.01%	0.002%
28	5.440	712	714	715	rVB	332	240	0.01%	0.002%
29	5.550	726	732	743	rBV3	1303	3967	0.23%	0.031%
30	5.793	770	772	774	rVB2	259	217	0.01%	0.002%
31	5.970	788	801	827	rBV2	574842	1725488	100.00%	13.598%
32	6.226	841	843	844	rVB	414	240	0.01%	0.002%
33	6.245	844	846	848	rBV2	329	278	0.02%	0.002%
34	6.373	866	867	873	rVB2	292	417	0.02%	0.003%
35	6.470	880	883	889	rBV2	341	529	0.03%	0.004%
36	6.671	913	916	917	rBV2	280	312	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035191.D
 Acq On : 19 Apr 2023 23:58
 Operator : JC/MD
 Sample : VIBLK625
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK625

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	6.763	921	931	951	rVV	466619	1125946	65.25%	8.873%
38	6.964	962	964	967	rBV2	276	212	0.01%	0.002%
39	7.116	983	989	1000	rVV2	4392	9916	0.57%	0.078%
40	7.196	1000	1002	1004	rVB2	320	285	0.02%	0.002%
41	7.305	1011	1020	1033	rBV	358511	791181	45.85%	6.235%
42	7.452	1042	1044	1046	rVB2	394	240	0.01%	0.002%
43	7.482	1046	1049	1053	rVV4	1083	1817	0.11%	0.014%
44	7.531	1055	1057	1059	rVB2	458	352	0.02%	0.003%
45	7.946	1119	1125	1128	rBV2	1406	2590	0.15%	0.020%
46	8.074	1144	1146	1149	rBV	287	195	0.01%	0.002%
47	8.128	1152	1155	1160	rVB2	198	284	0.02%	0.002%
48	8.226	1167	1171	1172	rBV2	202	217	0.01%	0.002%
49	8.324	1181	1187	1197	rBV	202083	331478	19.21%	2.612%
50	8.494	1213	1215	1216	rBV2	601	527	0.03%	0.004%
51	8.647	1234	1240	1257	rVV	853527	1367356	79.24%	10.776%
52	8.951	1284	1290	1302	rBV	141620	212412	12.31%	1.674%
53	9.238	1331	1337	1340	rBV4	309	713	0.04%	0.006%
54	9.262	1340	1341	1343	rBV	441	387	0.02%	0.003%
55	9.384	1356	1361	1379	rBV	544697	775637	44.95%	6.113%
56	9.732	1416	1418	1419	rBV	301	262	0.02%	0.002%
57	9.774	1423	1425	1427	rVV2	401	281	0.02%	0.002%
58	9.793	1427	1428	1431	rVB	305	227	0.01%	0.002%
59	10.055	1465	1471	1482	rBV	934032	1261295	73.10%	9.940%
60	10.476	1538	1540	1543	rVB2	332	264	0.02%	0.002%
61	10.652	1567	1569	1571	rVV	286	232	0.01%	0.002%
62	10.671	1571	1572	1575	rVV2	220	216	0.01%	0.002%
63	10.707	1577	1578	1580	rVV	345	225	0.01%	0.002%
64	10.817	1593	1596	1599	rBV	315	359	0.02%	0.003%
65	10.878	1602	1606	1607	rBV2	325	370	0.02%	0.003%
66	11.000	1624	1626	1628	rBV	323	256	0.01%	0.002%
67	11.189	1652	1657	1667	rBV	609588	779632	45.18%	6.144%
68	11.299	1674	1675	1677	rBV2	264	220	0.01%	0.002%
69	11.360	1683	1685	1687	rVB3	275	231	0.01%	0.002%
70	11.408	1690	1693	1695	rBV2	349	501	0.03%	0.004%
71	11.677	1735	1737	1739	rBV	226	199	0.01%	0.002%
72	11.707	1739	1742	1745	rVB2	648	684	0.04%	0.005%
73	11.762	1749	1751	1753	rBV3	304	284	0.02%	0.002%
74	11.853	1762	1766	1769	rBV3	168	207	0.01%	0.002%
75	11.933	1775	1779	1781	rBV2	221	215	0.01%	0.002%
76	11.975	1782	1786	1788	rBV2	513	646	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035191.D
 Acq On : 19 Apr 2023 23:58
 Operator : JC/MD
 Sample : VIBLK625
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK625

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	12.024	1788	1794	1804	rBV	865596	1142225	66.20%	9.001%
78	12.213	1823	1825	1830	rBV2	459	670	0.04%	0.005%
79	12.317	1837	1842	1849	rBV	896426	1147170	66.48%	9.040%
80	12.554	1880	1881	1883	rBV	260	255	0.01%	0.002%
81	12.695	1901	1904	1905	rBV2	273	227	0.01%	0.002%
82	12.756	1912	1914	1917	rVB	550	452	0.03%	0.004%
83	12.902	1937	1938	1942	rBV3	192	213	0.01%	0.002%
84	12.975	1948	1950	1952	rBV	405	395	0.02%	0.003%
85	13.201	1986	1987	1990	rVB2	366	247	0.01%	0.002%
86	13.249	1991	1995	1997	rVB2	255	335	0.02%	0.003%
87	13.530	2039	2041	2043	rBV2	245	195	0.01%	0.002%
88	13.591	2048	2051	2057	rBV2	2794	3764	0.22%	0.030%
89	13.847	2091	2093	2095	rBV2	321	313	0.02%	0.002%
90	13.890	2098	2100	2101	rVV	275	234	0.01%	0.002%
91	13.963	2111	2112	2116	rBV3	557	633	0.04%	0.005%
92	14.042	2123	2125	2127	rBV2	407	416	0.02%	0.003%
93	14.127	2137	2139	2145	rVV4	549	920	0.05%	0.007%
94	14.194	2145	2150	2151	rVV4	454	578	0.03%	0.005%
95	14.365	2176	2178	2181	rBV2	336	361	0.02%	0.003%
96	14.432	2188	2189	2192	rVB2	438	321	0.02%	0.003%
97	14.463	2192	2194	2195	rBV	377	268	0.02%	0.002%
98	14.902	2265	2266	2267	rBV	541	275	0.02%	0.002%
99	15.078	2294	2295	2296	rBV	571	346	0.02%	0.003%
100	15.914	2430	2432	2434	rBV3	702	496	0.03%	0.004%


Sum of corrected areas: 12689343

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035191.D
Acq On : 19 Apr 2023 23:58
Operator : JC/MD
Sample : VIBLK625
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK625

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

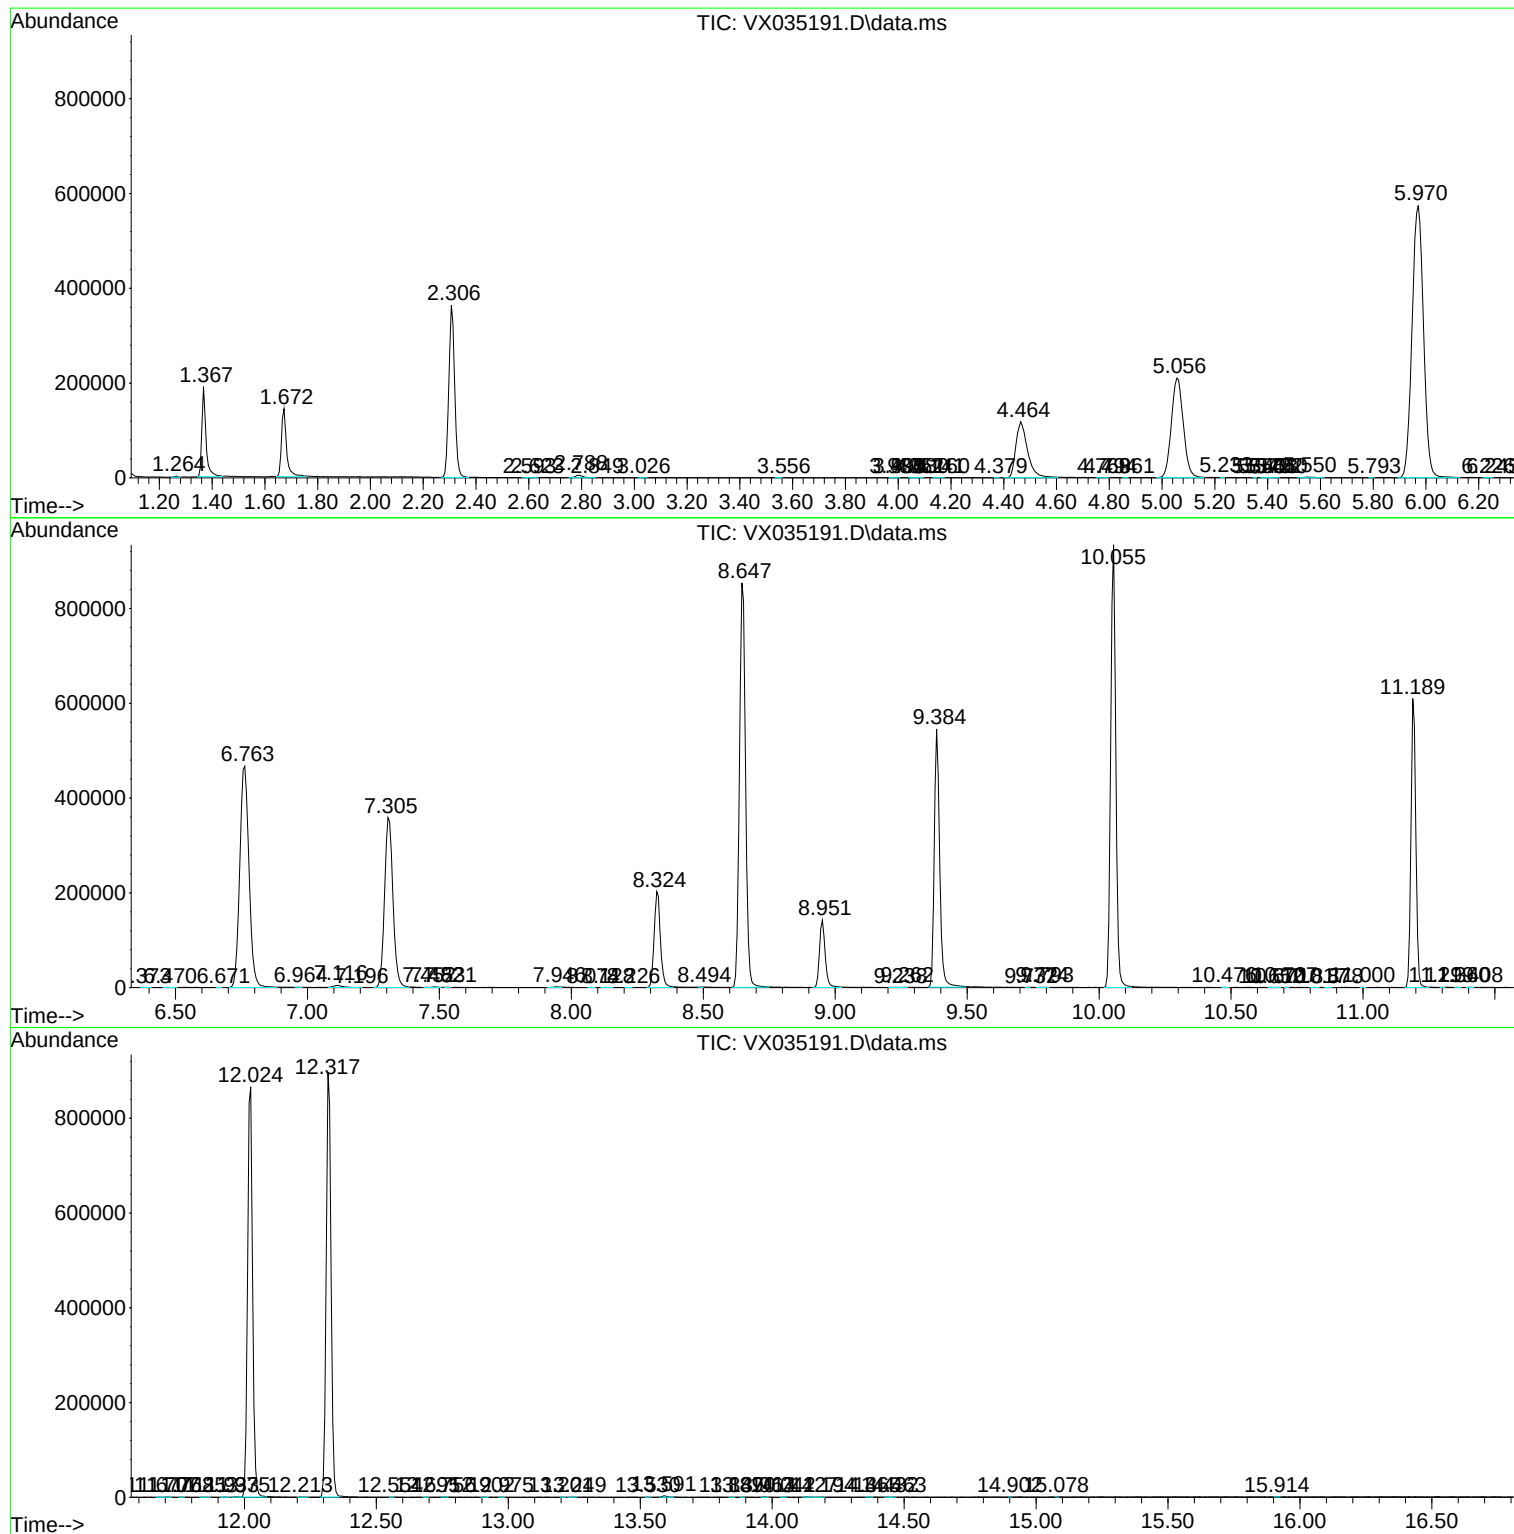

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035191.D
Acq On : 19 Apr 2023 23:58
Operator : JC/MD
Sample : VIBLK625
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK625

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035191.D
Acq On : 19 Apr 2023 23:58
Operator : JC/MD
Sample : VIBLK625
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK625

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------