

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035192.D
 Acq On : 20 Apr 2023 00:21
 Operator : JC/MD
 Sample : 02378-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMK2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M

Title : VOC Analysis

Signal : TIC: VX035192.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	25	28	31	rBV2	4561	4765	0.28%	0.036%
2	1.368	42	46	58	rVB	182164	199580	11.67%	1.495%
3	1.672	91	96	109	rBV	140344	185887	10.87%	1.393%
4	2.306	194	200	210	rBV	350915	539305	31.54%	4.041%
5	2.562	240	242	246	rBV3	305	445	0.03%	0.003%
6	2.623	249	252	255	rBV	361	440	0.03%	0.003%
7	2.788	277	279	285	rVB3	1018	1319	0.08%	0.010%
8	2.867	290	292	294	rBV2	210	206	0.01%	0.002%
9	2.940	298	304	312	rVB4	1857	4319	0.25%	0.032%
10	3.038	318	320	322	rBV	300	266	0.02%	0.002%
11	3.123	327	334	339	rBV4	700	1510	0.09%	0.011%
12	3.318	364	366	368	rVB	258	180	0.01%	0.001%
13	3.361	372	373	377	rVB	353	239	0.01%	0.002%
14	3.416	377	382	383	rVB	263	236	0.01%	0.002%
15	3.434	383	385	388	rBV	207	230	0.01%	0.002%
16	3.568	406	407	409	rBV2	261	226	0.01%	0.002%
17	3.672	423	424	427	rBV2	290	216	0.01%	0.002%
18	3.739	431	435	438	rBV2	243	409	0.02%	0.003%
19	3.922	462	465	467	rBV2	201	228	0.01%	0.002%
20	4.288	524	525	526	rBV	301	197	0.01%	0.001%
21	4.458	542	553	570	rBV	111775	341581	19.98%	2.559%
22	4.794	606	608	609	rBV	416	212	0.01%	0.002%
23	4.849	614	617	618	rVV2	360	319	0.02%	0.002%
24	4.867	618	620	623	rVB2	332	228	0.01%	0.002%
25	5.056	638	651	668	rBV	209089	654892	38.31%	4.907%
26	5.379	702	704	711	rBV4	614	1171	0.07%	0.009%
27	5.562	727	734	742	rVB4	1440	3419	0.20%	0.026%
28	5.739	761	763	766	rVB2	282	296	0.02%	0.002%
29	5.763	766	767	769	rBV	414	218	0.01%	0.002%
30	5.970	789	801	807	rBV2	576435	1709641	100.00%	12.810%
31	6.367	864	866	867	rBV2	266	191	0.01%	0.001%
32	6.397	870	871	875	rBV2	184	211	0.01%	0.002%
33	6.482	883	885	886	rBV	365	218	0.01%	0.002%
34	6.507	886	889	891	rVV2	193	230	0.01%	0.002%
35	6.757	921	930	948	rBV	454484	1094739	64.03%	8.203%
36	7.056	977	979	982	rBV3	226	206	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035192.D
 Acq On : 20 Apr 2023 00:21
 Operator : JC/MD
 Sample : 02378-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMK2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	7.117	982	989	999	rBV6	3753	8490	0.50%	0.064%
38	7.306	1011	1020	1043	rVV	354601	778607	45.54%	5.834%
39	7.476	1046	1048	1049	rBV	621	463	0.03%	0.003%
40	7.598	1066	1068	1072	rVB	331	395	0.02%	0.003%
41	7.635	1072	1074	1077	rBV	351	450	0.03%	0.003%
42	7.787	1097	1099	1102	rBV2	167	182	0.01%	0.001%
43	7.866	1111	1112	1113	rBV	484	207	0.01%	0.002%
44	7.946	1120	1125	1130	rBV3	1139	2450	0.14%	0.018%
45	8.226	1170	1171	1174	rBV2	224	184	0.01%	0.001%
46	8.324	1181	1187	1204	rBV	197233	329748	19.29%	2.471%
47	8.647	1234	1240	1257	rBV	864952	1354137	79.21%	10.146%
48	8.952	1284	1290	1303	rBV	140765	208922	12.22%	1.565%
49	9.153	1321	1323	1325	rBV2	231	232	0.01%	0.002%
50	9.214	1328	1333	1334	rVB2	486	629	0.04%	0.005%
51	9.226	1334	1335	1337	rBV2	290	228	0.01%	0.002%
52	9.275	1339	1343	1347	rBV2	1630	2633	0.15%	0.020%
53	9.384	1356	1361	1380	rBV	535513	749545	43.84%	5.616%
54	9.927	1448	1450	1451	rBV	250	186	0.01%	0.001%
55	9.994	1460	1461	1463	rBV2	215	189	0.01%	0.001%
56	10.055	1465	1471	1473	rBV	940443	1350563	79.00%	10.119%
57	10.244	1500	1502	1504	rVB2	457	328	0.02%	0.002%
58	10.470	1537	1539	1542	rVB	277	227	0.01%	0.002%
59	10.592	1557	1559	1562	rBV2	321	415	0.02%	0.003%
60	10.756	1585	1586	1588	rBV	324	218	0.01%	0.002%
61	11.000	1625	1626	1628	rVB2	450	267	0.02%	0.002%
62	11.024	1628	1630	1634	rVB2	250	350	0.02%	0.003%
63	11.055	1634	1635	1638	rBV2	260	196	0.01%	0.001%
64	11.091	1638	1641	1643	rBV	376	368	0.02%	0.003%
65	11.189	1652	1657	1671	rBV	576275	765182	44.76%	5.733%
66	11.311	1675	1677	1681	rVB4	1401	1880	0.11%	0.014%
67	11.366	1684	1686	1689	rBV2	279	208	0.01%	0.002%
68	11.408	1691	1693	1699	rVB	259	422	0.02%	0.003%
69	11.463	1699	1702	1704	rBV2	298	304	0.02%	0.002%
70	11.713	1740	1743	1745	rVV2	706	594	0.03%	0.004%
71	11.969	1780	1785	1789	rBV	30399	38640	2.26%	0.290%
72	12.024	1789	1794	1807	rVB2	910898	1500722	87.78%	11.244%
73	12.219	1822	1826	1830	rBV4	2292	3717	0.22%	0.028%
74	12.323	1837	1843	1859	rBV2	933910	1433717	83.86%	10.742%
75	12.500	1868	1872	1874	rVB3	601	476	0.03%	0.004%
76	12.768	1910	1916	1920	rVB2	545	767	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035192.D
 Acq On : 20 Apr 2023 00:21
 Operator : JC/MD
 Sample : 02378-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMK2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	12.817	1920	1924	1928	rBV3	1938	3494	0.20%	0.026%
78	12.945	1944	1945	1946	rBV	398	255	0.01%	0.002%
79	12.994	1951	1953	1954	rBV2	342	187	0.01%	0.001%
80	13.054	1961	1963	1966	rVB	313	299	0.02%	0.002%
81	13.250	1994	1995	1998	rBV2	204	244	0.01%	0.002%
82	13.420	2021	2023	2026	rBV2	205	228	0.01%	0.002%
83	13.518	2036	2039	2041	rBV2	276	352	0.02%	0.003%
84	13.591	2046	2051	2059	rVV	31560	42497	2.49%	0.318%
85	13.695	2066	2068	2069	rVV	416	290	0.02%	0.002%
86	13.762	2077	2079	2080	rVB	368	220	0.01%	0.002%
87	13.786	2080	2083	2085	rBV2	522	602	0.04%	0.005%
88	13.902	2098	2102	2103	rBV2	293	261	0.02%	0.002%
89	13.920	2103	2105	2106	rVV	374	281	0.02%	0.002%
90	13.963	2108	2112	2119	rVB2	3707	4876	0.29%	0.037%
91	14.091	2131	2133	2137	rBV2	335	361	0.02%	0.003%
92	14.121	2137	2138	2140	rVV	351	202	0.01%	0.002%
93	14.164	2144	2145	2147	rBV2	643	393	0.02%	0.003%
94	14.201	2149	2151	2153	rVB3	576	305	0.02%	0.002%
95	14.225	2153	2155	2156	rBV	337	286	0.02%	0.002%
96	14.414	2185	2186	2189	rBV	435	368	0.02%	0.003%
97	14.786	2244	2247	2254	rBV4	1199	2199	0.13%	0.016%
98	14.859	2257	2259	2261	rBV	395	339	0.02%	0.003%
99	15.249	2320	2323	2330	rBV5	1141	1886	0.11%	0.014%
100	16.139	2467	2469	2470	rBV2	656	466	0.03%	0.003%


Sum of corrected areas: 13346304

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035192.D
Acq On : 20 Apr 2023 00:21
Operator : JC/MD
Sample : 02378-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMK2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

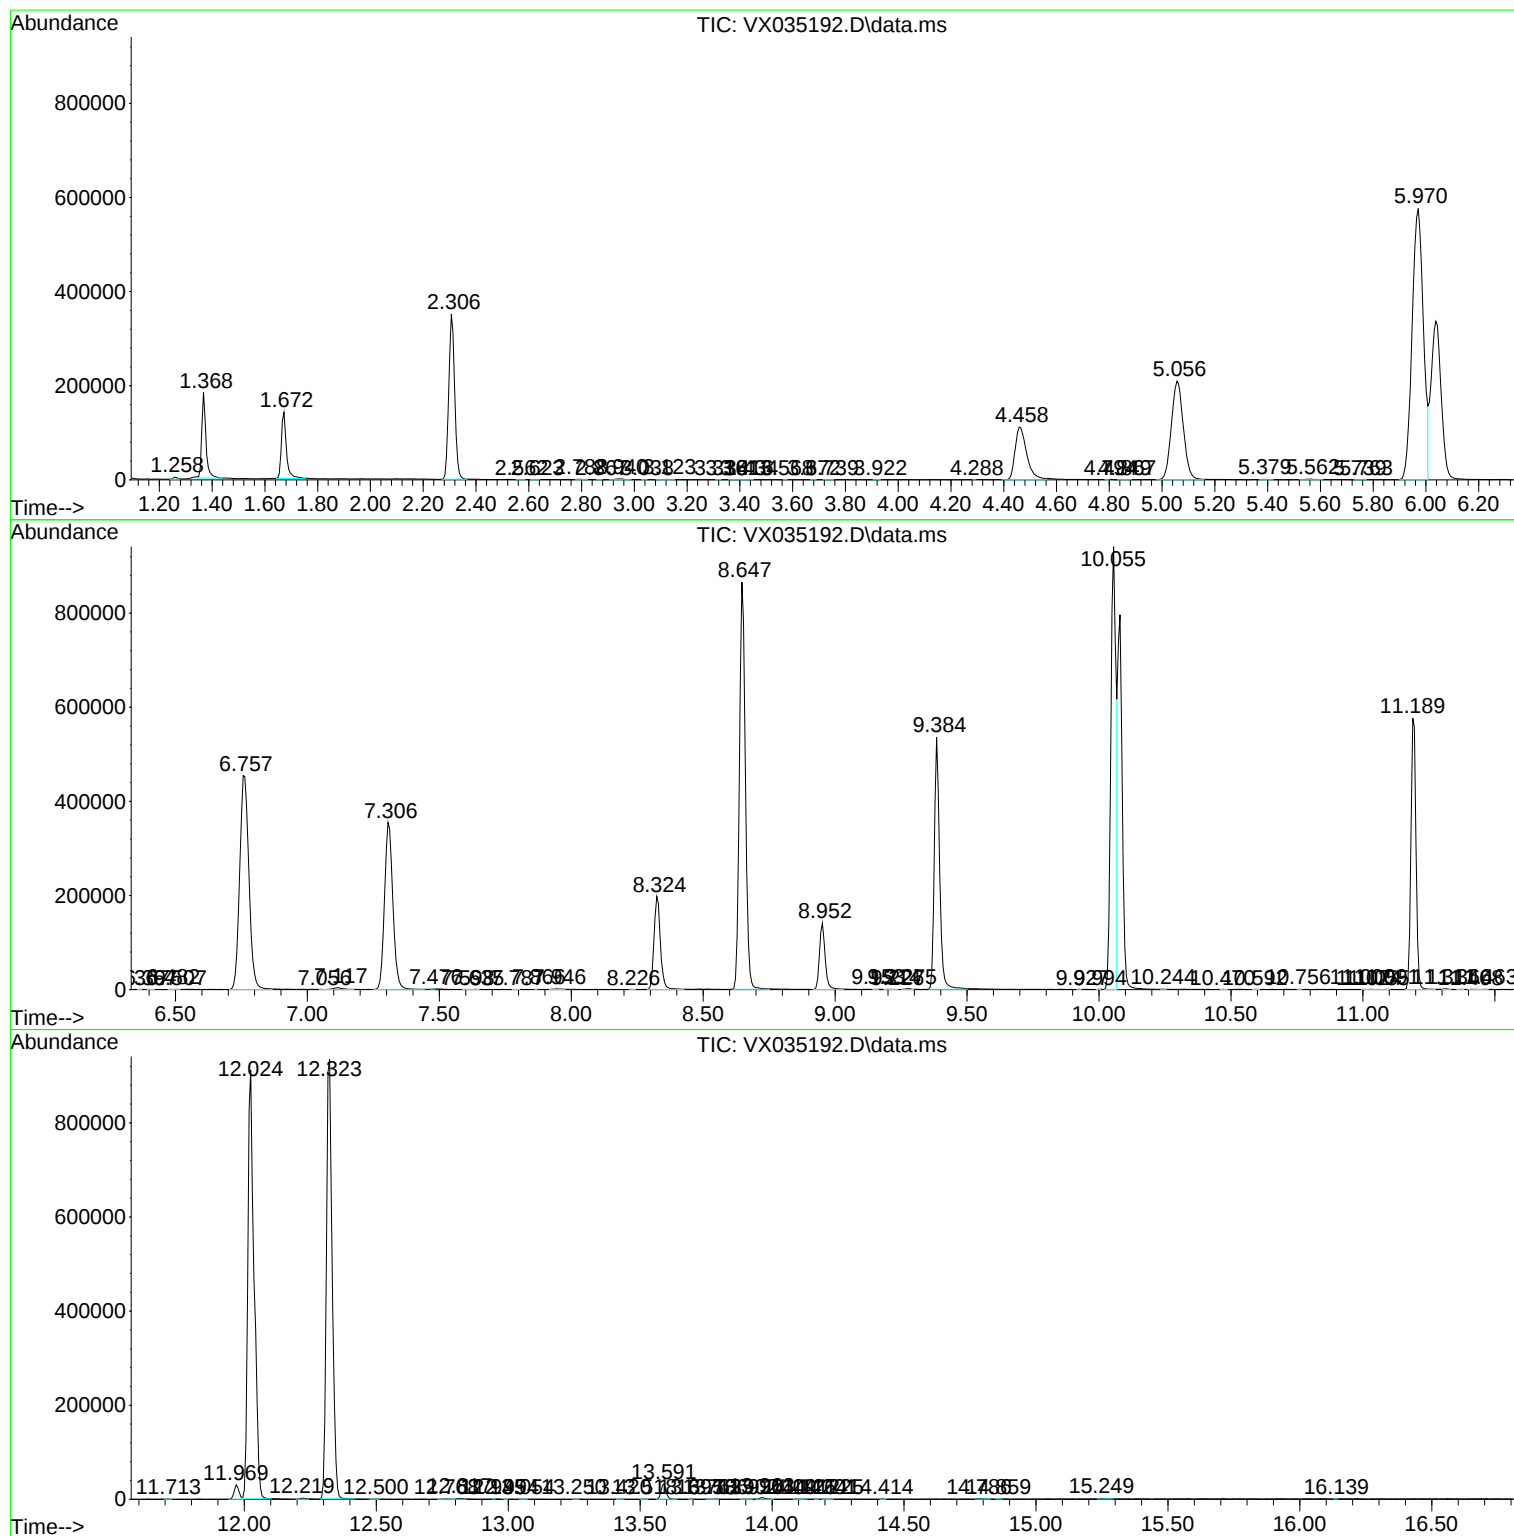

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035192.D
Acq On : 20 Apr 2023 00:21
Operator : JC/MD
Sample : 02378-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0MK2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035192.D
Acq On : 20 Apr 2023 00:21
Operator : JC/MD
Sample : 02378-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0MK2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc