

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035195.D
 Acq On : 20 Apr 2023 01:30
 Operator : JC/MD
 Sample : 02378-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M

Title : VOC Analysis

Signal : TIC: VX035195.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	11	rBV2	732	575	0.00%	0.000%
2	1.264	25	29	30	rBV2	2715	2976	0.01%	0.002%
3	1.301	30	35	42	rVV2	11366	32718	0.07%	0.017%
4	1.368	42	46	59	rVB	179750	200328	0.42%	0.104%
5	1.666	91	95	108	rVB	133408	181402	0.38%	0.094%
6	2.307	194	200	209	rBV	348363	549846	1.16%	0.286%
7	2.386	211	213	219	rVB2	3166	3682	0.01%	0.002%
8	2.520	230	235	241	rVB6	668	1264	0.00%	0.001%
9	2.788	273	279	284	rBV4	2183	4115	0.01%	0.002%
10	2.867	288	292	299	rVV4	1955	3864	0.01%	0.002%
11	2.941	301	304	309	rVB3	579	850	0.00%	0.000%
12	3.111	328	332	338	rVV4	870	1496	0.00%	0.001%
13	3.441	382	386	387	rBV2	445	489	0.00%	0.000%
14	3.837	447	451	452	rBV2	302	458	0.00%	0.000%
15	4.044	482	485	489	rVB2	295	339	0.00%	0.000%
16	4.300	518	527	537	rVB4	3997	11160	0.02%	0.006%
17	4.453	542	552	568	rBV	113368	332175	0.70%	0.173%
18	4.642	581	583	584	rVB2	646	388	0.00%	0.000%
19	5.087	639	656	676	rBV3	508327	2057306	4.33%	1.071%
20	5.233	679	680	685	rVB4	927	905	0.00%	0.000%
21	5.391	701	706	712	rVB4	1084	2349	0.00%	0.001%
22	5.465	712	718	727	rVB5	2455	6784	0.01%	0.004%
23	5.550	727	732	735	rBV4	1317	2216	0.00%	0.001%
24	5.684	742	754	764	rBV2	33872	102653	0.22%	0.053%
25	6.050	804	814	845	rVB	16638024	47479329	100.00%	24.722%
26	6.763	921	931	947	rBV	466264	1120645	2.36%	0.584%
27	7.129	984	991	1003	rVB5	8782	23106	0.05%	0.012%
28	7.306	1011	1020	1037	rBV	338662	753272	1.59%	0.392%
29	7.476	1045	1048	1049	rBV2	1094	1088	0.00%	0.001%
30	7.550	1058	1060	1062	rVB2	433	348	0.00%	0.000%
31	7.720	1086	1088	1090	rBV2	374	366	0.00%	0.000%
32	7.775	1094	1097	1099	rVV	278	367	0.00%	0.000%
33	7.824	1100	1105	1113	rVB	4491	8940	0.02%	0.005%
34	7.885	1113	1115	1119	rBV2	320	414	0.00%	0.000%
35	7.940	1119	1124	1129	rBV3	1999	3545	0.01%	0.002%
36	8.159	1158	1160	1163	rVB2	349	352	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035195.D
 Acq On : 20 Apr 2023 01:30
 Operator : JC/MD
 Sample : 02378-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	8.196	1163	1166	1167	rBV3	261	370	0.00%	0.000%
38	8.226	1169	1171	1174	rVB3	352	356	0.00%	0.000%
39	8.263	1174	1177	1178	rBV2	475	410	0.00%	0.000%
40	8.324	1178	1187	1201	rBV	204949	340500	0.72%	0.177%
41	8.488	1211	1214	1217	rBV3	1066	1400	0.00%	0.001%
42	8.647	1234	1240	1249	rBV	850061	1337180	2.82%	0.696%
43	8.952	1284	1290	1306	rBV	142854	218860	0.46%	0.114%
44	9.122	1315	1318	1321	rVB3	290	352	0.00%	0.000%
45	9.159	1321	1324	1328	rVB3	384	531	0.00%	0.000%
46	9.275	1336	1343	1349	rBV3	6960	11147	0.02%	0.006%
47	9.385	1355	1361	1380	rBV	516469	740478	1.56%	0.386%
48	9.586	1392	1394	1397	rBV3	400	365	0.00%	0.000%
49	9.695	1411	1412	1415	rBV3	320	351	0.00%	0.000%
50	9.811	1428	1431	1433	rVV2	402	431	0.00%	0.000%
51	9.866	1436	1440	1445	rBV3	372	644	0.00%	0.000%
52	9.933	1449	1451	1455	rBV3	323	531	0.00%	0.000%
53	10.086	1465	1476	1482	rBV	29242035	44967262	94.71%	23.414%
54	10.671	1570	1572	1574	rVB3	573	513	0.00%	0.000%
55	10.799	1590	1593	1597	rVB4	1033	1610	0.00%	0.001%
56	10.957	1618	1619	1623	rBV2	590	522	0.00%	0.000%
57	11.189	1652	1657	1670	rBV	586518	802817	1.69%	0.418%
58	11.293	1672	1674	1675	rVV	484	517	0.00%	0.000%
59	11.311	1675	1677	1682	rVV3	1782	2496	0.01%	0.001%
60	11.366	1682	1686	1692	rVV	11990	14609	0.03%	0.008%
61	11.463	1695	1702	1708	rVV3	4665	6982	0.01%	0.004%
62	11.610	1723	1726	1728	rBV2	354	416	0.00%	0.000%
63	11.640	1730	1731	1735	rVB2	435	420	0.00%	0.000%
64	11.683	1735	1738	1739	rBV	348	439	0.00%	0.000%
65	11.707	1739	1742	1746	rVB2	506	676	0.00%	0.000%
66	11.969	1779	1785	1790	rBV	6363369	7765473	16.36%	4.043%
67	12.043	1790	1797	1802	rVV	24365490	33470059	70.49%	17.428%
68	12.219	1823	1826	1831	rVB3	3744	5239	0.01%	0.003%
69	12.341	1837	1846	1851	rBV	29127883	40170154	84.61%	20.916%
70	12.701	1901	1905	1911	rBV7	1620	2778	0.01%	0.001%
71	12.805	1920	1922	1924	rBV2	384	343	0.00%	0.000%
72	12.860	1927	1931	1936	rBV7	3231	5351	0.01%	0.003%
73	12.921	1936	1941	1951	rVB2	34786	46967	0.10%	0.024%
74	13.061	1959	1964	1966	rBV3	8694	12934	0.03%	0.007%
75	13.103	1966	1971	1981	rVV	259702	349570	0.74%	0.182%
76	13.195	1982	1986	1992	rVB	27659	38086	0.08%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035195.D
 Acq On : 20 Apr 2023 01:30
 Operator : JC/MD
 Sample : 02378-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	13.384	2014	2017	2021	rVB4	2377	2886	0.01%	0.002%
78	13.585	2045	2050	2061	rBV	4838023	5980816	12.60%	3.114%
79	13.780	2080	2082	2086	rVB4	1090	1009	0.00%	0.001%
80	13.890	2098	2100	2102	rVB2	651	447	0.00%	0.000%
81	13.963	2106	2112	2129	rVB	1982811	2519299	5.31%	1.312%
82	14.170	2141	2146	2156	rBV2	11782	26332	0.06%	0.014%
83	14.262	2156	2161	2171	rVV	55448	82212	0.17%	0.043%
84	14.341	2172	2174	2187	rVB9	3784	10149	0.02%	0.005%
85	14.506	2196	2201	2206	rBV4	7297	11071	0.02%	0.006%
86	14.560	2208	2210	2211	rVB2	652	352	0.00%	0.000%
87	14.682	2228	2230	2232	rBV3	449	489	0.00%	0.000%
88	14.780	2237	2246	2252	rBV	36531	57438	0.12%	0.030%
89	14.877	2260	2262	2263	rBV	708	391	0.00%	0.000%
90	15.176	2309	2311	2313	rVB2	557	531	0.00%	0.000%
91	15.201	2313	2315	2317	rBV3	517	590	0.00%	0.000%
92	15.249	2317	2323	2330	rVV	102095	141676	0.30%	0.074%
93	15.304	2330	2332	2334	rVB3	619	392	0.00%	0.000%
94	15.615	2380	2383	2386	rBV3	691	723	0.00%	0.000%
95	15.932	2434	2435	2437	rBV2	449	377	0.00%	0.000%
96	16.036	2451	2452	2454	rBV2	591	384	0.00%	0.000%
97	16.274	2489	2491	2493	rVB3	549	424	0.00%	0.000%
98	16.414	2512	2514	2516	rBV2	426	362	0.00%	0.000%
99	16.469	2522	2523	2525	rBV2	578	418	0.00%	0.000%
100	16.517	2527	2531	2534	rVB5	635	1008	0.00%	0.001%




Sum of corrected areas: 192052025

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035195.D
Acq On : 20 Apr 2023 01:30
Operator : JC/MD
Sample : 02378-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

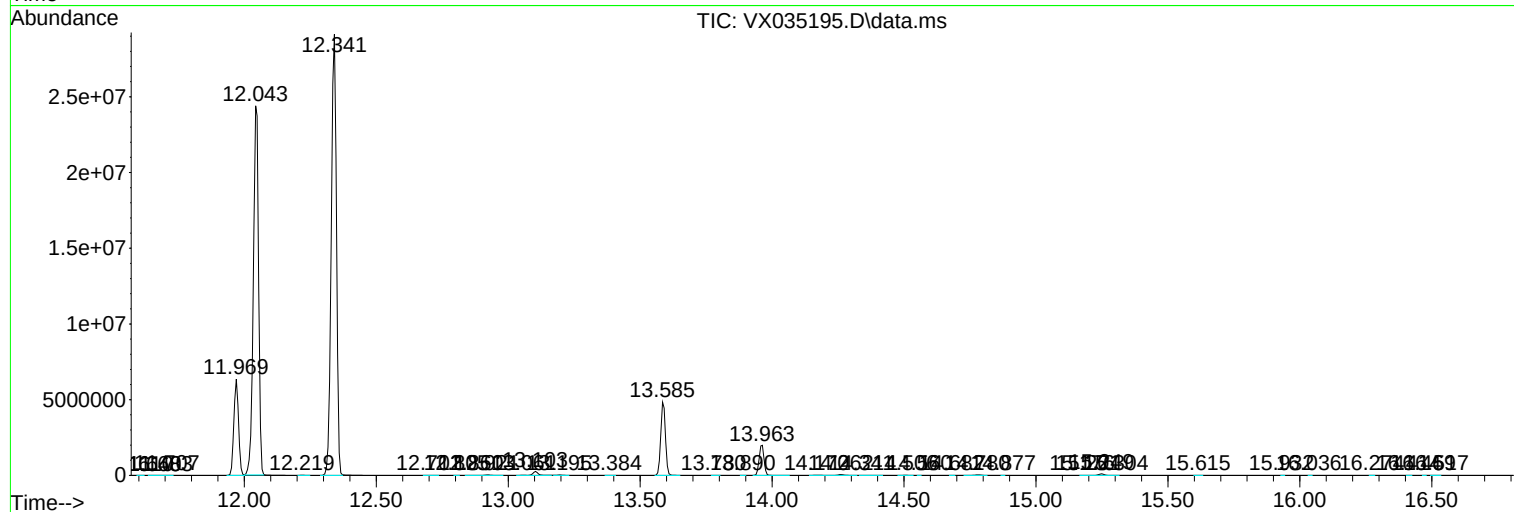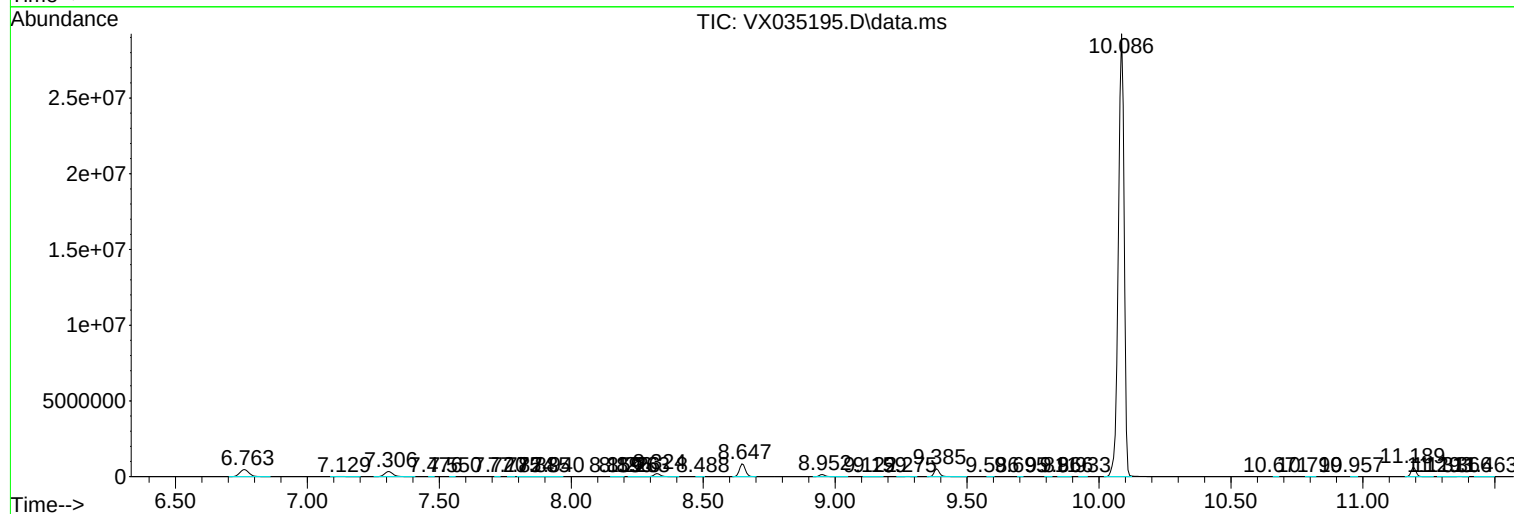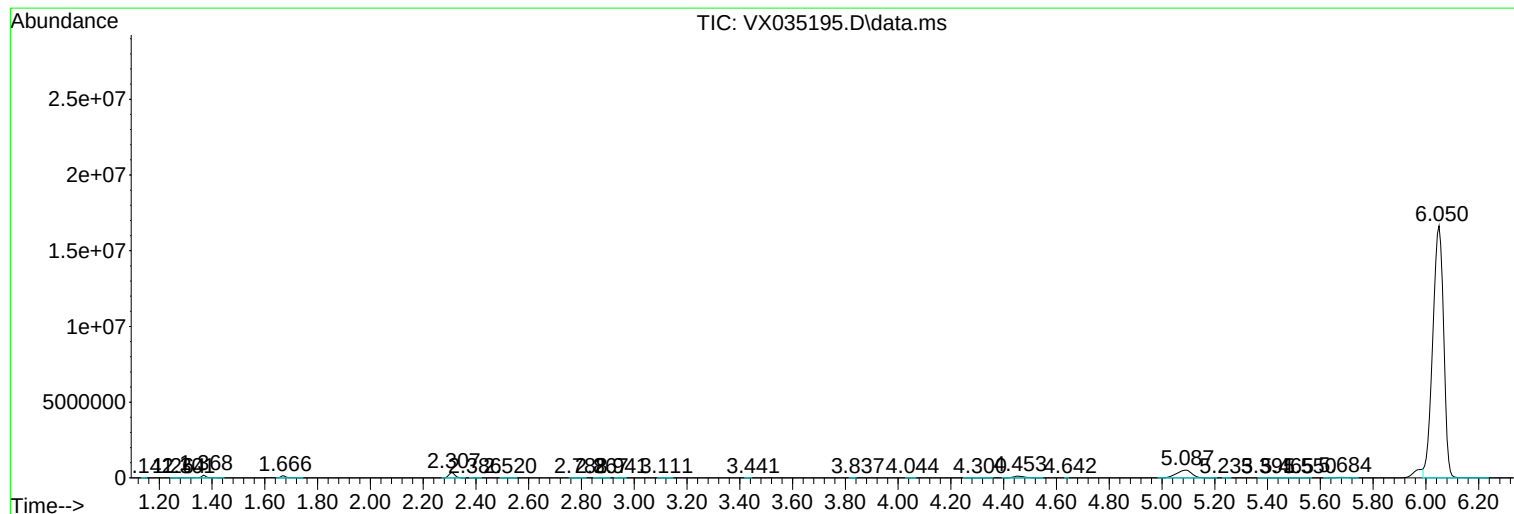

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035195.D
Acq On : 20 Apr 2023 01:30
Operator : JC/MD
Sample : 02378-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0MK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035195.D
Acq On : 20 Apr 2023 01:30
Operator : JC/MD
Sample : 02378-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0MK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc