

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035200.D
 Acq On : 20 Apr 2023 03:25
 Operator : JC/MD
 Sample : 02378-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035200.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	25	29	31	rBV3	3111	4496	0.01%	0.002%
2	1.367	43	46	65	rVB	173876	203877	0.42%	0.108%
3	1.672	92	96	109	rBV	131205	169862	0.35%	0.090%
4	2.306	194	200	210	rBV	321470	501803	1.03%	0.267%
5	2.617	248	251	252	rBV	313	227	0.00%	0.000%
6	2.660	257	258	261	rVB2	560	332	0.00%	0.000%
7	2.684	261	262	265	rBV2	333	271	0.00%	0.000%
8	2.708	265	266	268	rBV2	398	287	0.00%	0.000%
9	2.794	275	280	283	rBV4	1723	2847	0.01%	0.002%
10	2.867	287	292	299	rVV	2702	5489	0.01%	0.003%
11	2.940	299	304	311	rVV3	1569	3492	0.01%	0.002%
12	3.111	326	332	337	rVB6	930	2128	0.00%	0.001%
13	3.214	347	349	352	rVB2	281	309	0.00%	0.000%
14	3.239	352	353	355	rBV2	262	215	0.00%	0.000%
15	3.294	360	362	364	rVB2	381	266	0.00%	0.000%
16	3.324	364	367	368	rBV	387	313	0.00%	0.000%
17	3.464	388	390	391	rVB	338	203	0.00%	0.000%
18	3.507	394	397	400	rBV2	329	507	0.00%	0.000%
19	3.659	421	422	425	rVB2	445	257	0.00%	0.000%
20	3.708	428	430	431	rBV2	271	189	0.00%	0.000%
21	3.757	435	438	441	rBV2	211	293	0.00%	0.000%
22	3.855	452	454	456	rBV2	249	214	0.00%	0.000%
23	3.885	456	459	462	rVB2	268	259	0.00%	0.000%
24	3.970	470	473	476	rBV2	333	384	0.00%	0.000%
25	4.007	478	479	480	rBV	295	184	0.00%	0.000%
26	4.092	491	493	496	rVB3	335	345	0.00%	0.000%
27	4.208	510	512	515	rVV2	309	258	0.00%	0.000%
28	4.239	515	517	519	rVV2	293	322	0.00%	0.000%
29	4.306	519	528	539	rVB2	11114	31130	0.06%	0.017%
30	4.458	544	553	570	rBV2	107634	329463	0.68%	0.175%
31	4.671	586	588	590	rBV2	310	199	0.00%	0.000%
32	4.879	619	622	624	rVB2	257	229	0.00%	0.000%
33	4.903	624	626	627	rBV	429	200	0.00%	0.000%
34	4.921	627	629	631	rVB2	322	180	0.00%	0.000%
35	5.056	636	651	671	rBV	202666	660623	1.36%	0.351%
36	5.299	688	691	692	rBV3	346	337	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035200.D
 Acq On : 20 Apr 2023 03:25
 Operator : JC/MD
 Sample : 02378-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	5.476	712	720	725	rBV5	4201	11431	0.02%	0.006%
38	5.684	742	754	766	rBV4	14535	43920	0.09%	0.023%
39	5.793	768	772	775	rBV3	195	352	0.00%	0.000%
40	5.824	775	777	781	rBV3	523	539	0.00%	0.000%
41	5.976	789	802	803	rBV2	529891	1225983	2.53%	0.652%
42	6.043	805	813	845	rVB	11399049	31313673	64.50%	16.652%
43	6.683	914	918	921	rVB3	369	580	0.00%	0.000%
44	6.763	921	931	948	rBV	448520	1088219	2.24%	0.579%
45	6.909	953	955	957	rBV3	265	241	0.00%	0.000%
46	7.019	970	973	974	rBV3	261	315	0.00%	0.000%
47	7.116	987	989	997	rVB5	3471	5790	0.01%	0.003%
48	7.232	1007	1008	1011	rBV3	149	194	0.00%	0.000%
49	7.305	1011	1020	1039	rVV	324901	741235	1.53%	0.394%
50	7.476	1043	1048	1053	rBV7	1024	1836	0.00%	0.001%
51	7.622	1070	1072	1074	rBV2	281	364	0.00%	0.000%
52	7.653	1074	1077	1079	rVV2	569	504	0.00%	0.000%
53	7.811	1101	1103	1105	rVB2	428	320	0.00%	0.000%
54	7.842	1105	1108	1109	rBV	269	273	0.00%	0.000%
55	7.915	1115	1120	1121	rBV2	369	542	0.00%	0.000%
56	7.933	1121	1123	1124	rBV2	1503	1161	0.00%	0.001%
57	8.104	1150	1151	1152	rBV	589	347	0.00%	0.000%
58	8.220	1167	1170	1173	rVB3	325	389	0.00%	0.000%
59	8.262	1175	1177	1181	rBB3	273	274	0.00%	0.000%
60	8.323	1181	1187	1198	rBV	201372	332717	0.69%	0.177%
61	8.494	1212	1215	1216	rBV2	1084	809	0.00%	0.000%
62	8.646	1234	1240	1250	rBV	807907	1289613	2.66%	0.686%
63	8.951	1284	1290	1303	rBV	143082	215960	0.44%	0.115%
64	9.122	1317	1318	1319	rVB	640	234	0.00%	0.000%
65	9.158	1319	1324	1328	rVB4	399	612	0.00%	0.000%
66	9.274	1337	1343	1349	rBV2	7239	10694	0.02%	0.006%
67	9.384	1356	1361	1377	rBV	510197	724315	1.49%	0.385%
68	9.884	1441	1443	1444	rVV	300	178	0.00%	0.000%
69	9.902	1444	1446	1448	rVB2	290	213	0.00%	0.000%
70	10.085	1465	1476	1482	rBV	30606827	48547852	100.00%	25.816%
71	11.048	1632	1634	1636	rBV2	294	287	0.00%	0.000%
72	11.189	1652	1657	1668	rBV	552442	754713	1.55%	0.401%
73	11.311	1675	1677	1681	rVB4	1002	1356	0.00%	0.001%
74	11.365	1682	1686	1691	rVB	9585	11963	0.02%	0.006%
75	11.457	1698	1701	1710	rVB	4717	7058	0.01%	0.004%
76	11.524	1710	1712	1714	rVV2	239	188	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035200.D
 Acq On : 20 Apr 2023 03:25
 Operator : JC/MD
 Sample : 02378-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041823WMA.M
 Title : VOC Analysis

77	11.554	1715	1717	1719	rVB2	390	227	0.00%	0.000%
78	11.646	1730	1732	1733	rBV	436	320	0.00%	0.000%
79	11.682	1737	1738	1740	rBV2	346	346	0.00%	0.000%
80	11.707	1740	1742	1744	rVV3	668	471	0.00%	0.000%
81	11.835	1761	1763	1764	rBV2	411	305	0.00%	0.000%
82	11.969	1779	1785	1790	rBV	3067354	3797860	7.82%	2.020%
83	12.048	1790	1798	1803	rVV	28599662	39071510	80.48%	20.777%
84	12.341	1838	1846	1851	rBV	32542994	45875703	94.50%	24.395%
85	12.920	1937	1941	1952	rVB	23313	32459	0.07%	0.017%
86	13.060	1959	1964	1968	rBV	14607	27464	0.06%	0.015%
87	13.103	1968	1971	1982	rVV	32344	47596	0.10%	0.025%
88	13.194	1982	1986	1991	rVB2	12028	15889	0.03%	0.008%
89	13.268	1996	1998	1999	rVB2	481	225	0.00%	0.000%
90	13.383	2014	2017	2020	rVB4	2292	2937	0.01%	0.002%
91	13.591	2045	2051	2070	rVB	6435487	8311625	17.12%	4.420%
92	13.963	2106	2112	2122	rVB	1474586	1865635	3.84%	0.992%
93	14.084	2130	2132	2134	rBV2	625	377	0.00%	0.000%
94	14.261	2157	2161	2167	rBV3	7896	10378	0.02%	0.006%
95	14.383	2175	2181	2186	rVB7	2298	4543	0.01%	0.002%
96	14.542	2204	2207	2209	rBV4	863	836	0.00%	0.000%
97	14.621	2217	2220	2224	rBV3	1362	1684	0.00%	0.001%
98	14.779	2239	2246	2253	rBV	147353	214831	0.44%	0.114%
99	15.249	2317	2323	2332	rBV	352218	497002	1.02%	0.264%
100	16.511	2525	2530	2535	rVB3	6367	10404	0.02%	0.006%




Sum of corrected areas: 188049861

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035200.D
Acq On : 20 Apr 2023 03:25
Operator : JC/MD
Sample : 02378-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COML1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

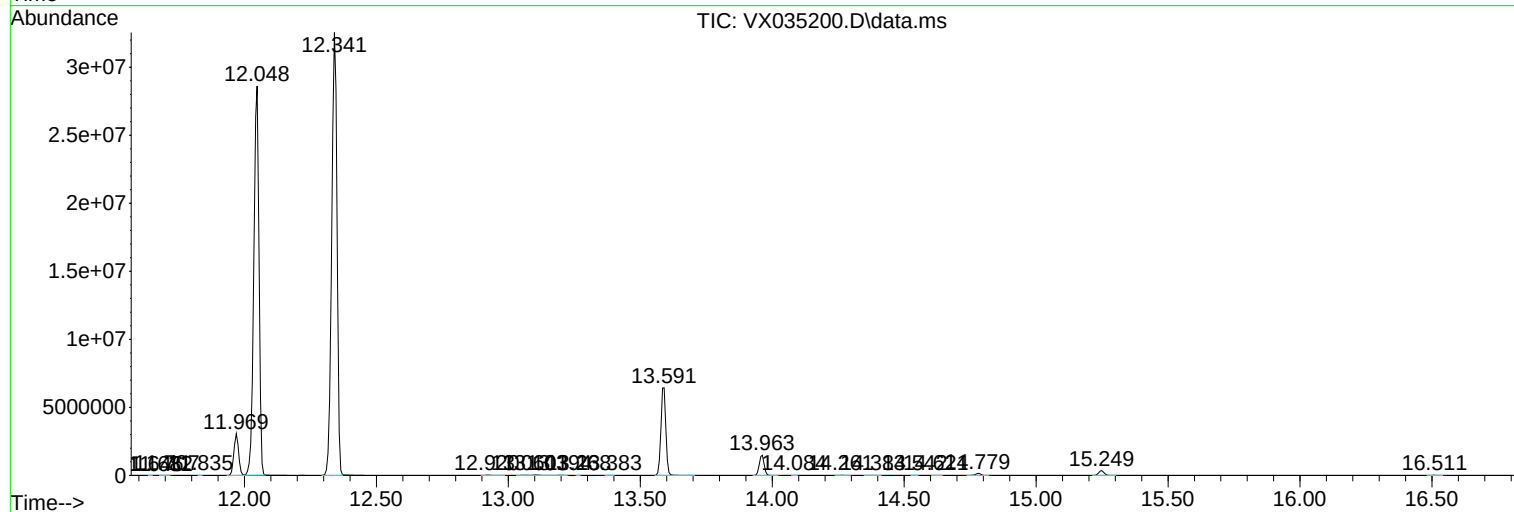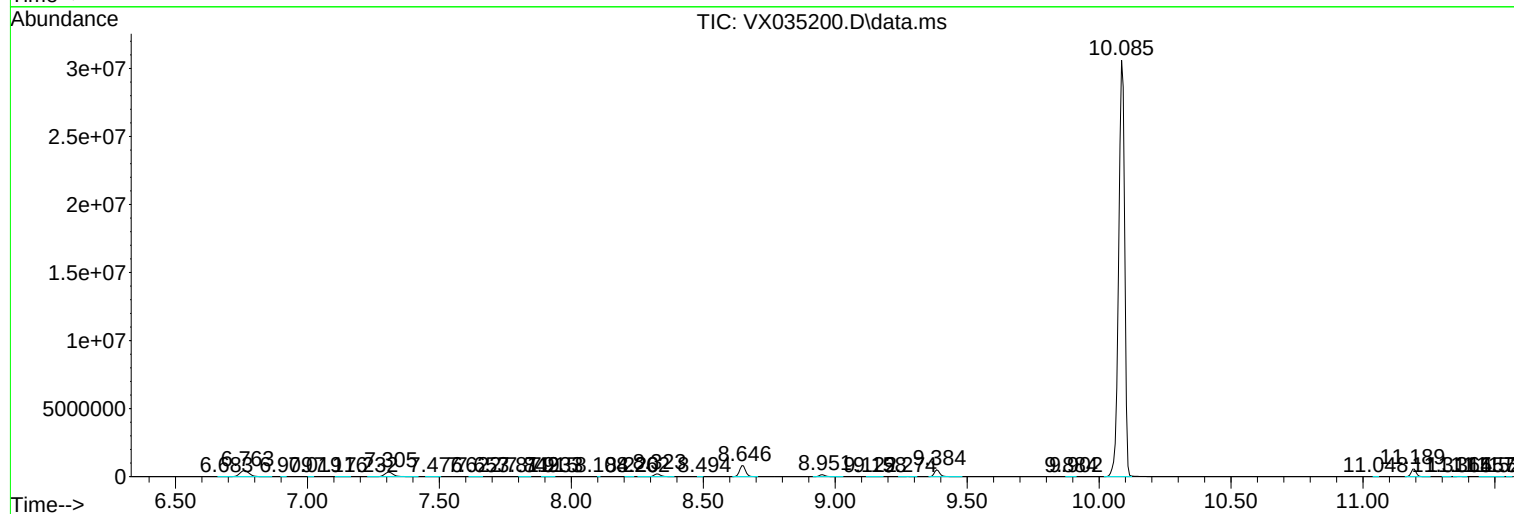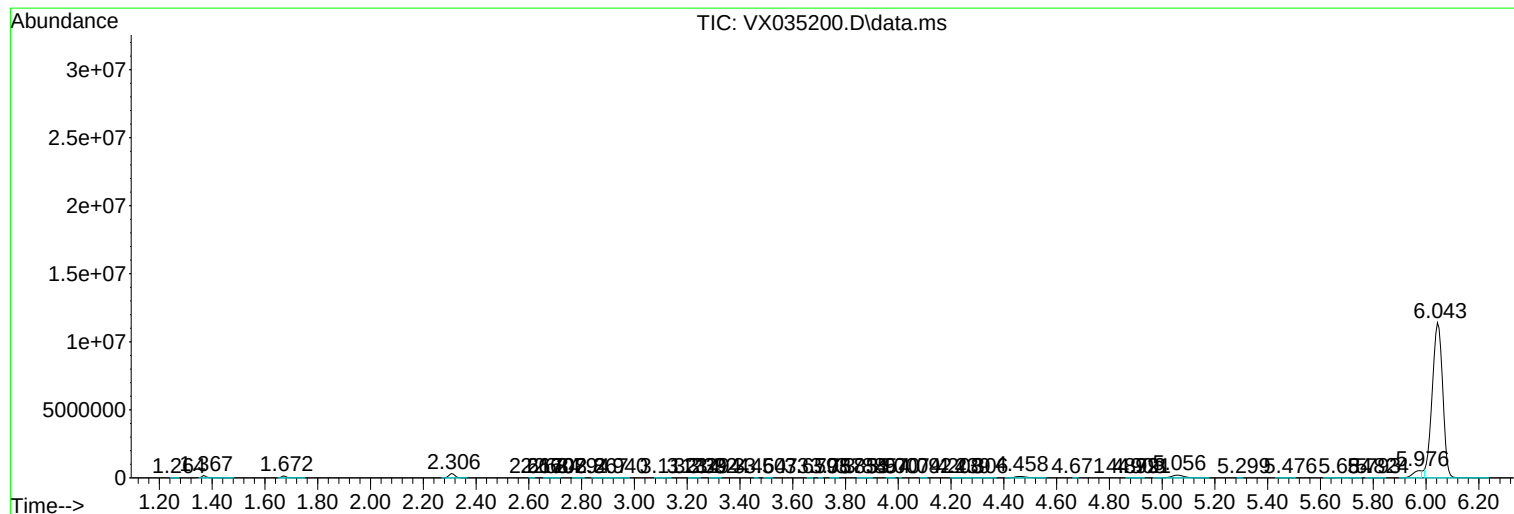

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035200.D
Acq On : 20 Apr 2023 03:25
Operator : JC/MD
Sample : 02378-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ML1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035200.D
Acq On : 20 Apr 2023 03:25
Operator : JC/MD
Sample : 02378-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ML1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------