

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035201.D
 Acq On : 20 Apr 2023 03:48
 Operator : JC/MD
 Sample : 02378-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035201.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.197	17	18	22	rVB	720	454	0.00%	0.000%
2	1.264	25	29	32	rBV3	2999	4397	0.01%	0.002%
3	1.367	42	46	58	rVB	170131	187788	0.33%	0.088%
4	1.672	92	96	113	rVB	134947	181924	0.32%	0.085%
5	1.892	129	132	136	rBV6	1243	1702	0.00%	0.001%
6	2.306	193	200	210	rBV	336290	527826	0.94%	0.247%
7	2.392	211	214	222	rVV3	2706	4789	0.01%	0.002%
8	2.514	230	234	241	rVB	973	1450	0.00%	0.001%
9	2.794	274	280	285	rBV5	1788	3827	0.01%	0.002%
10	2.867	286	292	298	rVB2	3403	6436	0.01%	0.003%
11	2.928	298	302	303	rBV4	573	506	0.00%	0.000%
12	2.946	303	305	309	rVB2	591	642	0.00%	0.000%
13	3.044	319	321	324	rBV2	477	501	0.00%	0.000%
14	3.111	324	332	337	rBV6	1362	3201	0.01%	0.001%
15	3.446	383	387	390	rBV4	505	751	0.00%	0.000%
16	3.513	394	398	402	rBV3	301	577	0.00%	0.000%
17	3.788	438	443	445	rBV3	314	441	0.00%	0.000%
18	4.300	518	527	540	rVB4	13531	40121	0.07%	0.019%
19	4.458	543	553	570	rBV	110421	338594	0.60%	0.158%
20	5.056	639	651	673	rBV	212515	696837	1.24%	0.326%
21	5.391	701	706	708	rBV3	488	761	0.00%	0.000%
22	5.464	711	718	719	rBV2	5010	7386	0.01%	0.003%
23	5.678	743	753	766	rVB2	18789	53898	0.10%	0.025%
24	5.818	771	776	779	rBV3	319	572	0.00%	0.000%
25	5.848	779	781	784	rVB2	419	489	0.00%	0.000%
26	5.976	789	802	803	rBV2	563409	1275310	2.27%	0.597%
27	6.043	804	813	842	rVB	13426003	38020284	67.65%	17.784%
28	6.342	861	862	864	rBV2	672	431	0.00%	0.000%
29	6.617	903	907	909	rVB3	440	594	0.00%	0.000%
30	6.763	919	931	951	rBV	415222	998126	1.78%	0.467%
31	7.116	983	989	999	rVB8	3363	8759	0.02%	0.004%
32	7.305	1011	1020	1031	rBV	340004	759042	1.35%	0.355%
33	7.446	1042	1043	1045	rBV2	392	408	0.00%	0.000%
34	7.488	1045	1050	1059	rVV6	1031	2991	0.01%	0.001%
35	7.659	1074	1078	1082	rVB3	948	1384	0.00%	0.001%
36	7.946	1117	1125	1128	rBV6	1444	2953	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035201.D
 Acq On : 20 Apr 2023 03:48
 Operator : JC/MD
 Sample : 02378-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	8.110	1146	1152	1158	rVB4	797	1497	0.00%	0.001%
38	8.324	1179	1187	1202	rBV	208211	343965	0.61%	0.161%
39	8.482	1210	1213	1214	rBV2	762	593	0.00%	0.000%
40	8.647	1234	1240	1250	rBV	851037	1342891	2.39%	0.628%
41	8.848	1270	1273	1277	rBV4	425	541	0.00%	0.000%
42	8.884	1277	1279	1282	rVB4	435	540	0.00%	0.000%
43	8.951	1284	1290	1308	rBV	144704	222032	0.40%	0.104%
44	9.275	1338	1343	1349	rVB2	8405	12453	0.02%	0.006%
45	9.384	1356	1361	1380	rBV	528503	746834	1.33%	0.349%
46	9.774	1422	1425	1426	rVB3	513	489	0.00%	0.000%
47	10.085	1465	1476	1482	rBV	33617024	56203514	100.00%	26.289%
48	10.476	1538	1540	1545	rVB3	1120	1095	0.00%	0.001%
49	10.982	1618	1623	1625	rVB2	472	541	0.00%	0.000%
50	11.055	1632	1635	1636	rBV2	480	519	0.00%	0.000%
51	11.085	1639	1640	1645	rVB3	683	598	0.00%	0.000%
52	11.189	1651	1657	1667	rBV	580497	784666	1.40%	0.367%
53	11.317	1674	1678	1682	rVB3	1787	2394	0.00%	0.001%
54	11.366	1682	1686	1691	rVB2	11018	14535	0.03%	0.007%
55	11.408	1691	1693	1695	rBV2	558	452	0.00%	0.000%
56	11.457	1695	1701	1706	rBV	5688	7580	0.01%	0.004%
57	11.658	1731	1734	1735	rBV2	304	407	0.00%	0.000%
58	11.713	1738	1743	1745	rVB4	538	747	0.00%	0.000%
59	11.811	1755	1759	1761	rVB4	370	409	0.00%	0.000%
60	11.969	1779	1785	1790	rBV	3642261	4440392	7.90%	2.077%
61	12.048	1790	1798	1803	rBV	32085508	44869354	79.83%	20.987%
62	12.341	1838	1846	1851	rBV	34829820	51260415	91.21%	23.976%
63	12.695	1901	1904	1906	rBV4	960	875	0.00%	0.000%
64	12.872	1930	1933	1936	rBV5	1205	1689	0.00%	0.001%
65	12.920	1937	1941	1946	rVV	23935	31414	0.06%	0.015%
66	13.060	1958	1964	1967	rBV2	10178	17571	0.03%	0.008%
67	13.103	1967	1971	1982	rVV	38357	56104	0.10%	0.026%
68	13.195	1982	1986	1992	rVB2	12386	17440	0.03%	0.008%
69	13.237	1992	1993	1996	rBV2	435	553	0.00%	0.000%
70	13.384	2014	2017	2021	rVB4	2054	2862	0.01%	0.001%
71	13.432	2021	2025	2026	rBV	441	457	0.00%	0.000%
72	13.585	2045	2050	2067	rVB	6287675	7904328	14.06%	3.697%
73	13.780	2077	2082	2089	rVB	2432	3514	0.01%	0.002%
74	13.963	2106	2112	2123	rVB	1299875	1661078	2.96%	0.777%
75	14.042	2123	2125	2129	rBV4	669	816	0.00%	0.000%
76	14.170	2144	2146	2148	rBV2	527	554	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
 Data File : VX035201.D
 Acq On : 20 Apr 2023 03:48
 Operator : JC/MD
 Sample : 02378-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	14.261	2157	2161	2168	rVV2	8557	11495	0.02%	0.005%
78	14.353	2173	2176	2177	rVV2	672	763	0.00%	0.000%
79	14.383	2177	2181	2185	rVV4	1904	2952	0.01%	0.001%
80	14.420	2185	2187	2191	rVB3	729	453	0.00%	0.000%
81	14.505	2198	2201	2204	rVV4	1408	1534	0.00%	0.001%
82	14.548	2205	2208	2211	rVB3	902	1120	0.00%	0.001%
83	14.627	2218	2221	2224	rVB2	1663	1615	0.00%	0.001%
84	14.725	2235	2237	2238	rBV	514	453	0.00%	0.000%
85	14.780	2239	2246	2253	rVV	143611	216581	0.39%	0.101%
86	14.859	2256	2259	2261	rVB4	484	464	0.00%	0.000%
87	14.926	2268	2270	2272	rVB2	650	453	0.00%	0.000%
88	14.969	2275	2277	2282	rVB4	608	762	0.00%	0.000%
89	15.036	2285	2288	2289	rBV2	401	420	0.00%	0.000%
90	15.249	2317	2323	2330	rBV	316194	444950	0.79%	0.208%
91	15.438	2352	2354	2357	rBV3	654	576	0.00%	0.000%
92	15.548	2369	2372	2373	rBV2	677	625	0.00%	0.000%
93	15.645	2386	2388	2390	rBV3	570	511	0.00%	0.000%
94	15.737	2401	2403	2404	rBV2	482	429	0.00%	0.000%
95	15.938	2434	2436	2438	rBV3	591	650	0.00%	0.000%
96	16.304	2495	2496	2499	rVB3	582	453	0.00%	0.000%
97	16.340	2499	2502	2503	rBV2	569	493	0.00%	0.000%
98	16.511	2525	2530	2538	rVB5	6412	11100	0.02%	0.005%
99	16.609	2544	2546	2549	rVB3	655	477	0.00%	0.000%
100	16.737	2566	2567	2570	rVB2	637	486	0.00%	0.000%

Sum of corrected areas: 213794675




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035201.D
Acq On : 20 Apr 2023 03:48
Operator : JC/MD
Sample : 02378-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COML2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

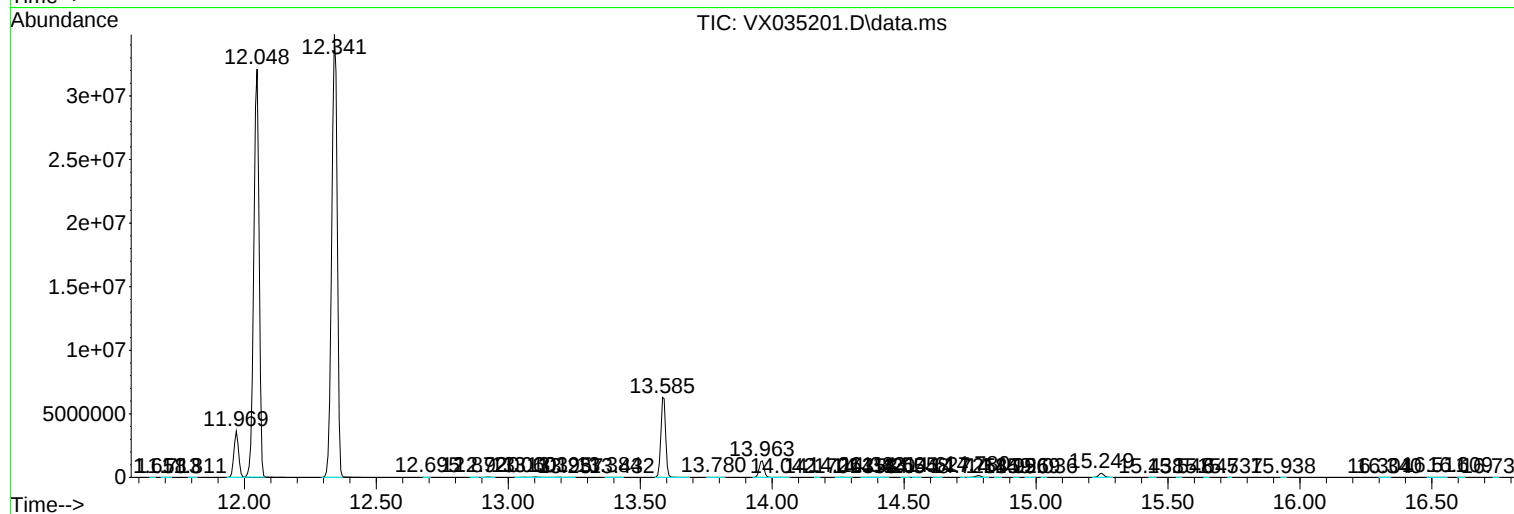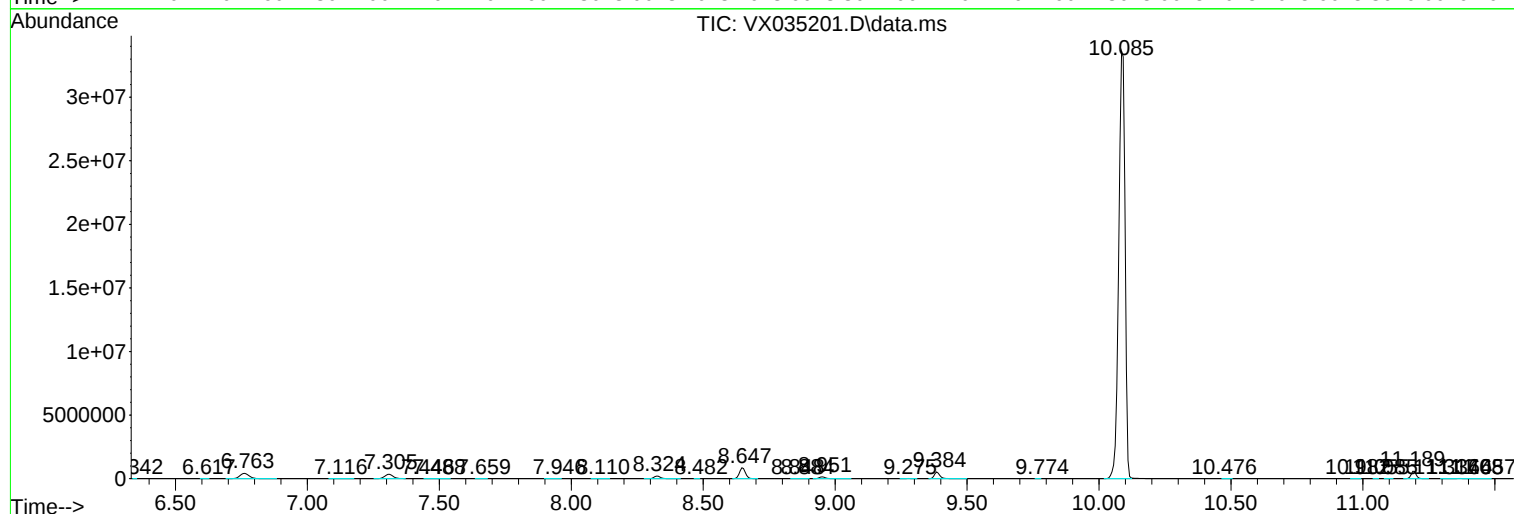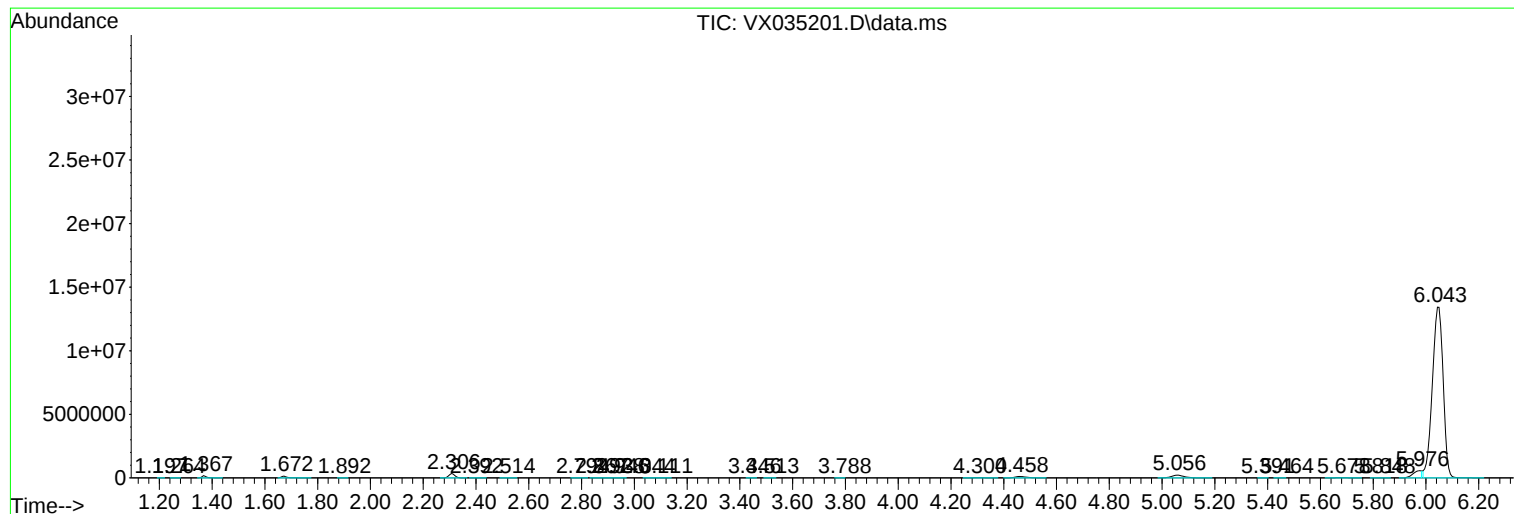

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035201.D
Acq On : 20 Apr 2023 03:48
Operator : JC/MD
Sample : 02378-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ML2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041923\
Data File : VX035201.D
Acq On : 20 Apr 2023 03:48
Operator : JC/MD
Sample : 02378-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ML2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc