

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041924\
 Data File : VX041175.D
 Acq On : 19 Apr 2024 14:04
 Operator : JC/MD
 Sample : P2121-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 1348RE

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041624W.M
 Title : SW846 8260

Signal : TIC: VX041175.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.294	31	34	42	rVB	59877	69268	1.54%	0.090%
2	1.453	56	60	68	rBV	120206	154554	3.43%	0.201%
3	2.300	192	199	208	rBV	26135	50030	1.11%	0.065%
4	2.404	208	216	241	rVV	262372	640133	14.20%	0.834%
5	4.239	508	517	530	rBV2	31205	95102	2.11%	0.124%
6	4.404	532	544	563	rVV2	11742	54336	1.20%	0.071%
7	4.574	563	572	602	rVV	48300	179420	3.98%	0.234%
8	5.385	692	705	720	rBV2	96874	288729	6.40%	0.376%
9	5.544	720	731	755	rVV	171254	514826	11.42%	0.671%
10	5.952	789	798	817	rBV	98601	269338	5.97%	0.351%
11	6.757	921	930	946	rVB	251570	605343	13.42%	0.789%
12	7.470	1041	1047	1061	rBV	27065	80346	1.78%	0.105%
13	7.647	1071	1076	1090	rVB3	16648	48093	1.07%	0.063%
14	8.647	1234	1240	1248	rBV	527437	814705	18.07%	1.062%
15	9.445	1364	1371	1380	rBV	27466	52927	1.17%	0.069%
16	9.537	1380	1386	1396	rVV2	23917	52779	1.17%	0.069%
17	10.055	1462	1471	1486	rBV	516201	735120	16.30%	0.958%
18	10.774	1583	1589	1595	rBV	37129	51641	1.15%	0.067%
19	11.079	1635	1639	1649	rVB	431470	579334	12.85%	0.755%
20	11.482	1700	1705	1712	rVB	45136	67573	1.50%	0.088%
21	11.671	1731	1736	1740	rBV	32448	49001	1.09%	0.064%
22	12.024	1789	1794	1802	rBV	564071	736217	16.33%	0.959%
23	12.146	1802	1814	1821	rVV8	20690	65110	1.44%	0.085%
24	12.420	1856	1859	1862	rBV	41964	45479	1.01%	0.059%
25	12.798	1912	1921	1928	rBV8	62810	143745	3.19%	0.187%
26	12.920	1938	1941	1944	rBV	45186	49410	1.10%	0.064%
27	12.963	1944	1948	1954	rVB	113864	172710	3.83%	0.225%
28	13.024	1954	1958	1959	rBV2	36390	46630	1.03%	0.061%
29	13.164	1974	1981	1985	rBV3	105390	172858	3.83%	0.225%
30	13.213	1985	1989	1992	rBV2	79458	98024	2.17%	0.128%
31	13.268	1992	1998	1999	rBV3	242937	353004	7.83%	0.460%
32	13.292	1999	2002	2006	rVV2	318472	439655	9.75%	0.573%
33	13.341	2006	2010	2019	rVB	2731483	3242085	71.89%	4.225%
34	13.420	2019	2023	2033	rVB3	378898	766335	16.99%	0.999%
35	13.506	2033	2037	2039	rBV2	74722	101041	2.24%	0.132%
36	13.548	2039	2044	2047	rBV	1166840	1411239	31.29%	1.839%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041924\
 Data File : VX041175.D
 Acq On : 19 Apr 2024 14:04
 Operator : JC/MD
 Sample : P2121-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 1348RE

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041624W.M
 Title : SW846 8260

37	13.579	2047	2049	2057	rVB3	188072	306810	6.80%	0.400%
38	13.670	2060	2064	2067	rBV3	123110	182213	4.04%	0.237%
39	13.713	2067	2071	2078	rBV5	187938	303828	6.74%	0.396%
40	13.774	2078	2081	2087	rVB	121790	181542	4.03%	0.237%
41	13.853	2087	2094	2100	rVB5	329427	809315	17.95%	1.055%
42	13.926	2100	2106	2111	rBV3	265359	528479	11.72%	0.689%
43	14.006	2116	2119	2120	rBV	62215	63360	1.41%	0.083%
44	14.036	2120	2124	2127	rVB3	297677	326272	7.24%	0.425%
45	14.073	2127	2130	2134	rBV2	280866	374352	8.30%	0.488%
46	14.146	2138	2142	2144	rBV	485409	643501	14.27%	0.839%
47	14.176	2144	2147	2151	rVV	2771291	3014608	66.85%	3.929%
48	14.225	2151	2155	2158	rVV3	1143695	1890204	41.92%	2.463%
49	14.262	2158	2161	2167	rVB	3274297	4058504	90.00%	5.289%
50	14.323	2167	2171	2176	rBV2	1202162	2167833	48.07%	2.825%
51	14.371	2176	2179	2184	rVB	3954078	4509544	100.00%	5.877%
52	14.475	2192	2196	2201	rBV2	1199638	1961810	43.50%	2.557%
53	14.591	2210	2215	2217	rBV	1130412	1471338	32.63%	1.918%
54	14.633	2217	2222	2225	rVV2	1094560	1992025	44.17%	2.596%
55	14.670	2225	2228	2233	rVB2	733608	1009693	22.39%	1.316%
56	14.725	2233	2237	2239	rBV5	180945	227719	5.05%	0.297%
57	14.780	2239	2246	2251	rBV4	754710	1625367	36.04%	2.118%
58	14.829	2251	2254	2258	rVV3	522572	916565	20.33%	1.195%
59	14.871	2258	2261	2262	rVV	590765	676610	15.00%	0.882%
60	14.902	2262	2266	2270	rVV2	1058716	1719270	38.13%	2.241%
61	14.987	2270	2280	2288	rVV3	1884970	3453614	76.58%	4.501%
62	15.109	2292	2300	2303	rVV	2733042	4300253	95.36%	5.604%
63	15.146	2303	2306	2309	rVV	2039296	2957267	65.58%	3.854%
64	15.182	2309	2312	2314	rVV3	1159179	1746270	38.72%	2.276%
65	15.207	2314	2316	2319	rVV2	834808	944471	20.94%	1.231%
66	15.255	2319	2324	2326	rVV3	311065	637843	14.14%	0.831%
67	15.310	2328	2333	2336	rVV	1299359	2347404	52.05%	3.059%
68	15.365	2336	2342	2353	rVV4	1490030	4425397	98.13%	5.767%
69	15.481	2356	2361	2371	rVV5	940554	2741566	60.79%	3.573%
70	15.566	2371	2375	2378	rVV2	385674	810452	17.97%	1.056%
71	15.615	2378	2383	2386	rVV	1065359	2068995	45.88%	2.696%
72	15.645	2386	2388	2398	rVV2	829768	1568775	34.79%	2.044%
73	15.743	2400	2404	2407	rVV3	261789	556345	12.34%	0.725%
74	15.780	2407	2410	2414	rVV2	385284	675696	14.98%	0.881%
75	15.841	2417	2420	2427	rVV4	277943	707191	15.68%	0.922%
76	15.908	2428	2431	2437	rVV	278701	474284	10.52%	0.618%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041924\
Data File : VX041175.D
Acq On : 19 Apr 2024 14:04
Operator : JC/MD
Sample : P2121-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1348RE

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041624W.M

Title : SW846 8260

77	15.987	2440	2444	2455	rVB4	340001	819447	18.17%	1.068%
78	16.084	2456	2460	2469	rBV6	134125	385260	8.54%	0.502%
79	16.170	2470	2474	2482	rVB2	255049	499979	11.09%	0.652%
80	16.255	2483	2488	2493	rBV2	133434	247514	5.49%	0.323%
81	16.414	2511	2514	2519	rBV4	24533	48074	1.07%	0.063%
82	16.657	2550	2554	2557	rBV	31775	58857	1.31%	0.077%




Sum of corrected areas: 76731856

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041924\
Data File : VX041175.D
Acq On : 19 Apr 2024 14:04
Operator : JC/MD
Sample : P2121-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1348RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041624W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

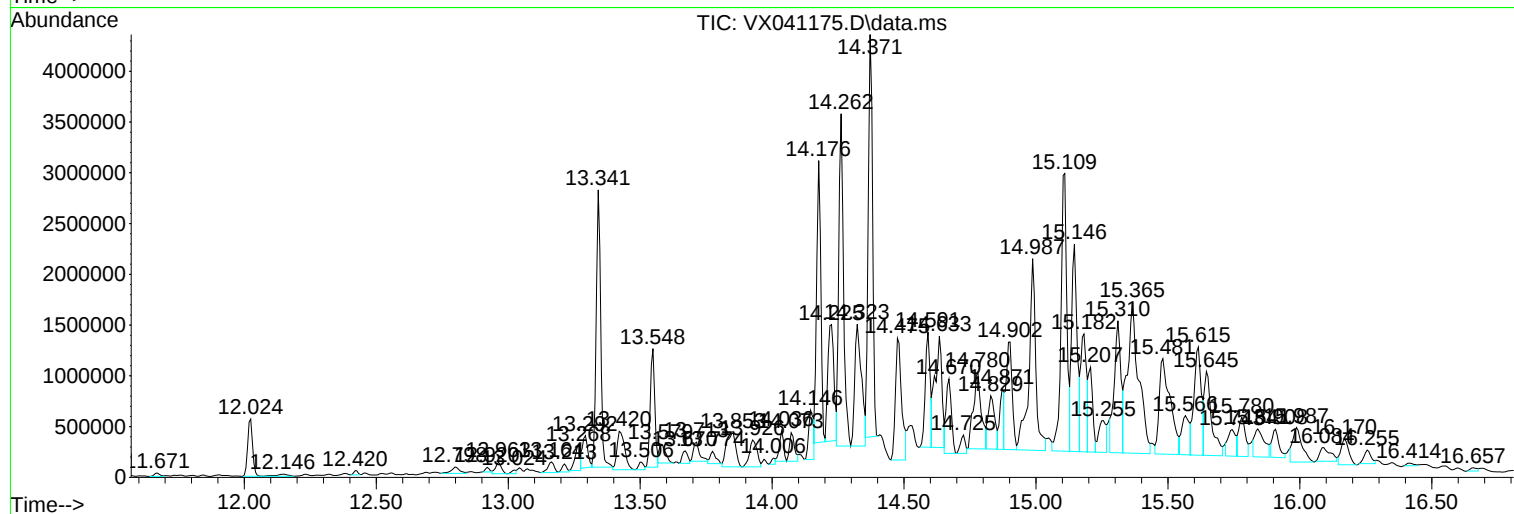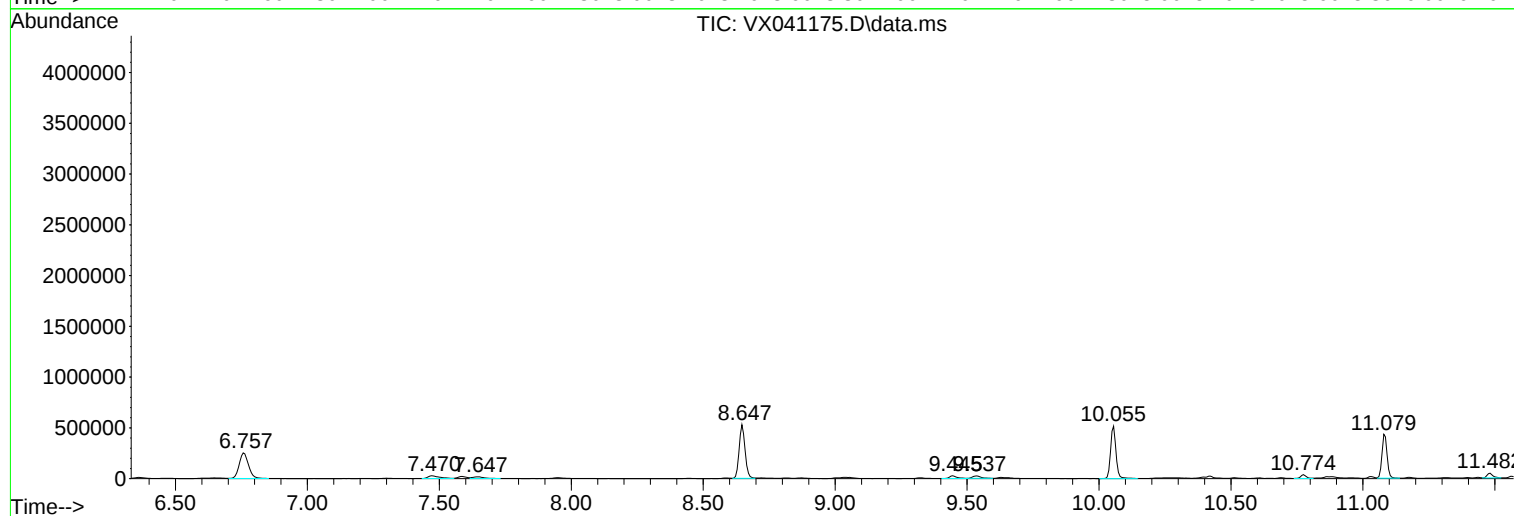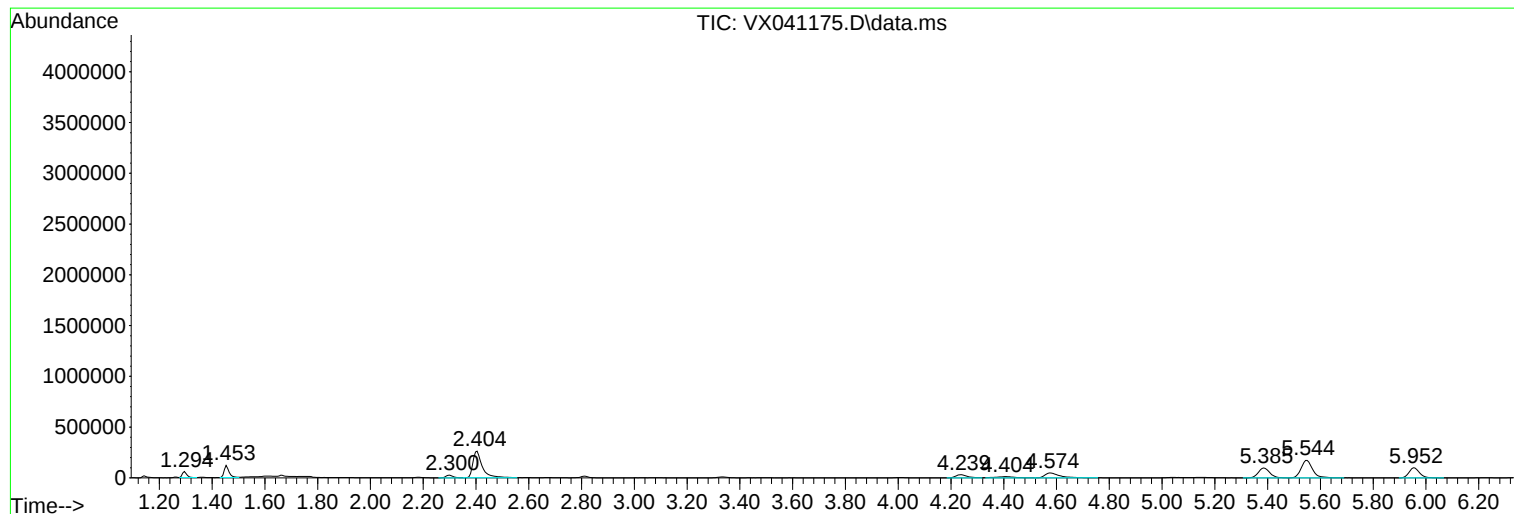

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041924\
Data File : VX041175.D
Acq On : 19 Apr 2024 14:04
Operator : JC/MD
Sample : P2121-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1348RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041624W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041924\
Data File : VX041175.D
Acq On : 19 Apr 2024 14:04
Operator : JC/MD
Sample : P2121-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1348RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041624W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------