



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041924\
Data File : VX041165.D
Acq On : 19 Apr 2024 08:58
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041624W.M
Title : SW846 8260
Last Update : Wed Apr 17 02:04:44 2024

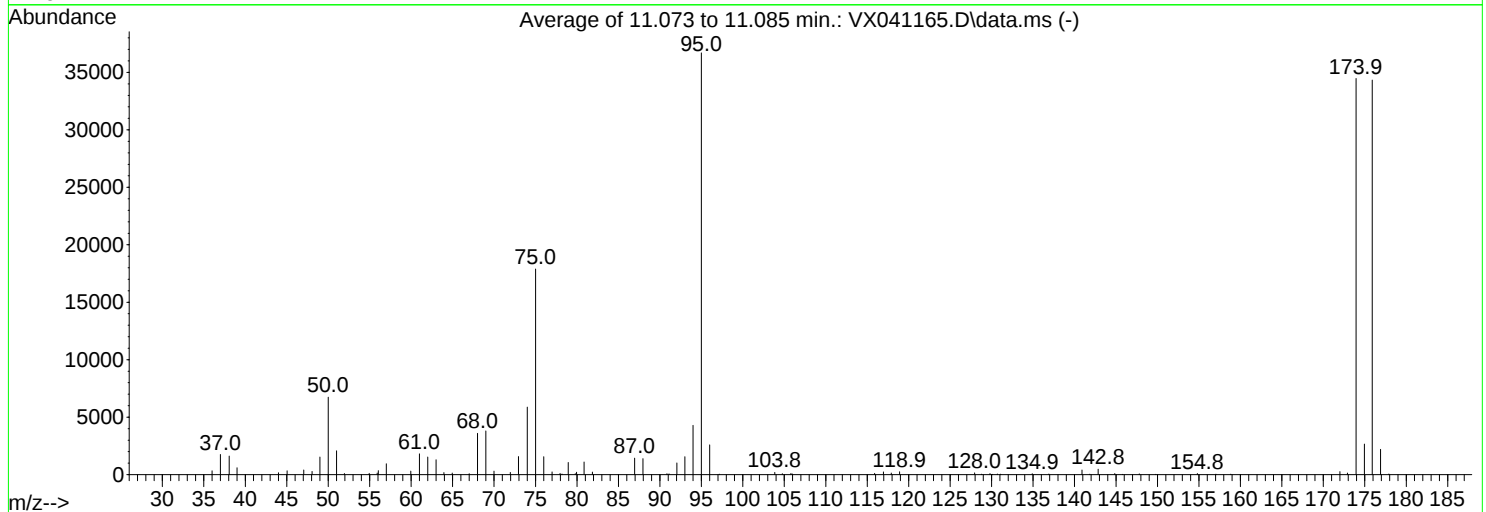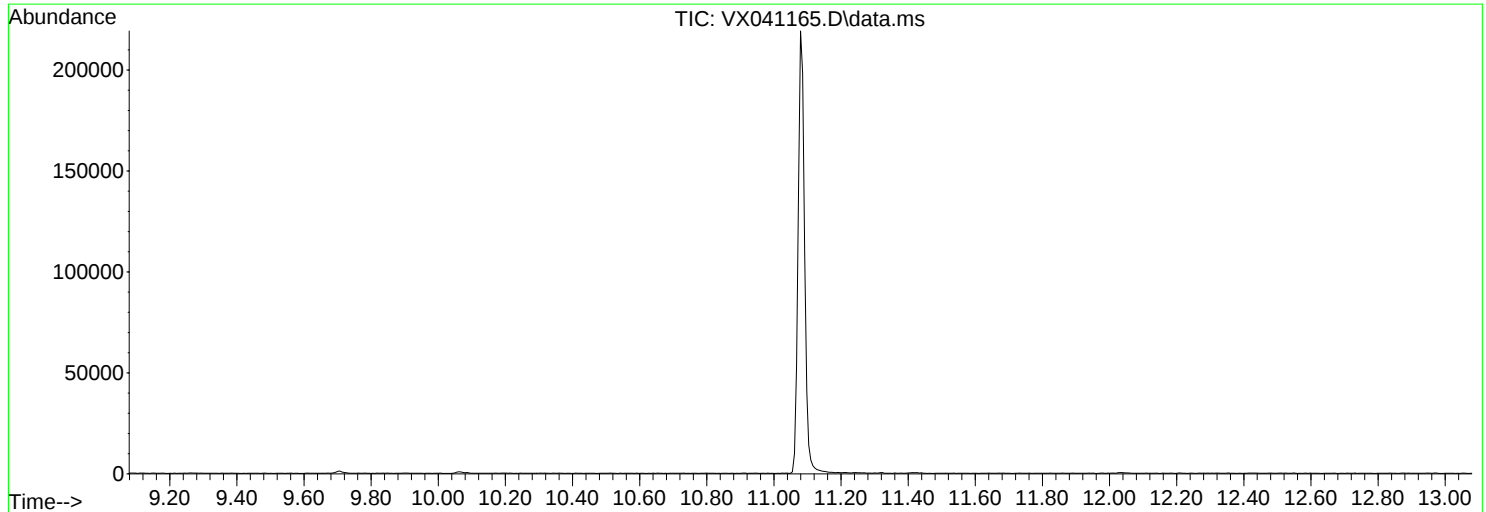

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	6740	PASS
75	95	30	60	48.7	17890	PASS
95	95	100	100	100.0	36699	PASS
96	95	5	9	7.1	2590	PASS
173	174	0.00	2	0.4	143	PASS
174	95	50	100	93.9	34469	PASS
175	174	5	9	7.7	2665	PASS
176	174	95	101	99.6	34325	PASS
177	176	5	9	6.4	2207	PASS