


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX042020\  
Data File : VX015756.D  
Acq On : 20 Apr 2020 09:41  
Operator : JC/SP  
Sample : BFB  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X032720W.M  
Title : SW846 8260  
Last Update : Fri Mar 27 09:35:51 2020

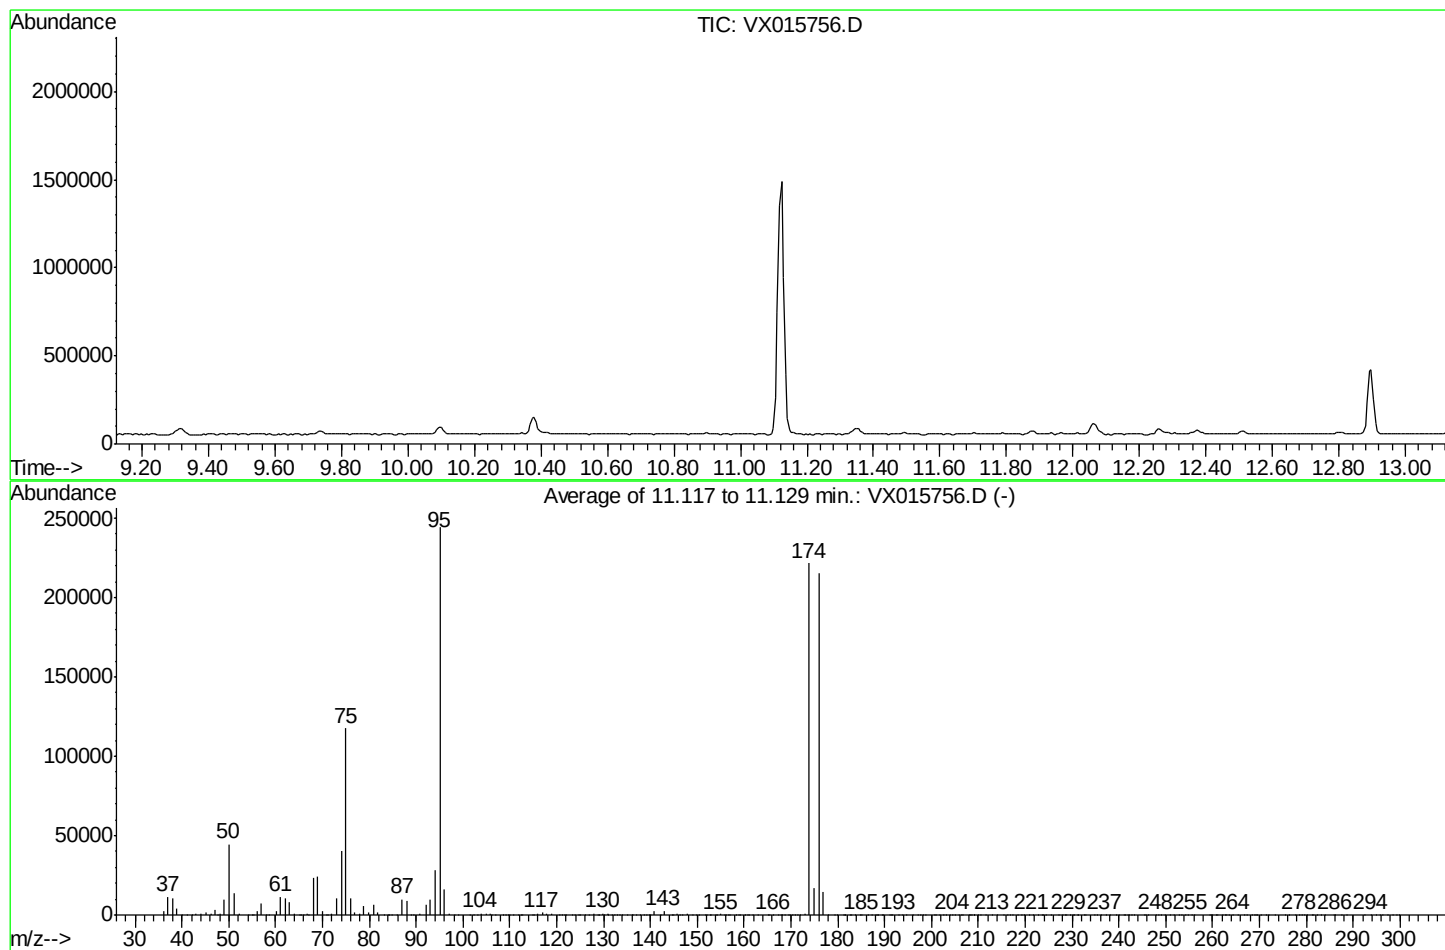

AutoFind: Scans 1678, 1679, 1680; Background Corrected with Scan 1671

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 18.3      | 44780   | PASS             |
| 75          | 95           | 30           | 60           | 48.2      | 117664  | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 244267  | PASS             |
| 96          | 95           | 5            | 9            | 6.5       | 15831   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.5       | 1042    | PASS             |
| 174         | 95           | 50           | 100          | 90.7      | 221525  | PASS             |
| 175         | 174          | 5            | 9            | 7.6       | 16828   | PASS             |
| 176         | 174          | 95           | 101          | 97.1      | 215138  | PASS             |
| 177         | 176          | 5            | 9            | 6.7       | 14416   | PASS             |