


Chloromethane

Response Ratio

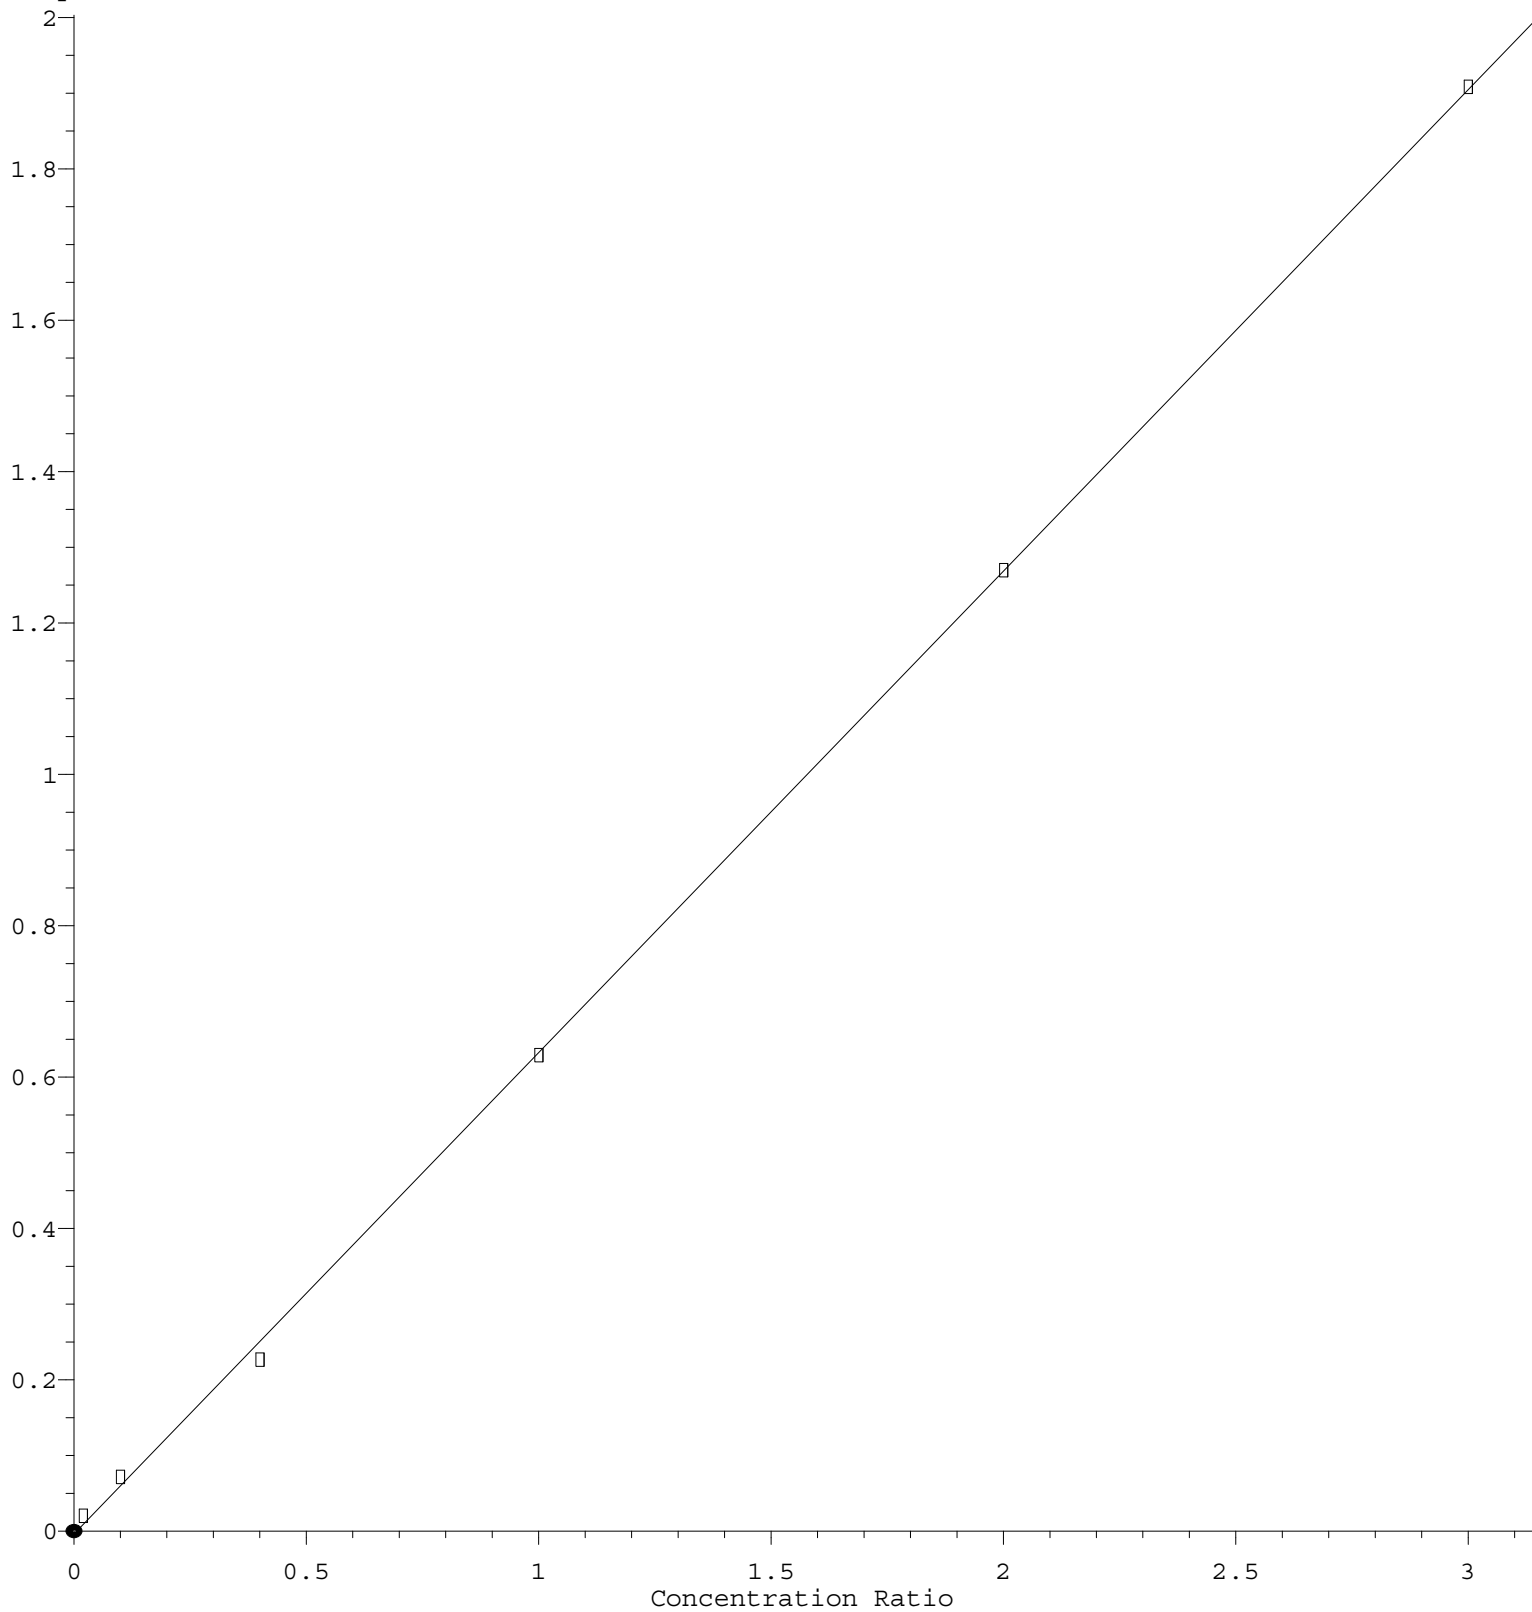

$$\text{Response} = 6.363\text{e-}001 * \text{Amt} - 3.849\text{e-}003$$


Coef of Det (r^2) = 0.999695 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X042021W.M

Calibration Table Last Updated: Tue Apr 20 13:46:22 2021

Methyl Iodide

Response Ratio

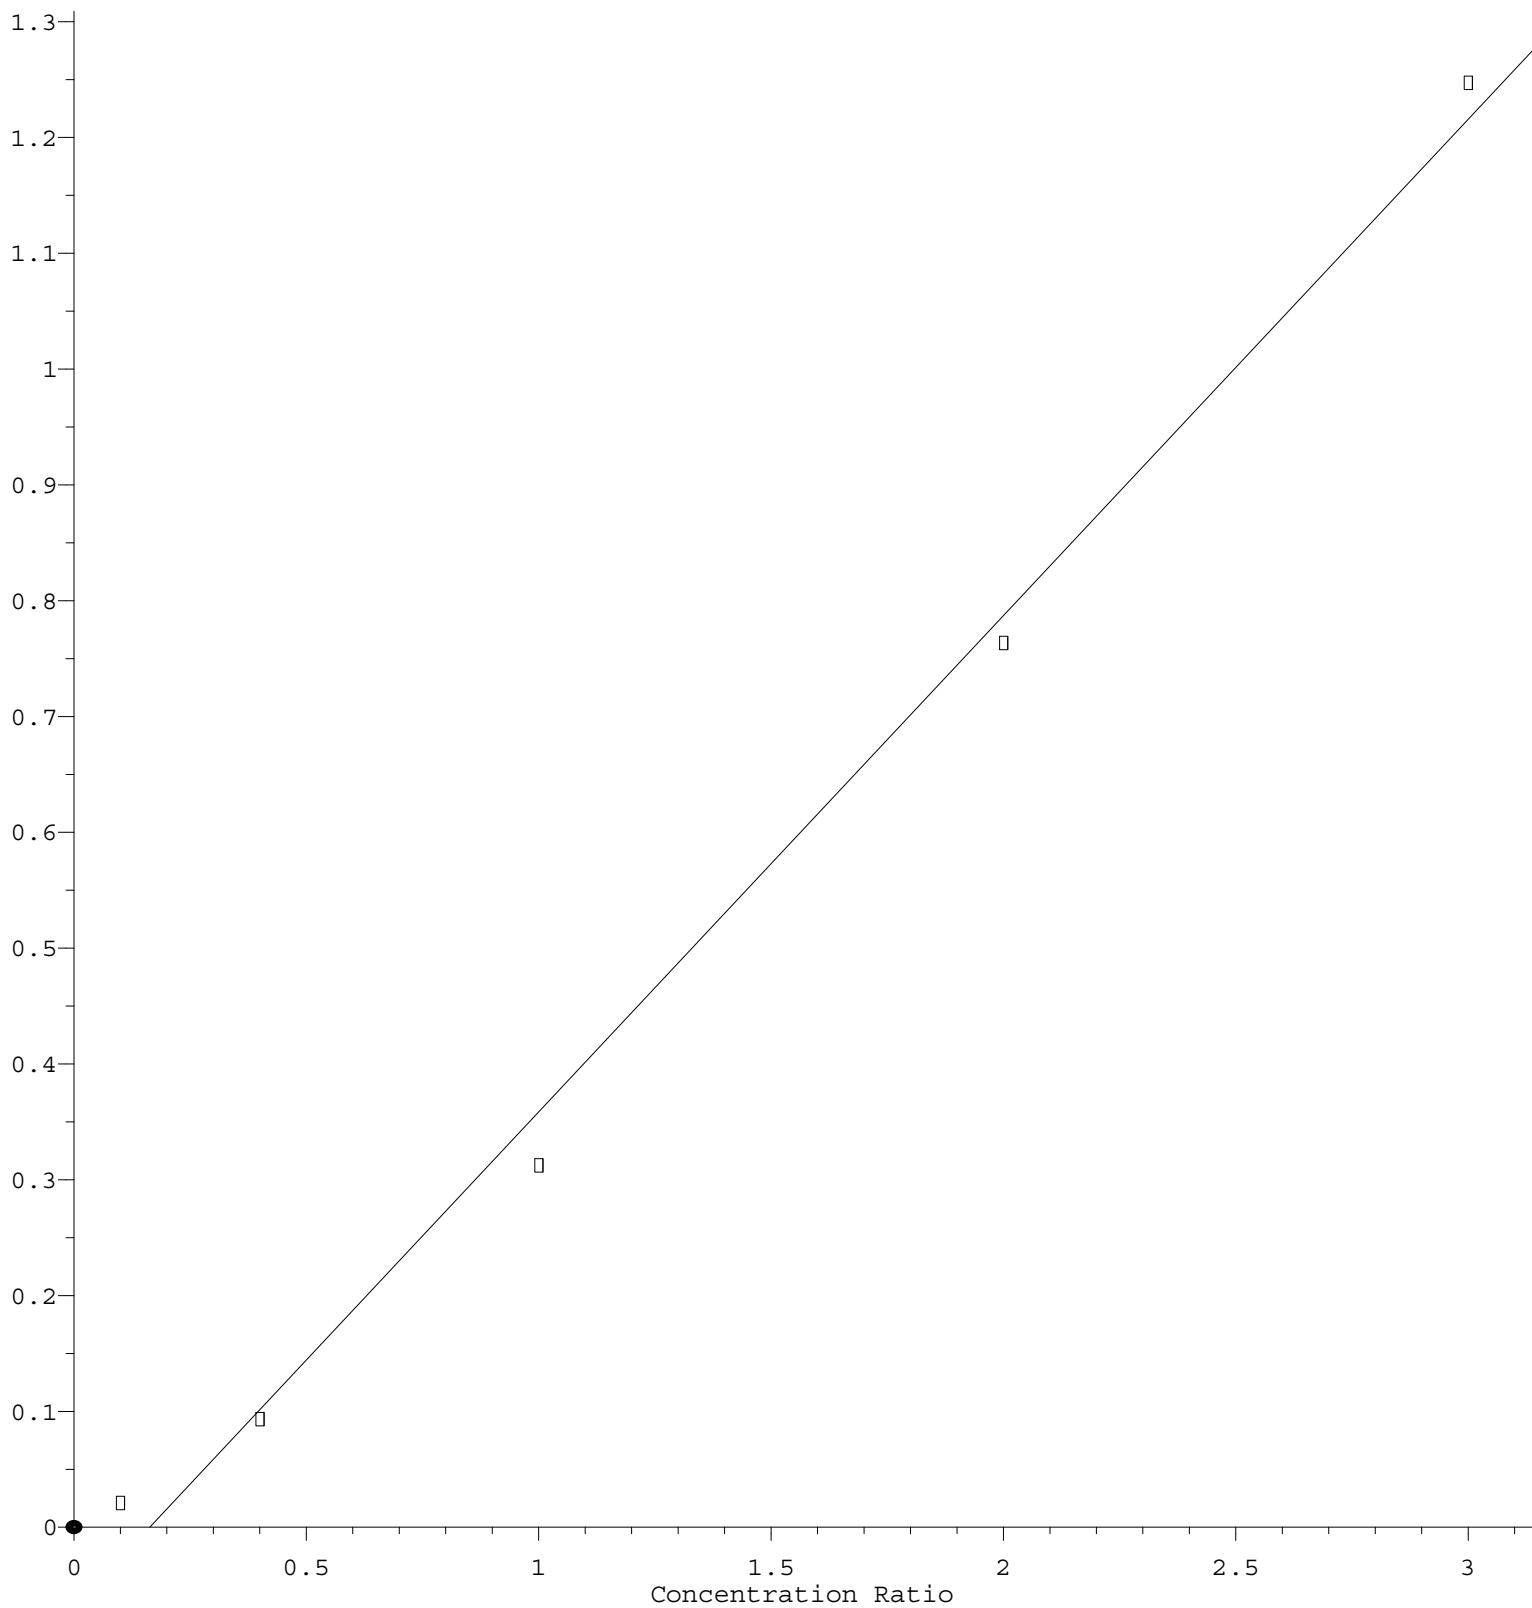

$$\text{Response} = 4.286\text{e-}001 * \text{Amt} - 6.982\text{e-}002$$

Coef of Det (r^2) = 0.994272 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X042021W.M

Calibration Table Last Updated: Tue Apr 20 13:46:22 2021