

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042021\
 Data File : VX021763.D
 Acq On : 20 Apr 2021 19:05
 Operator : JC/MD
 Sample : M2064-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-5

Quant Time: Apr 21 11:23:00 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 20 13:46:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.629	168	154337	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.830	114	258606	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.092	117	225389	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.061	152	97003	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.031	65	87820	50.16	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	100.32%
35) Dibromofluoromethane	5.465	113	82078	49.63	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.26%
50) Toluene-d8	8.696	98	306672	48.23	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	96.46%
62) 4-Bromofluorobenzene	11.116	95	105466	44.41	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	88.82%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042021\
Data File : VX021763.D
Acq On : 20 Apr 2021 19:05
Operator : JC/MD
Sample : M2064-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Time: Apr 21 11:23:00 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 20 13:46:22 2021
Response via : Initial Calibration




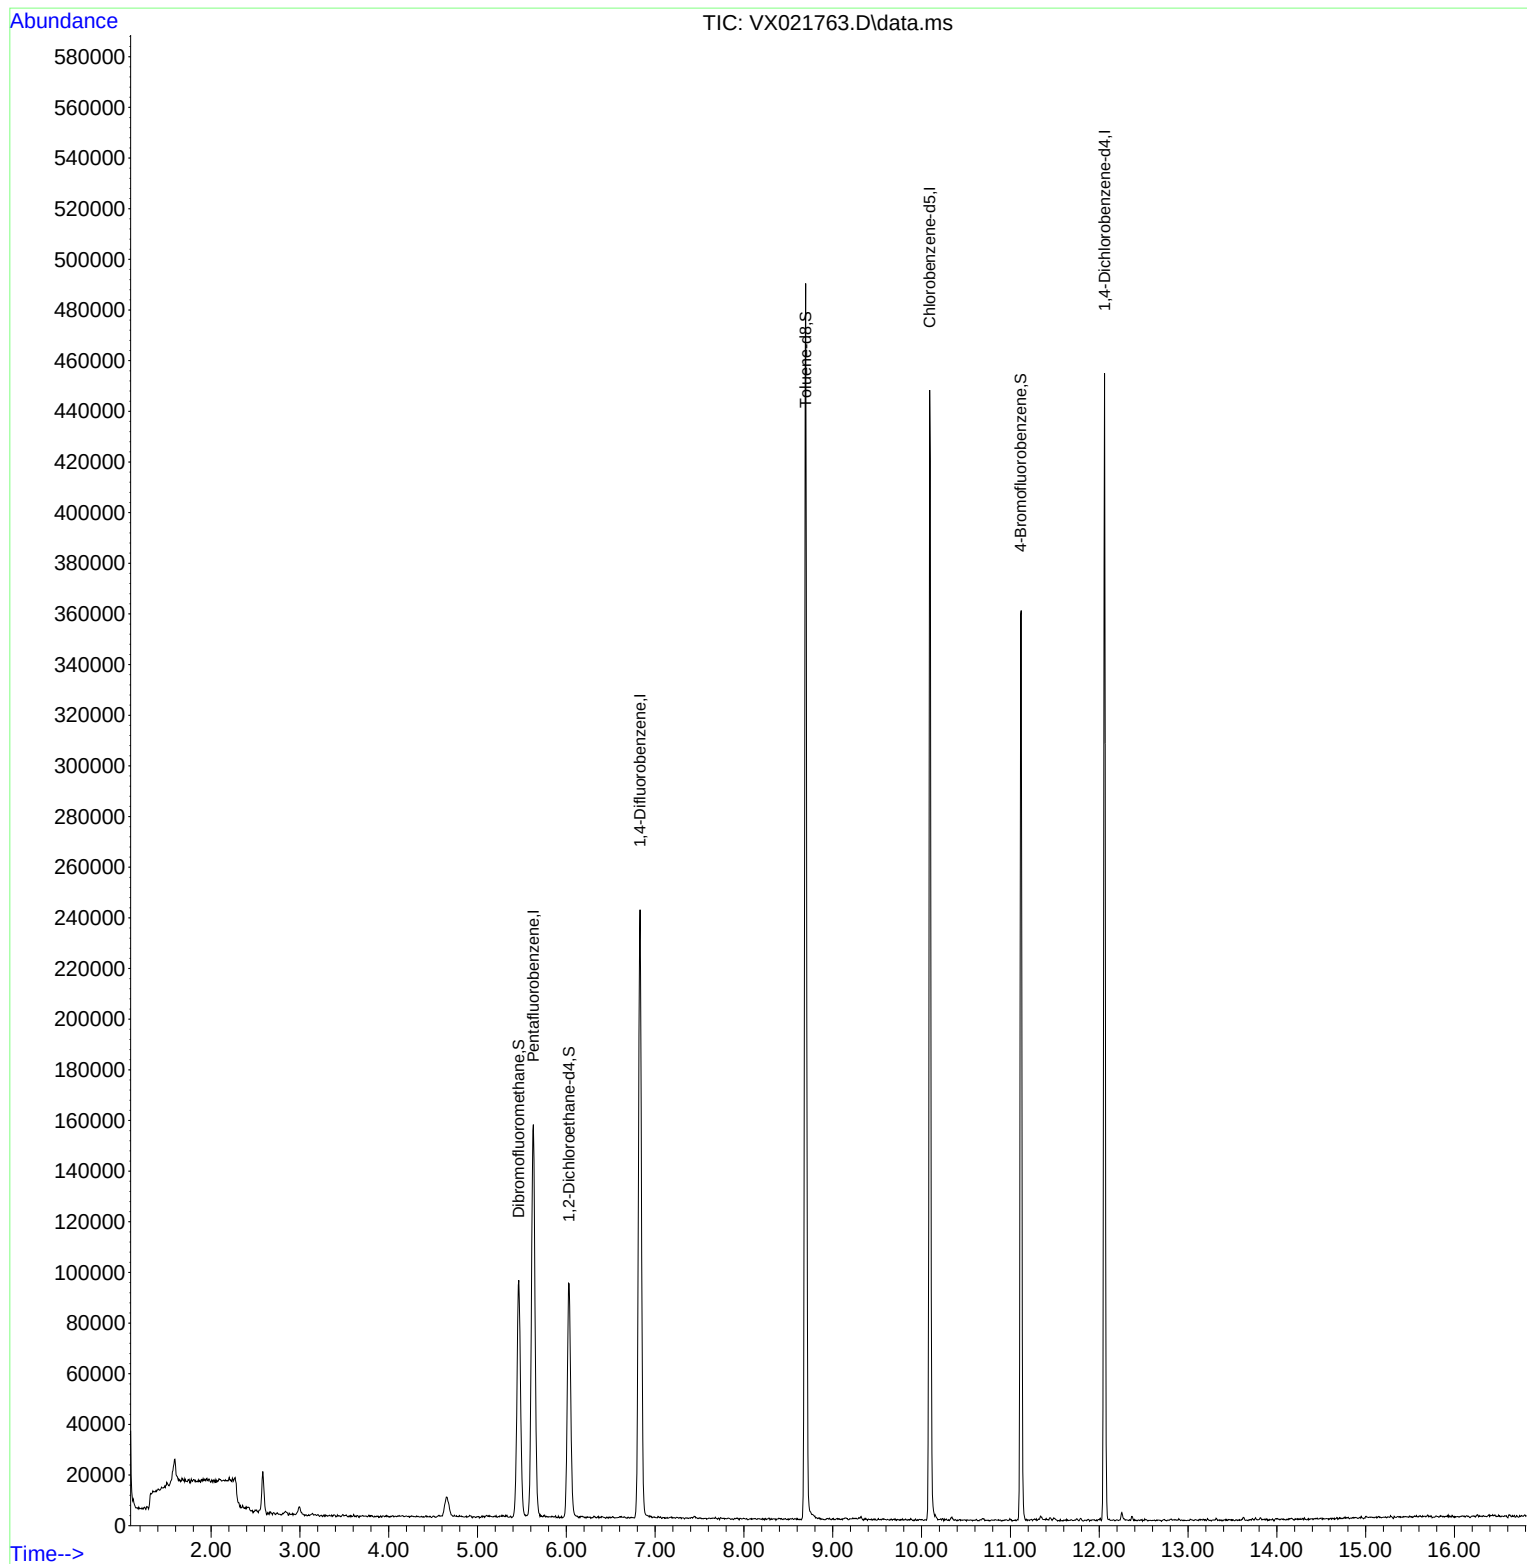


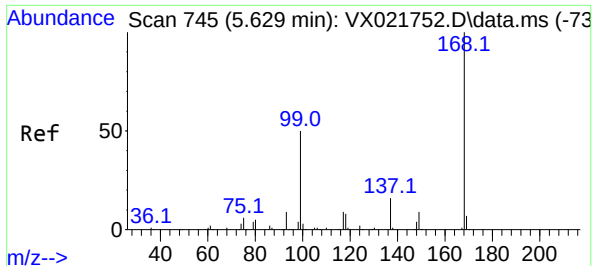

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.629 min Scan# 745
Delta R.T. 0.000 min
Lab File: VX021763.D
Acq: 20 Apr 2021 19:05




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion:168 Resp: 154337
Ion Ratio Lower Upper
168 100
99 54.5 45.8 68.6

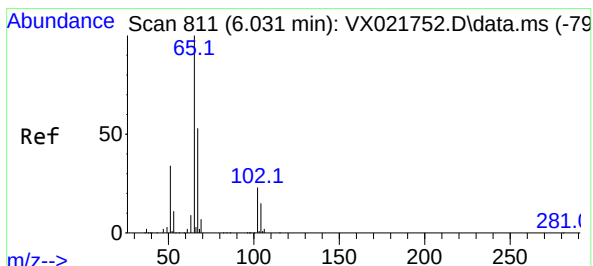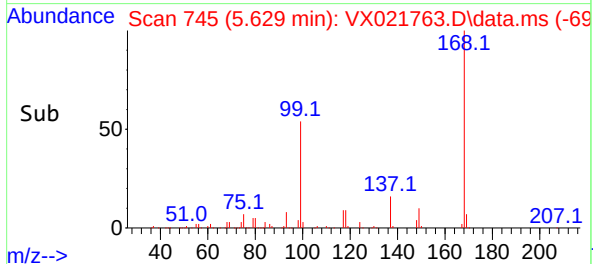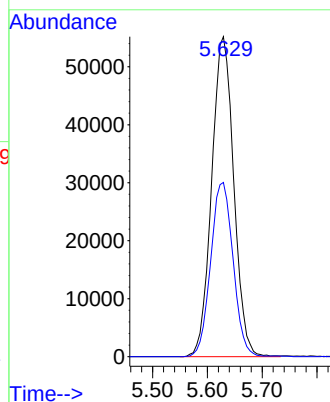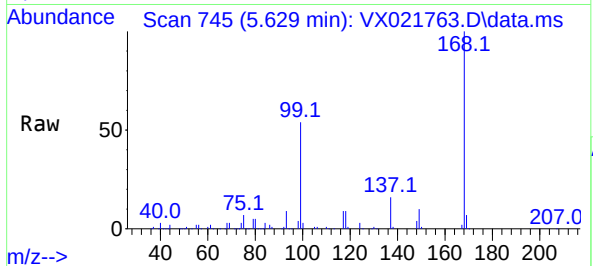

#33
1,2-Dichloroethane-d4
Concen: 50.16 ug/l
RT: 6.031 min Scan# 811
Delta R.T. 0.000 min
Lab File: VX021763.D
Acq: 20 Apr 2021 19:05

Tgt Ion: 65 Resp: 87820
Ion Ratio Lower Upper
65 100
67 54.4 0.0 105.4


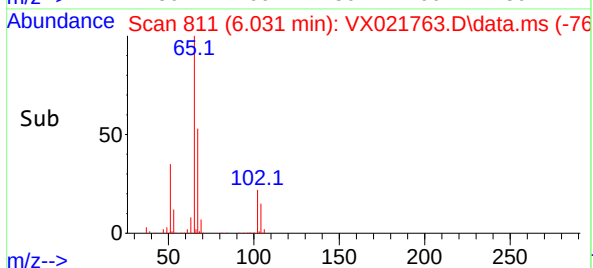
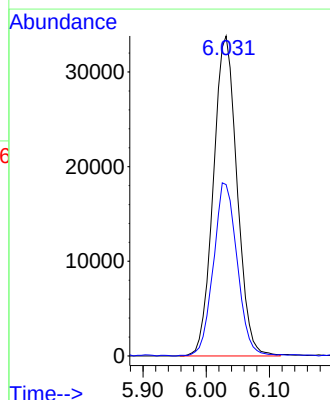
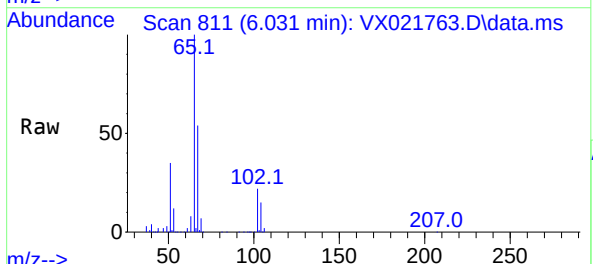


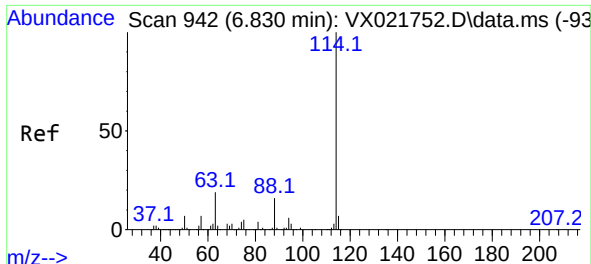

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.830 min Scan# 942
Delta R.T. 0.000 min
Lab File: VX021763.D
Acq: 20 Apr 2021 19:05




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion:	114	Resp:	258606
Ion	Ratio	Lower	Upper
114	100		
63	18.8	0.0	40.8
88	15.9	0.0	32.8

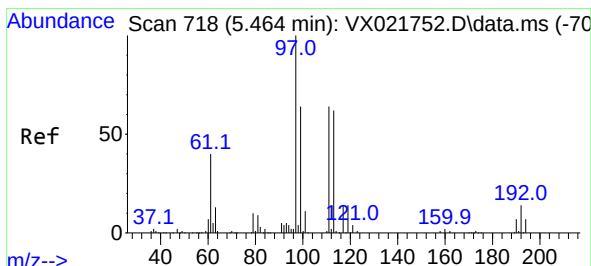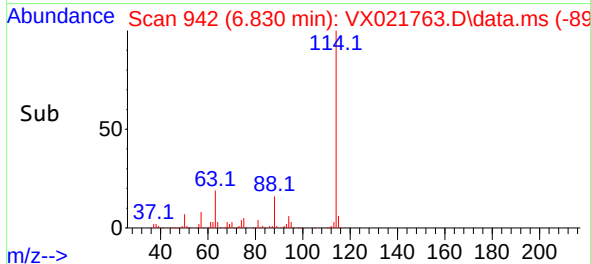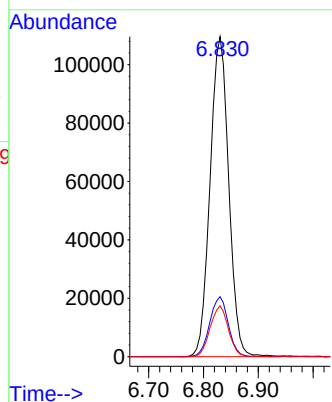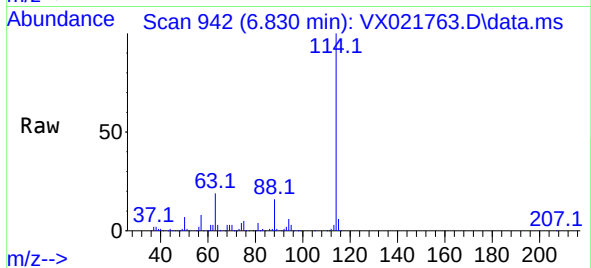

#35
Dibromofluoromethane
Concen: 49.63 ug/l
RT: 5.465 min Scan# 718
Delta R.T. 0.000 min
Lab File: VX021763.D
Acq: 20 Apr 2021 19:05

Tgt Ion:	113	Resp:	82078
Ion	Ratio	Lower	Upper
113	100		
111	101.3	81.9	122.9
192	20.8	16.7	25.1


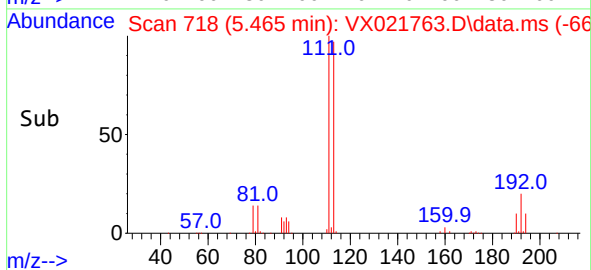
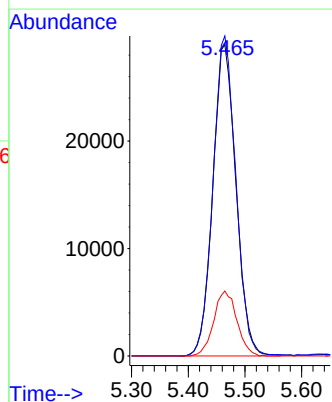
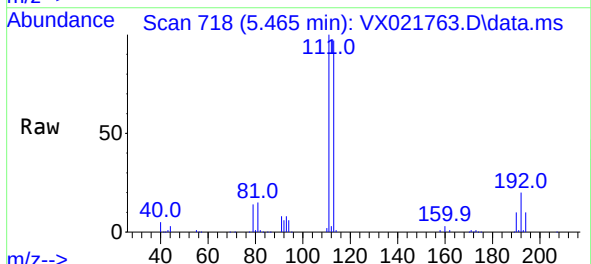


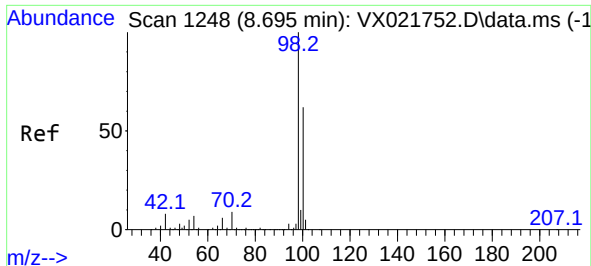

#50
Toluene-d8
Concen: 48.23 ug/l
RT: 8.696 min Scan# 1248
Delta R.T. 0.001 min
Lab File: VX021763.D
Acq: 20 Apr 2021 19:05




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion: 98 Resp: 306672
Ion Ratio Lower Upper
98 100
100 64.6 51.9 77.9

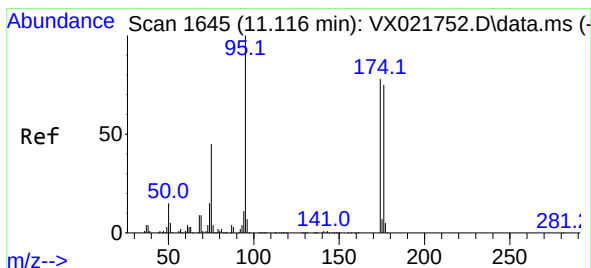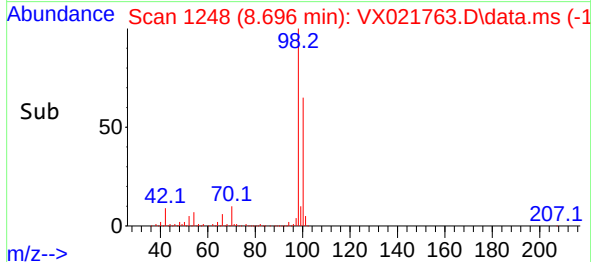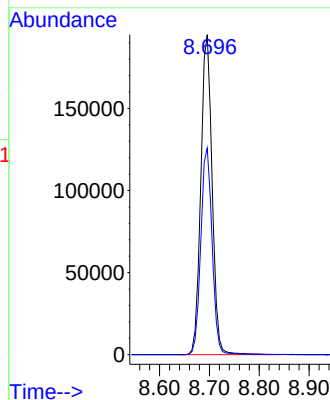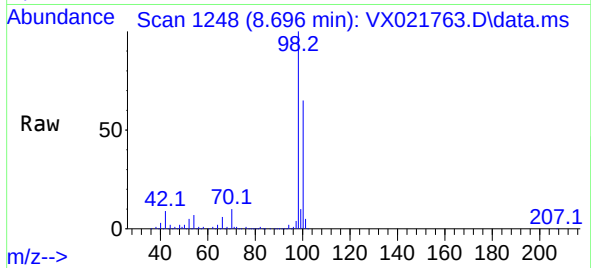

#62
4-Bromofluorobenzene
Concen: 44.41 ug/l
RT: 11.116 min Scan# 1645
Delta R.T. -0.000 min
Lab File: VX021763.D
Acq: 20 Apr 2021 19:05

Tgt Ion: 95 Resp: 105466
Ion Ratio Lower Upper
95 100
174 80.8 0.0 154.6
176 77.9 0.0 155.8


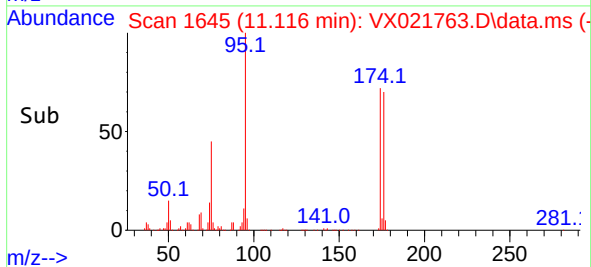
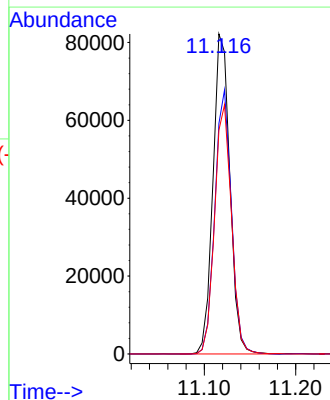
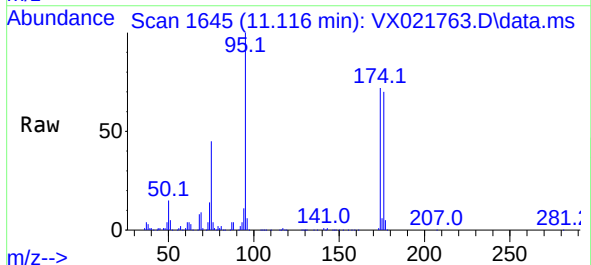


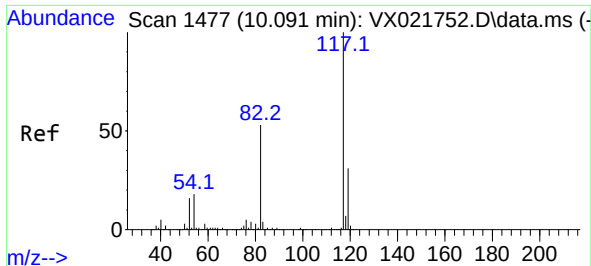

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.092 min Scan# 1477
Delta R.T. 0.001 min
Lab File: VX021763.D
Acq: 20 Apr 2021 19:05

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Tgt Ion:117 Resp: 225389
Ion Ratio Lower Upper
117 100
82 51.6 47.4 71.2
119 31.4 26.6 39.8

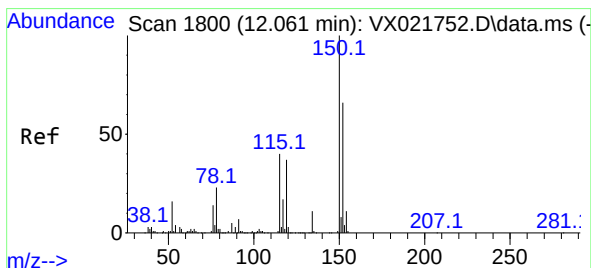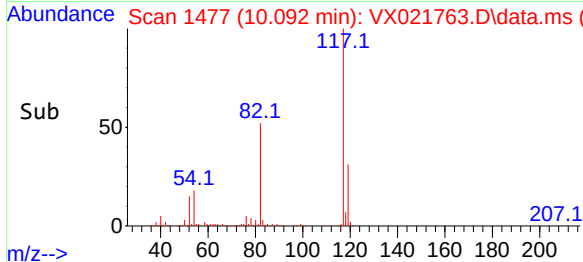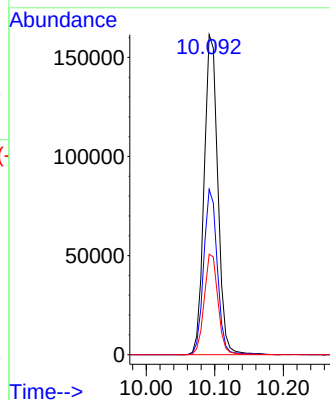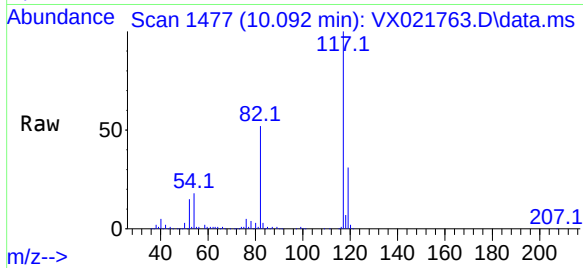

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.061 min Scan# 1800
Delta R.T. -0.000 min
Lab File: VX021763.D
Acq: 20 Apr 2021 19:05

Tgt Ion:152 Resp: 97003
Ion Ratio Lower Upper
152 100
115 59.1 41.1 123.3
150 156.4 0.0 349.0

