
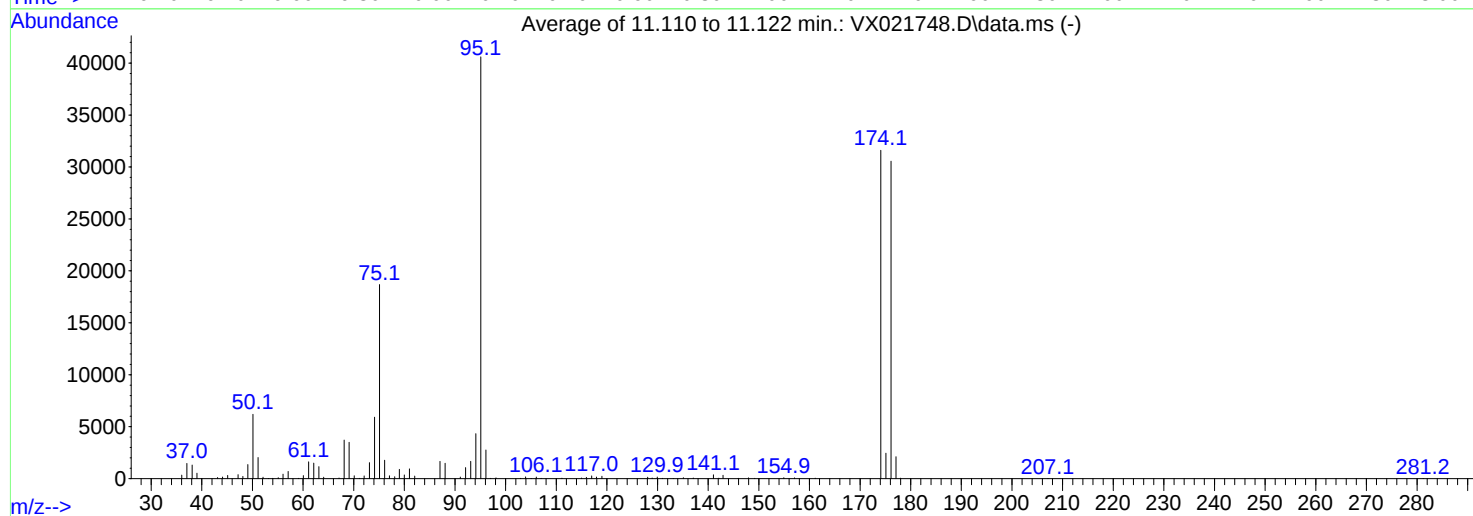


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042021\
 Data File : VX021748.D
 Acq On : 20 Apr 2021 10:46
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
 Title : SW846 8260
 Last Update : Tue Apr 20 13:46:22 2021

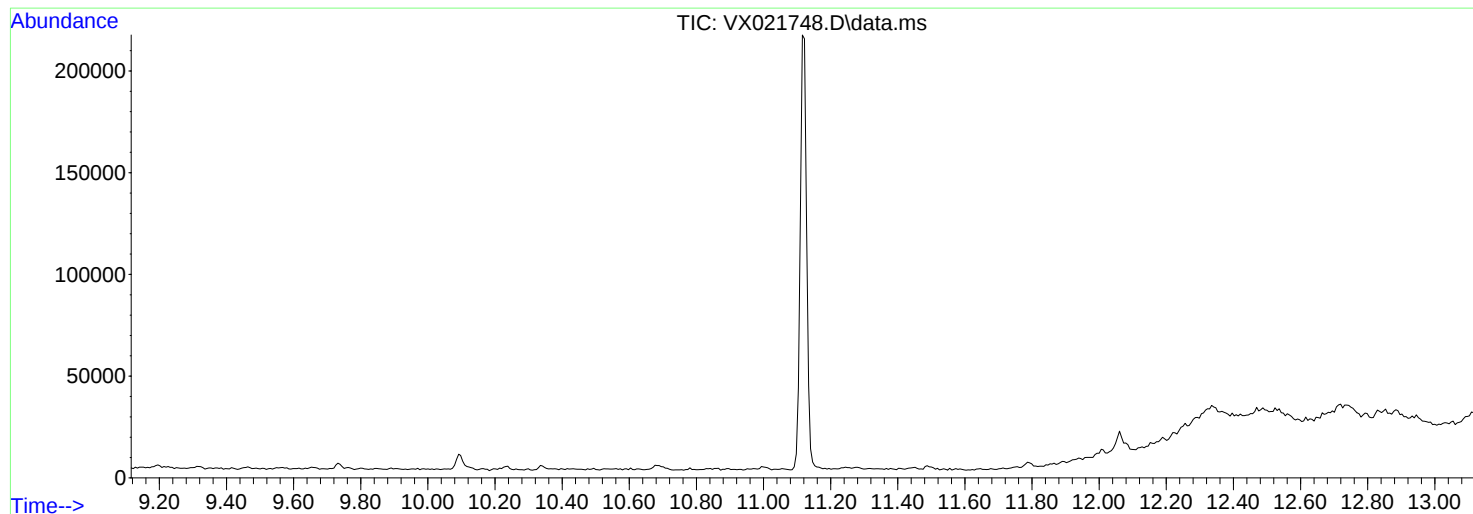

AutoFind: Scans 1644, 1645, 1646; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	6194	PASS
75	95	30	60	46.0	18683	PASS
95	95	100	100	100.0	40603	PASS
96	95	5	9	6.8	2752	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	77.8	31608	PASS
175	174	5	9	7.8	2455	PASS
176	174	95	101	96.7	30565	PASS
177	176	5	9	6.9	2107	PASS