
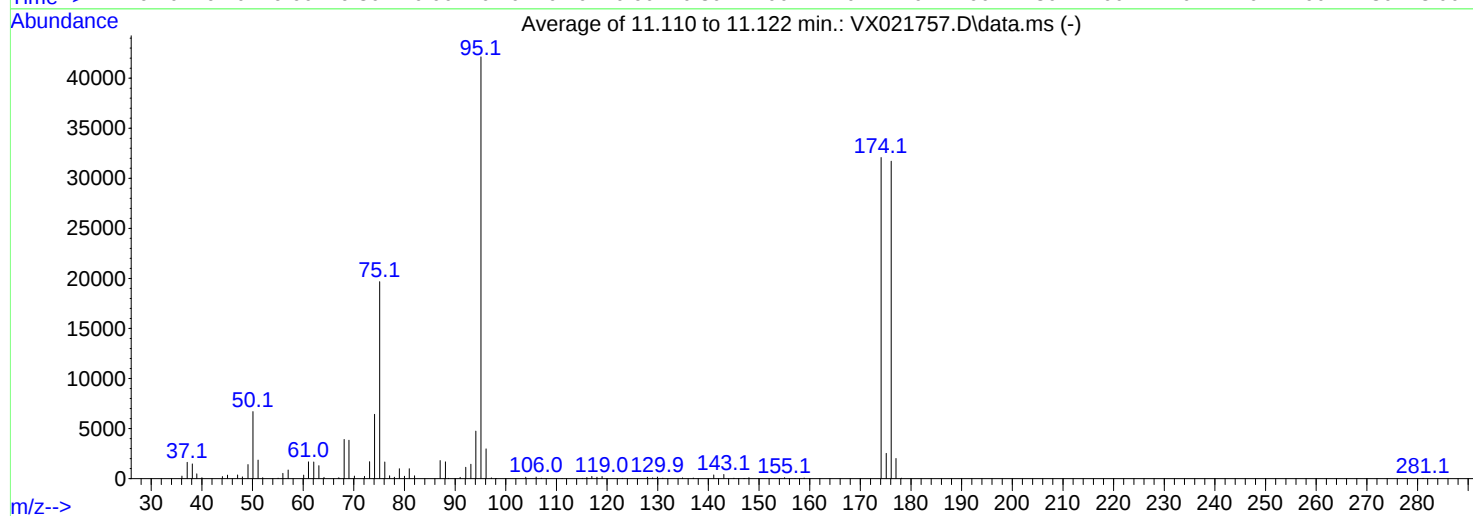


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042021\
Data File : VX021757.D
Acq On : 20 Apr 2021 15:59
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
Title : SW846 8260
Last Update : Tue Apr 20 13:46:22 2021

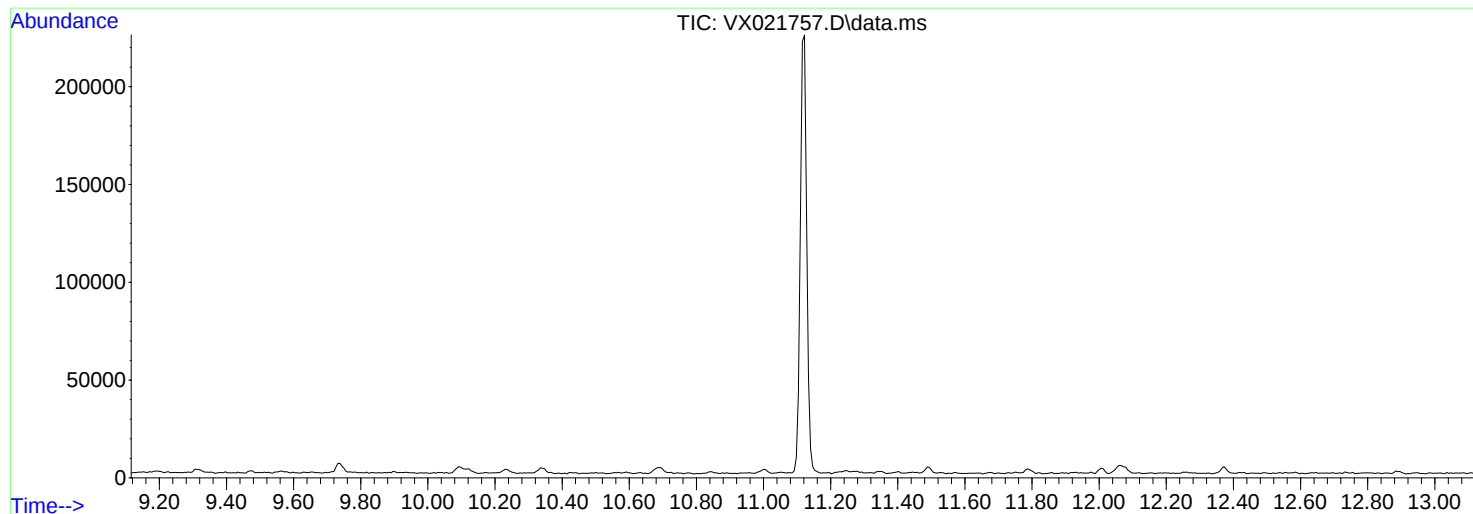

AutoFind: Scans 1644, 1645, 1646; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	6700	PASS
75	95	30	60	46.7	19670	PASS
95	95	100	100	100.0	42131	PASS
96	95	5	9	7.0	2969	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	76.1	32080	PASS
175	174	5	9	7.9	2519	PASS
176	174	95	101	98.9	31712	PASS
177	176	5	9	6.4	2016	PASS