

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042022\
 Data File : VX028192.D
 Acq On : 20 Apr 2022 13:02
 Operator : JC/MD
 Sample : N2468-09ME
 Misc : 4.05g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WC-15-1-8-GRME


Quant Time: Apr 21 06:11:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 19 13:38:04 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	448528	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	749284	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	713986	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	354569	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	255436	43.677	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	87.360%		
35) Dibromofluoromethane	5.391	113	246756	46.959	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	93.920%		
50) Toluene-d8	8.653	98	874473	43.329	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	86.660%		
62) 4-Bromofluorobenzene	11.079	95	331411	42.947	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	85.900%		
Target Compounds						
					Qvalue	
3) Chloromethane	1.294	50	461	Below Cal	#	78
5) Bromomethane	1.618	94	1061	Below Cal		94
6) Chloroethane	1.703	64	627	Below Cal	#	43
8) Diethyl Ether	2.136	74	43	Below Cal	#	1
10) Methyl Iodide	2.465	142	1164	5.444	ug/l	96
11) Tert butyl alcohol	2.941	59	7541	Below Cal	#	75
16) Acetone	2.380	43	6433	2.218	ug/l	91
20) Methylene Chloride	2.788	84	1232	0.284	ug/l #	83
25) 2-Butanone	4.568	43	2099	0.606	ug/l #	85
29) Tetrahydrofuran	5.044	42	477	0.211	ug/l #	35
36) 1,1-Dichloropropene	5.556	75	31424	4.585	ug/l #	50
38) Carbon Tetrachloride	5.556	117	43737	5.652	ug/l #	15
39) Methylcyclohexane	7.379	83	7243	0.837	ug/l	86
51) 4-Methyl-2-Pentanone	8.653	43	4772	0.657	ug/l #	1
55) 1,1,2-Trichloroethane	9.110	97	2143	0.378	ug/l #	22
71) Bromoform	10.689	173	78	3.589	ug/l #	29
73) Isopropylbenzene	10.963	105	22056	0.905	ug/l	98
74) N-amyl acetate	10.860	43	3412	0.405	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	11.220	83	3439	0.435	ug/l #	25
76) 1,2,3-Trichloropropane	11.079	75	163103	23.373	ug/l #	38
80) 1,3,5-Trimethylbenzene	11.451	105	7321	0.354	ug/l	93
81) trans-1,4-Dichloro-2-b...	11.079	75	163103	69.460	ug/l #	15
84) 1,2,4-Trimethylbenzene	11.756	105	13121	0.638	ug/l	99
85) sec-Butylbenzene	11.890	105	13888	0.545	ug/l #	74
89) n-Butylbenzene	12.335	91	14308	0.793	ug/l #	67
90) Hexachloroethane	12.616	117	5782	3.222	ug/l #	12
91) 1,2-Dichlorobenzene	12.341	146	4125	0.348	ug/l #	79
92) 1,2-Dibromo-3-Chloropr...	12.920	75	380	0.216	ug/l #	1
96) 1,2,3-Trichlorobenzene	13.975	180	3761	0.544	ug/l #	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Apr 21 06:11:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 19 13:38:04 2022
Response via : Initial Calibration




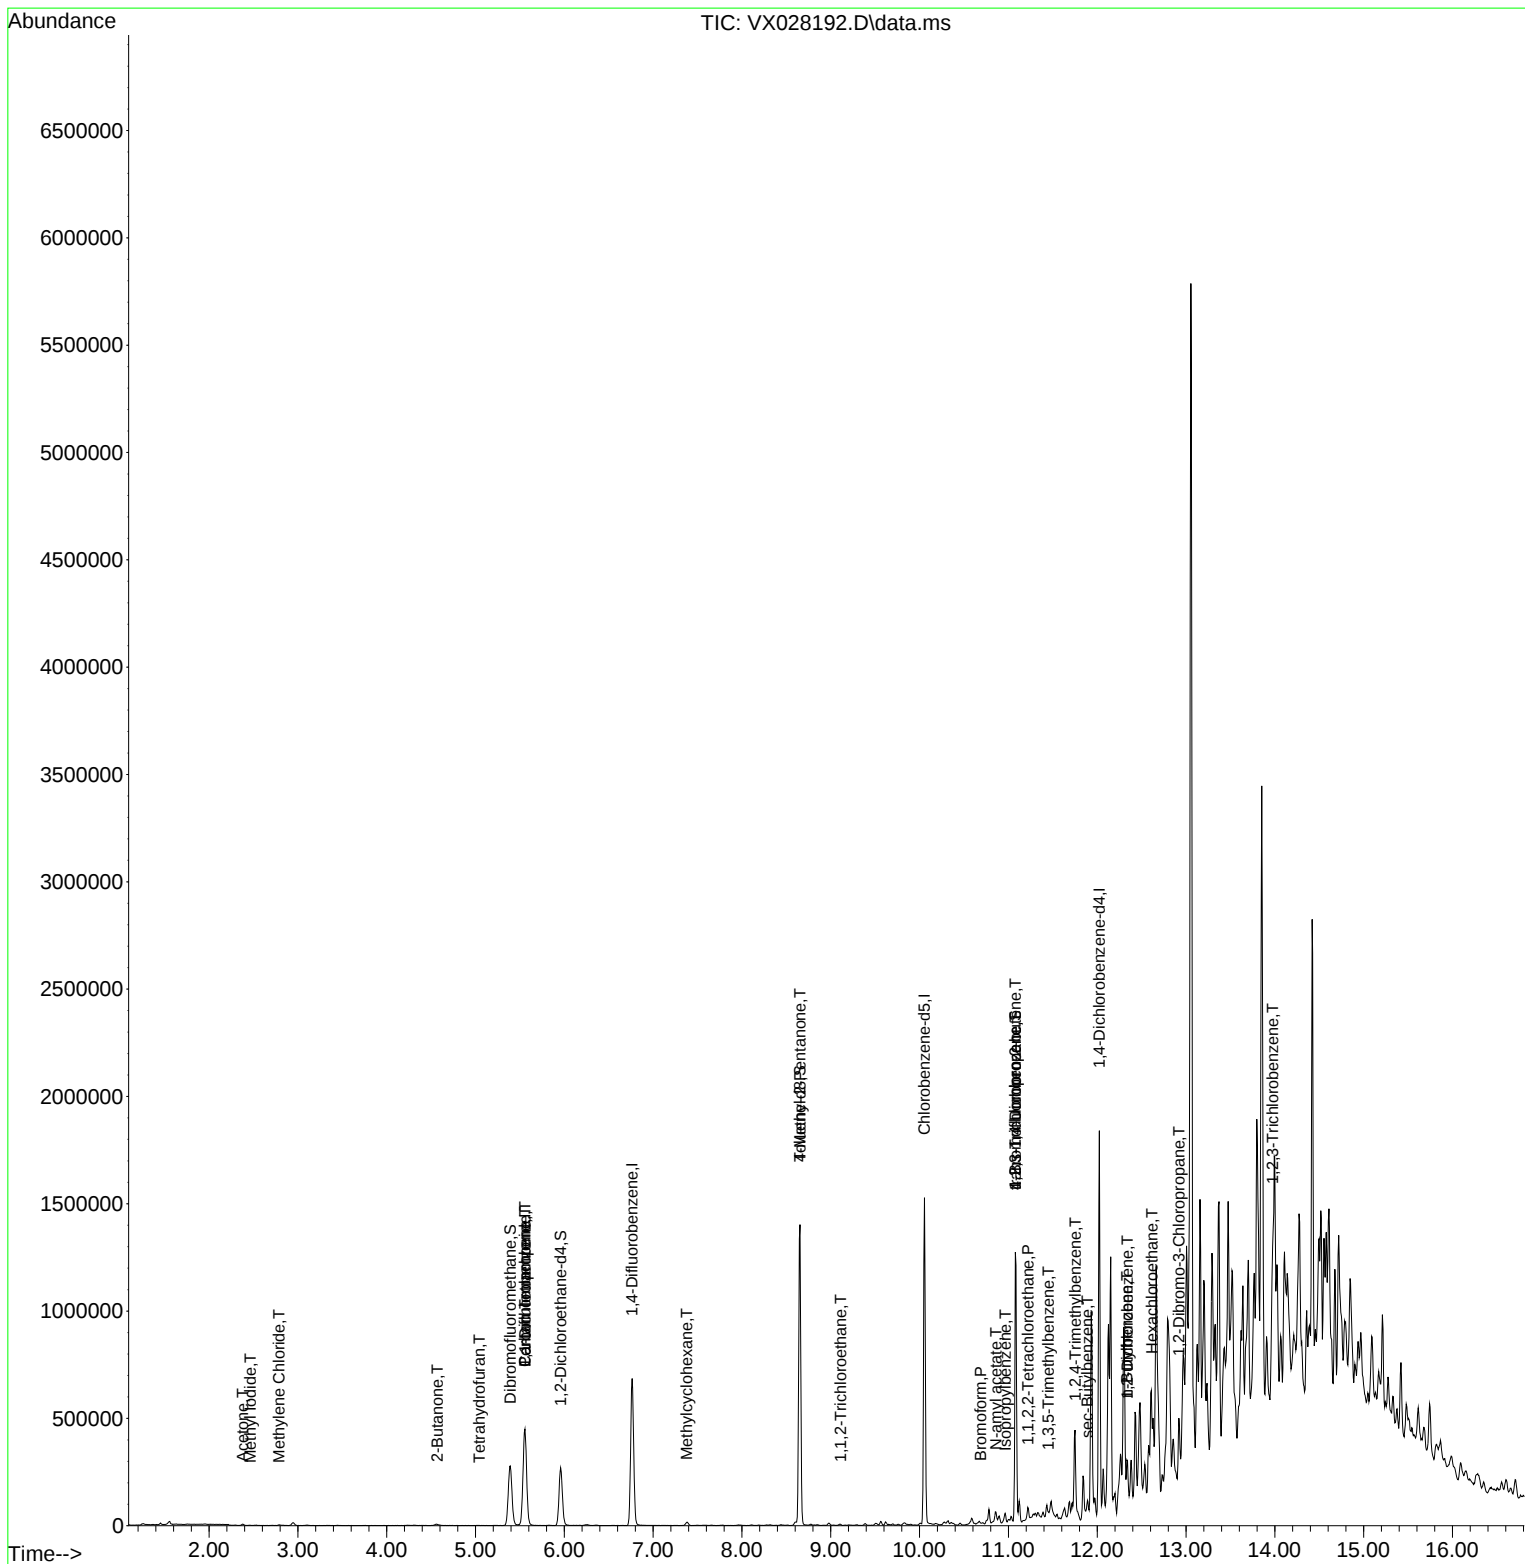




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-8-GRME


Tgt Ion:168 Resp: 448528
Ion Ratio Lower Upper
168 100
99 53.2 41.7 62.5

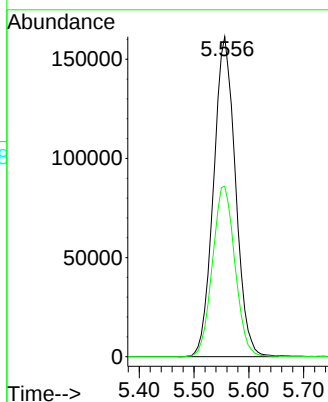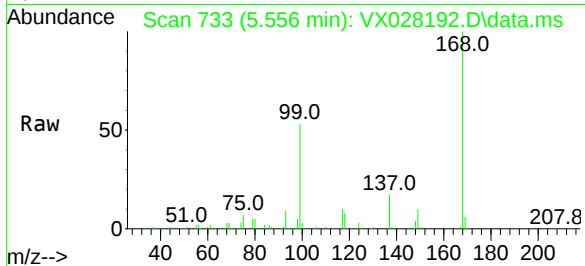

#3
Chloromethane
Concen: Below Cal
RT: 1.294 min Scan# 34
Delta R.T. 0.000 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02

Tgt Ion: 50 Resp: 461
Ion Ratio Lower Upper
50 100
52 20.3 26.4 39.6#


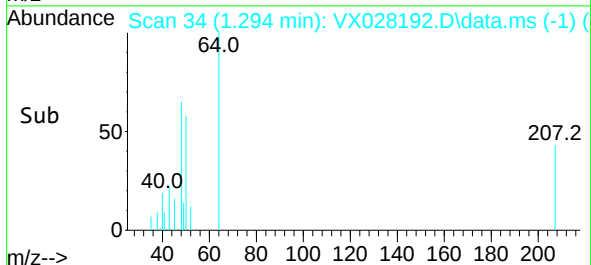
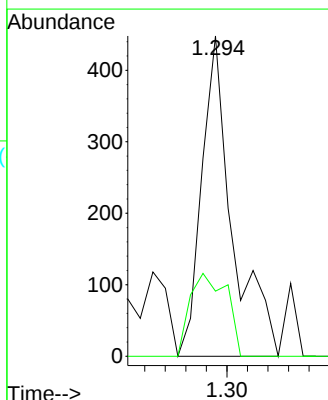
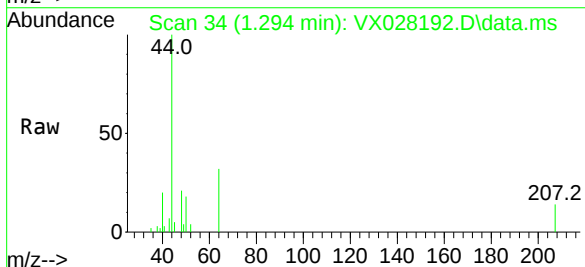


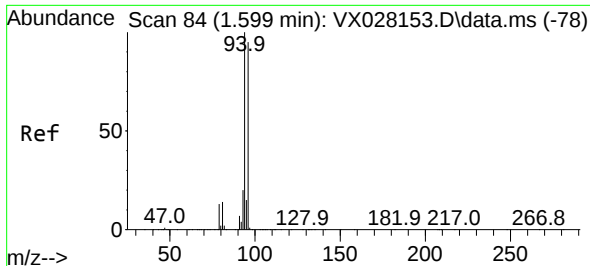

#5
Bromomethane
Concen: Below Cal
RT: 1.618 min Scan# 81
Delta R.T. 0.019 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-8-GRME


Tgt Ion: 94 Resp: 1061
Ion Ratio Lower Upper
94 100
96 87.9 75.3 112.9

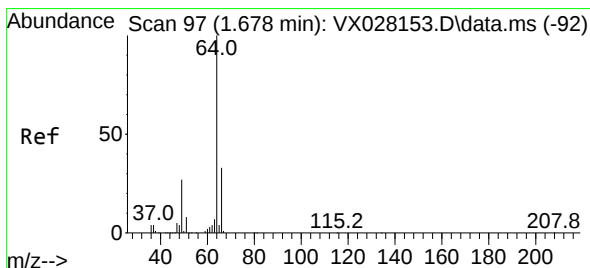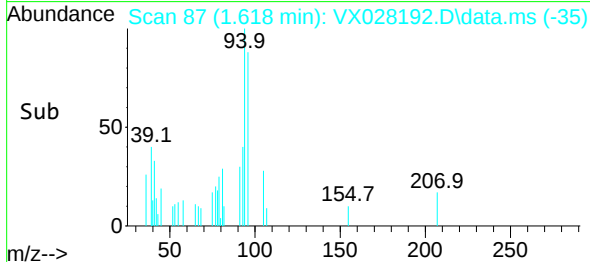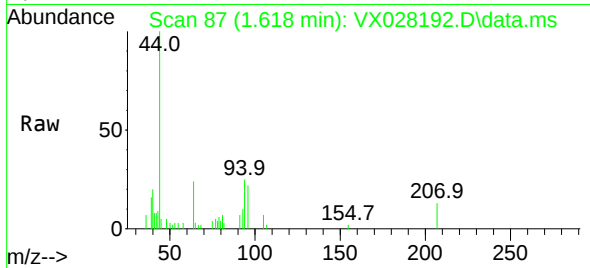

#6
Chloroethane
Concen: Below Cal
RT: 1.703 min Scan# 101
Delta R.T. 0.025 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02

Tgt Ion: 64 Resp: 627
Ion Ratio Lower Upper
64 100
66 0.0 25.3 37.9#


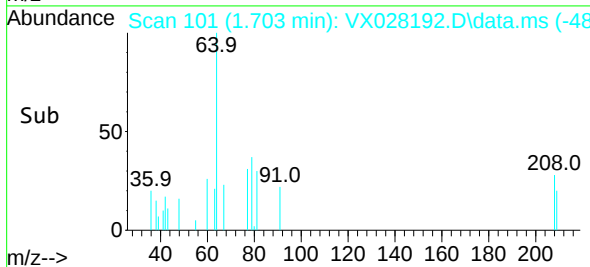

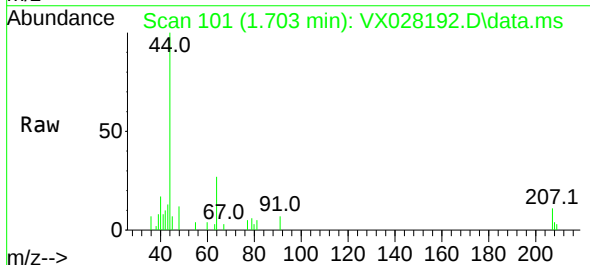




#8
Diethyl Ether
Concen: Below Cal
RT: 2.136 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-8-GRME


Tgt Ion: 74 Resp: 43
Ion Ratio Lower Upper
74 100
45 439.5 42.0 126.0#

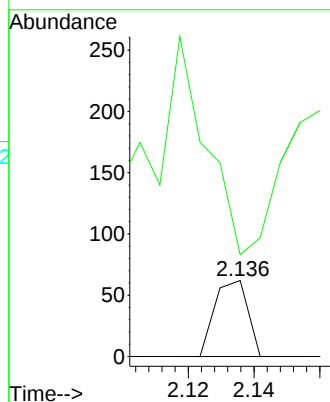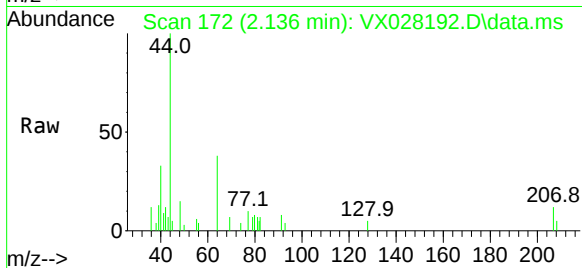

#10
Methyl Iodide
Concen: 5.444 ug/l
RT: 2.465 min Scan# 226
Delta R.T. 0.012 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02

Tgt Ion: 142 Resp: 1164
Ion Ratio Lower Upper
142 100
127 40.3 33.9 50.9
141 11.9 11.4 17.2


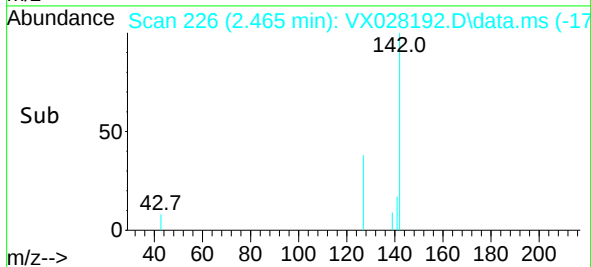
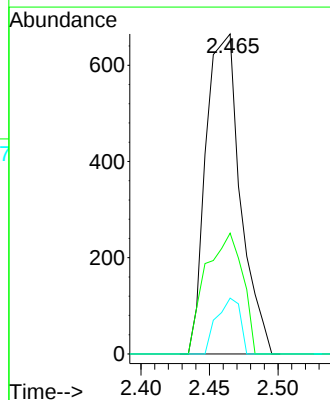
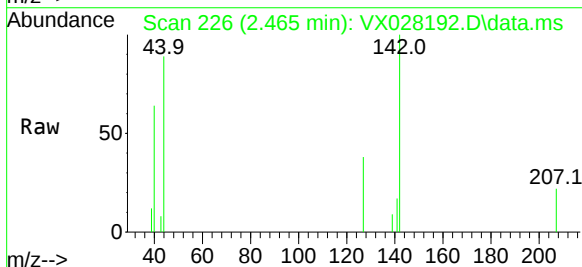


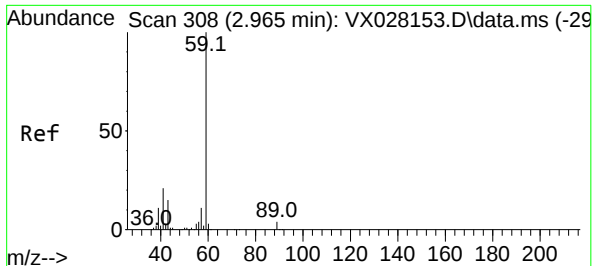

#11
Tert butyl alcohol
Concen: Below Cal
RT: 2.941 min Scan# 308
Delta R.T. -0.024 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-8-GRME


Tgt Ion: 59 Resp: 7541
Ion Ratio Lower Upper
59 100
57 1.0 8.3 12.5#

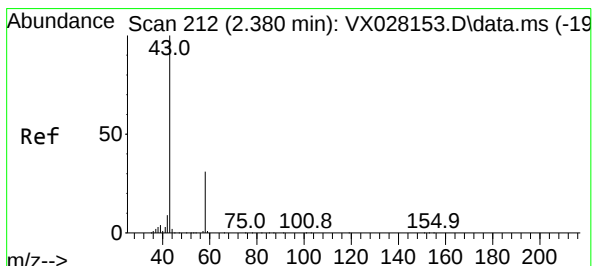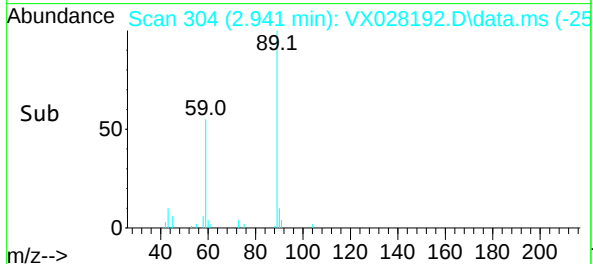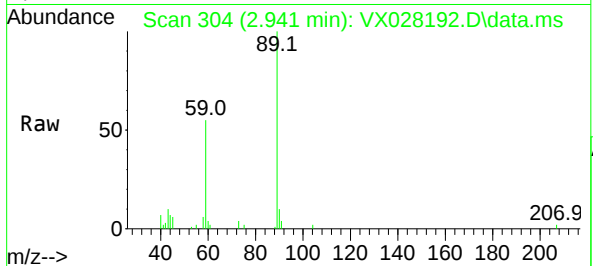

#16
Acetone
Concen: 2.218 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.000 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02


Tgt Ion: 43 Resp: 6433
Ion Ratio Lower Upper
43 100
58 30.7 28.8 43.2

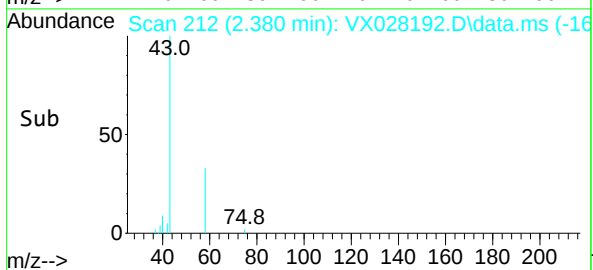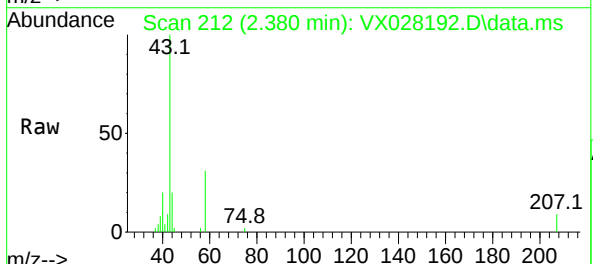






#20
Methylene Chloride
Concen: 0.284 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02

Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-8-GRME







Tgt Ion:	84	Resp:	1232
Ion	Ratio	Lower	Upper
84	100		
49	115.6	85.5	128.3
51	49.4	26.6	39.8#
86	85.2	51.5	77.3#

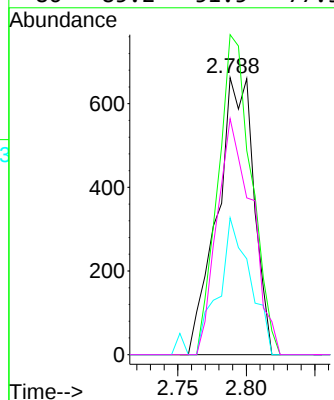

#25
2-Butanone
Concen: 0.606 ug/l
RT: 4.568 min Scan# 571
Delta R.T. 0.012 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02

Tgt Ion:	43	Resp:	2099
Ion	Ratio	Lower	Upper
43	100		
72	22.1	24.4	36.6#

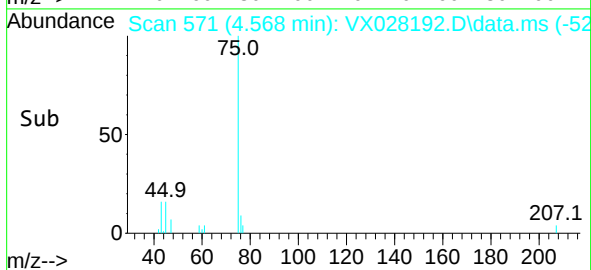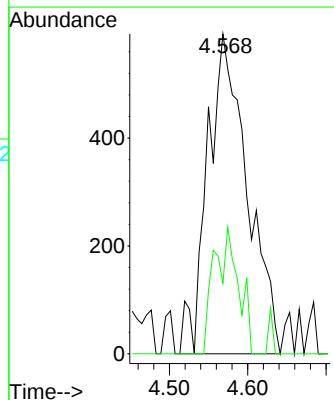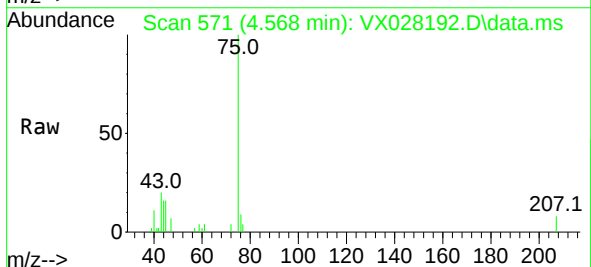



#29

Tetrahydrofuran

Concen: 0.211 ug/l

RT: 5.044 min Scan# 643

Delta R.T. 0.037 min

Lab File: VX028192.D


Acq: 20 Apr 2022 13:02

Instrument :




MSVOA_X

ClientSampleId :

WC-15-1-8-GRME

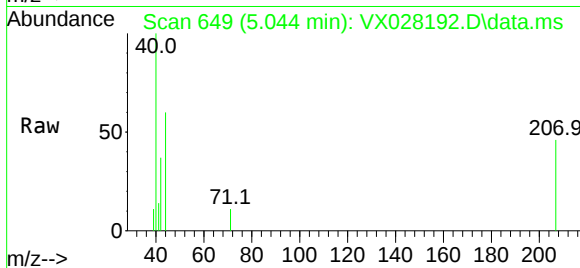

Tgt Ion:	42	Resp:	477
Ion	Ratio	Lower	Upper
42	100		
72	9.2	44.1	66.1#
71	5.0	40.5	60.7#

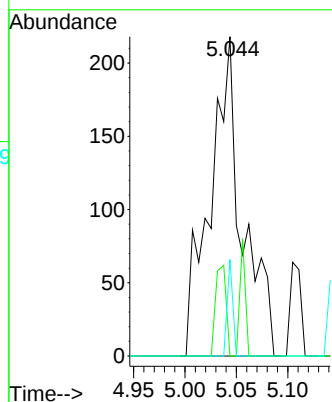

#33

1,2-Dichloroethane-d4

Concen: 43.677 ug/l




RT: 5.958 min Scan# 799


Delta R.T. 0.000 min

Lab File: VX028192.D

Acq: 20 Apr 2022 13:02

Tgt Ion:	65	Resp:	255436
Ion	Ratio	Lower	Upper
65	100		
67	52.1	0.0	107.4


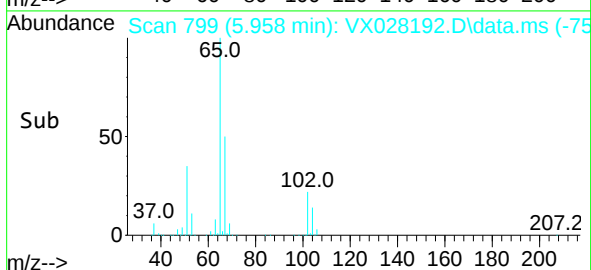
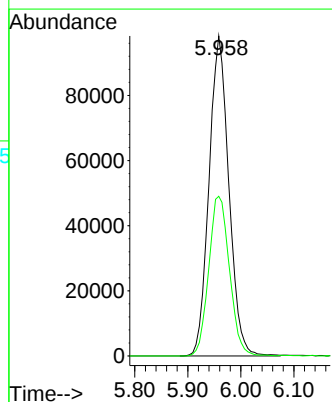
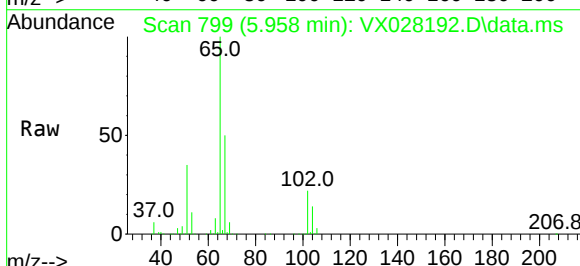




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-8-GRME


Tgt Ion:114 Resp: 749284
Ion Ratio Lower Upper
114 100
63 17.9 0.0 36.8
88 15.2 0.0 32.4

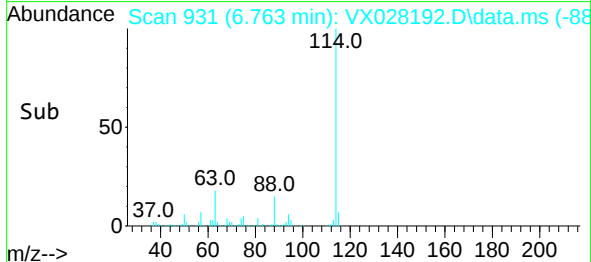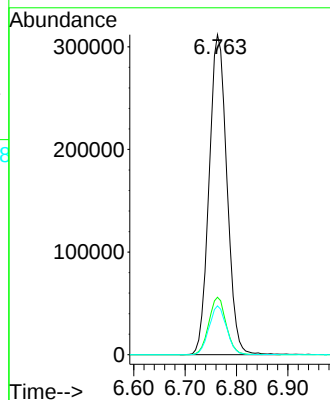

#35
Dibromofluoromethane
Concen: 46.959 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02

Tgt Ion:113 Resp: 246756
Ion Ratio Lower Upper
113 100
111 100.7 82.8 124.2
192 20.2 16.9 25.3


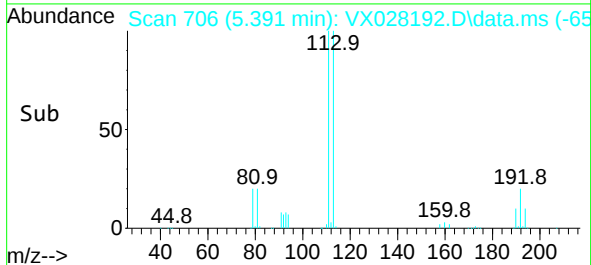
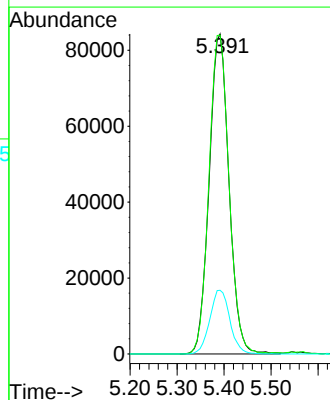
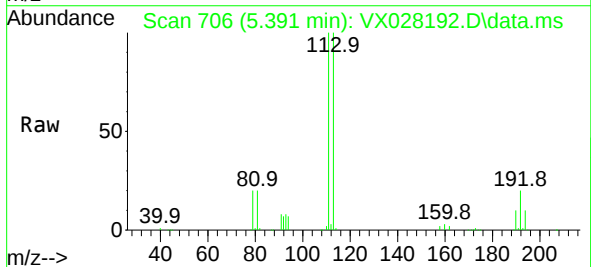




#36
1,1-Dichloropropene
Concen: 4.585 ug/l
RT: 5.556 min Scan# 711
Delta R.T. -0.140 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-8-GRME


Tgt Ion: 75 Resp: 31424
Ion Ratio Lower Upper
75 100
110 9.7 18.3 54.8#
77 0.0 24.8 37.2#

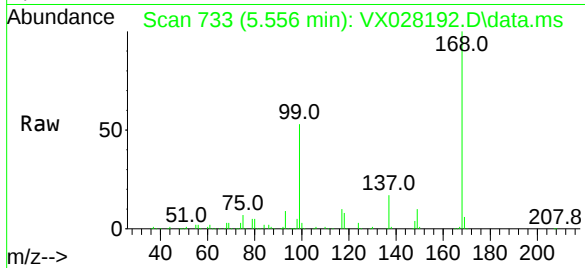

#38
Carbon Tetrachloride
Concen: 5.652 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.128 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02

Tgt Ion: 117 Resp: 43737
Ion Ratio Lower Upper
117 100
119 4.3 77.3 115.9#
121 0.0 24.2 36.2#

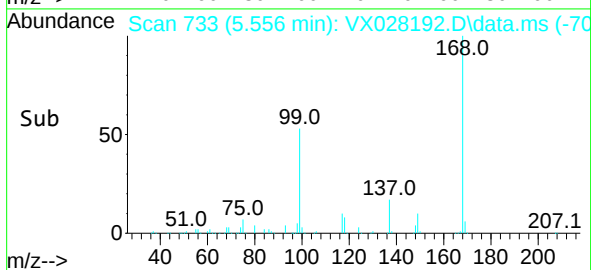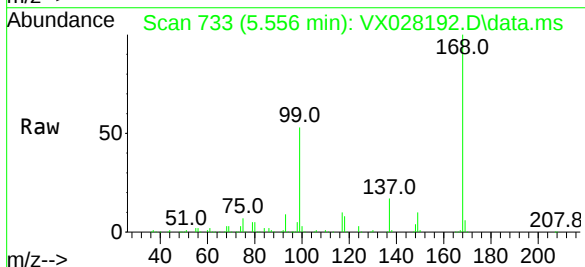



#39

Methylcyclohexane

Concen: 0.837 ug/l

RT: 7.379 min Scan# 1033

Delta R.T. -0.006 min

Lab File: VX028192.D

Acq: 20 Apr 2022 13:02

Instrument :

MSVOA_X

ClientSampleId :

WC-15-1-8-GRME





Tgt Ion: 83 Resp: 7243

Ion Ratio Lower Upper

83 100

55 56.1 54.6 81.8

98 37.8 37.4 56.2

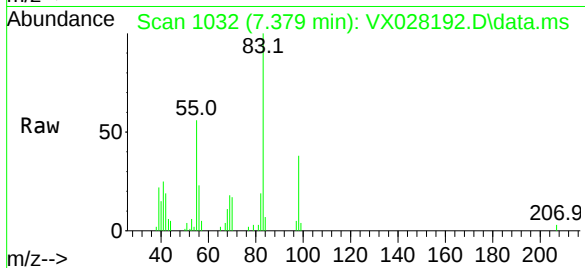

#50

Toluene-d8

Concen: 43.329 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX028192.D




Acq: 20 Apr 2022 13:02


Tgt Ion: 98 Resp: 874473

Ion Ratio Lower Upper

98 100

100 66.3 52.6 78.8


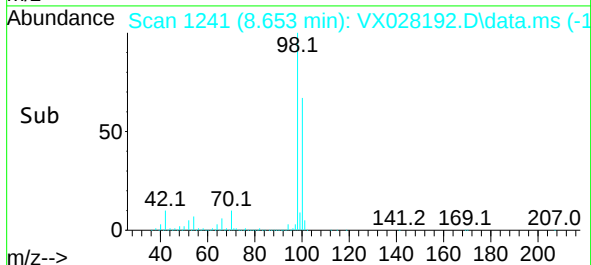
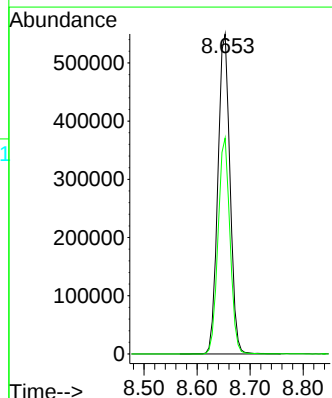
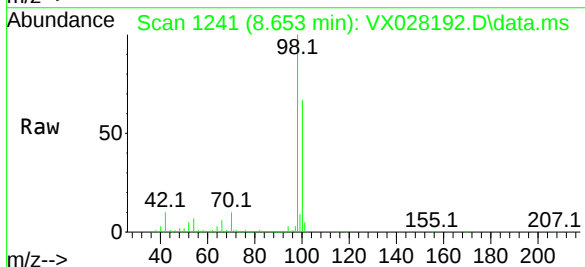


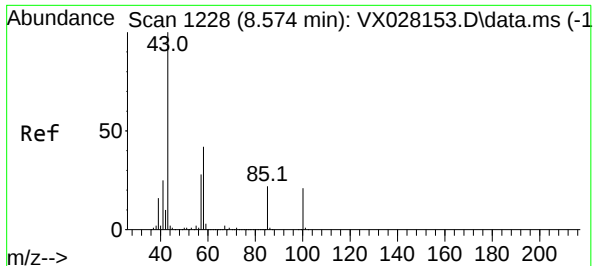

#51
4-Methyl-2-Pentanone
Concen: 0.657 ug/l
RT: 8.653 min Scan# 1316
Delta R.T. 0.079 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-8-GRME


Tgt Ion: 43 Resp: 4772
Ion Ratio Lower Upper
43 100
58 141.8 36.1 54.1#

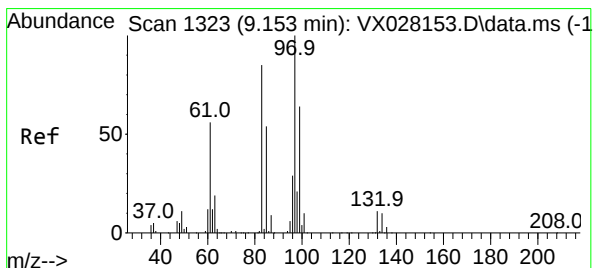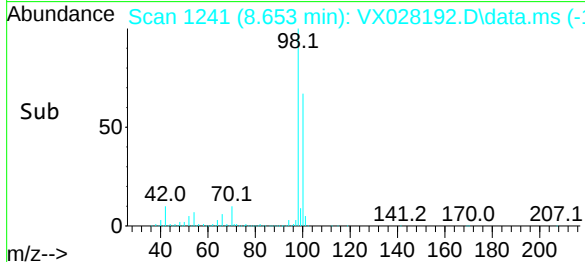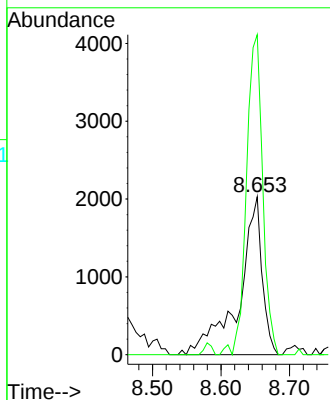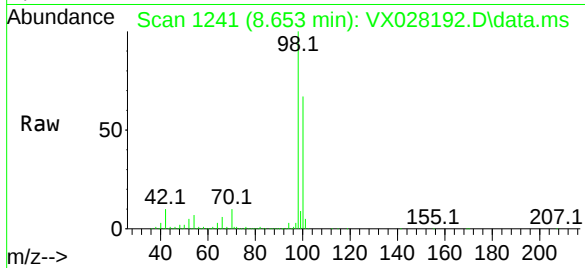

#55
1,1,2-Trichloroethane
Concen: 0.378 ug/l
RT: 9.110 min Scan# 1316
Delta R.T. -0.043 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02

Tgt Ion: 97 Resp: 2143
Ion Ratio Lower Upper
97 100
83 13.3 66.2 99.4#
85 0.0 42.9 64.3#
99 0.0 49.0 73.6#


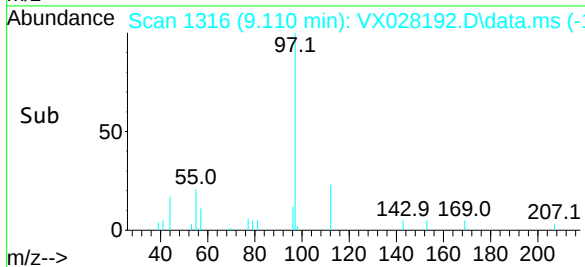
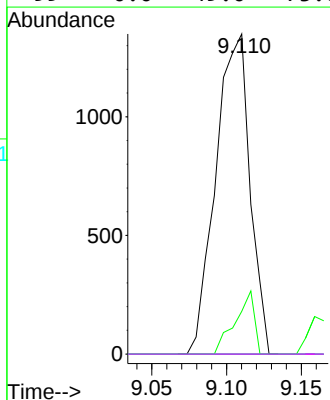
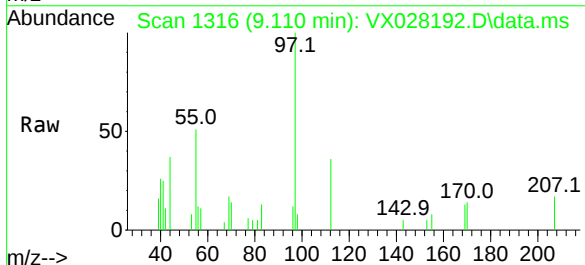




#62
4-Bromofluorobenzene
Concen: 42.947 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-8-GRME


Tgt Ion: 95 Resp: 331411
Ion Ratio Lower Upper
95 100
174 84.2 0.0 163.0
176 80.2 0.0 155.0

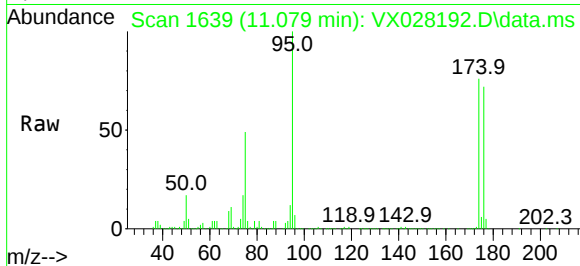

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02

Tgt Ion: 117 Resp: 713986
Ion Ratio Lower Upper
117 100
82 50.6 41.8 62.8
119 32.3 24.8 37.2


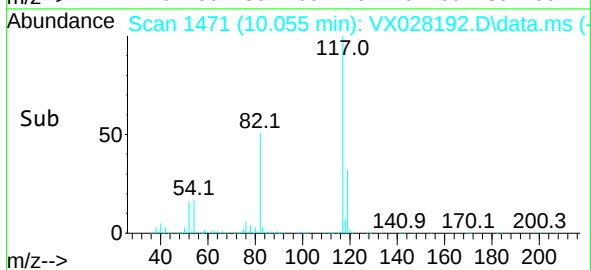

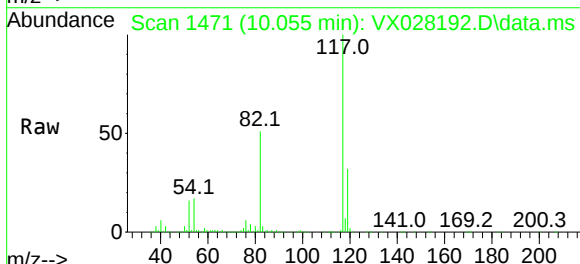




#71
Bromoform
Concen: 3.589 ug/l
RT: 10.689 min Scan# 1575
Delta R.T. -0.110 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-8-GRME


Tgt Ion:173 Resp: 78
Ion Ratio Lower Upper
173 100
175 0.0 24.1 72.2#
254 0.0 0.1 0.1#

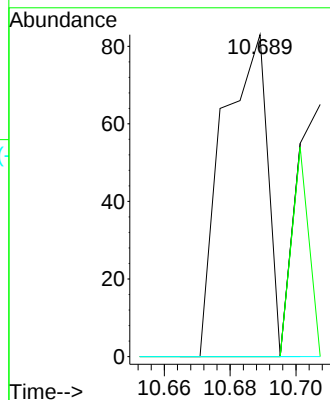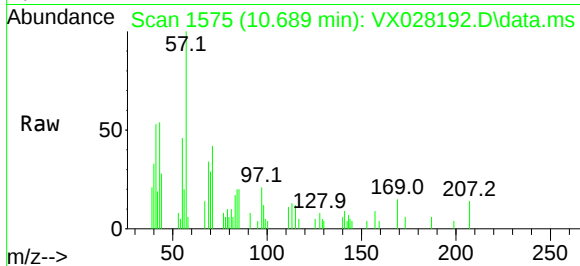

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02

Tgt Ion:152 Resp: 354569
Ion Ratio Lower Upper
152 100
115 58.1 37.5 112.7
150 156.9 0.0 338.2


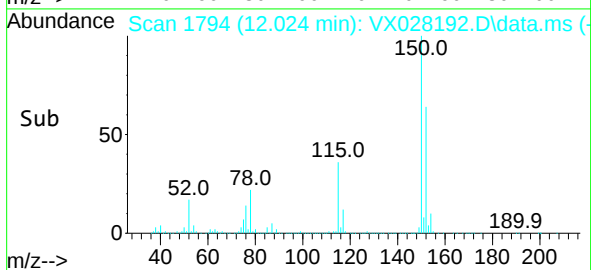
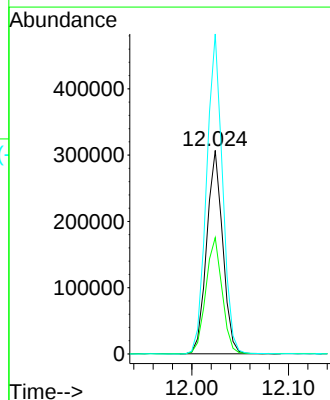
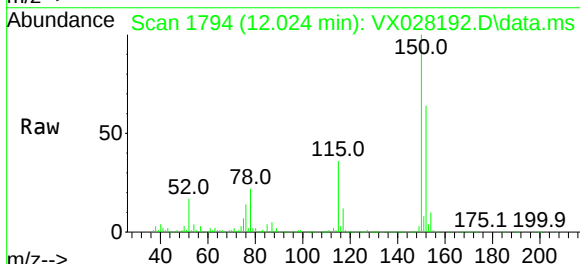




#73
Isopropylbenzene
Concen: 0.905 ug/l
RT: 10.963 min Scan# 1603
Delta R.T. 0.000 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-8-GRME


Tgt Ion:105 Resp: 22056
Ion Ratio Lower Upper
105 100
120 27.9 13.5 40.5

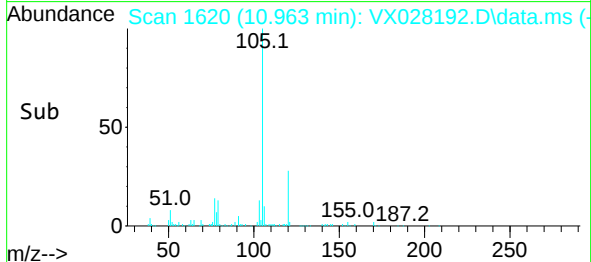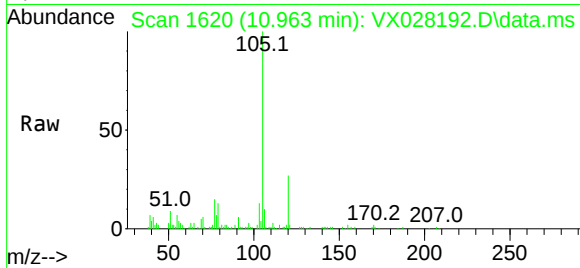

#74
N-ethyl acetate
Concen: 0.405 ug/l
RT: 10.860 min Scan# 1603
Delta R.T. 0.012 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02

Tgt Ion: 43 Resp: 3412
Ion Ratio Lower Upper
43 100
70 76.3 42.5 63.7#
55 428.4 23.1 34.7#
61 0.0 22.8 34.2#


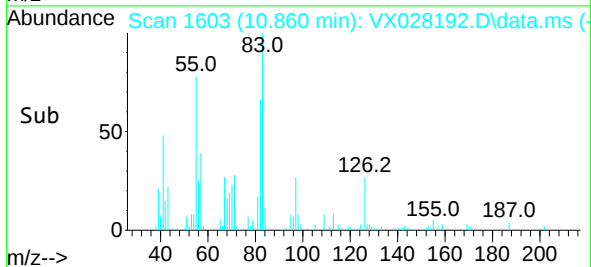

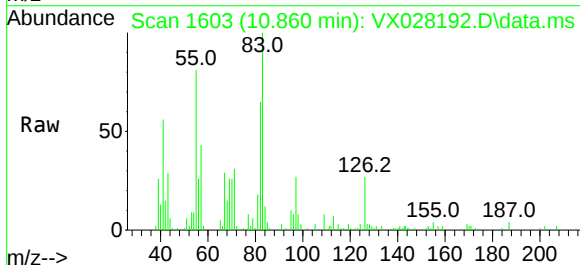




#75
1,1,2,2-Tetrachloroethane
Concen: 0.435 ug/l
RT: 11.220 min Scan# 1639
Delta R.T. 0.007 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-8-GRME


Tgt Ion: 83 Resp: 3439
Ion Ratio Lower Upper
83 100
131 0.6 5.1 15.3#
85 0.0 32.6 97.7#

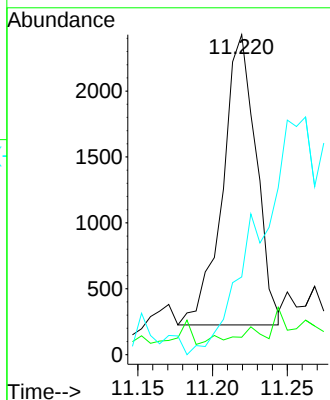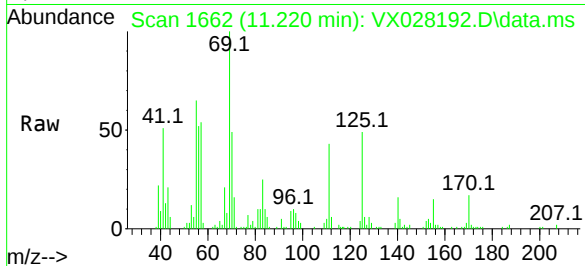

#76
1,2,3-Trichloropropane
Concen: 23.373 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02

Tgt Ion: 75 Resp: 163103
Ion Ratio Lower Upper
75 100
77 1.2 19.4 58.2#

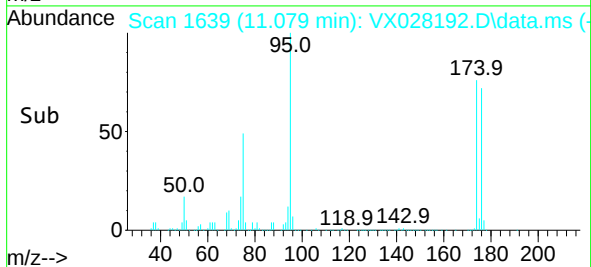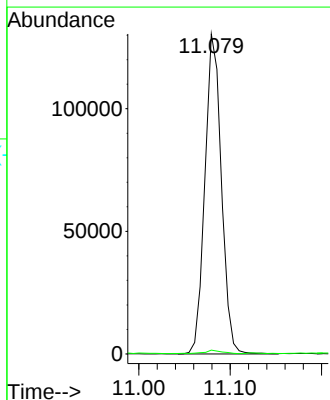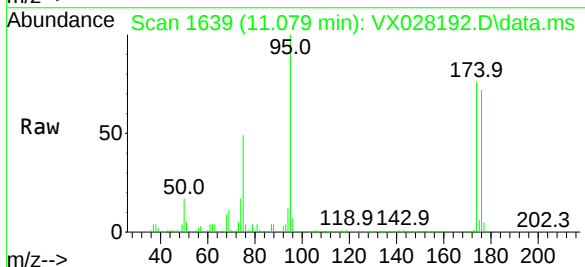



#80

1,3,5-Trimethylbenzene

Concen: 0.354 ug/l

RT: 11.451 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX028192.D

Acq: 20 Apr 2022 13:02

Instrument :

MSVOA_X

ClientSampleId :





WC-15-1-8-GRME

Tgt Ion:105 Resp: 7321

Ion Ratio Lower Upper

105 100

120 53.2 24.3 72.9

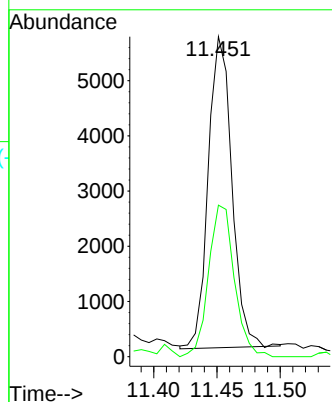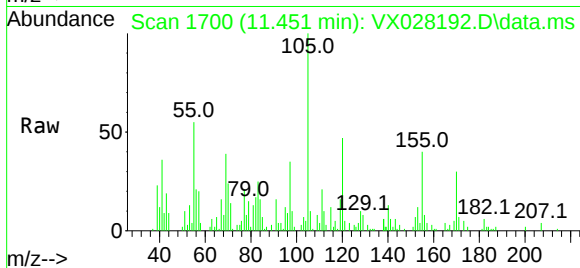

#81

trans-1,4-Dichloro-2-butene

Concen: 69.460 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX028192.D

Acq: 20 Apr 2022 13:02




Tgt Ion: 75 Resp: 163103


Ion Ratio Lower Upper

75 100

53 0.1 69.0 103.4#

89 0.0 37.0 55.6#


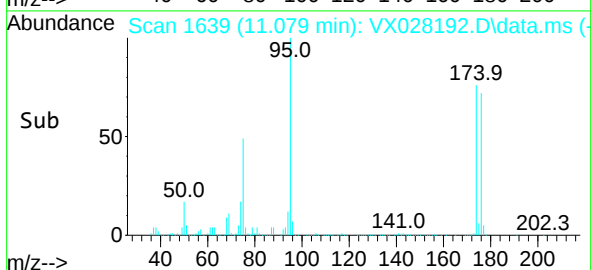

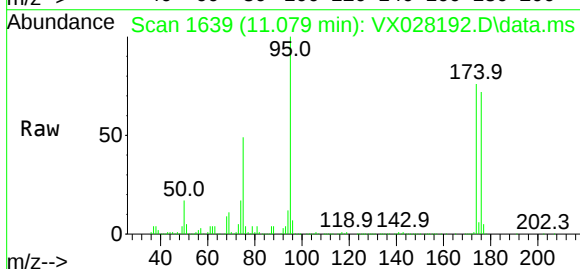


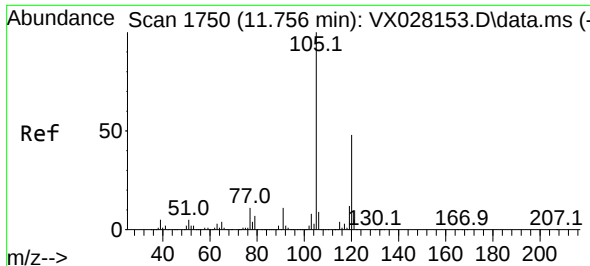

#84
1,2,4-Trimethylbenzene
Concen: 0.638 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-8-GRME


Tgt Ion:105 Resp: 13121
Ion Ratio Lower Upper
105 100
120 45.9 22.6 67.8

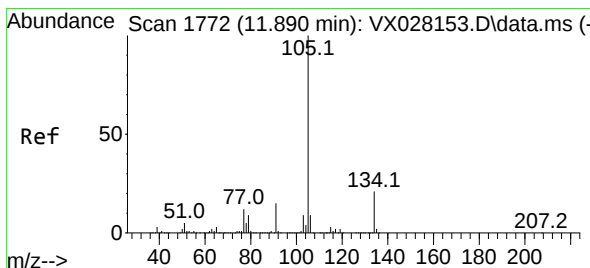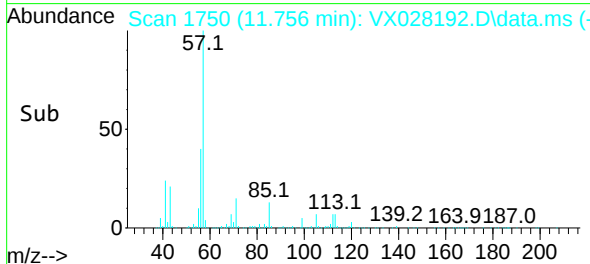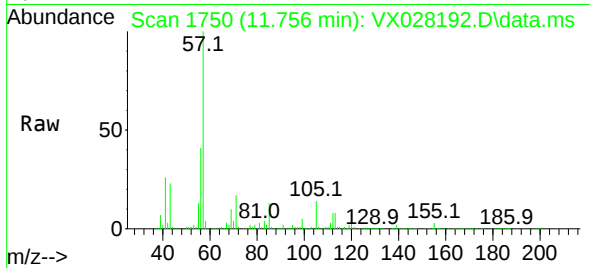

#85
sec-Butylbenzene
Concen: 0.545 ug/l
RT: 11.890 min Scan# 1772
Delta R.T. 0.000 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02

Tgt Ion:105 Resp: 13888
Ion Ratio Lower Upper
105 100
134 32.5 10.2 30.4#

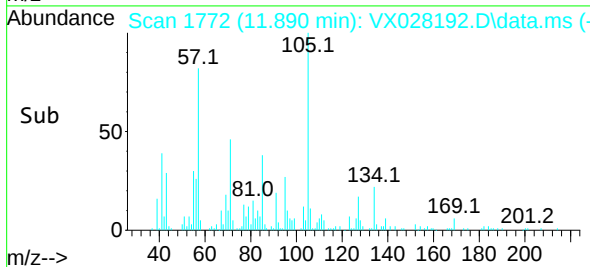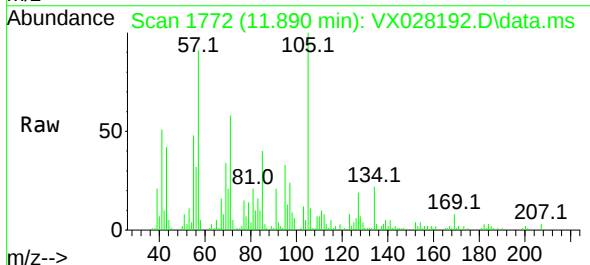



#89

n-Butylbenzene

Concen: 0.793 ug/l

RT: 12.335 min Scan# 1845

Delta R.T. 0.000 min

Lab File: VX028192.D

Acq: 20 Apr 2022 13:02

Instrument :

MSVOA_X

ClientSampleId :

WC-15-1-8-GRME





Tgt Ion: 91 Resp: 14308

Ion Ratio Lower Upper

91 100

92 40.5 27.8 83.3

134 57.1 13.3 39.8#

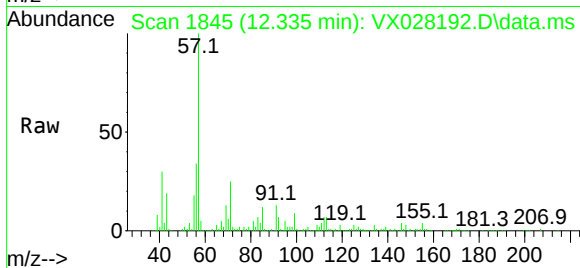

#90

Hexachloroethane

Concen: 3.222 ug/l

RT: 12.616 min Scan# 1891

Delta R.T. 0.074 min

Lab File: VX028192.D




Acq: 20 Apr 2022 13:02


Tgt Ion: 117 Resp: 5782

Ion Ratio Lower Upper

117 100

201 2.1 39.5 118.5#


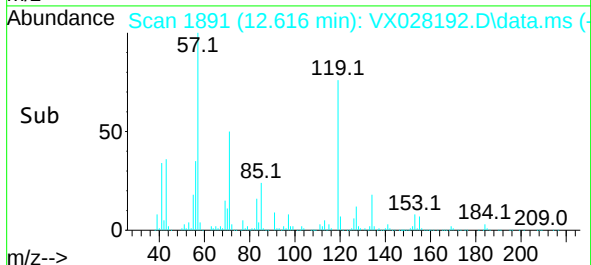
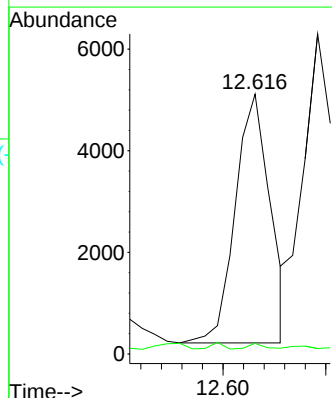
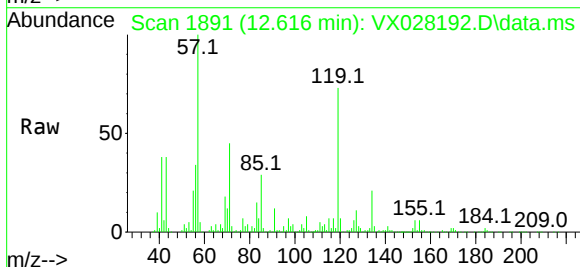




#91
1,2-Dichlorobenzene
Concen: 0.348 ug/l
RT: 12.341 min Scan# 1845
Delta R.T. 0.006 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-8-GRME


Tgt Ion:146 Resp: 4125
Ion Ratio Lower Upper
146 100
111 71.7 21.0 63.0#
148 61.2 32.6 97.7

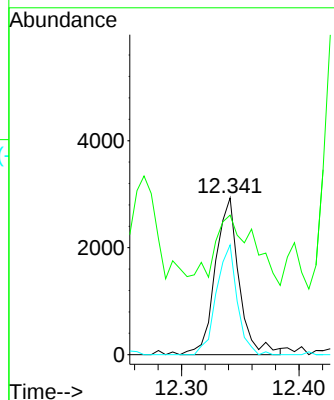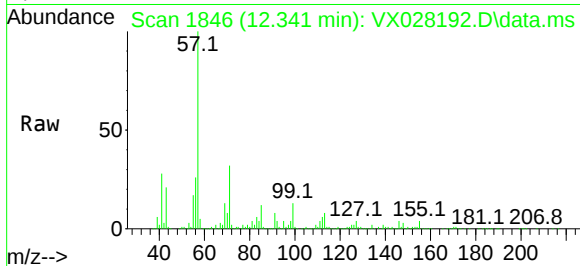

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.216 ug/l
RT: 12.920 min Scan# 1941
Delta R.T. -0.025 min
Lab File: VX028192.D
Acq: 20 Apr 2022 13:02


Tgt Ion: 75 Resp: 380
Ion Ratio Lower Upper
75 100
155 867.1 47.0 141.2#
157 0.0 57.9 173.6#

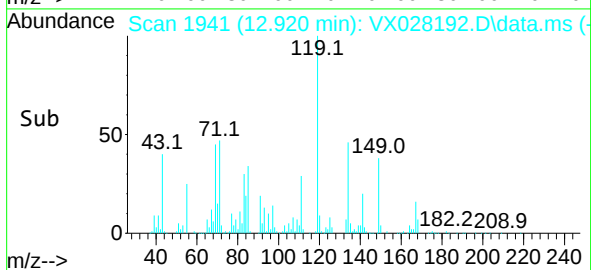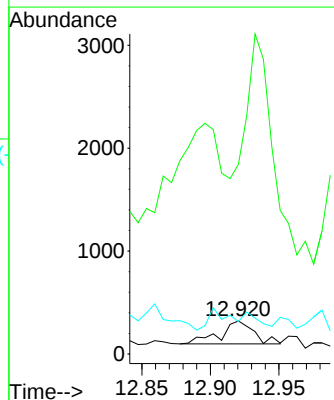

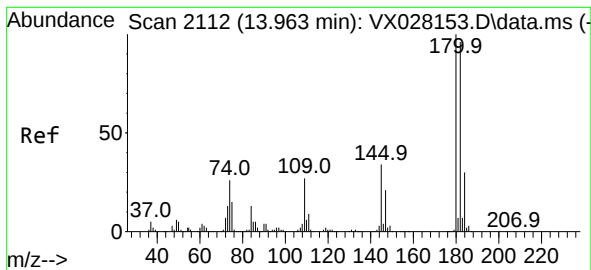

#96
 1,2,3-Trichlorobenzene
 Concen: 0.544 ug/l
 RT: 13.975 min Scan# 2114
 Delta R.T. 0.012 min
 Lab File: VX028192.D
 Acq: 20 Apr 2022 13:02

Instrument :
 MSVOA_X
 ClientSampleId :
 WC-15-1-8-GRME

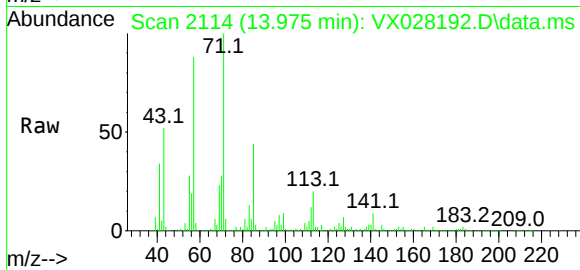

Tgt Ion:180 Resp: 3761
 Ion Ratio Lower Upper
 180 100
 182 0.0 50.0 149.8#
 145 166.7 16.2 48.5#

