

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042022\
 Data File : VX028188.D
 Acq On : 20 Apr 2022 11:15
 Operator : JC/MD
 Sample : VX0420MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0420MBL01

Quant Time: Apr 20 15:17:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 19 13:38:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	403293	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	661358	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	577833	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	254780	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	228662	43.484	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	86.960%
35) Dibromofluoromethane	5.385	113	206758	44.579	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	89.160%
50) Toluene-d8	8.647	98	757013	42.496	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	85.000%
62) 4-Bromofluorobenzene	11.079	95	258045	37.885	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	75.780%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042022\
Data File : VX028188.D
Acq On : 20 Apr 2022 11:15
Operator : JC/MD
Sample : VX0420MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0420MBL01

Quant Time: Apr 20 15:17:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 19 13:38:04 2022
Response via : Initial Calibration




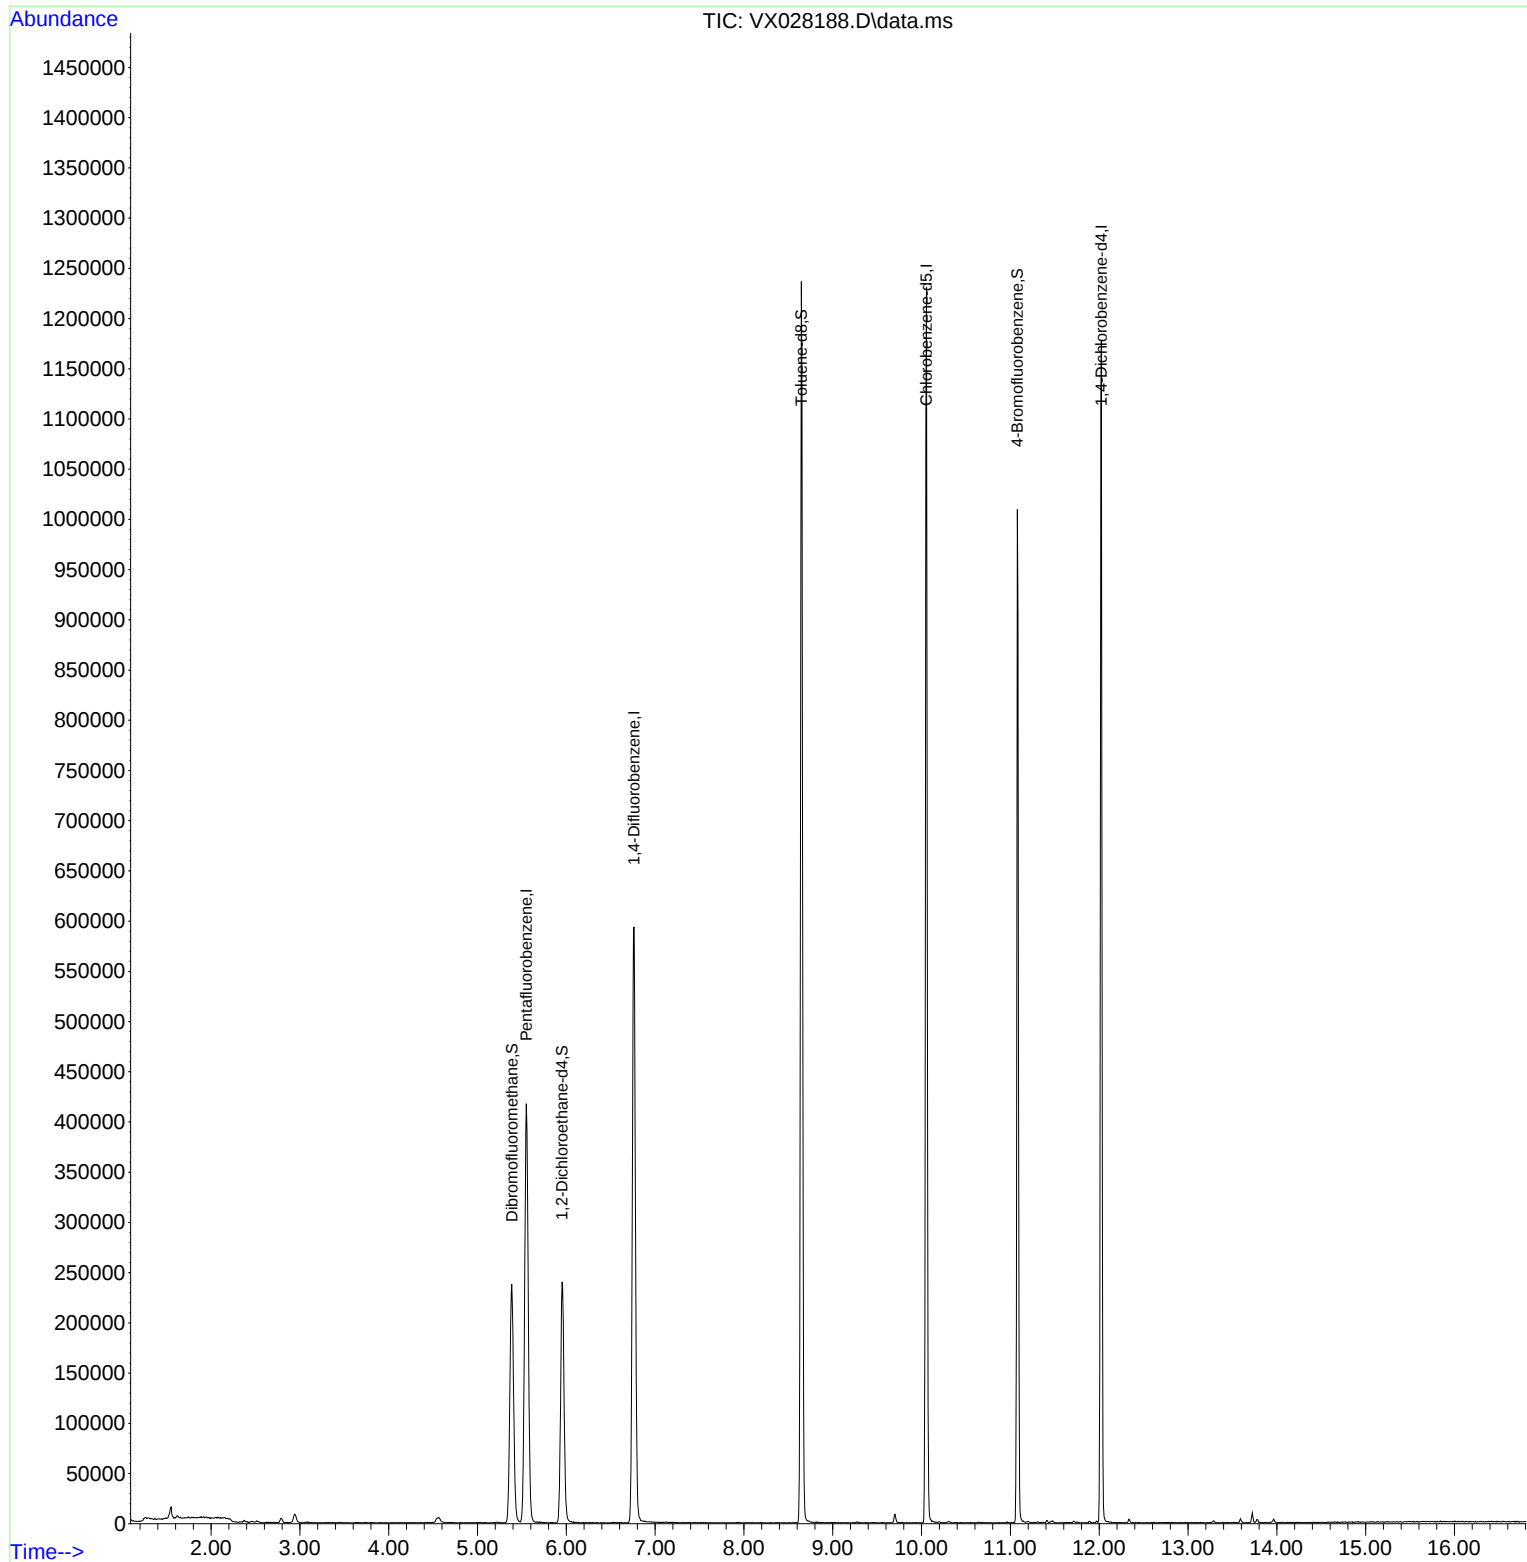


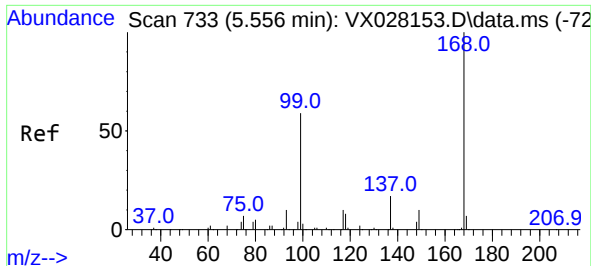

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 713
Delta R.T. -0.006 min
Lab File: VX028188.D
Acq: 20 Apr 2022 11:15




Instrument :
MSVOA_X
ClientSampleId :
VX0420MBL01


Tgt Ion:168 Resp: 403293
Ion Ratio Lower Upper
168 100
99 59.5 41.7 62.5

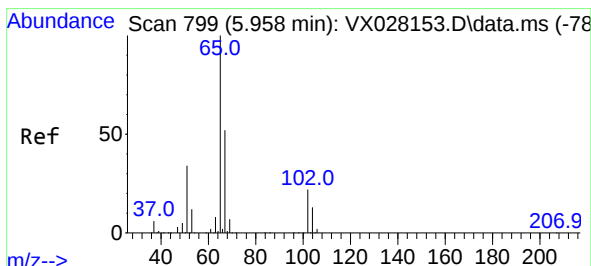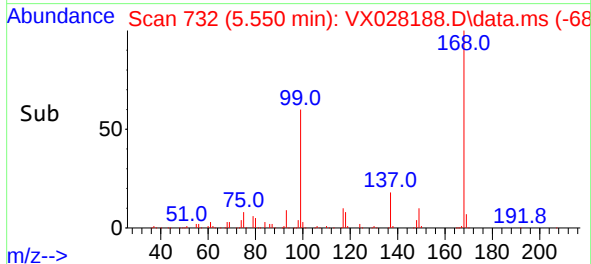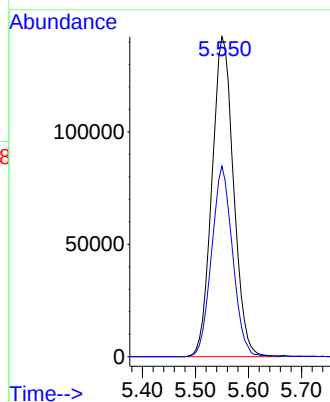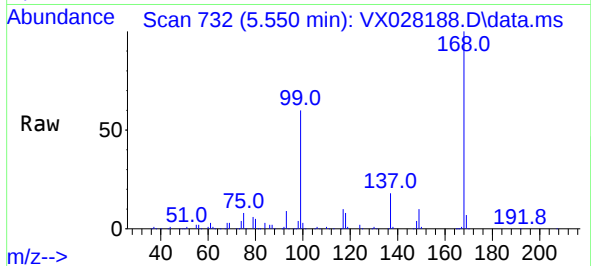

#33
1,2-Dichloroethane-d4
Concen: 43.484 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX028188.D
Acq: 20 Apr 2022 11:15


Tgt Ion: 65 Resp: 228662
Ion Ratio Lower Upper
65 100
67 51.7 0.0 107.4

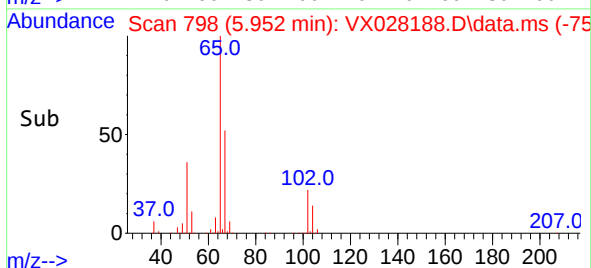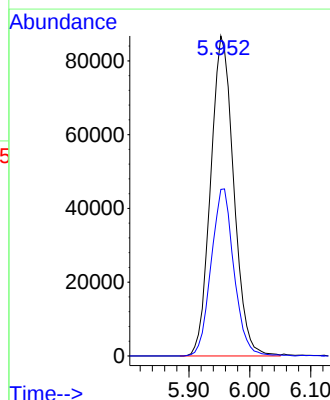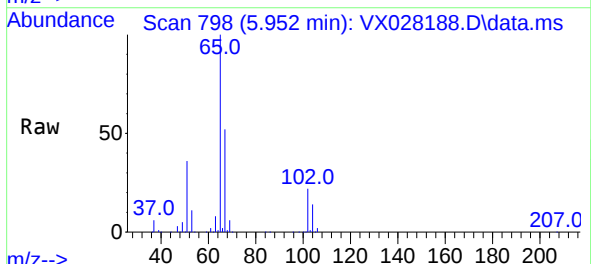



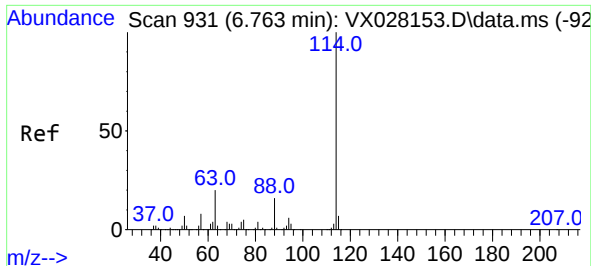


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX028188.D
Acq: 20 Apr 2022 11:15

Instrument :
MSVOA_X
ClientSampleId :
VX0420MBL01



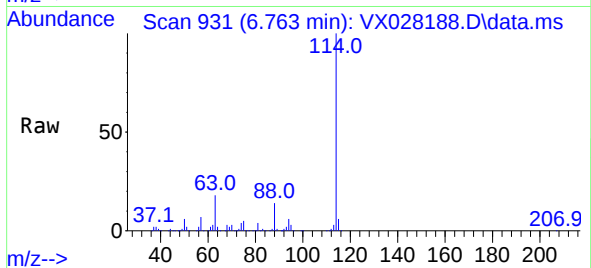


Tgt Ion:114 Resp: 661358
Ion Ratio Lower Upper
114 100
63 17.6 0.0 36.8
88 14.5 0.0 32.4

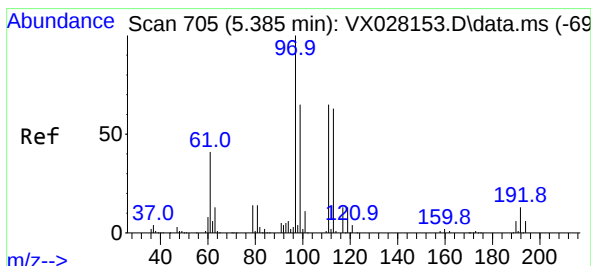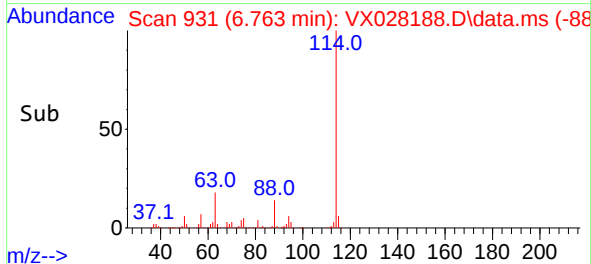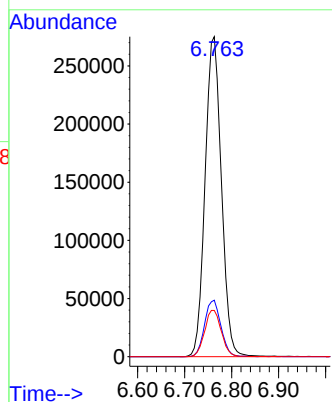

#35
Dibromofluoromethane
Concen: 44.579 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX028188.D
Acq: 20 Apr 2022 11:15

Tgt Ion:113 Resp: 206758
Ion Ratio Lower Upper
113 100
111 101.6 82.8 124.2
192 20.1 16.9 25.3


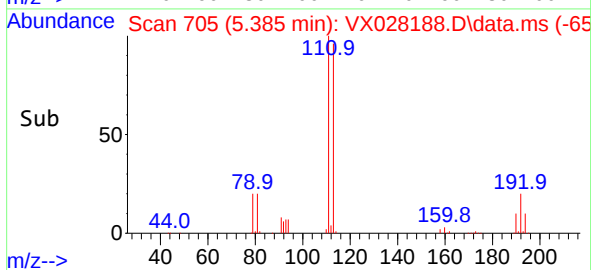
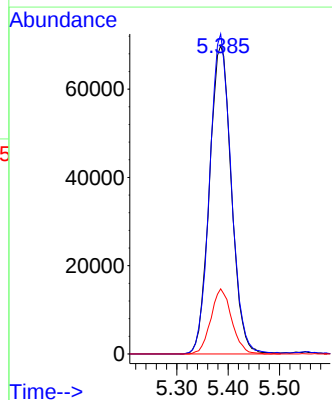
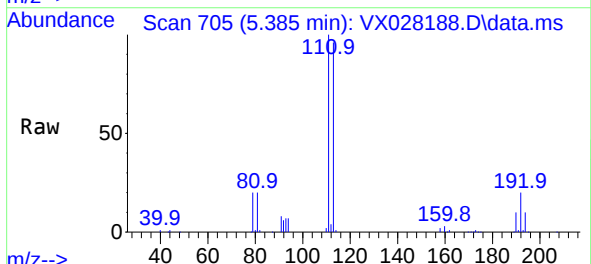




#50
Toluene-d8
Concen: 42.496 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX028188.D
Acq: 20 Apr 2022 11:15




Instrument :
MSVOA_X
ClientSampleId :
VX0420MBL01


Tgt Ion: 98 Resp: 757013
Ion Ratio Lower Upper
98 100
100 66.3 52.6 78.8

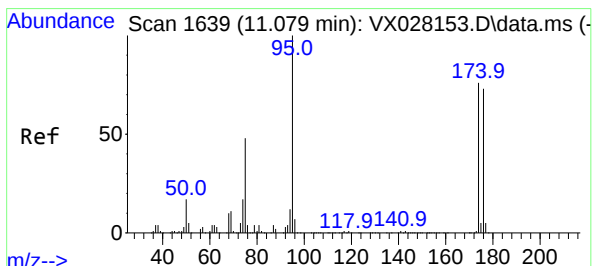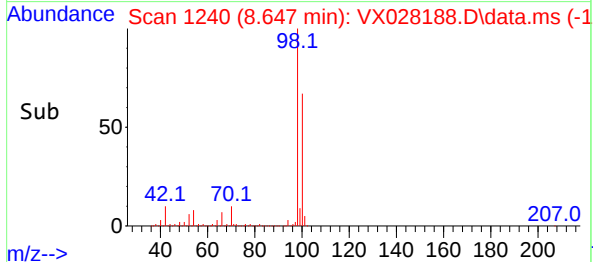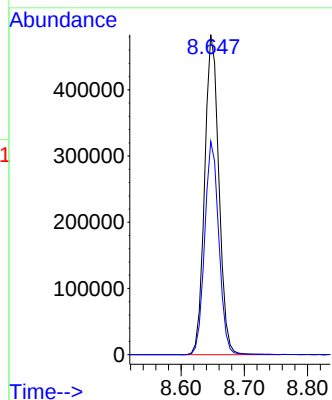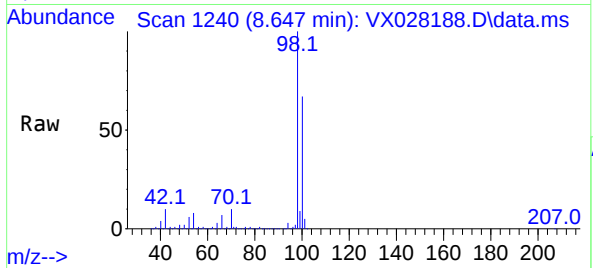

#62
4-Bromofluorobenzene
Concen: 37.885 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX028188.D
Acq: 20 Apr 2022 11:15

Tgt Ion: 95 Resp: 258045
Ion Ratio Lower Upper
95 100
174 82.6 0.0 163.0
176 79.4 0.0 155.0


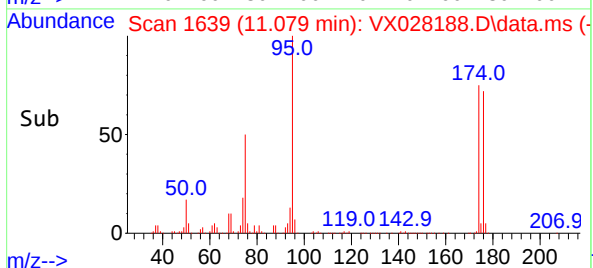
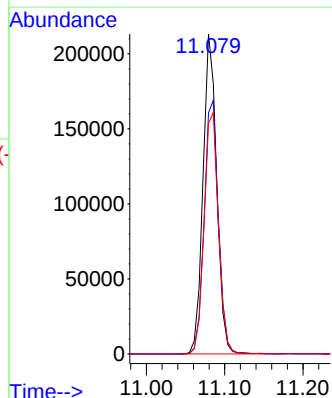
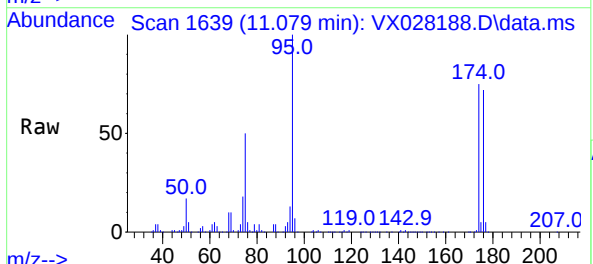


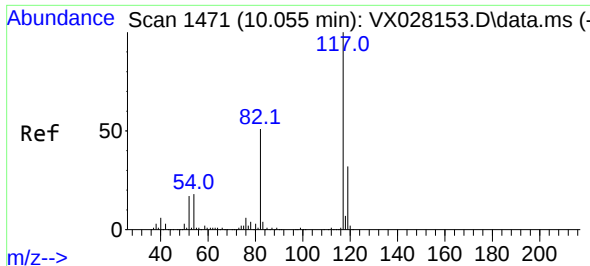

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX028188.D
Acq: 20 Apr 2022 11:15

Instrument :
MSVOA_X
ClientSampleId :
VX0420MBL01

Tgt Ion:117 Resp: 577833
Ion Ratio Lower Upper
117 100
82 51.6 41.8 62.8
119 32.7 24.8 37.2

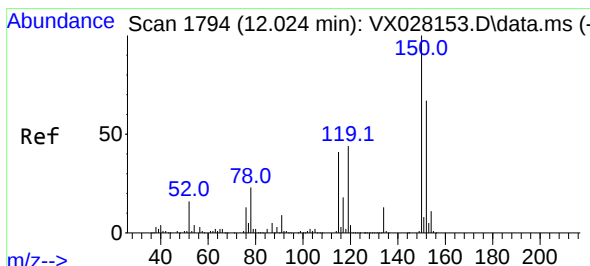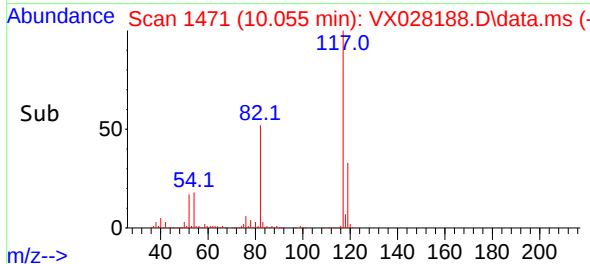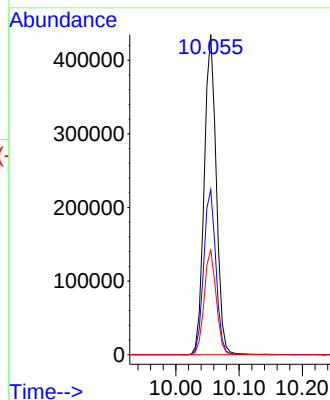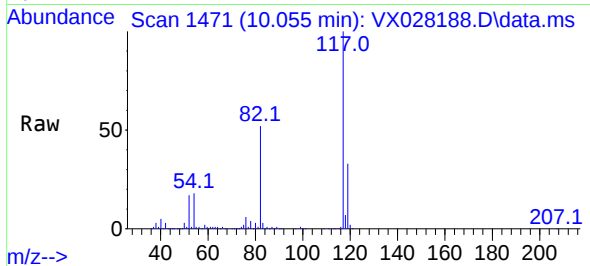

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX028188.D
Acq: 20 Apr 2022 11:15

Tgt Ion:152 Resp: 254780
Ion Ratio Lower Upper
152 100
115 58.4 37.5 112.7
150 156.5 0.0 338.2

