

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042022\
 Data File : VX028202.D
 Acq On : 20 Apr 2022 16:58
 Operator : JC/MD
 Sample : N2450-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SOIL-REF-6

Quant Time: Apr 21 06:14:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 19 13:38:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	374283	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	640123	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	603589	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	277384	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	267546	54.823	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	109.640%
35) Dibromofluoromethane	5.391	113	245903	54.777	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	109.560%
50) Toluene-d8	8.653	98	882662	51.193	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	102.380%
62) 4-Bromofluorobenzene	11.079	95	318371	48.292	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	96.580%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042022\
Data File : VX028202.D
Acq On : 20 Apr 2022 16:58
Operator : JC/MD
Sample : N2450-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Quant Time: Apr 21 06:14:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 19 13:38:04 2022
Response via : Initial Calibration




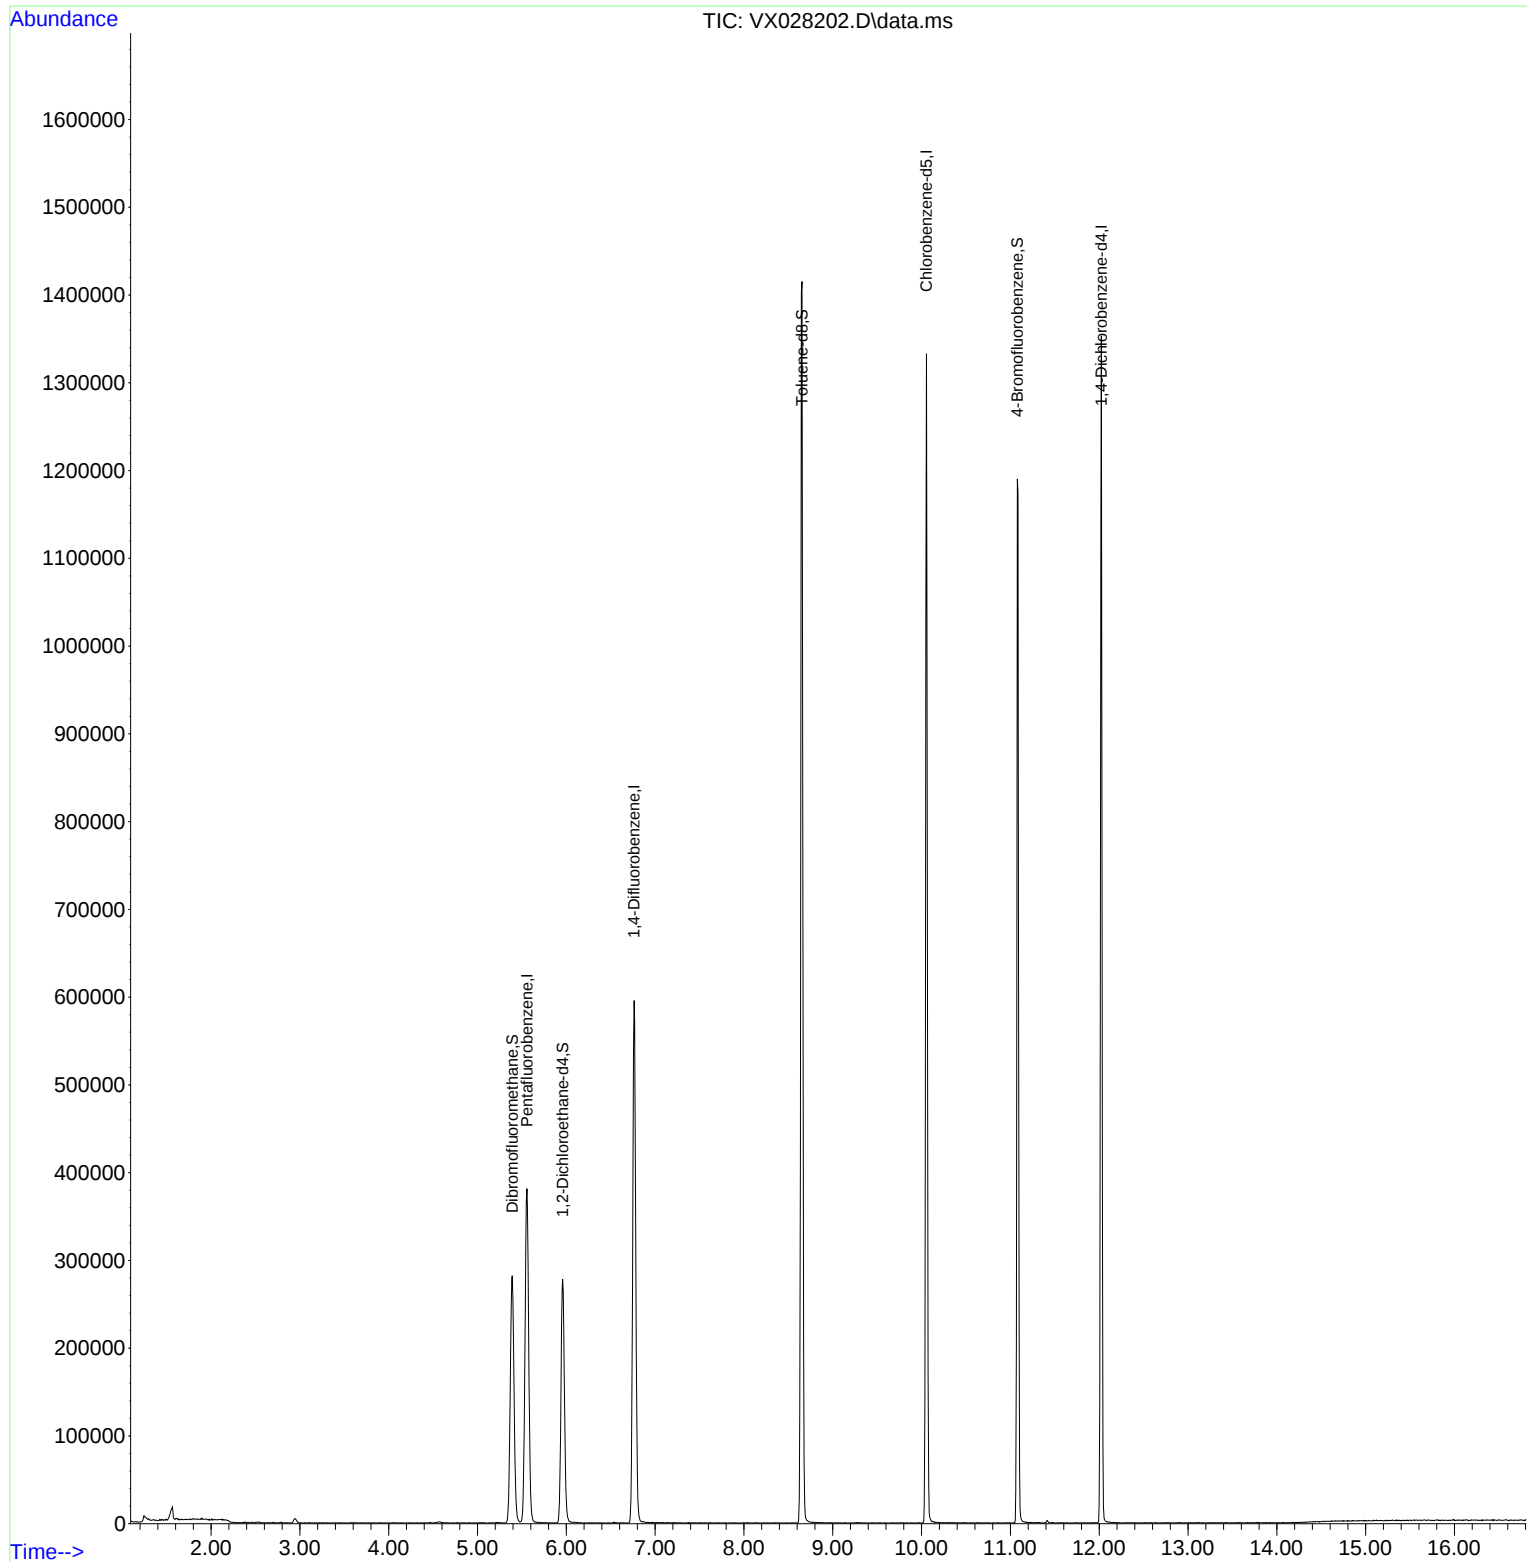




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 713
Delta R.T. -0.000 min
Lab File: VX028202.D
Acq: 20 Apr 2022 16:58




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion:168 Resp: 374283
Ion Ratio Lower Upper
168 100
99 56.9 41.7 62.5

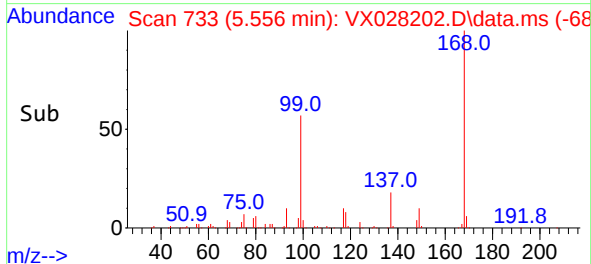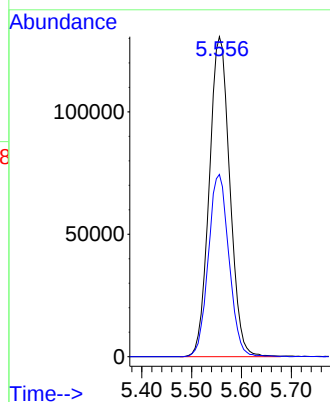

#33
1,2-Dichloroethane-d4
Concen: 54.823 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.000 min
Lab File: VX028202.D
Acq: 20 Apr 2022 16:58

Tgt Ion: 65 Resp: 267546
Ion Ratio Lower Upper
65 100
67 52.1 0.0 107.4

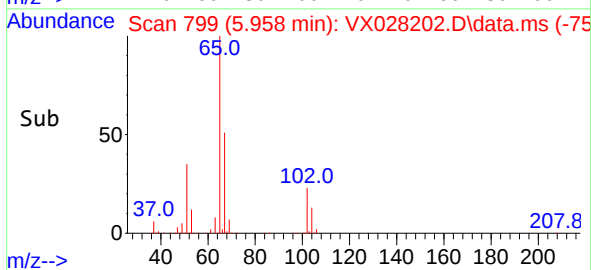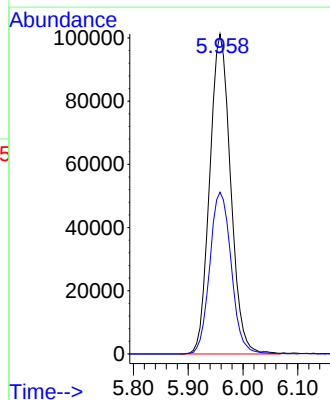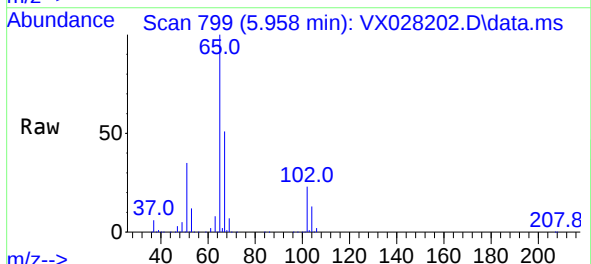







#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX028202.D
Acq: 20 Apr 2022 16:58

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Tgt Ion:114 Resp: 640123




Ion	Ratio	Lower	Upper
114	100		
63	19.3	0.0	36.8
88	15.3	0.0	32.4

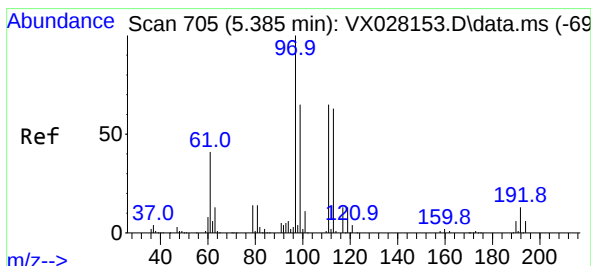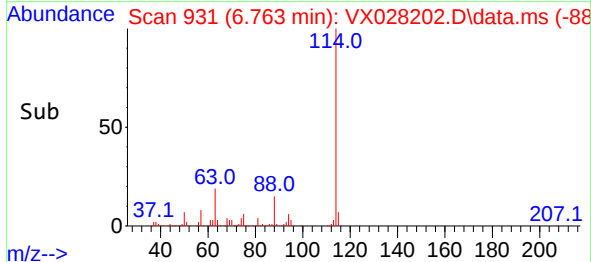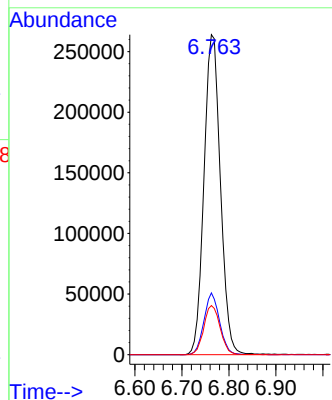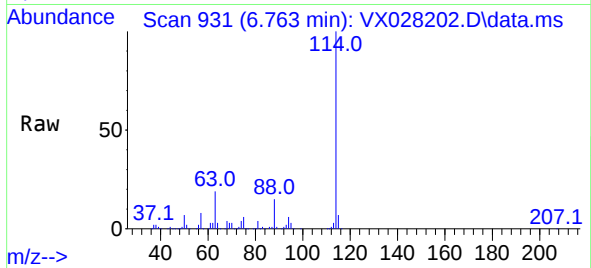


#35
Dibromofluoromethane
Concen: 54.777 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX028202.D
Acq: 20 Apr 2022 16:58

Tgt Ion:113 Resp: 245903

Ion	Ratio	Lower	Upper
113	100		
111	102.9	82.8	124.2
192	19.8	16.9	25.3


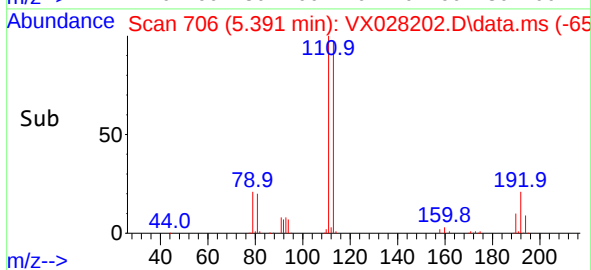
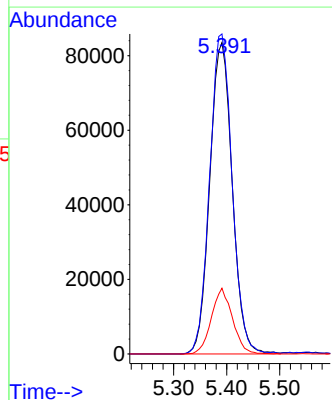
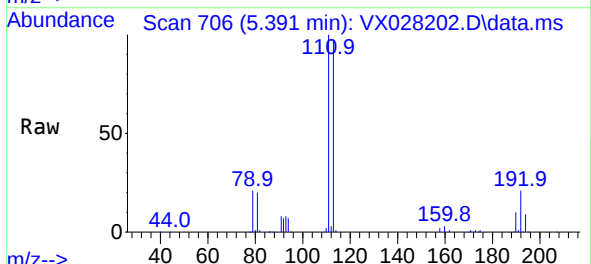




#50
Toluene-d8
Concen: 51.193 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX028202.D
Acq: 20 Apr 2022 16:58




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion: 98 Resp: 882662
Ion Ratio Lower Upper
98 100
100 65.8 52.6 78.8

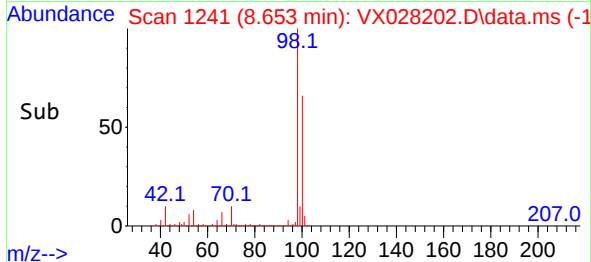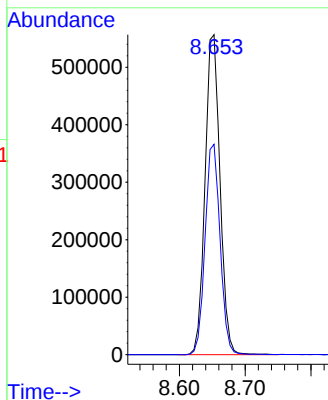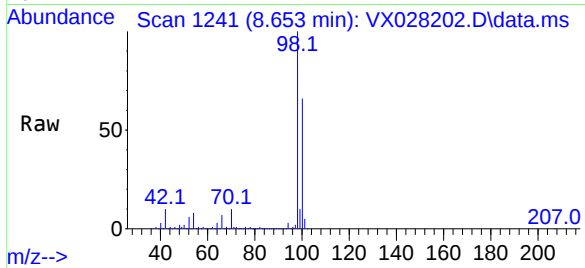

#62
4-Bromofluorobenzene
Concen: 48.292 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX028202.D
Acq: 20 Apr 2022 16:58

Tgt Ion: 95 Resp: 318371
Ion Ratio Lower Upper
95 100
174 82.9 0.0 163.0
176 80.3 0.0 155.0


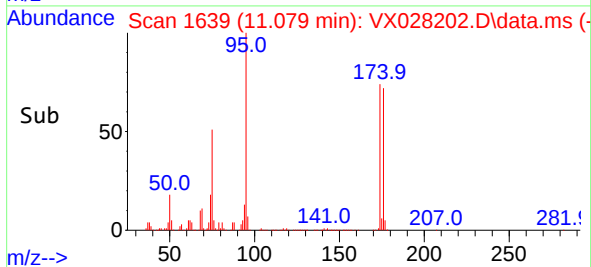
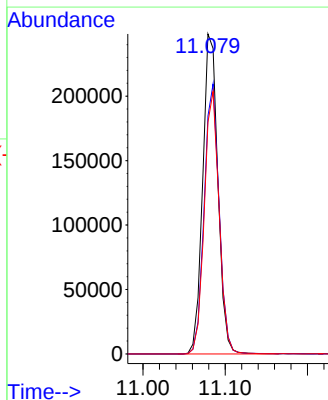
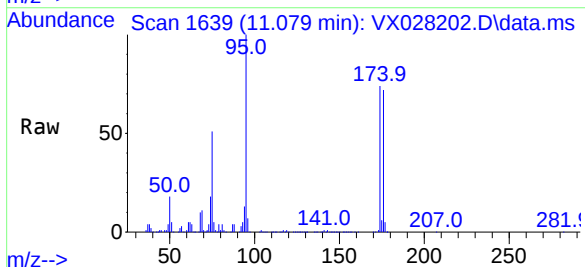




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX028202.D
Acq: 20 Apr 2022 16:58

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Tgt Ion:117 Resp: 603589
Ion Ratio Lower Upper
117 100
82 53.2 41.8 62.8
119 33.0 24.8 37.2

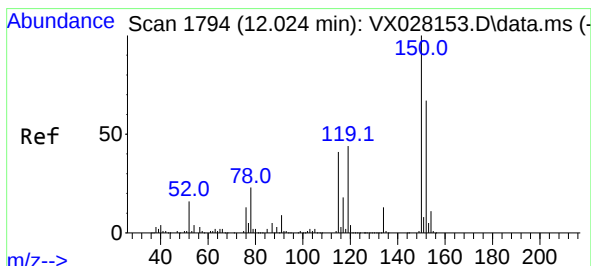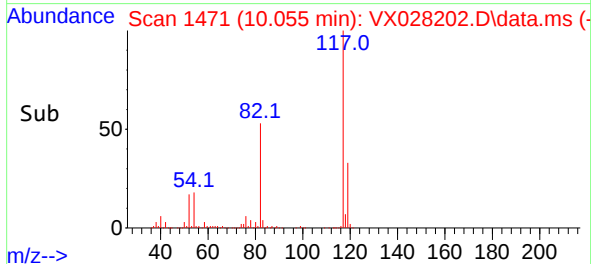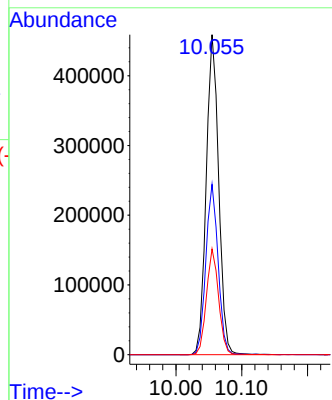

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX028202.D
Acq: 20 Apr 2022 16:58

Tgt Ion:152 Resp: 277384
Ion Ratio Lower Upper
152 100
115 58.6 37.5 112.7
150 156.8 0.0 338.2

