

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042022\
 Data File : VX028197.D
 Acq On : 20 Apr 2022 15:02
 Operator : JC/MD
 Sample : N2448-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E14ST-B6-041522-GW-DUP

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
 Title : SW846 8260

Signal : TIC: VX028197.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.557	69	77	81	rBV5	13880	28315	1.16%	0.229%
2	2.526	230	236	247	rVB	16152	33482	1.38%	0.271%
3	5.105	647	659	671	rBV2	58258	181940	7.49%	1.473%
4	5.391	693	706	722	rBV	303513	884400	36.39%	7.160%
5	5.556	722	733	750	rVB	401357	1146490	47.17%	9.282%
6	5.958	787	799	819	rBV	314280	811483	33.39%	6.570%
7	6.763	921	931	946	rBV	632224	1493789	61.46%	12.094%
8	7.824	1099	1105	1114	rBV3	12507	25433	1.05%	0.206%
9	8.653	1234	1241	1249	rBV	1536301	2430544	100.00%	19.678%
10	10.055	1465	1471	1481	rBV	1436002	1852397	76.21%	14.997%
11	11.085	1634	1640	1652	rBV	1311598	1686921	69.41%	13.657%
12	12.024	1788	1794	1802	rBV	1466159	1776600	73.09%	14.383%




Sum of corrected areas: 12351794

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042022\
Data File : VX028197.D
Acq On : 20 Apr 2022 15:02
Operator : JC/MD
Sample : N2448-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E14ST-B6-041522-GW-DUP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

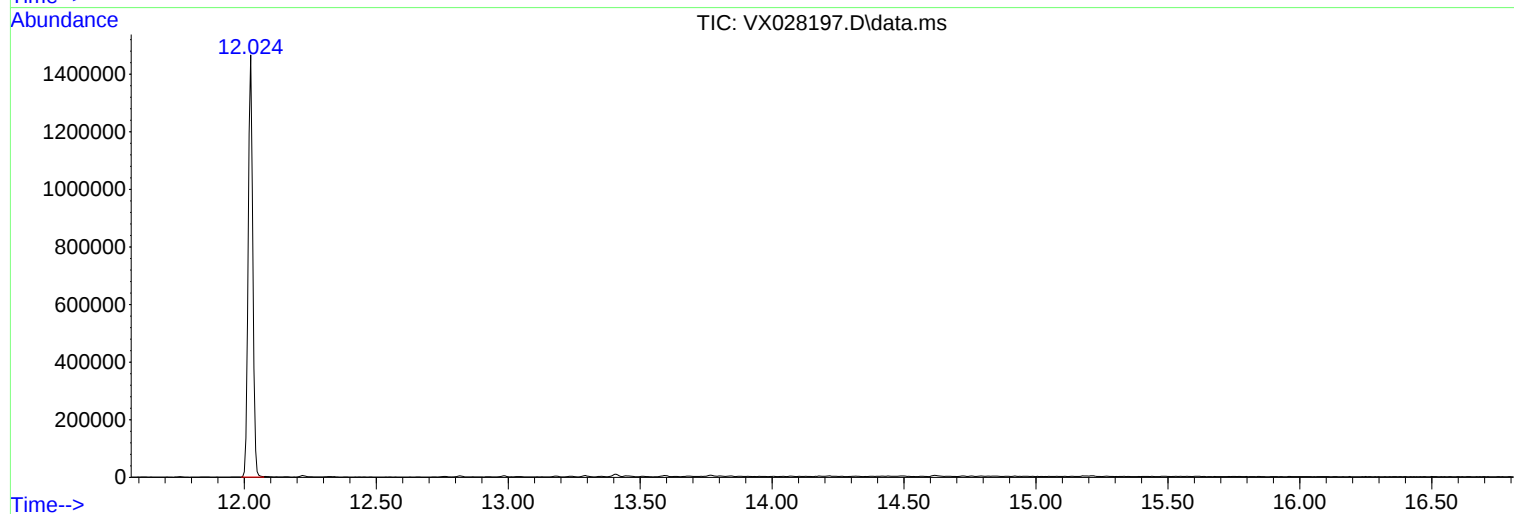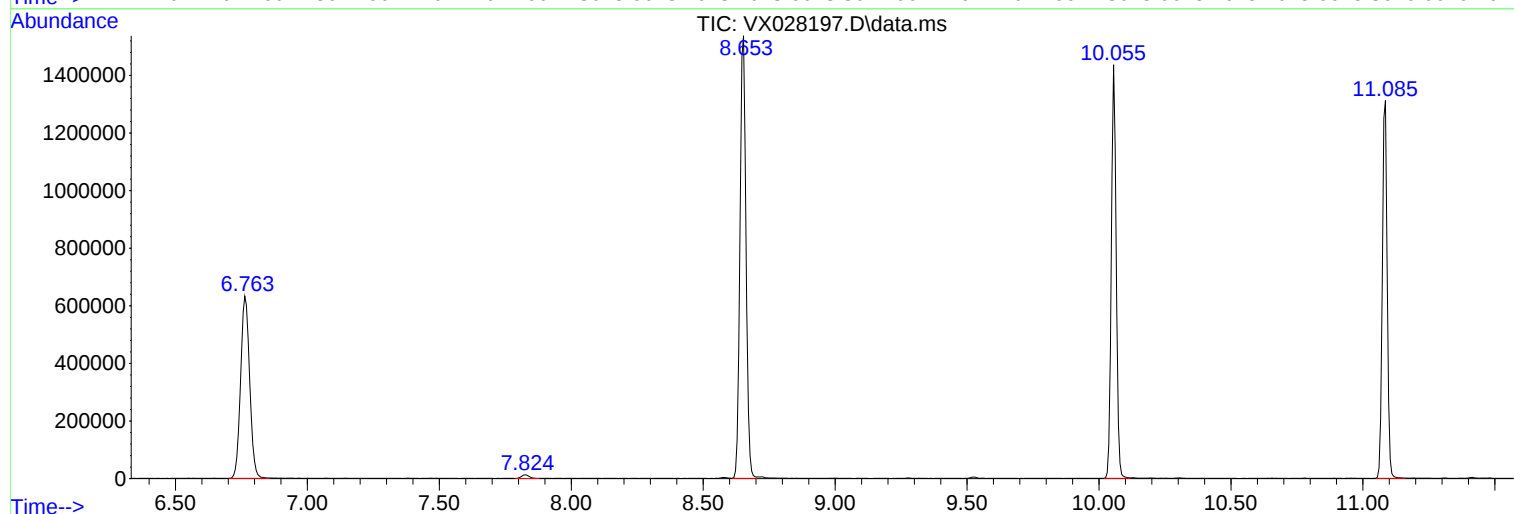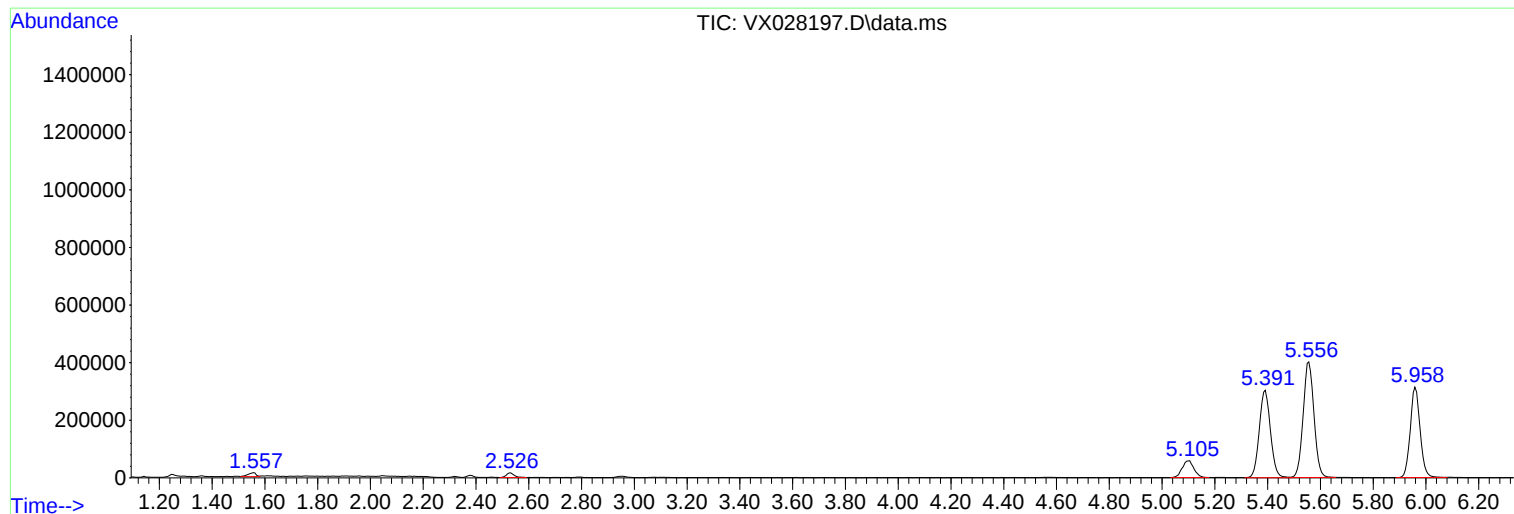

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042022\
Data File : VX028197.D
Acq On : 20 Apr 2022 15:02
Operator : JC/MD
Sample : N2448-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E14ST-B6-041522-GW-DUP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042022\
Data File : VX028197.D
Acq On : 20 Apr 2022 15:02
Operator : JC/MD
Sample : N2448-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E14ST-B6-041522-GW-DUP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc