

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035214.D
 Acq On : 20 Apr 2023 14:40
 Operator : JC/MD
 Sample : 02378-18DL 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML1DL

Quant Time: Apr 20 23:30:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 20 23:27:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	475849	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	409792	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	197971	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	100048	32.607	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	65.220%	
7) Chloroethane-d5	1.672	69	87723	39.566	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	79.140%	
11) 1,1-Dichloroethene-d2	2.307	65	53372	36.354	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	72.700%	
21) 2-Butanone-d5	4.465	46	219672	107.435	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	107.440%	
24) Chloroform-d	5.056	84	253180	43.817	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	87.640%	
26) 1,2-Dichloroethane-d4	5.952	65	173777	46.833	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	93.660%	
32) Benzene-d6	5.977	84	522146	44.356	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	88.720%	
36) 1,2-Dichloropropane-d6	7.306	67	169800	47.221	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	94.440%	
41) Toluene-d8	8.647	98	452777	42.085	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	84.180%	
43) trans-1,3-Dichloroprop...	8.952	79	63622	40.486	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	80.980%	
47) 2-Hexanone-d5	9.385	63	152233	105.425	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	105.420%	
56) 1,1,2,2-Tetrachloroeth...	11.189	84	220465	50.063	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	100.120%	
66) 1,2-Dichlorobenzene-d4	12.317	152	176528	46.013	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	92.020%	
Target Compounds						
					Qvalue	
33) Benzene	6.038	78	379882	30.611	ug/L	100
51) Chlorobenzene	10.080	112	462207	54.489	ug/L	99
64) 1,3-Dichlorobenzene	11.969	146	21010	3.422	ug/L	98
65) 1,4-Dichlorobenzene	12.043	146	254556	40.519	ug/L	98
67) 1,2-Dichlorobenzene	12.335	146	305990	49.154	ug/L	99
70) 1,2,4-trichlorobenzene	13.591	180	27401	7.710	ug/L	98
72) 1,2,3-Trichlorobenzene	13.963	180	5586	1.592	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035214.D
Acq On : 20 Apr 2023 14:40
Operator : JC/MD
Sample : 02378-18DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COML1DL

Quant Time: Apr 20 23:30:00 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 20 23:27:37 2023
Response via : Initial Calibration




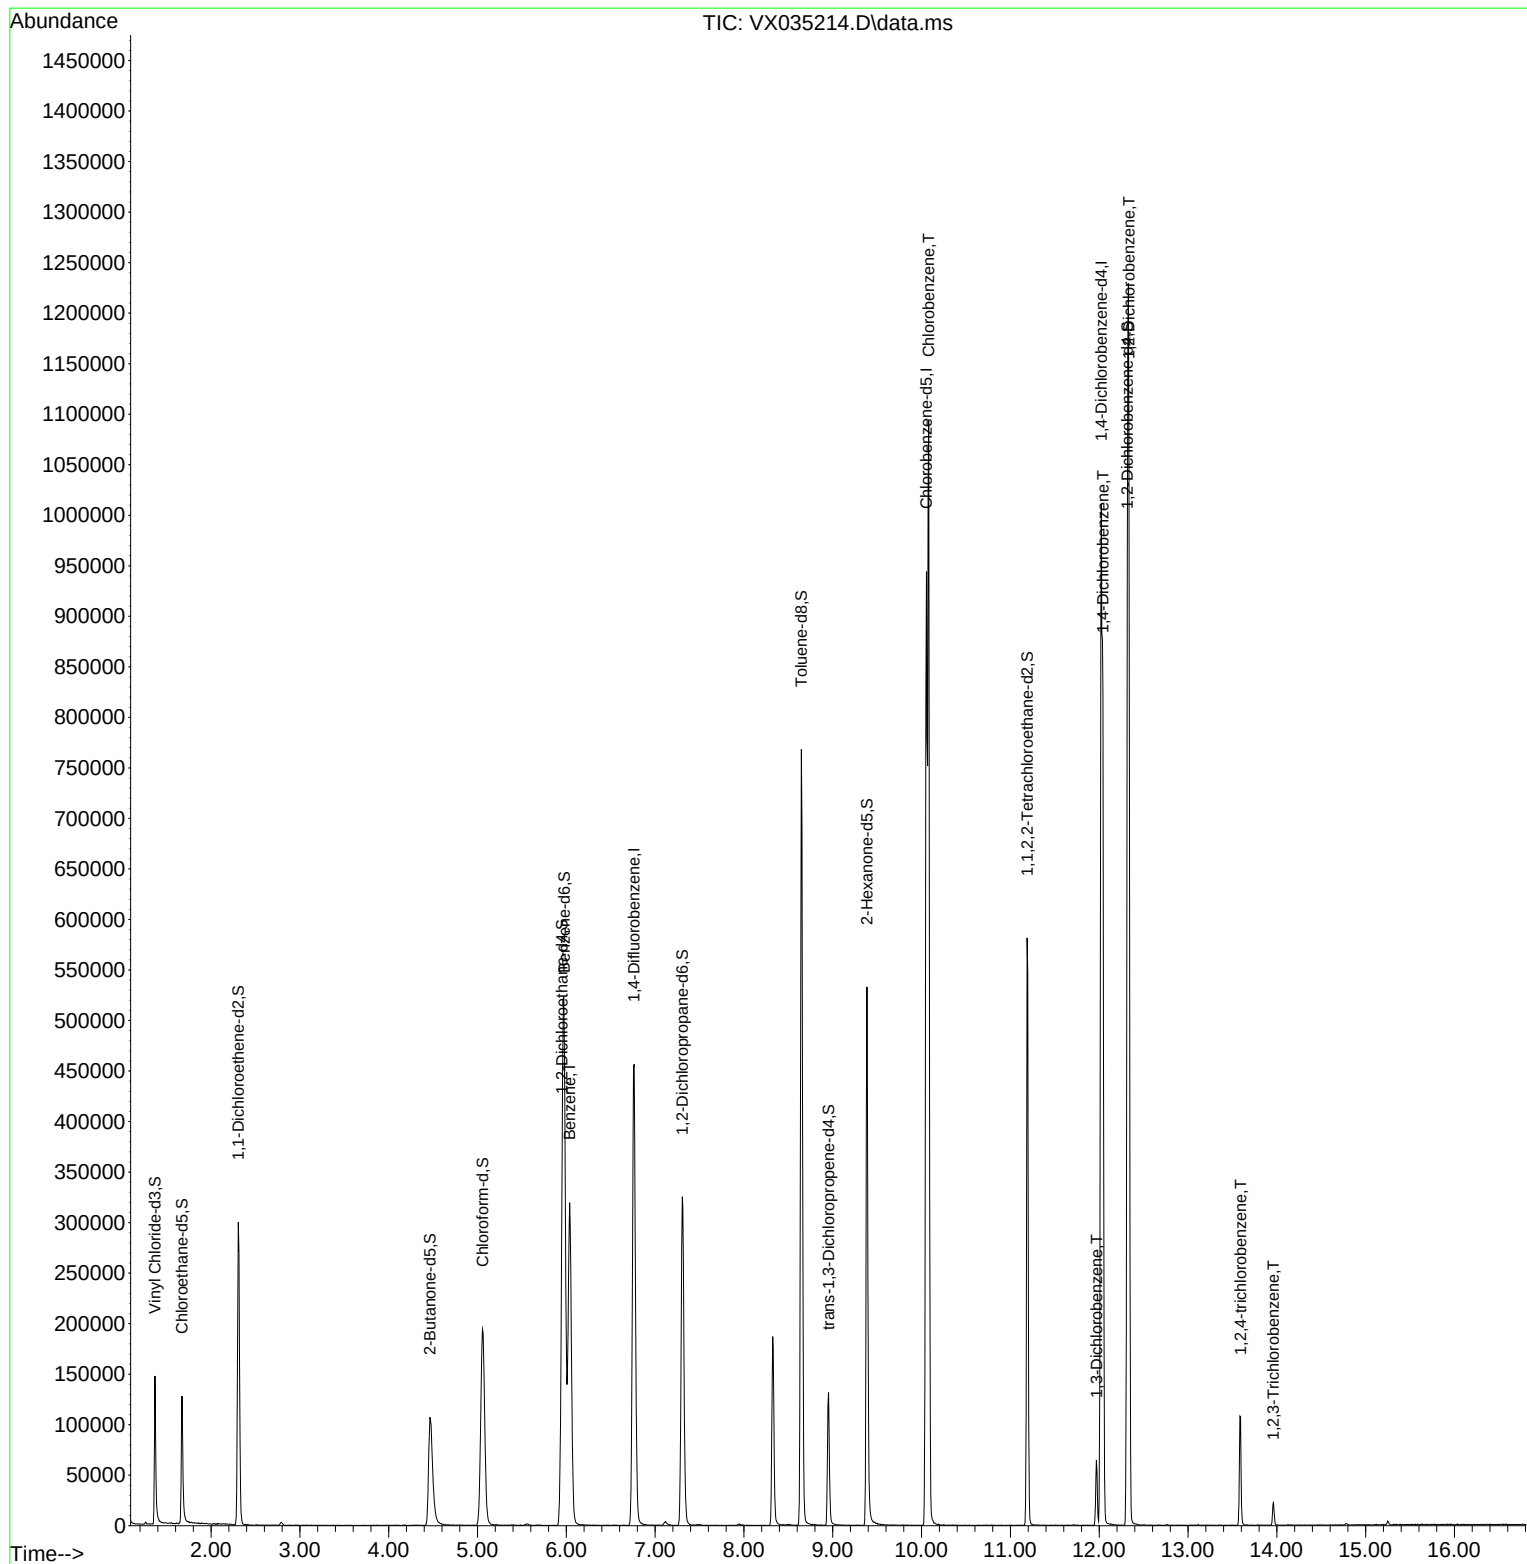


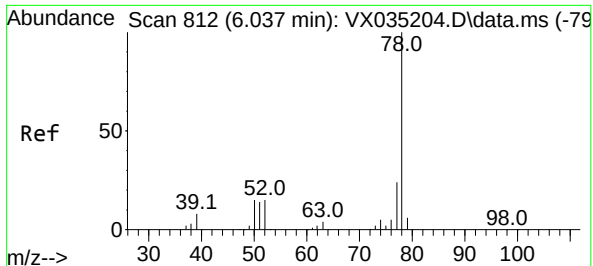

#33
Benzene
Concen: 30.611 ug/L
RT: 6.038 min Scan# 812
Delta R.T. 0.000 min
Lab File: VX035214.D
Acq: 20 Apr 2023 14:40




Instrument :
MSVOA_X
ClientSampleId :
COML1DL


Tgt Ion: 78 Resp: 379882

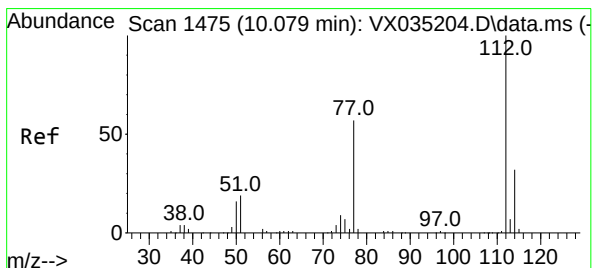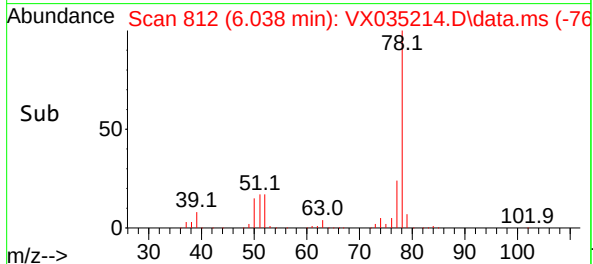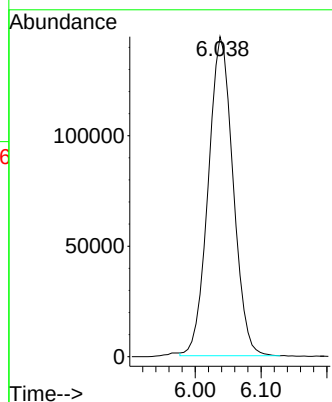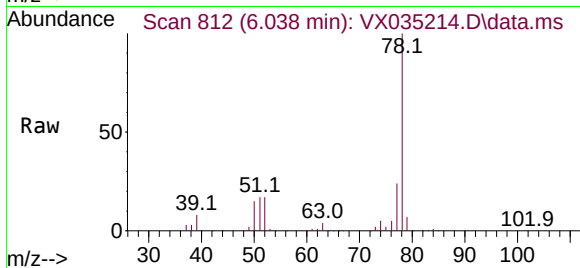

#51
Chlorobenzene
Concen: 54.489 ug/L
RT: 10.080 min Scan# 1475
Delta R.T. 0.000 min
Lab File: VX035214.D
Acq: 20 Apr 2023 14:40

Tgt Ion:112 Resp: 462207
Ion Ratio Lower Upper
112 100
114 32.6 22.4 41.6
77 59.3 47.0 70.6


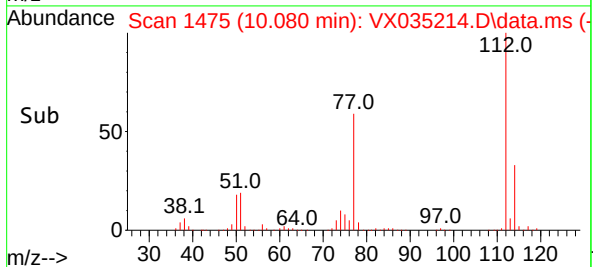
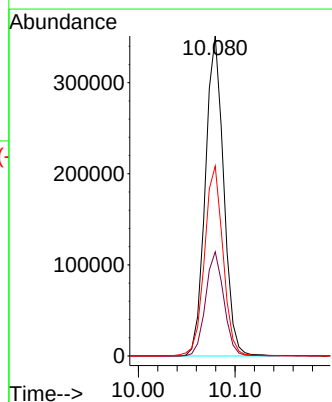
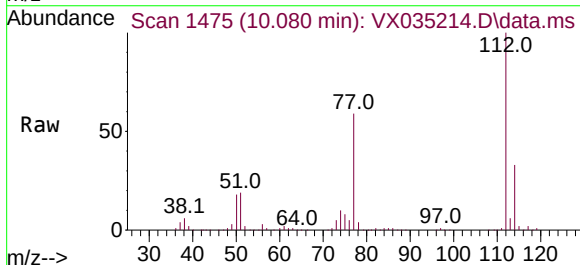


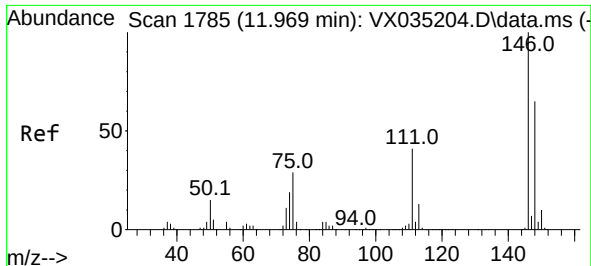

#64
1,3-Dichlorobenzene
Concen: 3.422 ug/L
RT: 11.969 min Scan# 1785
Delta R.T. 0.000 min
Lab File: VX035214.D
Acq: 20 Apr 2023 14:40




Instrument :
MSVOA_X
ClientSampleId :
COML1DL


Tgt Ion:146 Resp: 21010
Ion Ratio Lower Upper
146 100
111 43.2 28.9 53.7
148 62.3 44.3 82.3

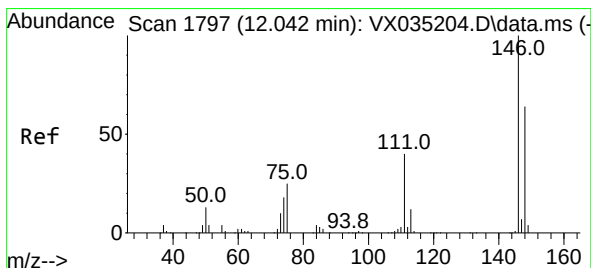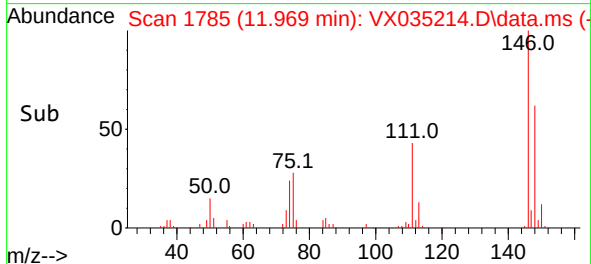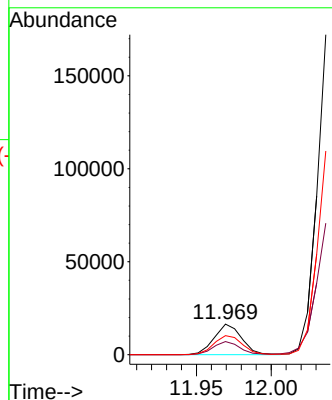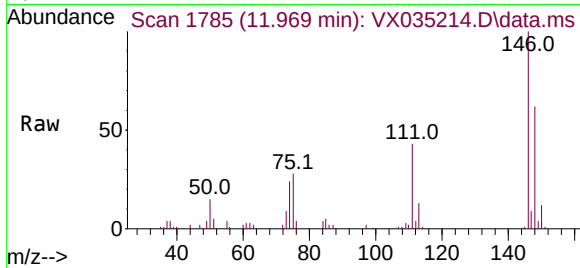

#65
1,4-Dichlorobenzene
Concen: 40.519 ug/L
RT: 12.043 min Scan# 1797
Delta R.T. 0.000 min
Lab File: VX035214.D
Acq: 20 Apr 2023 14:40

Tgt Ion:146 Resp: 254556
Ion Ratio Lower Upper
146 100
111 38.2 27.9 51.7
148 64.4 45.9 85.3

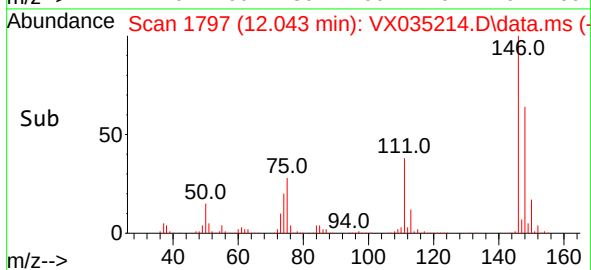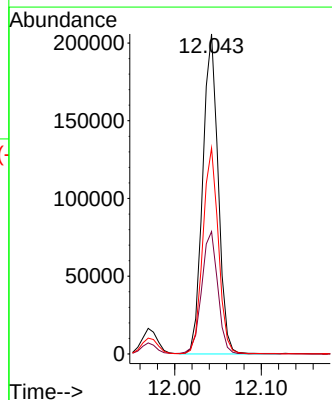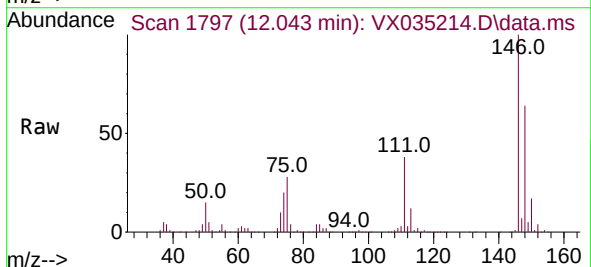

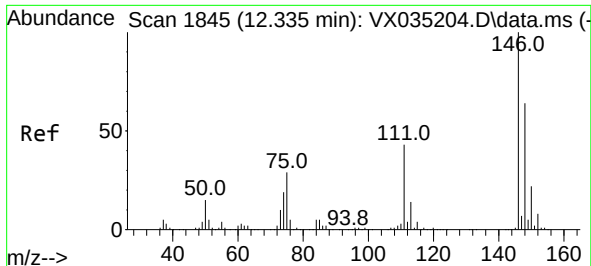

#67

1,2-Dichlorobenzene

Concen: 49.154 ug/L

RT: 12.335 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX035214.D

Acq: 20 Apr 2023 14:40

Instrument :

MSVOA_X

ClientSampleId :

COML1DL





Tgt Ion:146 Resp: 305990

Ion Ratio Lower Upper

146 100

111 43.3 34.7 52.1

148 65.8 52.1 78.1

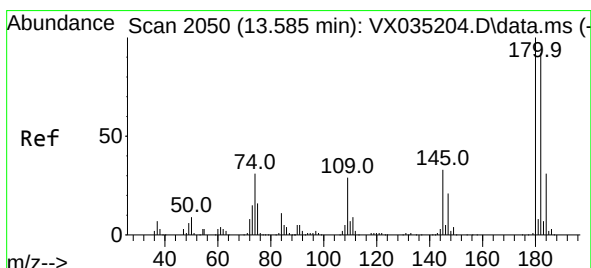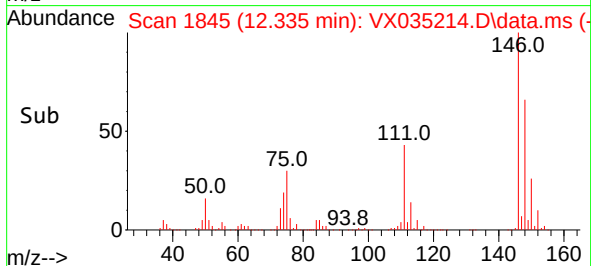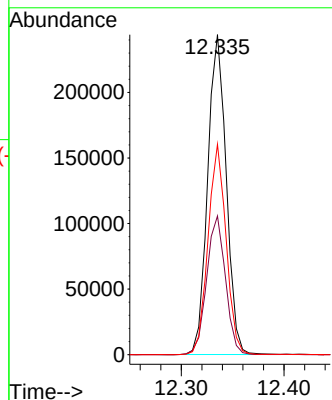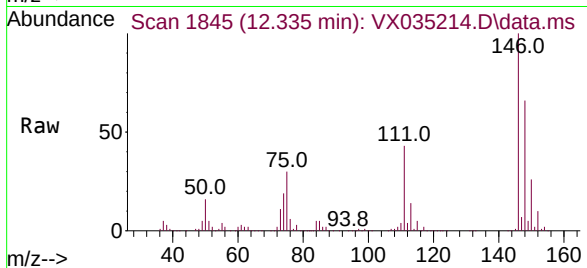

#70

1,2,4-trichlorobenzene

Concen: 7.710 ug/L

RT: 13.591 min Scan# 2051

Delta R.T. 0.006 min

Lab File: VX035214.D

Acq: 20 Apr 2023 14:40




Tgt Ion:180 Resp: 27401


Ion Ratio Lower Upper

180 100

182 97.3 76.6 114.8


145 34.2 26.2 39.4

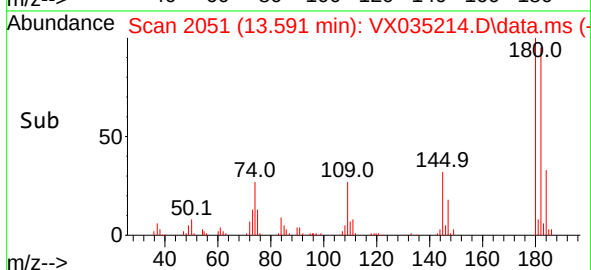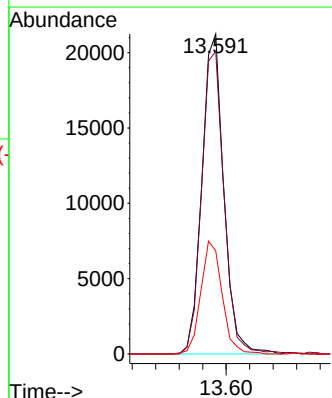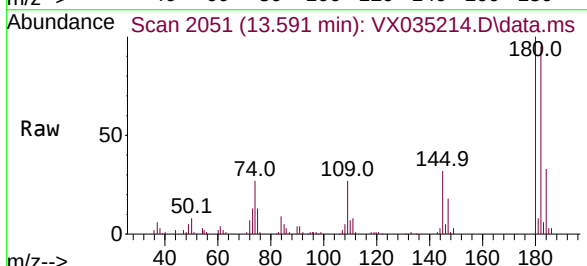

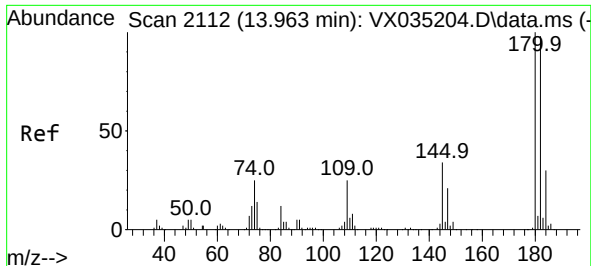

#72
 1,2,3-Trichlorobenzene
 Concen: 1.592 ug/L
 RT: 13.963 min Scan# 2112
 Delta R.T. 0.000 min
 Lab File: VX035214.D
 Acq: 20 Apr 2023 14:40

Instrument :
 MSVOA_X
 ClientSampleId :
 C0ML1DL

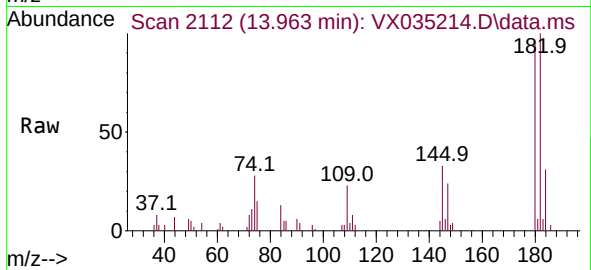

Tgt Ion:	180	Resp:	5586
Ion	Ratio	Lower	Upper
180	100		
182	101.3	75.0	112.6
145	34.6	27.1	40.7

