

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035205.D
 Acq On : 20 Apr 2023 10:29
 Operator : JC/MD
 Sample : VX0420WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK626

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035205.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	32	rBV4	2297	2166	0.14%	0.018%
2	1.368	42	46	57	rBV	174549	188535	11.93%	1.580%
3	1.672	91	96	108	rBV	129374	173682	10.99%	1.455%
4	2.306	194	200	212	rBV	334542	523142	33.09%	4.383%
5	2.441	220	222	223	rBV	344	232	0.01%	0.002%
6	2.605	247	249	252	rVB3	333	271	0.02%	0.002%
7	2.788	274	279	287	rBV3	3448	6296	0.40%	0.053%
8	2.904	296	298	300	rBV2	249	202	0.01%	0.002%
9	3.026	316	318	320	rBV2	375	222	0.01%	0.002%
10	3.392	374	378	381	rVV2	218	367	0.02%	0.003%
11	3.727	430	433	435	rVB3	344	326	0.02%	0.003%
12	3.757	435	438	441	rBV3	276	372	0.02%	0.003%
13	3.837	449	451	452	rBV	255	195	0.01%	0.002%
14	3.946	467	469	471	rBV2	287	205	0.01%	0.002%
15	4.184	507	508	512	rVB	249	234	0.01%	0.002%
16	4.349	534	535	540	rBV2	310	314	0.02%	0.003%
17	4.465	545	554	575	rBV2	100227	312116	19.74%	2.615%
18	5.056	636	651	670	rBV	192679	597565	37.80%	5.007%
19	5.214	675	677	681	rVV2	484	716	0.05%	0.006%
20	5.269	685	686	688	rBV	387	353	0.02%	0.003%
21	5.385	700	705	710	rBV4	1035	2215	0.14%	0.019%
22	5.477	717	720	722	rBV4	321	359	0.02%	0.003%
23	5.556	725	733	741	rVV6	1796	5449	0.34%	0.046%
24	5.702	756	757	760	rVB2	336	244	0.02%	0.002%
25	5.787	770	771	774	rBV2	221	219	0.01%	0.002%
26	5.824	774	777	778	rVV2	251	228	0.01%	0.002%
27	5.970	788	801	821	rBV2	528402	1580938	100.00%	13.246%
28	6.757	920	930	952	rBV	443768	1062608	67.21%	8.903%
29	7.007	969	971	974	rBB2	303	202	0.01%	0.002%
30	7.110	982	988	996	rBV6	4101	11071	0.70%	0.093%
31	7.184	999	1000	1003	rBV	475	262	0.02%	0.002%
32	7.306	1011	1020	1039	rBV	325486	716715	45.33%	6.005%
33	7.494	1046	1051	1055	rBV6	785	1236	0.08%	0.010%
34	7.592	1064	1067	1070	rVB2	253	309	0.02%	0.003%
35	7.623	1070	1072	1074	rBV	224	192	0.01%	0.002%
36	7.714	1083	1087	1093	rBV2	253	519	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035205.D
 Acq On : 20 Apr 2023 10:29
 Operator : JC/MD
 Sample : VX0420WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK626

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	7.872	1111	1113	1115	rBV2	237	191	0.01%	0.002%
38	7.946	1121	1125	1129	rBV3	1096	1524	0.10%	0.013%
39	8.049	1140	1142	1145	rBV	266	192	0.01%	0.002%
40	8.324	1180	1187	1202	rBV	199944	328292	20.77%	2.751%
41	8.500	1212	1216	1219	rBV3	783	1277	0.08%	0.011%
42	8.647	1233	1240	1252	rBV	804698	1271060	80.40%	10.650%
43	8.952	1284	1290	1311	rBV	140239	209812	13.27%	1.758%
44	9.281	1340	1344	1347	rVB2	1208	1311	0.08%	0.011%
45	9.311	1347	1349	1354	rVB	266	208	0.01%	0.002%
46	9.384	1356	1361	1375	rBV	479450	676957	42.82%	5.672%
47	9.829	1432	1434	1438	rVB2	339	357	0.02%	0.003%
48	9.872	1438	1441	1443	rBV2	262	295	0.02%	0.002%
49	9.933	1449	1451	1452	rBV2	313	258	0.02%	0.002%
50	10.055	1465	1471	1483	rBV	851971	1216906	76.97%	10.196%
51	10.195	1491	1494	1501	rBV3	765	1341	0.08%	0.011%
52	10.299	1509	1511	1518	rVB4	966	1665	0.11%	0.014%
53	10.354	1518	1520	1521	rBV2	298	252	0.02%	0.002%
54	10.415	1527	1530	1534	rBV2	275	353	0.02%	0.003%
55	10.531	1545	1549	1550	rBV	224	249	0.02%	0.002%
56	10.591	1558	1559	1562	rVB2	398	372	0.02%	0.003%
57	10.640	1562	1567	1568	rBV3	813	956	0.06%	0.008%
58	10.927	1610	1614	1616	rBV2	295	320	0.02%	0.003%
59	10.963	1616	1620	1623	rBV3	705	1116	0.07%	0.009%
60	11.091	1638	1641	1644	rVB2	396	508	0.03%	0.004%
61	11.189	1652	1657	1668	rBV	543444	710122	44.92%	5.950%
62	11.372	1684	1687	1690	rBV2	267	284	0.02%	0.002%
63	11.451	1696	1700	1707	rVB4	954	1938	0.12%	0.016%
64	11.518	1709	1711	1713	rVB	321	255	0.02%	0.002%
65	11.549	1713	1716	1718	rBV3	303	442	0.03%	0.004%
66	11.707	1739	1742	1745	rVB2	662	630	0.04%	0.005%
67	11.762	1745	1751	1755	rBV3	919	1601	0.10%	0.013%
68	11.884	1770	1771	1773	rBV2	318	263	0.02%	0.002%
69	11.969	1780	1785	1788	rBV	4612	6243	0.39%	0.052%
70	12.024	1788	1794	1804	rVV	853289	1156049	73.12%	9.686%
71	12.317	1837	1842	1854	rBV	851463	1109109	70.16%	9.293%
72	12.530	1875	1877	1882	rVB4	318	346	0.02%	0.003%
73	12.579	1882	1885	1888	rBV2	430	483	0.03%	0.004%
74	12.695	1903	1904	1906	rBV2	249	236	0.01%	0.002%
75	12.737	1909	1911	1913	rBV2	367	330	0.02%	0.003%
76	12.762	1913	1915	1917	rBV2	649	561	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035205.D
 Acq On : 20 Apr 2023 10:29
 Operator : JC/MD
 Sample : VX0420WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK626

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	12.981	1949	1951	1954	rVB3	305	320	0.02%	0.003%
78	13.115	1970	1973	1979	rVB3	1702	2082	0.13%	0.017%
79	13.225	1990	1991	1995	rVB2	431	388	0.02%	0.003%
80	13.280	1995	2000	2001	rBV	373	649	0.04%	0.005%
81	13.432	2024	2025	2027	rVV	339	210	0.01%	0.002%
82	13.469	2030	2031	2034	rBV	282	301	0.02%	0.003%
83	13.530	2039	2041	2043	rVB	397	226	0.01%	0.002%
84	13.554	2043	2045	2046	rBV2	297	215	0.01%	0.002%
85	13.591	2046	2051	2059	rBV	16400	21758	1.38%	0.182%
86	13.701	2068	2069	2071	rBV2	261	198	0.01%	0.002%
87	13.737	2073	2075	2077	rVV	544	399	0.03%	0.003%
88	13.780	2077	2082	2088	rVB4	1904	3065	0.19%	0.026%
89	13.835	2088	2091	2094	rBV2	267	377	0.02%	0.003%
90	13.865	2094	2096	2100	rBV3	488	433	0.03%	0.004%
91	13.969	2109	2113	2119	rVB3	3600	5251	0.33%	0.044%
92	14.127	2136	2139	2144	rBV3	935	1402	0.09%	0.012%
93	14.268	2160	2162	2163	rVB	435	205	0.01%	0.002%
94	14.359	2174	2177	2178	rBV	470	349	0.02%	0.003%
95	14.475	2194	2196	2198	rBV2	315	250	0.02%	0.002%
96	14.505	2198	2201	2202	rBV	358	408	0.03%	0.003%
97	15.133	2302	2304	2306	rBV2	449	401	0.03%	0.003%
98	15.152	2306	2307	2308	rBV	540	308	0.02%	0.003%
99	15.993	2443	2445	2446	rBV2	622	397	0.03%	0.003%
100	16.761	2569	2571	2572	rBV	636	311	0.02%	0.003%


Sum of corrected areas: 11934844

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035205.D
Acq On : 20 Apr 2023 10:29
Operator : JC/MD
Sample : VX0420WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK626

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

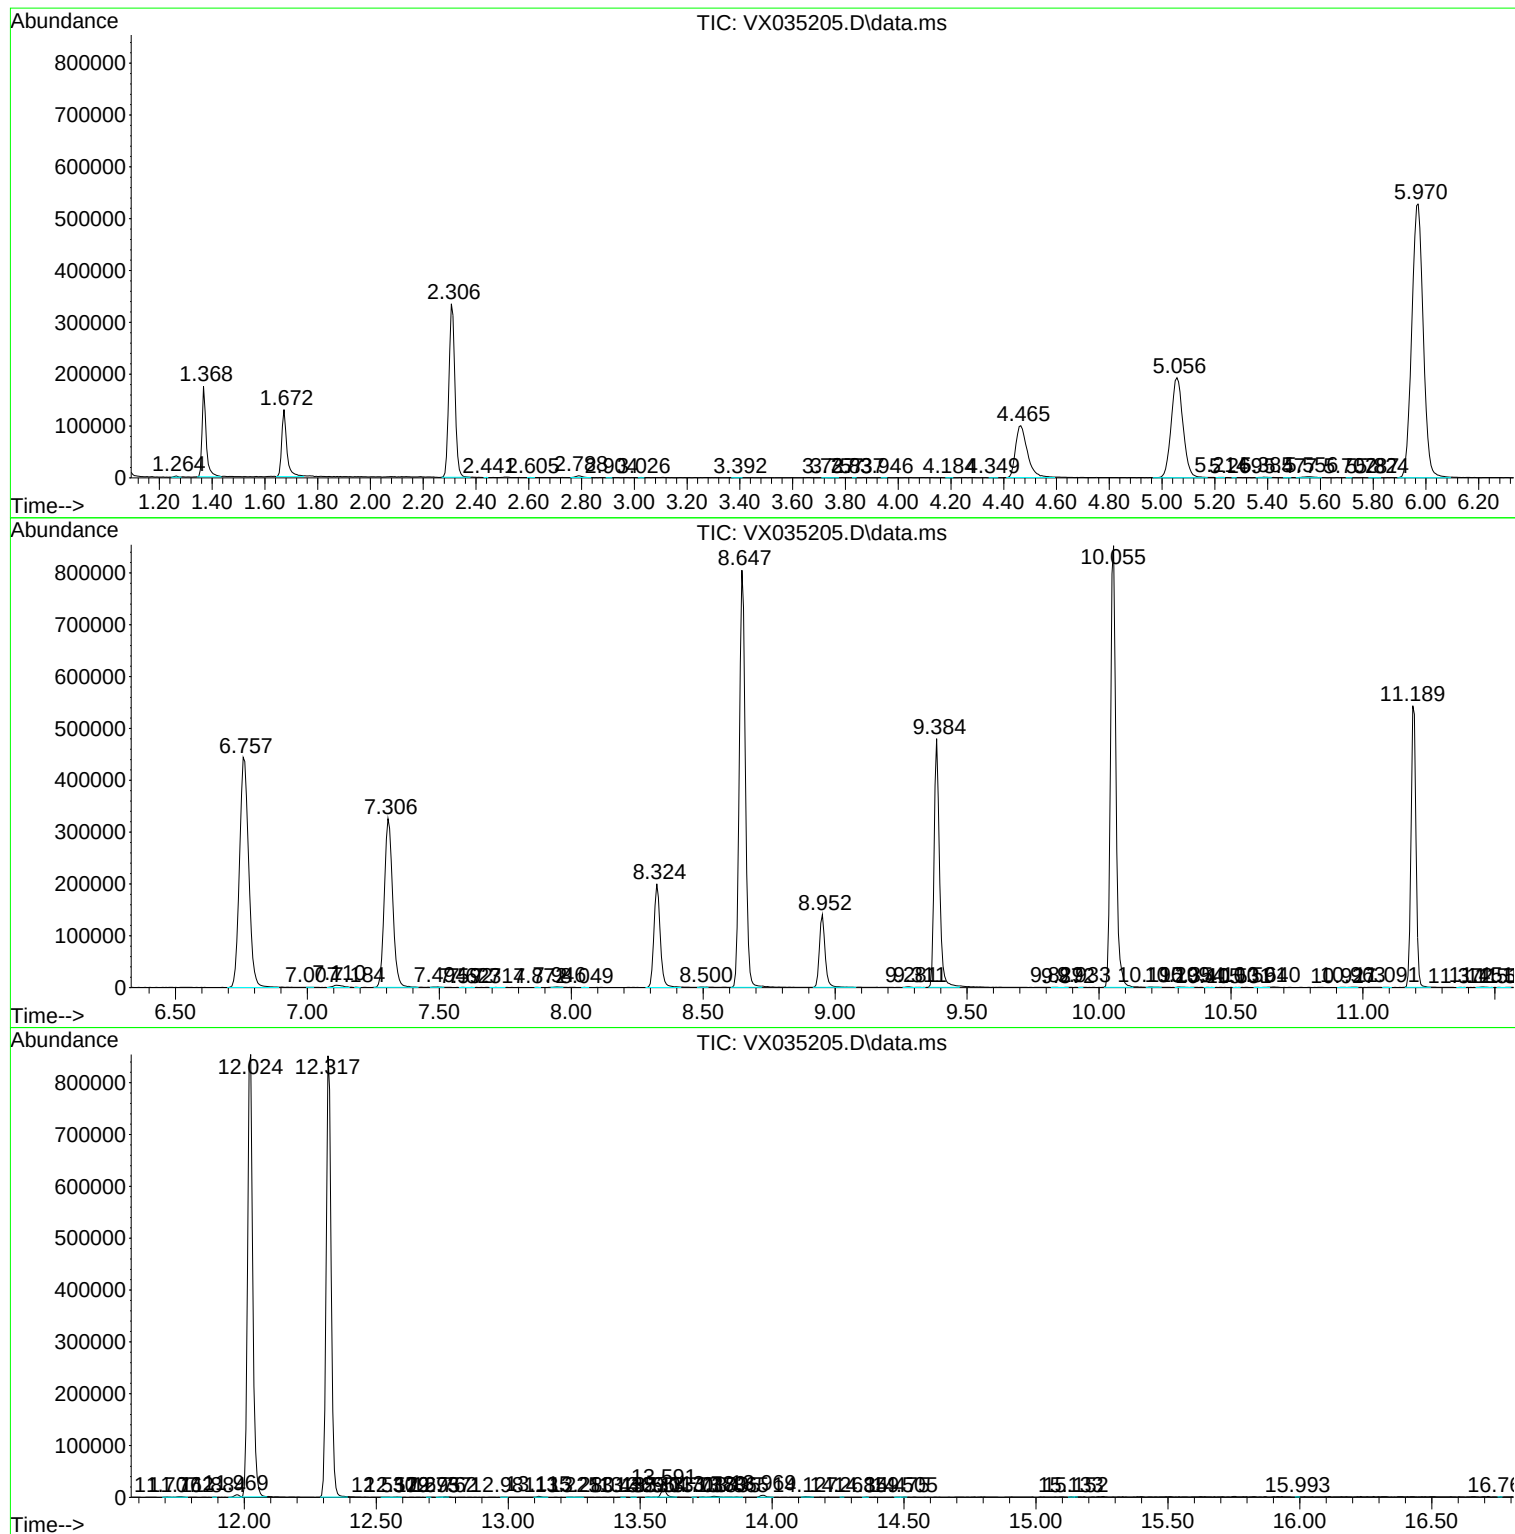

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035205.D
Acq On : 20 Apr 2023 10:29
Operator : JC/MD
Sample : VX0420WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK626

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035205.D
Acq On : 20 Apr 2023 10:29
Operator : JC/MD
Sample : VX0420WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK626

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc