

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035206.D
 Acq On : 20 Apr 2023 11:06
 Operator : JC/MD
 Sample : 02333-13DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMG8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035206.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	58	rBV	152110	172582	9.01%	1.260%
2	1.672	91	96	110	rBV	118235	160919	8.40%	1.175%
3	2.306	194	200	212	rVB	307972	475175	24.82%	3.469%
4	2.501	230	232	233	rBV	639	468	0.02%	0.003%
5	2.788	274	279	285	rBV2	4150	7056	0.37%	0.052%
6	2.940	300	304	309	rBV3	395	766	0.04%	0.006%
7	3.056	322	323	327	rVV2	190	213	0.01%	0.002%
8	3.129	330	335	338	rVV3	228	405	0.02%	0.003%
9	3.306	361	364	366	rBV	221	257	0.01%	0.002%
10	3.501	394	396	400	rVB2	207	232	0.01%	0.002%
11	3.684	422	426	428	rVB3	352	425	0.02%	0.003%
12	3.751	436	437	442	rVB2	212	287	0.01%	0.002%
13	3.800	442	445	446	rBV	335	280	0.01%	0.002%
14	3.958	468	471	472	rBV	291	317	0.02%	0.002%
15	4.282	523	524	526	rVB	373	219	0.01%	0.002%
16	4.306	526	528	530	rBV2	348	281	0.01%	0.002%
17	4.458	543	553	572	rBV	105210	321667	16.80%	2.348%
18	4.824	612	613	616	rBV2	364	368	0.02%	0.003%
19	4.916	625	628	631	rVB3	390	375	0.02%	0.003%
20	5.050	637	650	670	rBV	192208	610507	31.89%	4.457%
21	5.269	684	686	689	rBV2	254	263	0.01%	0.002%
22	5.354	697	700	701	rBV2	273	286	0.01%	0.002%
23	5.373	701	703	704	rBV2	462	376	0.02%	0.003%
24	5.550	726	732	742	rVB2	2266	4920	0.26%	0.036%
25	5.684	747	754	757	rVB3	775	1830	0.10%	0.013%
26	5.763	765	767	769	rBB	340	251	0.01%	0.002%
27	5.806	771	774	777	rVB2	279	330	0.02%	0.002%
28	5.964	787	800	807	rBV2	516221	1580847	82.57%	11.540%
29	6.257	847	848	850	rVB2	401	268	0.01%	0.002%
30	6.287	850	853	856	rVB2	232	264	0.01%	0.002%
31	6.440	875	878	880	rBV	331	306	0.02%	0.002%
32	6.556	890	897	905	rVB4	464	1312	0.07%	0.010%
33	6.616	905	907	910	rBV2	311	346	0.02%	0.003%
34	6.757	920	930	947	rBV	507945	1215915	63.51%	8.876%
35	6.964	962	964	967	rBV3	283	241	0.01%	0.002%
36	7.110	982	988	997	rBV3	3646	8242	0.43%	0.060%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035206.D
 Acq On : 20 Apr 2023 11:06
 Operator : JC/MD
 Sample : 02333-13DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMG8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	7.171	997	998	1002	rVB	328	214	0.01%	0.002%
38	7.305	1009	1020	1033	rBV	331849	718030	37.50%	5.242%
39	7.482	1044	1049	1054	rBV5	976	2331	0.12%	0.017%
40	7.933	1118	1123	1131	rBV3	1332	3124	0.16%	0.023%
41	8.074	1142	1146	1148	rBV	275	280	0.01%	0.002%
42	8.122	1153	1154	1156	rBV2	228	224	0.01%	0.002%
43	8.244	1172	1174	1178	rVB	183	247	0.01%	0.002%
44	8.323	1181	1187	1202	rBV	193606	322655	16.85%	2.355%
45	8.494	1211	1215	1218	rBV2	1134	1966	0.10%	0.014%
46	8.647	1233	1240	1250	rBV	787703	1217655	63.60%	8.889%
47	8.951	1284	1290	1305	rBV	134045	208974	10.91%	1.526%
48	9.275	1337	1343	1347	rBV2	1236	1729	0.09%	0.013%
49	9.384	1355	1361	1376	rBV	476925	694324	36.27%	5.069%
50	9.640	1401	1403	1405	rBV2	326	213	0.01%	0.002%
51	9.732	1416	1418	1421	rBV2	264	353	0.02%	0.003%
52	9.915	1446	1448	1451	rBV3	196	257	0.01%	0.002%
53	10.055	1465	1471	1473	rBV	1013614	1590209	83.06%	11.608%
54	10.287	1505	1509	1510	rBV	395	412	0.02%	0.003%
55	10.390	1522	1526	1527	rVB2	278	247	0.01%	0.002%
56	10.408	1527	1529	1532	rBV2	486	448	0.02%	0.003%
57	10.567	1553	1555	1557	rVB2	245	212	0.01%	0.002%
58	10.610	1560	1562	1565	rVB2	310	266	0.01%	0.002%
59	10.646	1565	1568	1570	rBV2	464	563	0.03%	0.004%
60	10.725	1578	1581	1583	rBV	245	225	0.01%	0.002%
61	10.786	1589	1591	1594	rVV	386	315	0.02%	0.002%
62	10.817	1594	1596	1598	rVV3	373	258	0.01%	0.002%
63	10.841	1598	1600	1602	rVV2	250	244	0.01%	0.002%
64	10.963	1617	1620	1623	rBV2	590	799	0.04%	0.006%
65	11.049	1632	1634	1636	rBV	241	225	0.01%	0.002%
66	11.091	1638	1641	1645	rVB	381	550	0.03%	0.004%
67	11.189	1652	1657	1671	rVV	569270	726187	37.93%	5.301%
68	11.402	1690	1692	1697	rBV2	276	497	0.03%	0.004%
69	11.445	1697	1699	1701	rBV2	358	383	0.02%	0.003%
70	11.500	1706	1708	1711	rBV	263	278	0.01%	0.002%
71	11.707	1740	1742	1745	rVB2	445	451	0.02%	0.003%
72	11.756	1748	1750	1754	rVB2	445	373	0.02%	0.003%
73	11.829	1761	1762	1767	rVB3	327	371	0.02%	0.003%
74	11.896	1767	1773	1775	rBV2	205	380	0.02%	0.003%
75	11.969	1779	1785	1789	rBV2	30825	41028	2.14%	0.300%
76	12.024	1789	1794	1806	rVB2	1057807	1914566	100.00%	13.976%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035206.D
 Acq On : 20 Apr 2023 11:06
 Operator : JC/MD
 Sample : 02333-13DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMG8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	12.323	1837	1843	1852	rBV2	940616	1585533	82.81%	11.574%
78	12.762	1912	1915	1920	rBV4	884	1303	0.07%	0.010%
79	12.932	1940	1943	1945	rBV	314	300	0.02%	0.002%
80	12.957	1945	1947	1949	rVB	350	243	0.01%	0.002%
81	12.981	1949	1951	1952	rBV	339	220	0.01%	0.002%
82	13.115	1970	1973	1977	rVB3	969	1074	0.06%	0.008%
83	13.591	2045	2051	2059	rBV	49863	68944	3.60%	0.503%
84	13.664	2062	2063	2065	rVB	334	224	0.01%	0.002%
85	13.682	2065	2066	2068	rBV2	299	283	0.01%	0.002%
86	13.762	2077	2079	2080	rBV	461	378	0.02%	0.003%
87	13.780	2080	2082	2085	rVV2	1119	1246	0.07%	0.009%
88	13.823	2087	2089	2092	rBV3	364	346	0.02%	0.003%
89	13.902	2101	2102	2105	rVB2	334	285	0.01%	0.002%
90	13.963	2107	2112	2116	rBV2	7036	8879	0.46%	0.065%
91	14.036	2123	2124	2126	rBV2	369	351	0.02%	0.003%
92	14.091	2129	2133	2135	rVV3	358	550	0.03%	0.004%
93	14.121	2135	2138	2144	rVB4	1076	2051	0.11%	0.015%
94	14.304	2166	2168	2172	rBV3	406	442	0.02%	0.003%
95	14.353	2174	2176	2179	rBV3	338	420	0.02%	0.003%
96	14.853	2255	2258	2259	rBV2	418	447	0.02%	0.003%
97	14.889	2262	2264	2266	rVB2	772	497	0.03%	0.004%
98	15.121	2299	2302	2303	rBV2	459	533	0.03%	0.004%
99	15.249	2319	2323	2326	rBV4	1840	2689	0.14%	0.020%
100	16.560	2537	2538	2541	rVB2	999	578	0.03%	0.004%




Sum of corrected areas: 13698675

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035206.D
Acq On : 20 Apr 2023 11:06
Operator : JC/MD
Sample : 02333-13DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMG8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

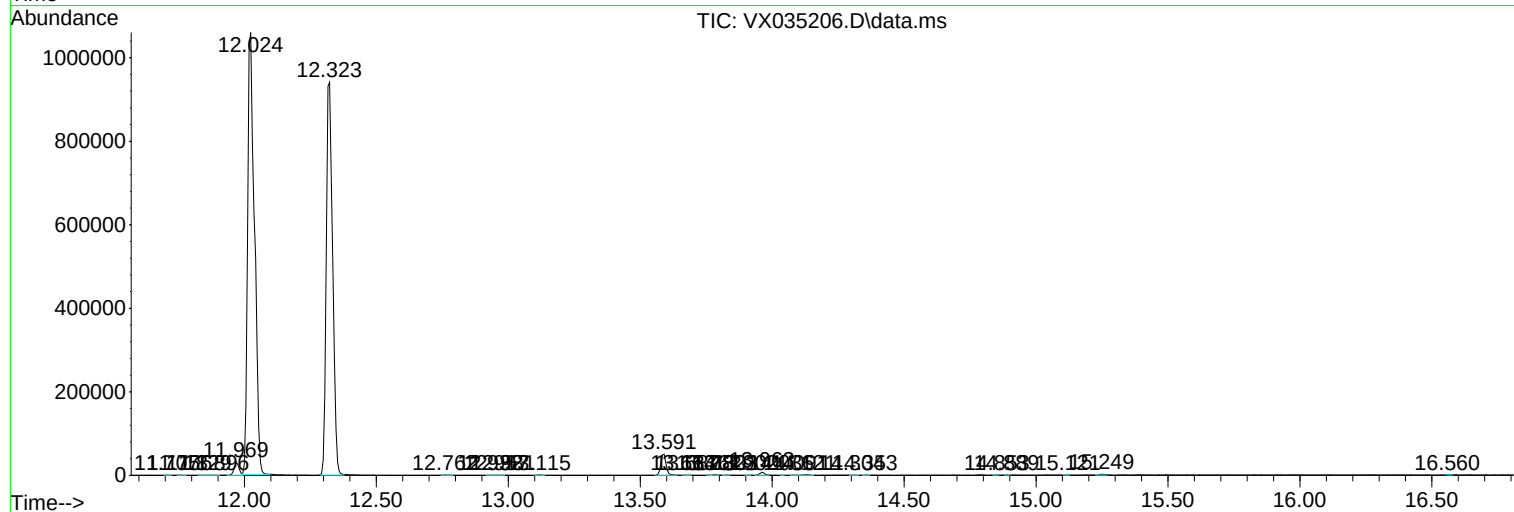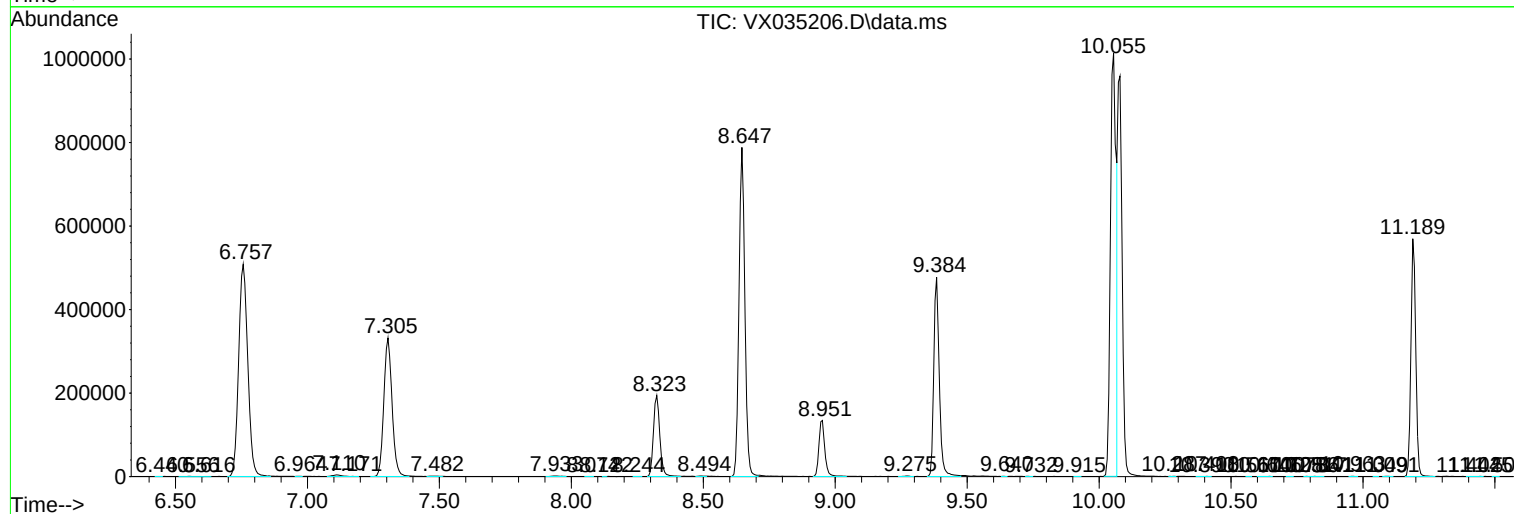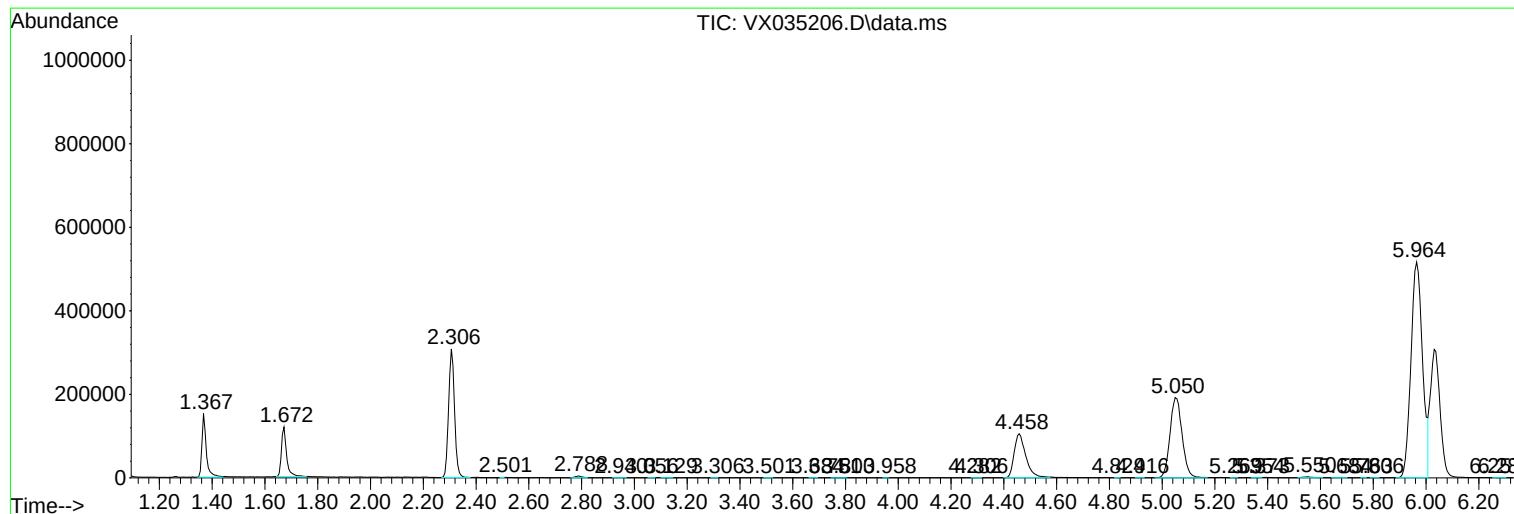

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035206.D
Acq On : 20 Apr 2023 11:06
Operator : JC/MD
Sample : 02333-13DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0MG8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035206.D
Acq On : 20 Apr 2023 11:06
Operator : JC/MD
Sample : 02333-13DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0MG8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------