

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035207.D
 Acq On : 20 Apr 2023 11:29
 Operator : JC/MD
 Sample : 02397-16DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035207.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	32	rBV3	2062	2246	0.07%	0.015%
2	1.367	42	46	57	rBV	147720	170994	5.34%	1.147%
3	1.672	91	96	109	rBV	123438	163238	5.09%	1.095%
4	2.306	194	200	210	rBV	303992	472787	14.76%	3.171%
5	2.489	228	230	231	rBV2	378	272	0.01%	0.002%
6	2.788	272	279	285	rBV4	3600	6695	0.21%	0.045%
7	2.892	295	296	299	rVB	280	211	0.01%	0.001%
8	2.922	299	301	302	rBV	206	153	0.00%	0.001%
9	3.074	325	326	328	rBV	252	208	0.01%	0.001%
10	3.093	328	329	331	rVB2	328	202	0.01%	0.001%
11	3.148	336	338	340	rVB	325	275	0.01%	0.002%
12	3.507	395	397	399	rVB	286	192	0.01%	0.001%
13	3.654	417	421	424	rVB3	338	573	0.02%	0.004%
14	3.678	424	425	427	rBV	256	243	0.01%	0.002%
15	3.702	427	429	430	rVB2	265	149	0.00%	0.001%
16	3.873	455	457	458	rBV	220	167	0.01%	0.001%
17	3.891	458	460	464	rVV3	201	254	0.01%	0.002%
18	3.928	464	466	468	rVV2	179	151	0.00%	0.001%
19	4.135	498	500	504	rBV2	300	339	0.01%	0.002%
20	4.464	545	554	576	rBV	106490	329697	10.29%	2.211%
21	5.056	639	651	671	rBV	199161	618361	19.30%	4.148%
22	5.227	677	679	683	rVB2	721	623	0.02%	0.004%
23	5.318	690	694	696	rBV3	299	359	0.01%	0.002%
24	5.556	724	733	742	rBV4	2336	6724	0.21%	0.045%
25	5.720	758	760	763	rVB	206	154	0.00%	0.001%
26	5.873	783	785	786	rVB	216	146	0.00%	0.001%
27	5.891	786	788	789	rBV	185	161	0.01%	0.001%
28	5.970	789	801	820	rBV2	519458	1565744	48.87%	10.502%
29	6.190	835	837	839	rVB	346	219	0.01%	0.001%
30	6.470	881	883	884	rBV2	240	232	0.01%	0.002%
31	6.525	890	892	894	rBV2	302	321	0.01%	0.002%
32	6.549	894	896	899	rVB2	503	478	0.01%	0.003%
33	6.617	905	907	910	rBV2	206	175	0.01%	0.001%
34	6.757	921	930	948	rBV	479848	1161671	36.26%	7.792%
35	6.982	965	967	968	rVB2	434	284	0.01%	0.002%
36	7.110	982	988	998	rVB6	3689	8937	0.28%	0.060%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035207.D
 Acq On : 20 Apr 2023 11:29
 Operator : JC/MD
 Sample : 02397-16DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	7.305	1011	1020	1035	rVV	329048	717098	22.38%	4.810%
38	7.555	1060	1061	1064	rVB2	337	221	0.01%	0.001%
39	7.598	1064	1068	1069	rBV2	283	286	0.01%	0.002%
40	7.702	1083	1085	1087	rVV	266	166	0.01%	0.001%
41	7.732	1089	1090	1094	rVB2	312	238	0.01%	0.002%
42	7.836	1105	1107	1110	rBV2	253	348	0.01%	0.002%
43	7.879	1112	1114	1116	rBV	199	225	0.01%	0.002%
44	7.939	1120	1124	1126	rBV4	1177	1969	0.06%	0.013%
45	8.049	1140	1142	1143	rBV	294	174	0.01%	0.001%
46	8.128	1154	1155	1159	rVB3	252	215	0.01%	0.001%
47	8.256	1171	1176	1181	rBV2	670	1174	0.04%	0.008%
48	8.324	1181	1187	1199	rBV	192744	322982	10.08%	2.166%
49	8.494	1211	1215	1219	rBV3	857	1326	0.04%	0.009%
50	8.647	1234	1240	1258	rVV	767114	1212696	37.85%	8.134%
51	8.903	1279	1282	1283	rBV3	395	366	0.01%	0.002%
52	8.951	1284	1290	1302	rVV	131791	202857	6.33%	1.361%
53	9.281	1339	1344	1348	rVB4	1067	1705	0.05%	0.011%
54	9.384	1356	1361	1380	rBV	497765	707832	22.09%	4.748%
55	9.896	1442	1445	1448	rBV3	363	400	0.01%	0.003%
56	9.951	1448	1454	1458	rVB2	437	829	0.03%	0.006%
57	9.982	1458	1459	1461	rBV	187	192	0.01%	0.001%
58	10.055	1465	1471	1473	rBV	979028	1357004	42.35%	9.102%
59	10.287	1507	1509	1510	rBV	215	148	0.00%	0.001%
60	10.384	1523	1525	1528	rBV	493	441	0.01%	0.003%
61	10.530	1548	1549	1550	rBV	311	166	0.01%	0.001%
62	10.677	1571	1573	1575	rVB	361	237	0.01%	0.002%
63	10.707	1575	1578	1579	rBV	264	261	0.01%	0.002%
64	10.963	1619	1620	1627	rVB3	357	590	0.02%	0.004%
65	11.189	1652	1657	1673	rBV	547511	720081	22.47%	4.830%
66	11.500	1704	1708	1709	rBV	381	304	0.01%	0.002%
67	11.622	1725	1728	1730	rBV2	242	332	0.01%	0.002%
68	11.652	1731	1733	1736	rVB2	398	361	0.01%	0.002%
69	11.683	1736	1738	1740	rBV2	366	347	0.01%	0.002%
70	11.707	1740	1742	1744	rVV2	514	407	0.01%	0.003%
71	11.792	1754	1756	1758	rBV2	195	150	0.00%	0.001%
72	11.969	1780	1785	1789	rBV	45657	59742	1.86%	0.401%
73	12.024	1789	1794	1807	rVB2	970579	1474094	46.01%	9.887%
74	12.329	1837	1844	1859	rBV2	1870544	3204052	100.00%	21.491%
75	12.506	1871	1873	1874	rBV	653	468	0.01%	0.003%
76	12.670	1898	1900	1906	rBV	400	415	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035207.D
 Acq On : 20 Apr 2023 11:29
 Operator : JC/MD
 Sample : 02397-16DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMM8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041823WMA.M
 Title : VOC Analysis

77	12.768	1912	1916	1918	rBV3	591	846	0.03%	0.006%
78	12.884	1933	1935	1938	rBV	238	245	0.01%	0.002%
79	12.926	1938	1942	1949	rVB4	1630	2689	0.08%	0.018%
80	12.993	1949	1953	1956	rVB2	433	587	0.02%	0.004%
81	13.036	1956	1960	1961	rBV2	280	414	0.01%	0.003%
82	13.121	1970	1974	1977	rBV3	753	892	0.03%	0.006%
83	13.201	1984	1987	1993	rVB4	697	955	0.03%	0.006%
84	13.262	1993	1997	1999	rVB	292	296	0.01%	0.002%
85	13.353	2009	2012	2013	rBV	265	317	0.01%	0.002%
86	13.481	2032	2033	2034	rBV	312	153	0.00%	0.001%
87	13.585	2045	2050	2064	rVB	256742	331830	10.36%	2.226%
88	13.682	2064	2066	2067	rVB	525	285	0.01%	0.002%
89	13.707	2067	2070	2072	rBV3	485	666	0.02%	0.004%
90	13.847	2091	2093	2096	rBV2	294	417	0.01%	0.003%
91	13.963	2107	2112	2117	rBV	44237	55482	1.73%	0.372%
92	14.060	2126	2128	2131	rVB3	320	432	0.01%	0.003%
93	14.127	2136	2139	2143	rBV4	1238	1778	0.06%	0.012%
94	14.286	2164	2165	2166	rBV	375	218	0.01%	0.001%
95	14.341	2172	2174	2175	rBV	276	161	0.01%	0.001%
96	14.414	2184	2186	2190	rVB3	375	297	0.01%	0.002%
97	14.755	2240	2242	2243	rBV2	337	199	0.01%	0.001%
98	14.786	2243	2247	2250	rVV4	1741	2228	0.07%	0.015%
99	15.152	2306	2307	2309	rBV	632	390	0.01%	0.003%
100	16.554	2535	2537	2540	rBV3	705	615	0.02%	0.004%




Sum of corrected areas: 14908926

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035207.D
Acq On : 20 Apr 2023 11:29
Operator : JC/MD
Sample : 02397-16DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

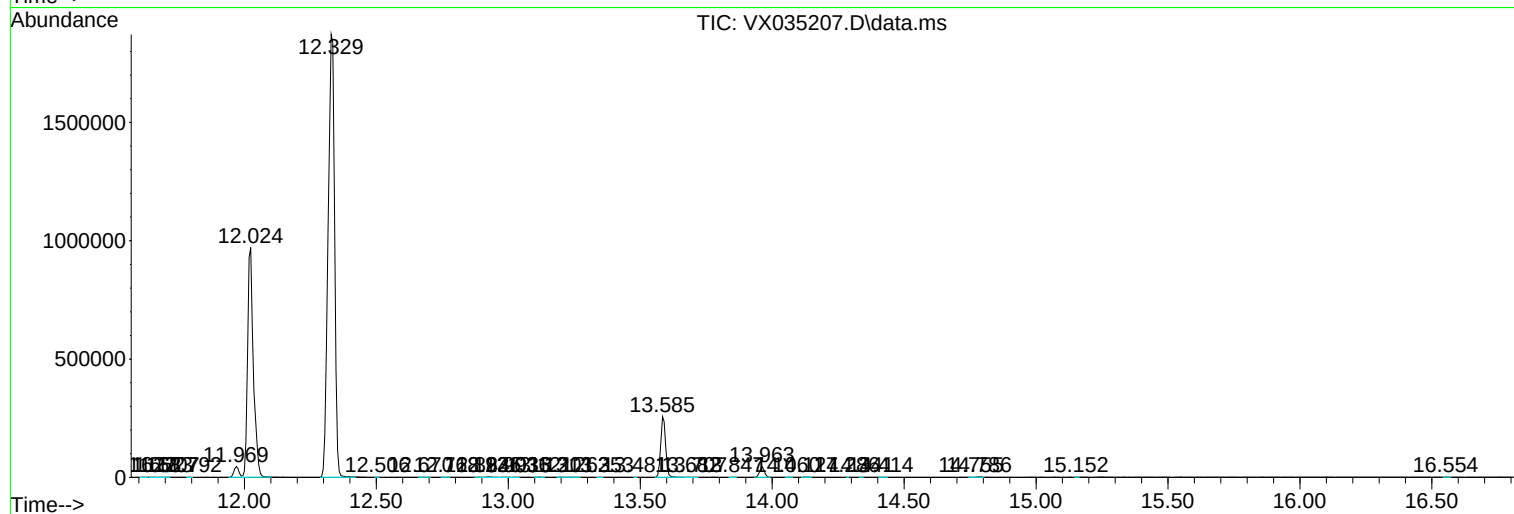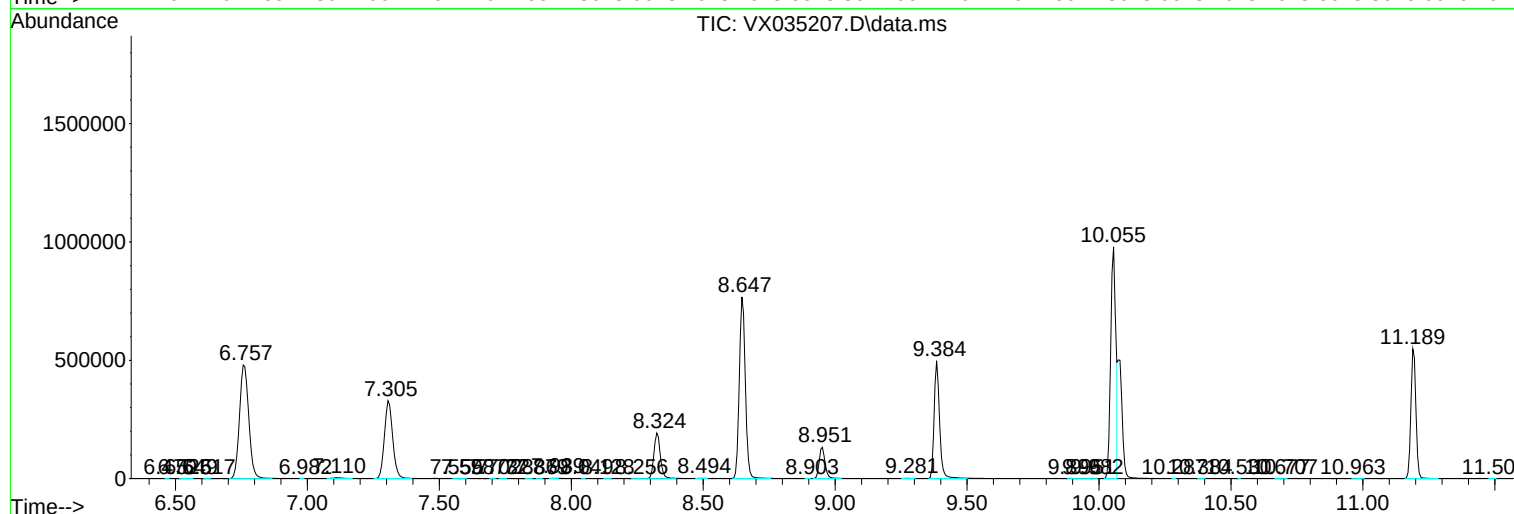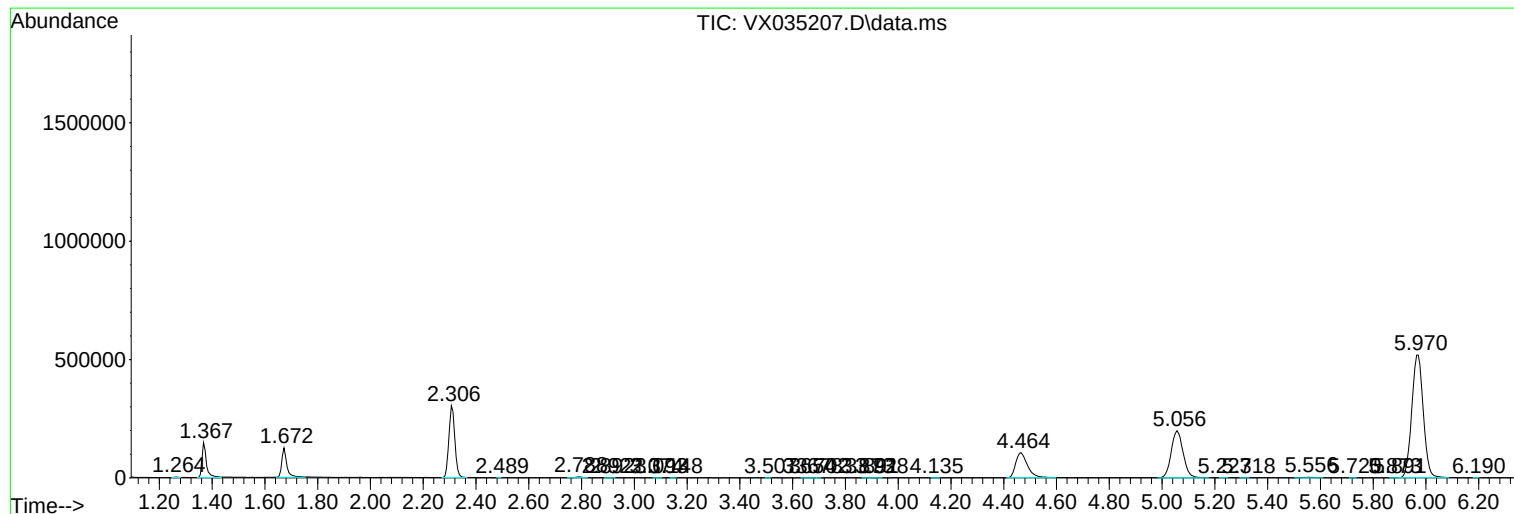

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035207.D
Acq On : 20 Apr 2023 11:29
Operator : JC/MD
Sample : 02397-16DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035207.D
Acq On : 20 Apr 2023 11:29
Operator : JC/MD
Sample : 02397-16DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMM8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------