

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035208.D
 Acq On : 20 Apr 2023 11:58
 Operator : JC/MD
 Sample : 02333-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035208.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	32	rVB5	2049	2022	0.13%	0.017%
2	1.368	42	46	57	rBV	175011	192506	12.00%	1.581%
3	1.672	91	96	112	rBV	133540	177444	11.07%	1.457%
4	2.306	194	200	214	rBV	359143	545372	34.01%	4.479%
5	2.453	222	224	227	rBV2	318	390	0.02%	0.003%
6	2.508	232	233	238	rVB3	911	1015	0.06%	0.008%
7	2.654	255	257	258	rBV	223	178	0.01%	0.001%
8	2.758	270	274	275	rBV2	240	297	0.02%	0.002%
9	2.788	275	279	284	rVV5	2886	5217	0.33%	0.043%
10	2.904	297	298	301	rBV2	304	257	0.02%	0.002%
11	3.038	315	320	321	rBV3	453	615	0.04%	0.005%
12	3.099	327	330	332	rBV	471	598	0.04%	0.005%
13	3.209	345	348	350	rVB3	236	262	0.02%	0.002%
14	3.373	372	375	376	rBV	214	209	0.01%	0.002%
15	3.453	385	388	390	rBV2	222	268	0.02%	0.002%
16	3.514	396	398	402	rVB2	313	333	0.02%	0.003%
17	3.575	402	408	409	rBV	278	398	0.02%	0.003%
18	3.873	455	457	460	rVB2	193	180	0.01%	0.001%
19	3.904	460	462	464	rVB	232	188	0.01%	0.002%
20	3.946	464	469	471	rBV2	283	383	0.02%	0.003%
21	3.989	471	476	479	rBV	188	403	0.03%	0.003%
22	4.050	484	486	487	rVV	329	208	0.01%	0.002%
23	4.135	497	500	503	rVB2	367	394	0.02%	0.003%
24	4.196	507	510	512	rBV2	321	425	0.03%	0.003%
25	4.282	521	524	526	rBV2	310	380	0.02%	0.003%
26	4.465	545	554	573	rBV	95582	305141	19.03%	2.506%
27	4.794	606	608	612	rBV3	274	329	0.02%	0.003%
28	4.971	636	637	639	rBV2	264	178	0.01%	0.001%
29	5.056	639	651	670	rVV	195097	611797	38.15%	5.024%
30	5.391	699	706	713	rVB5	894	2154	0.13%	0.018%
31	5.458	713	717	718	rVB2	292	345	0.02%	0.003%
32	5.483	718	721	722	rBV2	306	347	0.02%	0.003%
33	5.550	725	732	742	rBV2	1984	5169	0.32%	0.042%
34	5.745	763	764	767	rBV2	218	210	0.01%	0.002%
35	5.964	787	800	819	rBV2	537983	1603571	100.00%	13.169%
36	6.312	855	857	860	rBV2	226	195	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035208.D
 Acq On : 20 Apr 2023 11:58
 Operator : JC/MD
 Sample : 02333-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	6.367	862	866	871	rVB2	354	711	0.04%	0.006%
38	6.519	889	891	895	rBV3	242	343	0.02%	0.003%
39	6.757	920	930	946	rBV	461004	1105485	68.94%	9.078%
40	7.104	983	987	1001	rVB4	4311	10914	0.68%	0.090%
41	7.306	1011	1020	1034	rBV	332061	725475	45.24%	5.958%
42	7.476	1046	1048	1049	rBV2	526	548	0.03%	0.005%
43	7.556	1059	1061	1065	rBV2	232	316	0.02%	0.003%
44	7.629	1071	1073	1078	rVB2	405	278	0.02%	0.002%
45	7.946	1118	1125	1129	rBV4	1038	2167	0.14%	0.018%
46	8.068	1141	1145	1147	rBV2	223	220	0.01%	0.002%
47	8.238	1170	1173	1174	rBV	216	183	0.01%	0.002%
48	8.324	1180	1187	1199	rBV	199638	327436	20.42%	2.689%
49	8.464	1209	1210	1211	rBV	411	199	0.01%	0.002%
50	8.647	1233	1240	1252	rBV	824155	1302017	81.19%	10.692%
51	8.952	1284	1290	1304	rBV	133127	206590	12.88%	1.697%
52	9.153	1320	1323	1325	rBV3	316	279	0.02%	0.002%
53	9.269	1340	1342	1347	rVB3	675	940	0.06%	0.008%
54	9.305	1347	1348	1351	rBV	301	237	0.01%	0.002%
55	9.384	1356	1361	1386	rVV	472452	672455	41.93%	5.522%
56	9.671	1406	1408	1411	rVB	496	422	0.03%	0.003%
57	9.708	1411	1414	1417	rBV2	296	477	0.03%	0.004%
58	9.915	1446	1448	1449	rVB	326	183	0.01%	0.002%
59	9.939	1449	1452	1453	rBV	404	432	0.03%	0.004%
60	9.994	1459	1461	1462	rBV	263	172	0.01%	0.001%
61	10.055	1465	1471	1487	rVV	893670	1262281	78.72%	10.366%
62	10.640	1564	1567	1569	rBV2	523	573	0.04%	0.005%
63	10.799	1588	1593	1595	rBV3	226	370	0.02%	0.003%
64	10.842	1599	1600	1604	rVB2	261	243	0.02%	0.002%
65	10.927	1612	1614	1616	rBV2	233	274	0.02%	0.002%
66	11.037	1631	1632	1635	rVB2	261	216	0.01%	0.002%
67	11.073	1635	1638	1639	rBV2	310	292	0.02%	0.002%
68	11.091	1639	1641	1644	rVV2	395	420	0.03%	0.003%
69	11.116	1644	1645	1648	rVV2	247	296	0.02%	0.002%
70	11.189	1652	1657	1676	rVV	535663	704411	43.93%	5.785%
71	11.341	1680	1682	1686	rVB2	294	286	0.02%	0.002%
72	11.463	1698	1702	1704	rVB3	606	866	0.05%	0.007%
73	11.488	1704	1706	1708	rVB2	278	224	0.01%	0.002%
74	11.524	1710	1712	1715	rVB	327	319	0.02%	0.003%
75	11.555	1715	1717	1718	rBV	178	184	0.01%	0.002%
76	11.713	1739	1743	1745	rVV3	500	620	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035208.D
 Acq On : 20 Apr 2023 11:58
 Operator : JC/MD
 Sample : 02333-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	11.756	1748	1750	1755	rVB3	558	534	0.03%	0.004%
78	11.872	1767	1769	1771	rVB2	265	182	0.01%	0.001%
79	11.969	1779	1785	1788	rBV4	2842	4109	0.26%	0.034%
80	12.018	1788	1793	1803	rVV	903534	1208252	75.35%	9.922%
81	12.317	1837	1842	1857	rBV	877408	1142532	71.25%	9.383%
82	12.756	1911	1914	1918	rBV4	803	1051	0.07%	0.009%
83	12.792	1918	1920	1922	rBV2	251	174	0.01%	0.001%
84	12.817	1922	1924	1927	rBV	327	221	0.01%	0.002%
85	13.048	1961	1962	1964	rVB2	334	188	0.01%	0.002%
86	13.329	2005	2008	2010	rVB2	370	400	0.02%	0.003%
87	13.365	2012	2014	2016	rBV	292	240	0.01%	0.002%
88	13.481	2032	2033	2039	rVB	356	467	0.03%	0.004%
89	13.536	2039	2042	2045	rBV2	251	394	0.02%	0.003%
90	13.591	2046	2051	2060	rVB	15553	20470	1.28%	0.168%
91	13.774	2079	2081	2083	rBV3	388	424	0.03%	0.003%
92	13.932	2105	2107	2108	rBV	328	199	0.01%	0.002%
93	13.963	2108	2112	2119	rVB2	3079	4012	0.25%	0.033%
94	14.054	2125	2127	2129	rBV	224	256	0.02%	0.002%
95	14.134	2136	2140	2144	rVB3	1245	1699	0.11%	0.014%
96	14.170	2144	2146	2150	rBV2	246	343	0.02%	0.003%
97	14.396	2182	2183	2186	rVB	396	277	0.02%	0.002%
98	14.463	2192	2194	2196	rBV3	362	384	0.02%	0.003%
99	14.798	2248	2249	2253	rBV3	368	390	0.02%	0.003%
100	16.737	2565	2567	2569	rVB2	529	278	0.02%	0.002%




Sum of corrected areas: 12177208

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035208.D
Acq On : 20 Apr 2023 11:58
Operator : JC/MD
Sample : 02333-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

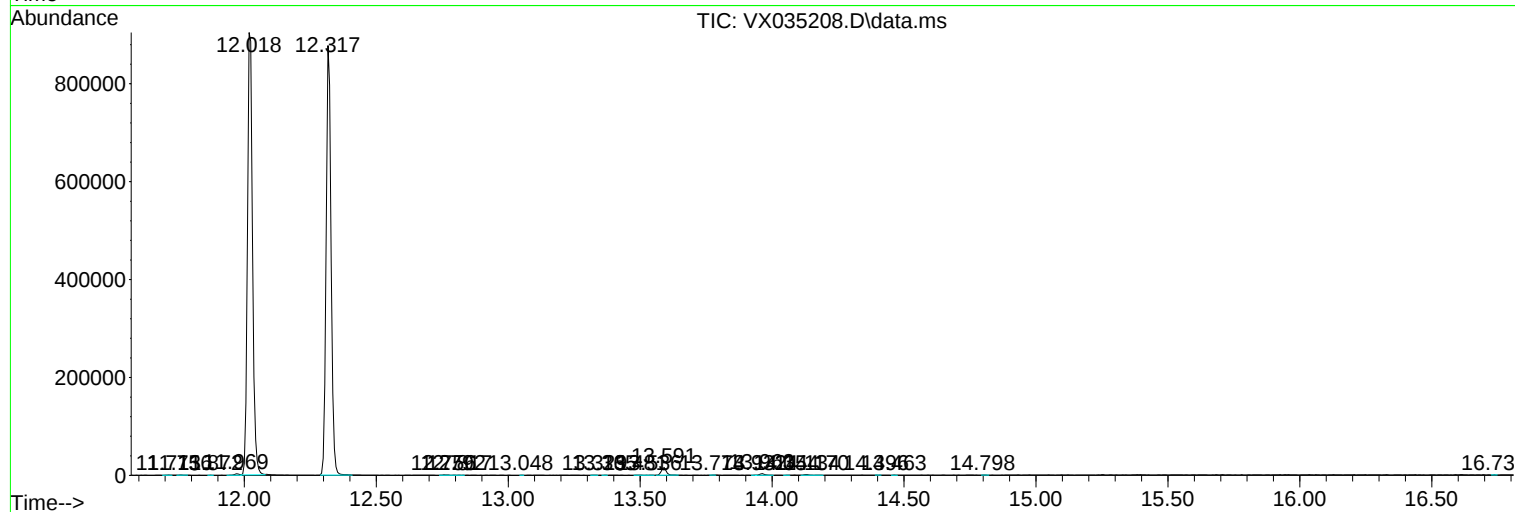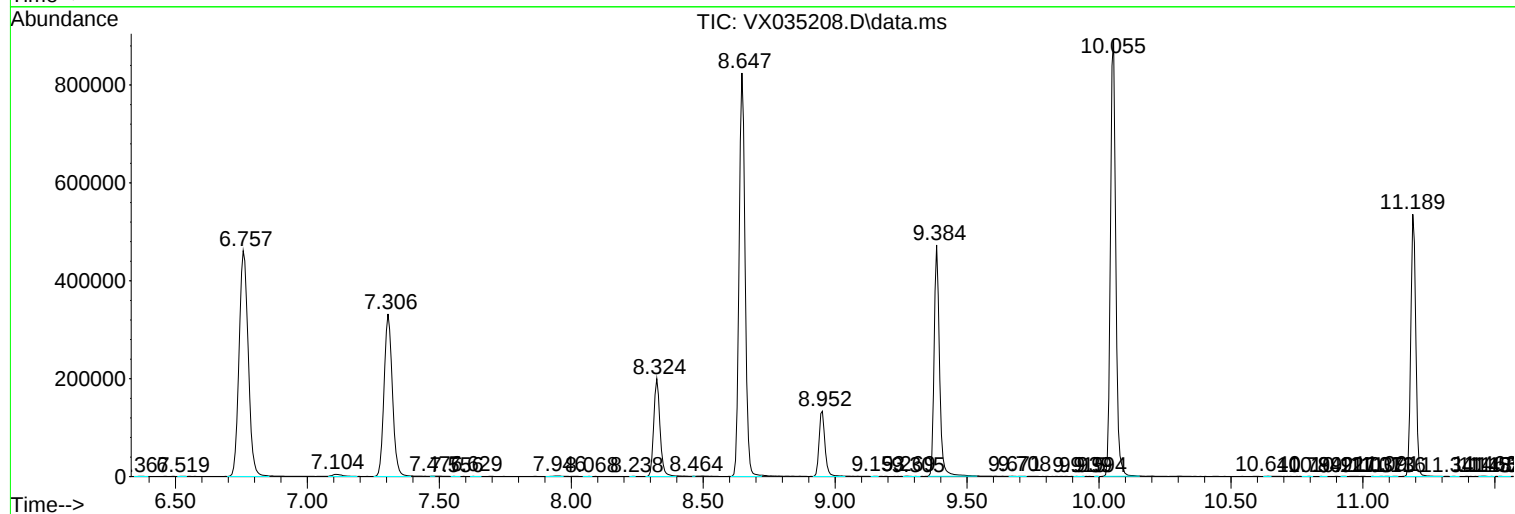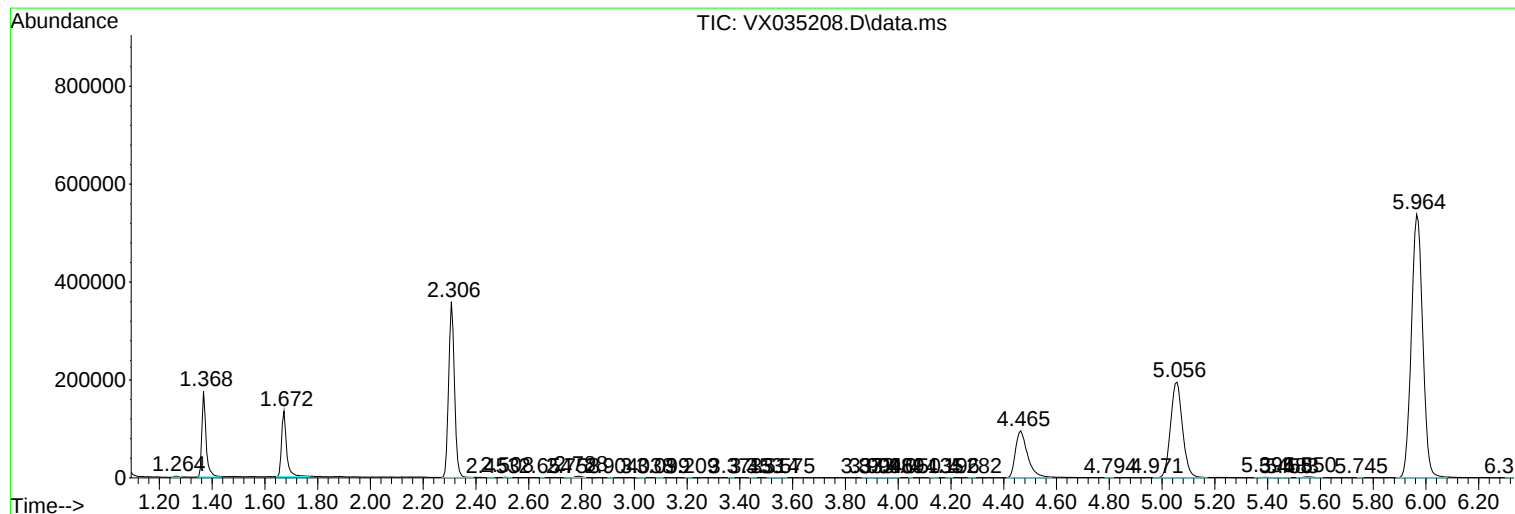

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035208.D
Acq On : 20 Apr 2023 11:58
Operator : JC/MD
Sample : 02333-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035208.D
Acq On : 20 Apr 2023 11:58
Operator : JC/MD
Sample : 02333-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------