

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035211.D
 Acq On : 20 Apr 2023 13:30
 Operator : JC/MD
 Sample : 02378-19DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035211.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	25	28	32	rBV2	2491	3001	0.06%	0.014%
2	1.368	42	46	58	rBV	149230	169321	3.53%	0.780%
3	1.672	92	96	107	rBV	123266	160370	3.34%	0.739%
4	2.306	194	200	214	rBV	322554	482237	10.05%	2.222%
5	2.550	238	240	243	rVB2	327	274	0.01%	0.001%
6	2.575	243	244	245	rBV	282	174	0.00%	0.001%
7	2.648	254	256	258	rBV2	324	370	0.01%	0.002%
8	2.721	264	268	270	rBV4	273	394	0.01%	0.002%
9	2.788	274	279	288	rVB4	3245	6223	0.13%	0.029%
10	2.861	288	291	292	rBV	266	230	0.00%	0.001%
11	2.922	298	301	303	rBV2	276	263	0.01%	0.001%
12	3.026	315	318	319	rBV2	240	207	0.00%	0.001%
13	3.068	324	325	329	rVV2	180	189	0.00%	0.001%
14	3.105	329	331	333	rVV2	320	260	0.01%	0.001%
15	3.136	333	336	339	rVV2	357	370	0.01%	0.002%
16	3.172	339	342	346	rVV2	242	367	0.01%	0.002%
17	3.270	356	358	361	rVB2	354	236	0.00%	0.001%
18	3.337	367	369	371	rBV2	202	217	0.00%	0.001%
19	3.422	380	383	386	rBV	236	242	0.01%	0.001%
20	3.696	427	428	431	rVB	429	225	0.00%	0.001%
21	3.721	431	432	434	rBV	254	189	0.00%	0.001%
22	3.763	437	439	440	rBV2	283	198	0.00%	0.001%
23	3.837	448	451	452	rBV	294	241	0.01%	0.001%
24	4.080	489	491	493	rVB2	447	275	0.01%	0.001%
25	4.141	499	501	504	rVB	255	208	0.00%	0.001%
26	4.465	545	554	572	rBV	111795	346777	7.23%	1.598%
27	4.727	595	597	600	rBV2	305	336	0.01%	0.002%
28	4.897	622	625	628	rVB3	287	331	0.01%	0.002%
29	5.056	637	651	670	rBV	200775	629591	13.12%	2.901%
30	5.263	683	685	687	rBV2	392	301	0.01%	0.001%
31	5.300	690	691	693	rBV	230	208	0.00%	0.001%
32	5.379	700	704	705	rBV3	1175	1321	0.03%	0.006%
33	5.550	725	732	746	rBV4	3906	9932	0.21%	0.046%
34	5.678	746	753	758	rBV5	883	2293	0.05%	0.011%
35	5.806	772	774	777	rVB2	221	226	0.00%	0.001%
36	5.879	784	786	788	rBV2	274	294	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035211.D
 Acq On : 20 Apr 2023 13:30
 Operator : JC/MD
 Sample : 02378-19DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	5.970	788	801	806	rBV2	540011	1586278	33.07%	7.309%
38	6.446	878	879	882	rBV2	346	247	0.01%	0.001%
39	6.525	890	892	894	rBV2	308	286	0.01%	0.001%
40	6.659	912	914	917	rBV2	279	276	0.01%	0.001%
41	6.763	921	931	948	rBV	478013	1140670	23.78%	5.256%
42	7.117	982	989	996	rBV5	4055	8698	0.18%	0.040%
43	7.305	1010	1020	1042	rBV	325860	736870	15.36%	3.395%
44	7.482	1047	1049	1054	rVB4	787	1090	0.02%	0.005%
45	7.562	1060	1062	1065	rVB2	233	223	0.00%	0.001%
46	7.592	1065	1067	1068	rBV	301	241	0.01%	0.001%
47	7.647	1074	1076	1078	rBV	180	176	0.00%	0.001%
48	7.940	1120	1124	1129	rBV5	1416	2994	0.06%	0.014%
49	8.141	1155	1157	1159	rBV	325	213	0.00%	0.001%
50	8.324	1181	1187	1200	rBV	198014	321731	6.71%	1.482%
51	8.500	1211	1216	1220	rBV5	907	2132	0.04%	0.010%
52	8.647	1234	1240	1256	rBV	792408	1248994	26.04%	5.755%
53	8.952	1284	1290	1301	rBV	138822	206759	4.31%	0.953%
54	9.275	1341	1343	1347	rVB3	704	748	0.02%	0.003%
55	9.384	1356	1361	1379	rBV	526838	754532	15.73%	3.477%
56	10.079	1465	1475	1493	rBV2	2594704	4796897	100.00%	22.102%
57	10.360	1519	1521	1522	rVB2	373	174	0.00%	0.001%
58	10.403	1525	1528	1530	rBV4	440	516	0.01%	0.002%
59	10.457	1535	1537	1538	rBV	236	187	0.00%	0.001%
60	10.537	1547	1550	1551	rBV2	286	284	0.01%	0.001%
61	10.774	1588	1589	1592	rVB2	268	209	0.00%	0.001%
62	10.823	1595	1597	1598	rBV	356	264	0.01%	0.001%
63	10.896	1606	1609	1611	rVB	402	338	0.01%	0.002%
64	10.963	1618	1620	1624	rVV2	246	265	0.01%	0.001%
65	11.012	1627	1628	1632	rVB2	376	271	0.01%	0.001%
66	11.085	1636	1640	1650	rBV4	3213	5760	0.12%	0.027%
67	11.189	1652	1657	1670	rVV	571824	754214	15.72%	3.475%
68	11.311	1672	1677	1683	rVB2	2331	3567	0.07%	0.016%
69	11.463	1700	1702	1706	rBV2	579	687	0.01%	0.003%
70	11.500	1706	1708	1711	rVV3	218	262	0.01%	0.001%
71	11.591	1721	1723	1725	rBV	184	221	0.00%	0.001%
72	11.707	1740	1742	1745	rBV3	478	475	0.01%	0.002%
73	11.756	1748	1750	1754	rVB2	593	613	0.01%	0.003%
74	11.817	1758	1760	1762	rVB2	352	207	0.00%	0.001%
75	11.896	1771	1773	1777	rBV2	256	278	0.01%	0.001%
76	11.969	1780	1785	1789	rBV	156694	196064	4.09%	0.903%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035211.D
 Acq On : 20 Apr 2023 13:30
 Operator : JC/MD
 Sample : 02378-19DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0ML2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	12.042	1789	1797	1812	rVB2	1957250	3651321	76.12%	16.824%
78	12.207	1822	1824	1826	rBV3	433	355	0.01%	0.002%
79	12.335	1837	1845	1863	rBV2	2429434	4016508	83.73%	18.506%
80	12.756	1912	1914	1918	rVB2	596	709	0.01%	0.003%
81	12.847	1927	1929	1932	rVV2	242	231	0.00%	0.001%
82	12.926	1939	1942	1946	rVB3	1045	1291	0.03%	0.006%
83	12.987	1949	1952	1953	rVB	317	221	0.00%	0.001%
84	13.024	1956	1958	1961	rBV2	195	219	0.00%	0.001%
85	13.109	1969	1972	1976	rBV3	1290	1725	0.04%	0.008%
86	13.195	1985	1986	1989	rBV2	247	232	0.00%	0.001%
87	13.262	1994	1997	1998	rBV2	336	336	0.01%	0.002%
88	13.280	1998	2000	2002	rBV3	205	217	0.00%	0.001%
89	13.585	2045	2050	2060	rBV	272332	344875	7.19%	1.589%
90	13.725	2071	2073	2076	rVB2	307	270	0.01%	0.001%
91	13.774	2079	2081	2082	rBV2	454	354	0.01%	0.002%
92	13.859	2093	2095	2098	rVB2	325	258	0.01%	0.001%
93	13.963	2107	2112	2120	rVB	54015	71179	1.48%	0.328%
94	14.024	2120	2122	2127	rVB3	389	413	0.01%	0.002%
95	14.066	2127	2129	2131	rBV2	295	281	0.01%	0.001%
96	14.134	2135	2140	2144	rBV3	1009	1893	0.04%	0.009%
97	14.786	2242	2247	2251	rVB3	4408	5628	0.12%	0.026%
98	15.085	2294	2296	2298	rBV3	569	462	0.01%	0.002%
99	15.249	2319	2323	2330	rVB2	8507	11460	0.24%	0.053%
100	16.621	2546	2548	2549	rBV	545	269	0.01%	0.001%




Sum of corrected areas: 21703509

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035211.D
Acq On : 20 Apr 2023 13:30
Operator : JC/MD
Sample : 02378-19DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COML2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

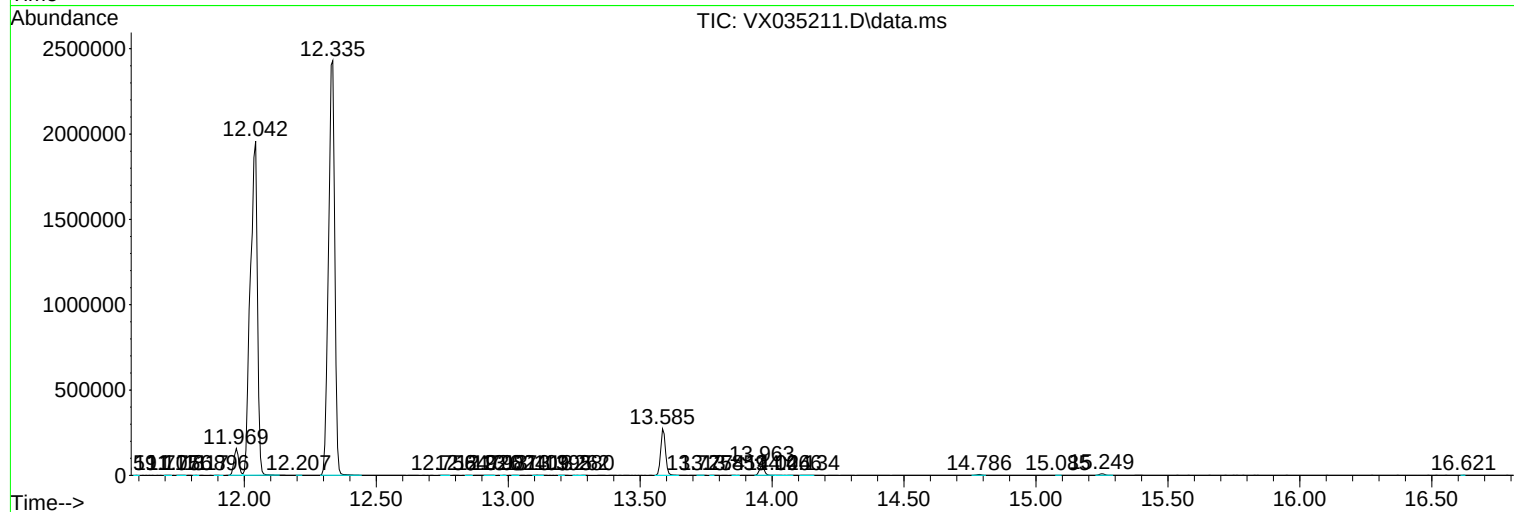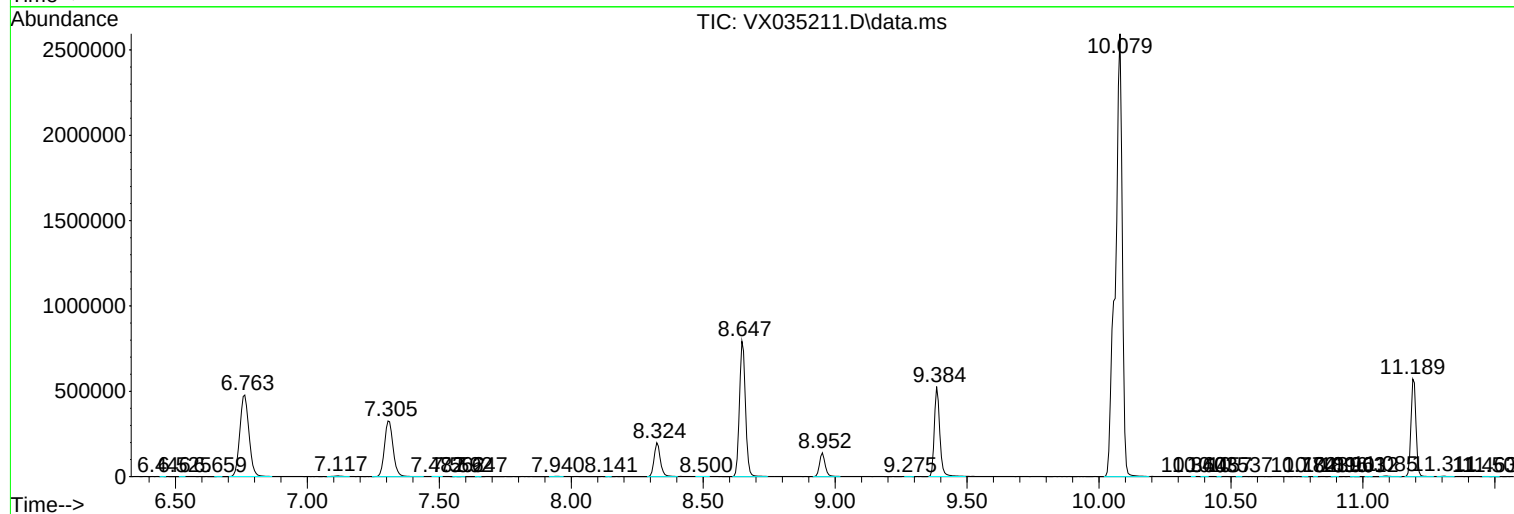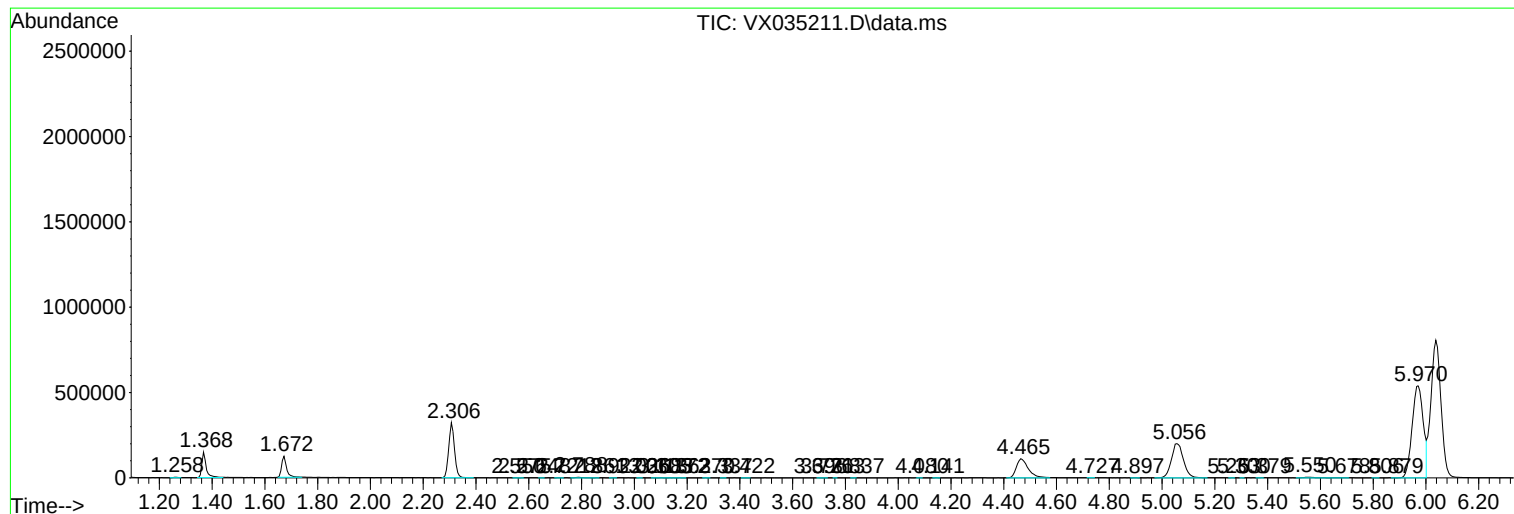

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035211.D
Acq On : 20 Apr 2023 13:30
Operator : JC/MD
Sample : 02378-19DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ML2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035211.D
Acq On : 20 Apr 2023 13:30
Operator : JC/MD
Sample : 02378-19DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ML2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------