

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035214.D
 Acq On : 20 Apr 2023 14:40
 Operator : JC/MD
 Sample : 02378-18DL 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035214.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	32	rBV2	2082	2141	0.09%	0.015%
2	1.368	42	46	59	rBV	146518	164717	7.16%	1.183%
3	1.672	92	96	106	rBV	125075	159858	6.95%	1.148%
4	2.307	194	200	212	rBV	299162	464158	20.17%	3.334%
5	2.636	250	254	255	rBV2	293	376	0.02%	0.003%
6	2.666	257	259	261	rVB	462	402	0.02%	0.003%
7	2.685	261	262	264	rBV	422	377	0.02%	0.003%
8	2.788	274	279	289	rVB3	3011	5895	0.26%	0.042%
9	2.855	289	290	292	rBV	222	192	0.01%	0.001%
10	2.941	302	304	307	rVB3	251	191	0.01%	0.001%
11	3.264	355	357	359	rBV	190	144	0.01%	0.001%
12	3.288	359	361	362	rVV	189	120	0.01%	0.001%
13	3.416	380	382	383	rVB2	190	101	0.00%	0.001%
14	3.453	386	388	392	rVB	300	383	0.02%	0.003%
15	3.489	392	394	395	rBV2	163	138	0.01%	0.001%
16	3.508	395	397	398	rBV2	177	128	0.01%	0.001%
17	3.837	448	451	453	rBV2	463	541	0.02%	0.004%
18	3.898	459	461	463	rBV2	213	160	0.01%	0.001%
19	3.946	467	469	470	rBV2	185	143	0.01%	0.001%
20	4.172	504	506	507	rBB	316	147	0.01%	0.001%
21	4.270	520	522	524	rVB2	257	159	0.01%	0.001%
22	4.312	525	529	531	rVB2	425	549	0.02%	0.004%
23	4.337	531	533	535	rBV2	270	204	0.01%	0.001%
24	4.367	535	538	540	rBV2	170	173	0.01%	0.001%
25	4.465	543	554	573	rBV	106981	351893	15.29%	2.527%
26	4.879	620	622	623	rBV2	238	219	0.01%	0.002%
27	4.952	632	634	635	rVB	312	149	0.01%	0.001%
28	5.056	639	651	670	rBV	193816	610852	26.55%	4.387%
29	5.306	690	692	693	rVB2	405	206	0.01%	0.001%
30	5.343	696	698	699	rBV	224	108	0.00%	0.001%
31	5.483	720	721	722	rBV	450	179	0.01%	0.001%
32	5.556	726	733	739	rVB3	1393	3602	0.16%	0.026%
33	5.605	739	741	743	rVB2	245	183	0.01%	0.001%
34	5.660	747	750	751	rBV	401	305	0.01%	0.002%
35	5.721	759	760	762	rBV	253	196	0.01%	0.001%
36	5.861	781	783	787	rVB3	225	221	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035214.D
 Acq On : 20 Apr 2023 14:40
 Operator : JC/MD
 Sample : 02378-18DL 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	5.971	788	801	807	rBV2	523602	1552153	67.45%	11.148%
38	6.294	852	854	856	rBV2	326	256	0.01%	0.002%
39	6.348	861	863	866	rBV2	383	333	0.01%	0.002%
40	6.458	880	881	885	rVV3	314	318	0.01%	0.002%
41	6.537	890	894	895	rBV2	329	323	0.01%	0.002%
42	6.763	921	931	944	rBV	456417	1087776	47.27%	7.812%
43	6.946	959	961	962	rBV	313	165	0.01%	0.001%
44	7.117	983	989	997	rVB5	3711	8231	0.36%	0.059%
45	7.306	1011	1020	1038	rBV	325239	715568	31.10%	5.139%
46	7.623	1070	1072	1074	rBV	176	133	0.01%	0.001%
47	7.684	1081	1082	1084	rBV	274	163	0.01%	0.001%
48	7.738	1090	1091	1092	rBV	223	127	0.01%	0.001%
49	7.879	1111	1114	1116	rBV	154	163	0.01%	0.001%
50	7.946	1120	1125	1129	rBV5	1253	2180	0.09%	0.016%
51	8.184	1161	1164	1165	rBV2	198	184	0.01%	0.001%
52	8.226	1167	1171	1173	rBV2	213	226	0.01%	0.002%
53	8.324	1181	1187	1202	rBV	186714	313397	13.62%	2.251%
54	8.494	1211	1215	1217	rBV3	849	1397	0.06%	0.010%
55	8.647	1233	1240	1258	rBV	767998	1202902	52.28%	8.639%
56	8.952	1284	1290	1309	rBV	131268	201487	8.76%	1.447%
57	9.385	1356	1361	1379	rBV	532661	754668	32.80%	5.420%
58	9.781	1424	1426	1428	rBV2	319	248	0.01%	0.002%
59	10.055	1465	1471	1473	rBV	943630	1419712	61.70%	10.196%
60	10.299	1509	1511	1513	rBV2	218	156	0.01%	0.001%
61	10.348	1517	1519	1522	rBV2	367	413	0.02%	0.003%
62	10.464	1537	1538	1540	rBV	305	163	0.01%	0.001%
63	10.482	1540	1541	1542	rBV	247	156	0.01%	0.001%
64	10.525	1547	1548	1550	rVV2	227	174	0.01%	0.001%
65	10.543	1550	1551	1553	rVB	317	153	0.01%	0.001%
66	10.689	1572	1575	1577	rBV2	355	482	0.02%	0.003%
67	10.762	1585	1587	1588	rBV	198	121	0.01%	0.001%
68	10.781	1588	1590	1593	rVV3	203	261	0.01%	0.002%
69	10.903	1607	1610	1615	rBV	307	464	0.02%	0.003%
70	10.964	1618	1620	1621	rVB2	224	102	0.00%	0.001%
71	10.988	1621	1624	1625	rBV2	238	204	0.01%	0.001%
72	11.085	1639	1640	1643	rVB	399	214	0.01%	0.002%
73	11.116	1643	1645	1646	rBV	224	150	0.01%	0.001%
74	11.189	1652	1657	1668	rBV	581339	747031	32.46%	5.365%
75	11.360	1684	1685	1687	rBV2	246	174	0.01%	0.001%
76	11.872	1768	1769	1770	rVB	337	123	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035214.D
 Acq On : 20 Apr 2023 14:40
 Operator : JC/MD
 Sample : 02378-18DL 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COML1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041823WMA.M
 Title : VOC Analysis

77	11.969	1780	1785	1789	rBV	64632	83535	3.63%	0.600%
78	12.024	1789	1794	1796	rBV	1006524	1567135	68.11%	11.255%
79	12.213	1823	1825	1828	rVB3	490	463	0.02%	0.003%
80	12.329	1837	1844	1863	rVB2	1228635	2301041	100.00%	16.526%
81	12.628	1892	1893	1897	rVB2	266	292	0.01%	0.002%
82	12.664	1897	1899	1900	rBV2	415	381	0.02%	0.003%
83	12.744	1909	1912	1913	rBV2	441	425	0.02%	0.003%
84	12.823	1923	1925	1927	rBV2	310	360	0.02%	0.003%
85	12.969	1947	1949	1950	rVB	258	128	0.01%	0.001%
86	13.061	1962	1964	1965	rBV2	285	269	0.01%	0.002%
87	13.116	1970	1973	1976	rBV2	741	772	0.03%	0.006%
88	13.347	2009	2011	2013	rVB2	344	234	0.01%	0.002%
89	13.536	2040	2042	2043	rVB	208	112	0.00%	0.001%
90	13.585	2045	2050	2060	rVV	108076	145755	6.33%	1.047%
91	13.719	2070	2072	2075	rVV2	336	180	0.01%	0.001%
92	13.786	2079	2083	2085	rVB3	526	574	0.02%	0.004%
93	13.963	2107	2112	2118	rBV	22349	29839	1.30%	0.214%
94	14.128	2135	2139	2141	rBV2	586	870	0.04%	0.006%
95	14.170	2144	2146	2147	rBV	382	190	0.01%	0.001%
96	14.256	2158	2160	2163	rBV	402	402	0.02%	0.003%
97	14.317	2168	2170	2173	rVB	552	405	0.02%	0.003%
98	14.780	2243	2246	2254	rVB4	1485	2424	0.11%	0.017%
99	15.249	2319	2323	2329	rVB6	3846	5328	0.23%	0.038%
100	15.310	2331	2333	2334	rBV	559	347	0.02%	0.002%




Sum of corrected areas: 13923622

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035214.D
Acq On : 20 Apr 2023 14:40
Operator : JC/MD
Sample : 02378-18DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COML1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

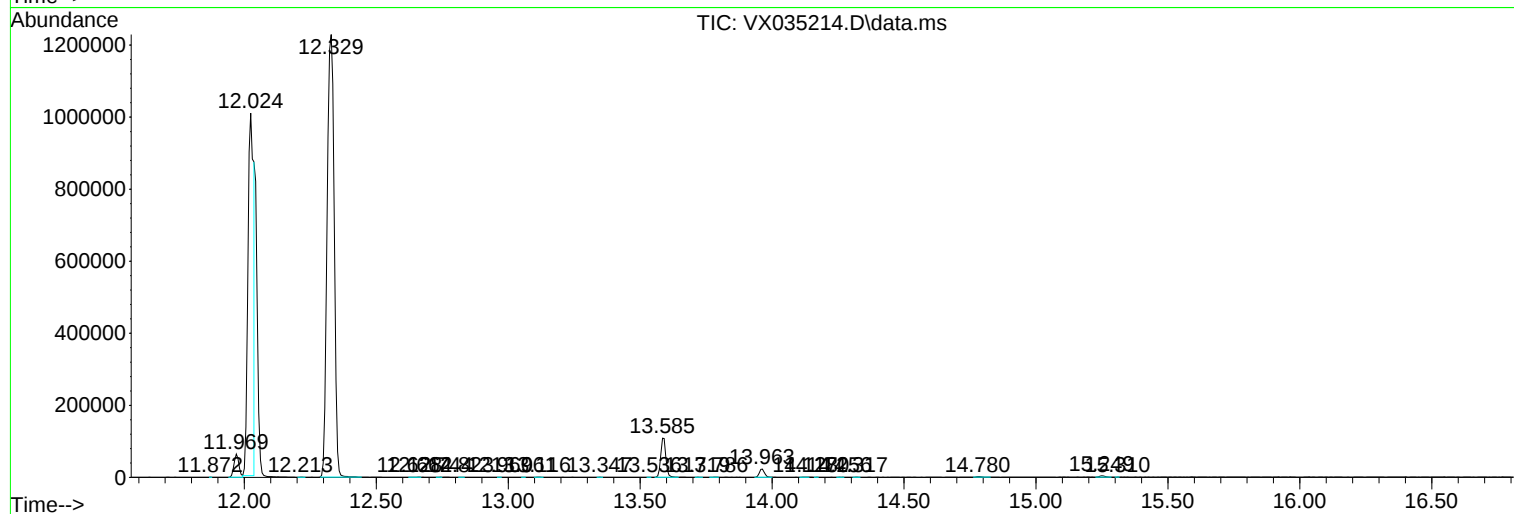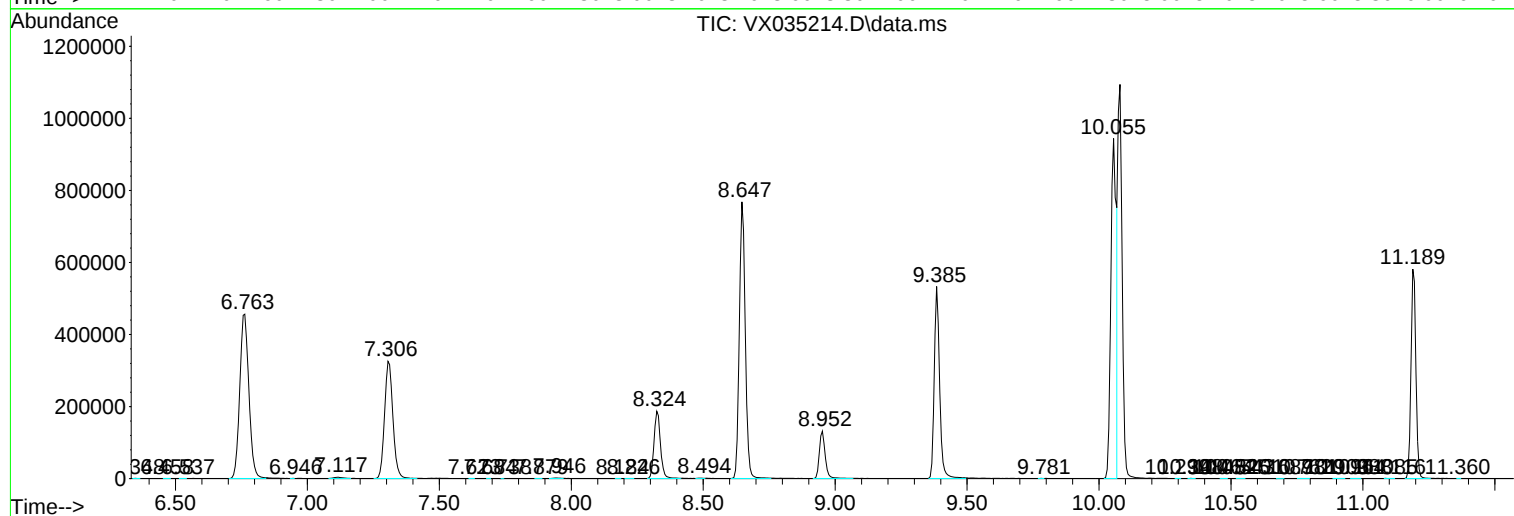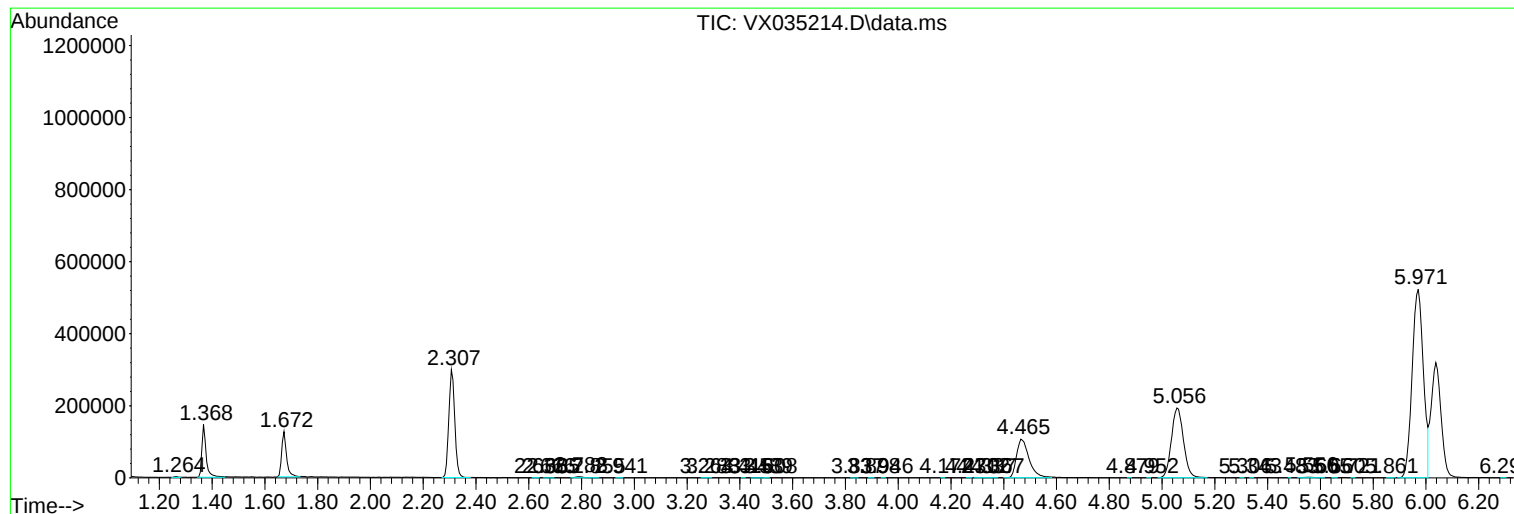

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035214.D
Acq On : 20 Apr 2023 14:40
Operator : JC/MD
Sample : 02378-18DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ML1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035214.D
Acq On : 20 Apr 2023 14:40
Operator : JC/MD
Sample : 02378-18DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ML1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------