

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035216.D
 Acq On : 20 Apr 2023 15:26
 Operator : JC/MD
 Sample : 02378-10 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035216.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	31	rBV2	2386	2120	0.15%	0.018%
2	1.368	42	46	59	rBV	130036	147173	10.19%	1.255%
3	1.672	92	96	110	rVB	112073	142683	9.88%	1.217%
4	2.307	194	200	213	rBV	268507	421831	29.20%	3.597%
5	2.508	231	233	237	rBV3	512	452	0.03%	0.004%
6	2.611	248	250	251	rBV	285	171	0.01%	0.001%
7	2.794	274	280	286	rVV3	2801	5755	0.40%	0.049%
8	2.947	303	305	307	rBV3	203	179	0.01%	0.002%
9	3.002	311	314	316	rVB	282	240	0.02%	0.002%
10	3.020	316	317	318	rBV	309	125	0.01%	0.001%
11	3.062	322	324	326	rVB2	395	300	0.02%	0.003%
12	3.087	326	328	331	rBV2	229	328	0.02%	0.003%
13	3.501	394	396	398	rBV	188	171	0.01%	0.001%
14	3.666	421	423	427	rVB3	189	219	0.02%	0.002%
15	3.825	447	449	453	rVB2	297	383	0.03%	0.003%
16	3.867	453	456	458	rBV2	244	233	0.02%	0.002%
17	3.983	472	475	476	rBV2	218	154	0.01%	0.001%
18	4.050	485	486	488	rBV	218	149	0.01%	0.001%
19	4.111	494	496	499	rVB	264	268	0.02%	0.002%
20	4.135	499	500	502	rBV	275	227	0.02%	0.002%
21	4.239	515	517	520	rBV2	247	260	0.02%	0.002%
22	4.465	545	554	577	rBV2	97426	320203	22.16%	2.730%
23	4.745	599	600	602	rBV2	325	183	0.01%	0.002%
24	4.946	631	633	635	rBV	365	311	0.02%	0.003%
25	4.965	635	636	638	rBV	247	187	0.01%	0.002%
26	5.056	638	651	667	rBV	175323	551459	38.17%	4.702%
27	5.330	694	696	698	rBV	245	187	0.01%	0.002%
28	5.373	700	703	704	rBV2	713	695	0.05%	0.006%
29	5.446	713	715	717	rVB	406	243	0.02%	0.002%
30	5.477	717	720	722	rBV	158	164	0.01%	0.001%
31	5.556	726	733	742	rVB3	2802	7753	0.54%	0.066%
32	5.635	744	746	750	rVB	245	223	0.02%	0.002%
33	5.672	750	752	753	rBV	257	189	0.01%	0.002%
34	5.763	763	767	768	rBV	306	274	0.02%	0.002%
35	5.855	780	782	786	rVB2	204	225	0.02%	0.002%
36	5.970	789	801	816	rBV2	467145	1407250	97.41%	11.999%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035216.D
 Acq On : 20 Apr 2023 15:26
 Operator : JC/MD
 Sample : 02378-10 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	6.324	857	859	861	rVB	244	140	0.01%	0.001%
38	6.355	862	864	865	rVB	346	168	0.01%	0.001%
39	6.391	868	870	871	rBV	293	241	0.02%	0.002%
40	6.446	877	879	881	rBV2	262	210	0.01%	0.002%
41	6.537	890	894	896	rBV3	493	772	0.05%	0.007%
42	6.763	921	931	946	rBV	519315	1248148	86.39%	10.643%
43	7.050	977	978	980	rBV2	274	163	0.01%	0.001%
44	7.117	983	989	998	rVV3	3868	9199	0.64%	0.078%
45	7.306	1011	1020	1038	rBV	298888	658430	45.57%	5.614%
46	7.476	1045	1048	1050	rBV2	710	936	0.06%	0.008%
47	7.549	1058	1060	1064	rVB2	212	218	0.02%	0.002%
48	7.604	1066	1069	1073	rVB2	199	326	0.02%	0.003%
49	7.635	1073	1074	1076	rBV2	278	201	0.01%	0.002%
50	7.720	1087	1088	1090	rBV	228	207	0.01%	0.002%
51	7.940	1118	1124	1130	rBV3	1612	3162	0.22%	0.027%
52	8.055	1139	1143	1145	rBV	248	379	0.03%	0.003%
53	8.324	1181	1187	1201	rVV	167011	284432	19.69%	2.425%
54	8.647	1234	1240	1250	rBV	695105	1088289	75.33%	9.280%
55	8.952	1284	1290	1306	rBV	118933	180846	12.52%	1.542%
56	9.153	1322	1323	1325	rBV	218	140	0.01%	0.001%
57	9.196	1327	1330	1332	rBV3	258	294	0.02%	0.003%
58	9.281	1340	1344	1347	rVB3	476	799	0.06%	0.007%
59	9.317	1348	1350	1353	rBV	213	187	0.01%	0.002%
60	9.384	1356	1361	1375	rBV	474769	684896	47.41%	5.840%
61	9.671	1407	1408	1412	rVB2	414	233	0.02%	0.002%
62	9.702	1412	1413	1415	rVB2	318	223	0.02%	0.002%
63	9.756	1420	1422	1423	rBV	413	307	0.02%	0.003%
64	9.927	1448	1450	1453	rVV4	289	298	0.02%	0.003%
65	10.055	1465	1471	1485	rBV	1013512	1444719	100.00%	12.319%
66	10.317	1510	1514	1515	rBV2	335	358	0.02%	0.003%
67	10.512	1544	1546	1548	rBV	285	176	0.01%	0.002%
68	10.659	1568	1570	1571	rBV	190	132	0.01%	0.001%
69	10.732	1580	1582	1584	rVB	163	127	0.01%	0.001%
70	10.762	1584	1587	1589	rBV	253	314	0.02%	0.003%
71	10.793	1590	1592	1595	rVV2	285	225	0.02%	0.002%
72	10.872	1603	1605	1607	rBV2	409	387	0.03%	0.003%
73	10.970	1618	1621	1623	rBV2	162	177	0.01%	0.002%
74	11.098	1638	1642	1645	rVB3	484	586	0.04%	0.005%
75	11.189	1652	1657	1669	rBV	517893	688056	47.63%	5.867%
76	11.549	1714	1716	1718	rVB	347	225	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035216.D
 Acq On : 20 Apr 2023 15:26
 Operator : JC/MD
 Sample : 02378-10 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041823WMA.M
 Title : VOC Analysis

77	11.707	1740	1742	1744	rVB2	479	413	0.03%	0.004%
78	11.738	1744	1747	1748	rVB2	310	198	0.01%	0.002%
79	11.756	1748	1750	1753	rBV2	161	126	0.01%	0.001%
80	11.799	1753	1757	1760	rBV3	296	411	0.03%	0.004%
81	11.975	1781	1786	1788	rBV3	2409	3236	0.22%	0.028%
82	12.024	1788	1794	1805	rVV	1010174	1355175	93.80%	11.555%
83	12.213	1823	1825	1827	rBV	369	386	0.03%	0.003%
84	12.317	1837	1842	1853	rBV	778838	1025707	71.00%	8.746%
85	12.683	1901	1902	1904	rBV2	273	164	0.01%	0.001%
86	12.719	1906	1908	1911	rBV2	315	348	0.02%	0.003%
87	12.756	1912	1914	1920	rVB4	832	1255	0.09%	0.011%
88	13.359	2011	2013	2018	rBV2	256	288	0.02%	0.002%
89	13.420	2022	2023	2025	rBV2	457	401	0.03%	0.003%
90	13.591	2046	2051	2057	rBV	14204	19821	1.37%	0.169%
91	13.713	2070	2071	2072	rBV	354	185	0.01%	0.002%
92	13.731	2072	2074	2076	rVB	288	191	0.01%	0.002%
93	13.908	2101	2103	2106	rVB2	356	375	0.03%	0.003%
94	13.939	2106	2108	2109	rBV2	345	369	0.03%	0.003%
95	13.963	2109	2112	2117	rVV2	3359	4308	0.30%	0.037%
96	14.018	2119	2121	2124	rBV2	290	391	0.03%	0.003%
97	14.103	2132	2135	2136	rBV	466	488	0.03%	0.004%
98	14.304	2166	2168	2169	rBV	492	314	0.02%	0.003%
99	14.585	2211	2214	2216	rBV	395	491	0.03%	0.004%
100	16.603	2543	2545	2546	rBV2	528	308	0.02%	0.003%




Sum of corrected areas: 11727642

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035216.D
Acq On : 20 Apr 2023 15:26
Operator : JC/MD
Sample : 02378-10 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

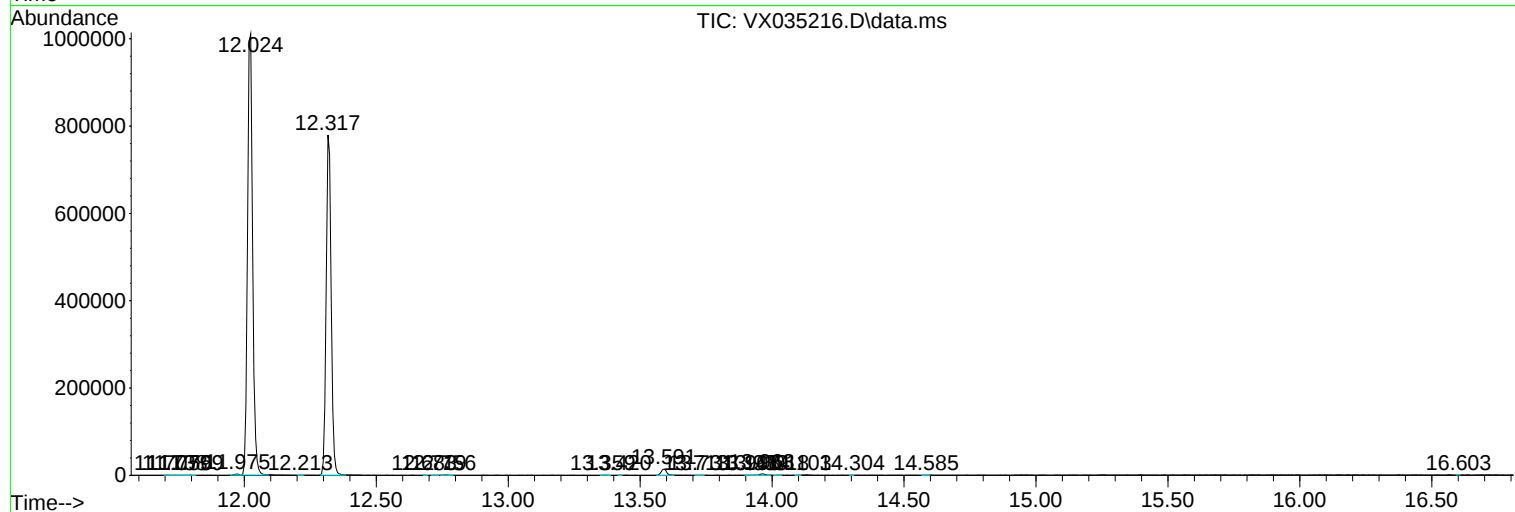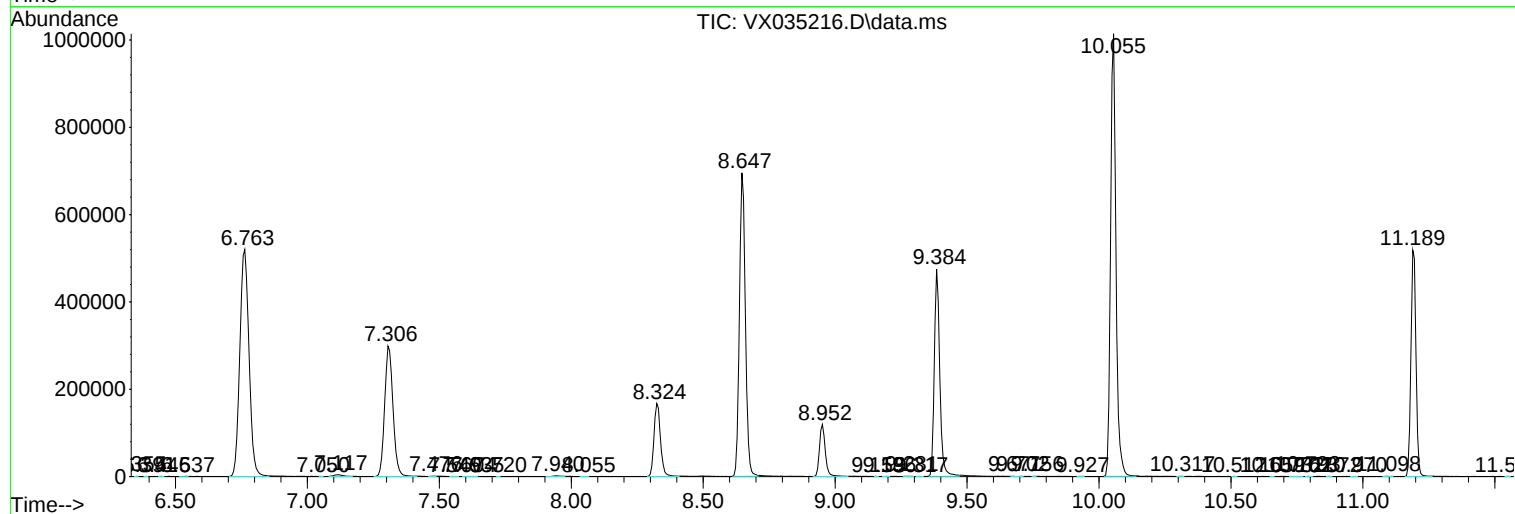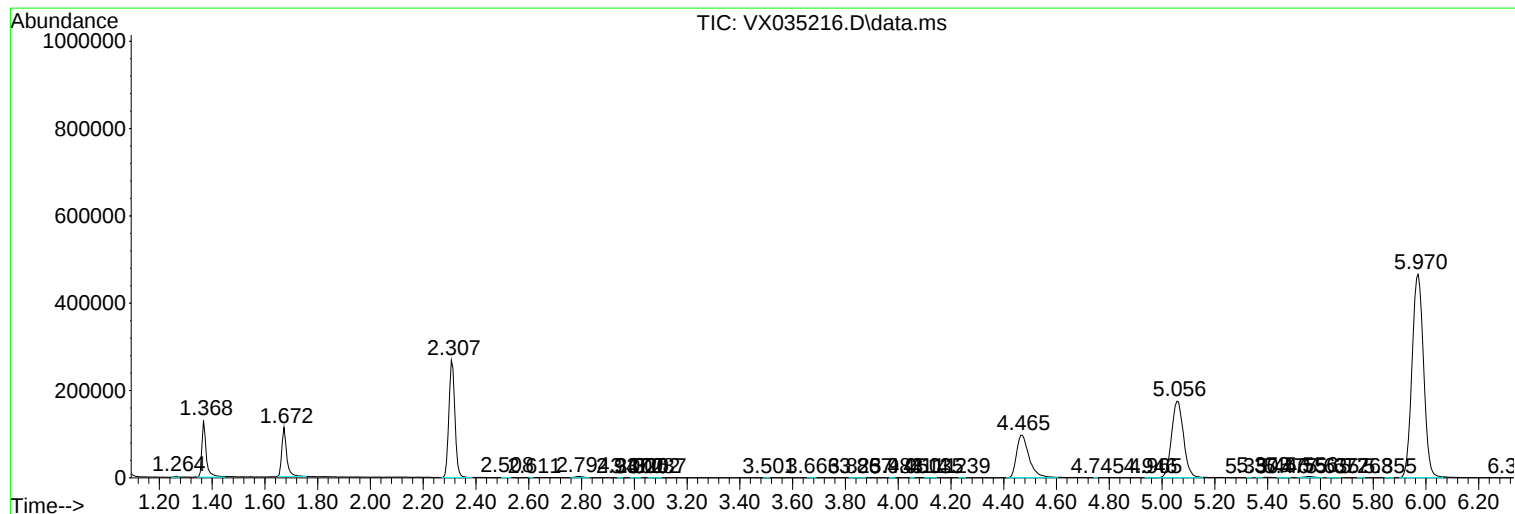

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035216.D
Acq On : 20 Apr 2023 15:26
Operator : JC/MD
Sample : 02378-10 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0MK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035216.D
Acq On : 20 Apr 2023 15:26
Operator : JC/MD
Sample : 02378-10 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0MK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------